

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL033020\
 Data File : PL057682.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Mar 2020 13:25
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 31 01:25:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031420.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 16 09:40:37 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.459	3.958	245.8E6	52946864	26.515	24.405
28)	SA Decachlor...	8.207	8.981	195.1E6	46361555	18.439	20.908
Target Compounds							
2)	A alpha-BHC	3.896	0.000	4142167	0	0.260	N.D. #
11)	B alpha-Chl...	5.452	0.000	786433	0	0.061	N.D. #
14)	MA Endrin	5.999	0.000	304343	0	0.027	N.D. #
15)	B Endosulfa...	6.284	0.000	4342589	0	0.400	N.D. #
19)	B Endosulfa...	6.691f	0.000	154976	0	0.015	N.D. #
20)	A Methoxychlor	6.922	0.000	29882	0	0.006	N.D. #
22)	Mirex	7.344	0.000	493747	0	0.061	N.D. #
23)	Chlordane-1	4.357f	0.000	2833290	0	8.729	N.D. #
24)	Chlordane-2	4.830	0.000	1791669	0	4.931	N.D. #
26)	Chlordane-4	5.452	0.000	786433	0	0.820	N.D. #
27)	Chlordane-5	6.284	0.000	4342589	0	11.935	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL033020\
Data File : PL057682.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Mar 2020 13:25
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 31 01:25:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031420.M
Quant Title : GC Extractables
QLast Update : Mon Mar 16 09:40:37 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

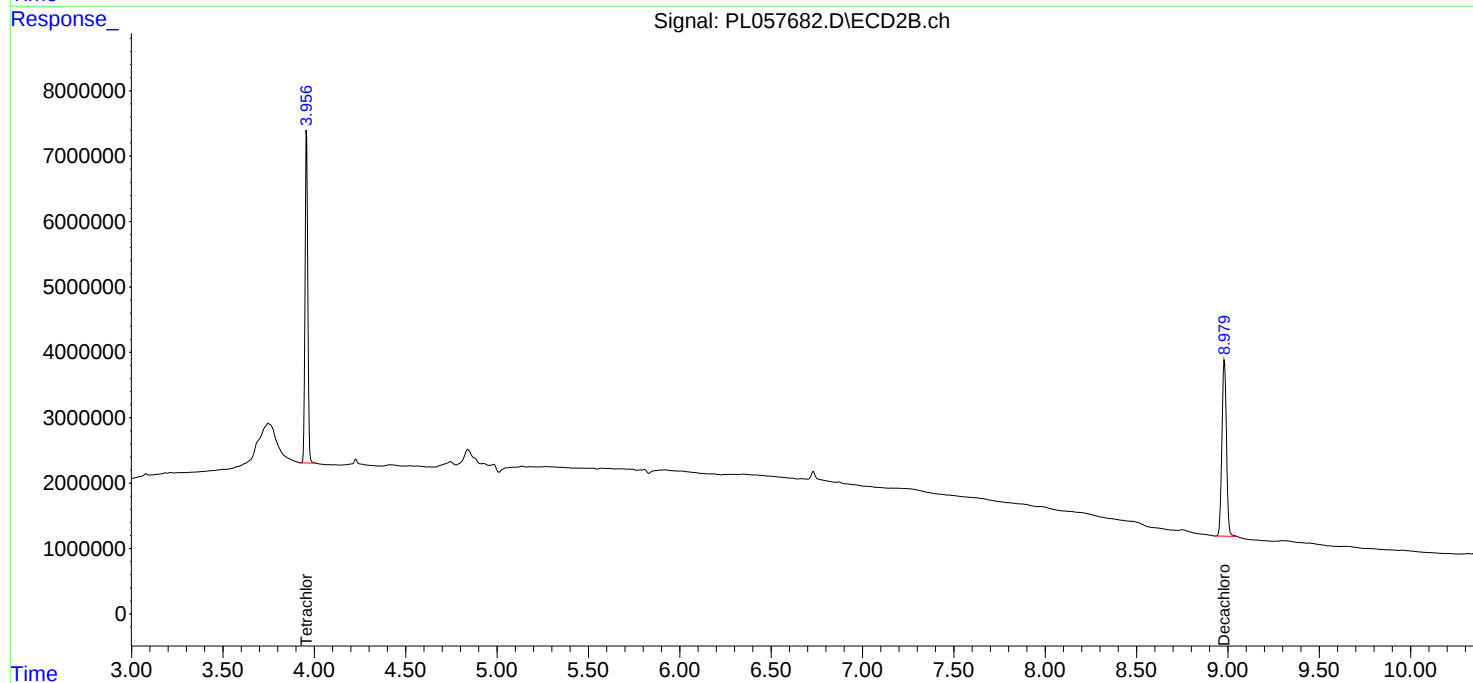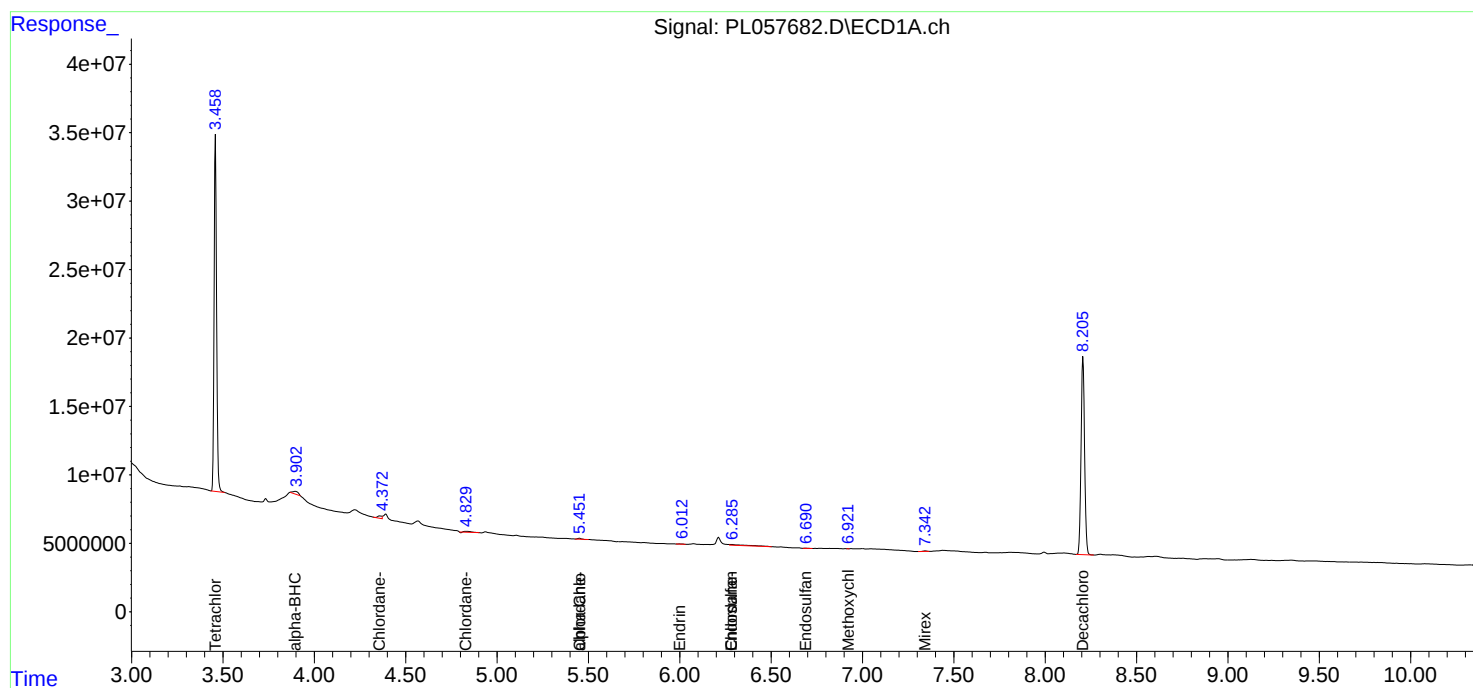


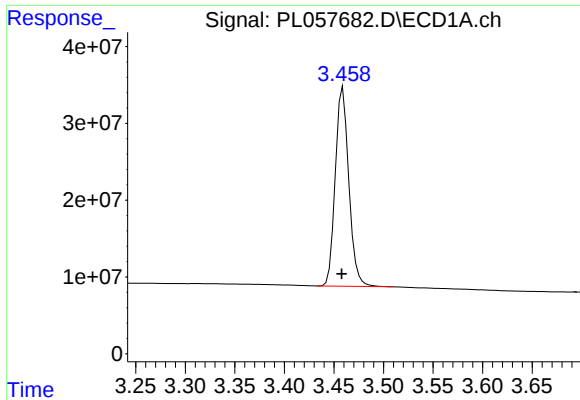

#1 Tetrachloro-m-xylene


R.T.: 3.459 min
Delta R.T.: 0.001 min
Response: 245780097
Conc: 26.52 ng/ml

Instrument :
ECD_L
ClientSampleId :

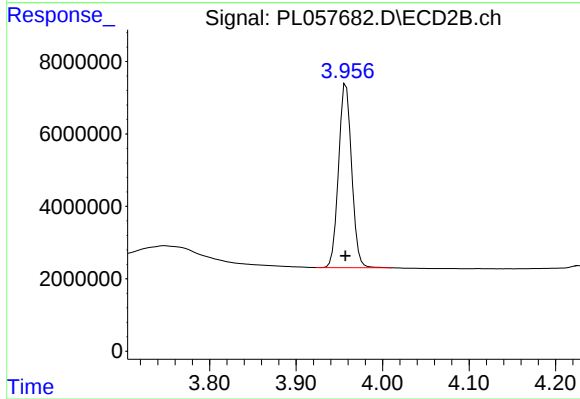


#1 Tetrachloro-m-xylene

R.T.: 3.958 min
Delta R.T.: 0.000 min
Response: 52946864
Conc: 24.40 ng/ml

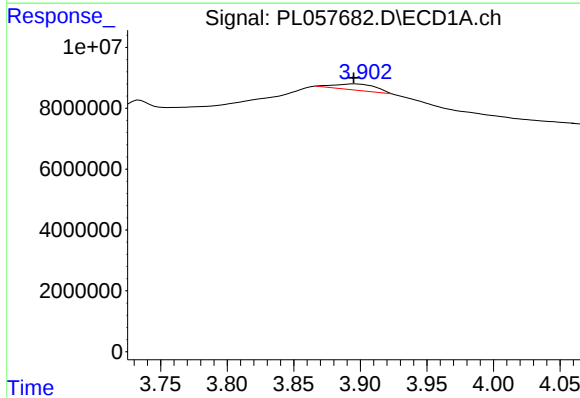


#2 alpha-BHC

R.T.: 3.896 min
Delta R.T.: 0.001 min
Response: 4142167
Conc: 0.26 ng/ml

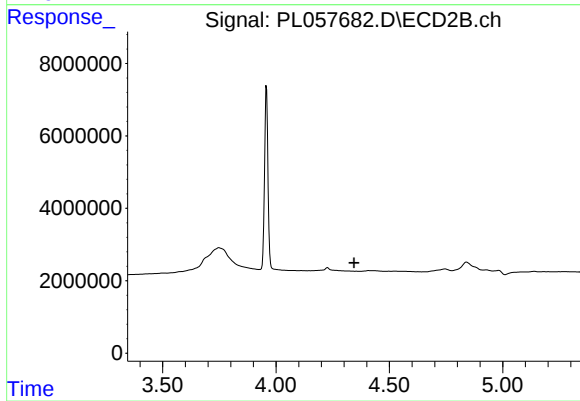

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.345 min
Response: 0
Conc: N.D.

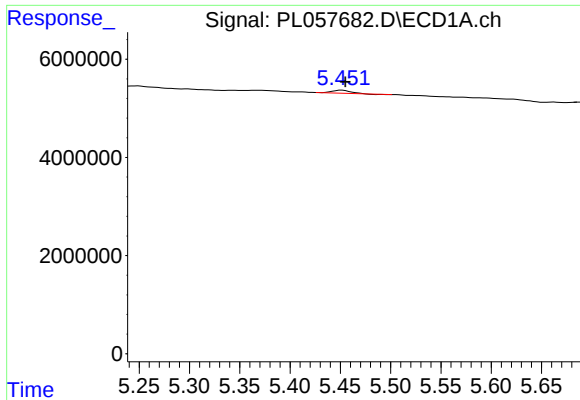

#11 alpha-Chlordane


R.T.: 5.452 min
Delta R.T.: -0.003 min
Response: 786433
Conc: 0.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

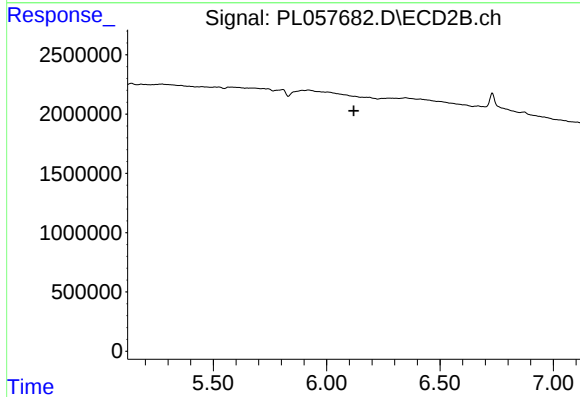


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.120 min
Response: 0
Conc: N.D.

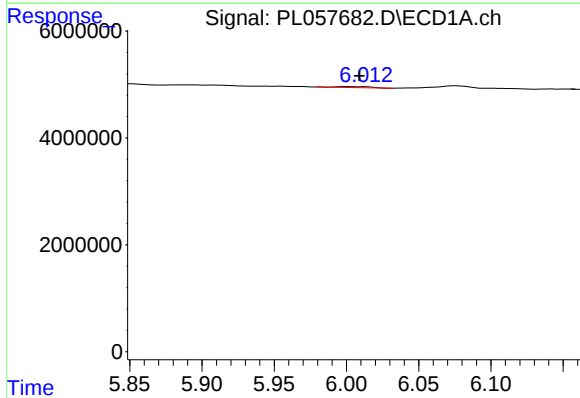


#14 Endrin

R.T.: 5.999 min
Delta R.T.: -0.010 min
Response: 304343
Conc: 0.03 ng/ml

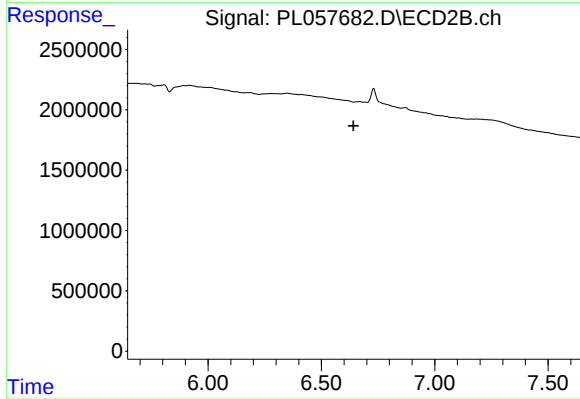

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.642 min
Response: 0
Conc: N.D.

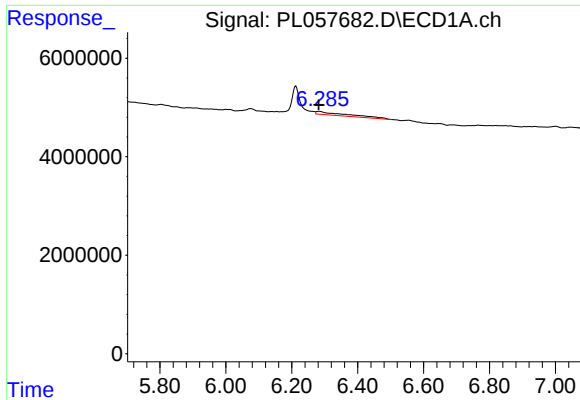

#15 Endosulfan II


R.T.: 6.284 min
Delta R.T.: 0.002 min
Response: 4342589
Conc: 0.40 ng/ml

Instrument :
ECD_L
ClientSampleId :

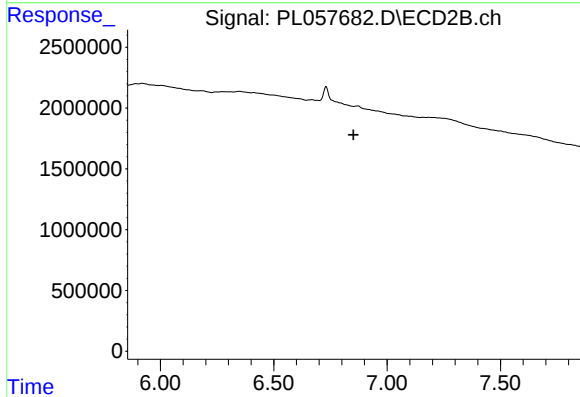


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.852 min
Response: 0
Conc: N.D.

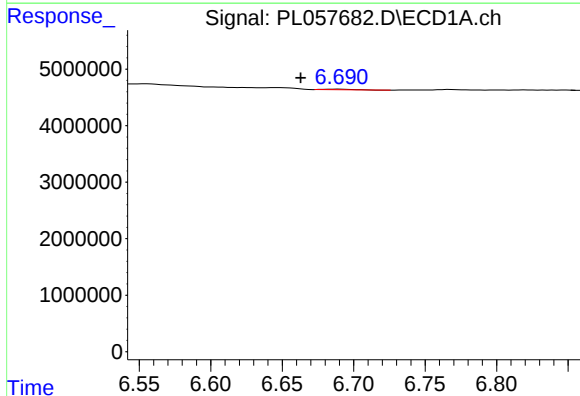


#19 Endosulfan Sulfate

R.T.: 6.691 min
Delta R.T.: 0.028 min
Response: 154976
Conc: 0.02 ng/ml

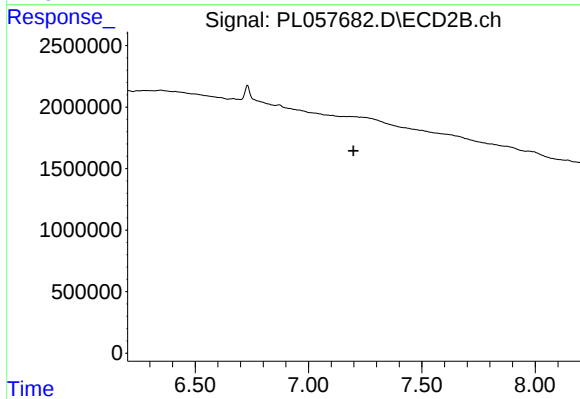

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 7.199 min
Response: 0
Conc: N.D.

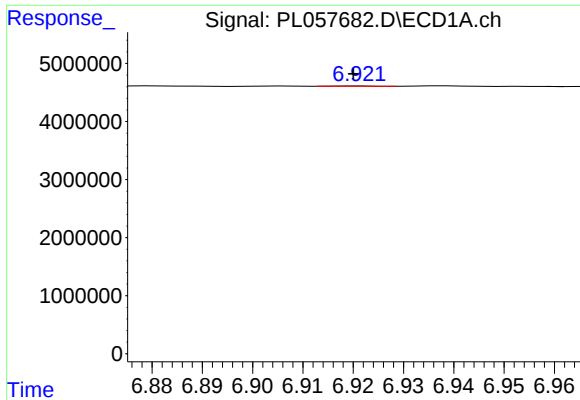

#20 Methoxychlor


R.T.: 6.922 min
Delta R.T.: 0.002 min
Response: 29882
Conc: 0.01 ng/ml

Instrument :
ECD_L
ClientSampleId :

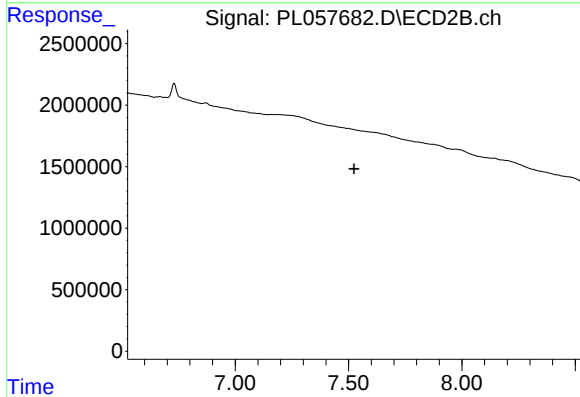


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.524 min
Response: 0
Conc: N.D.

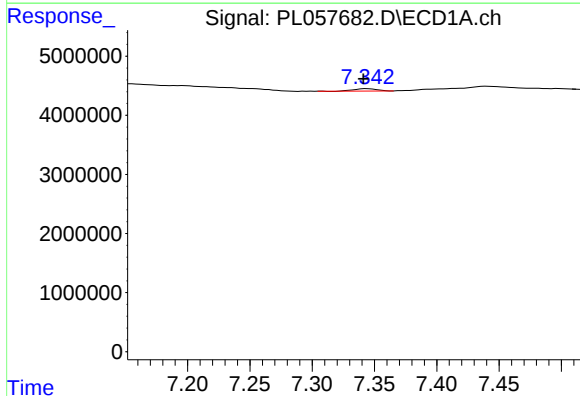


#22 Mirex

R.T.: 7.344 min
Delta R.T.: 0.003 min
Response: 493747
Conc: 0.06 ng/ml

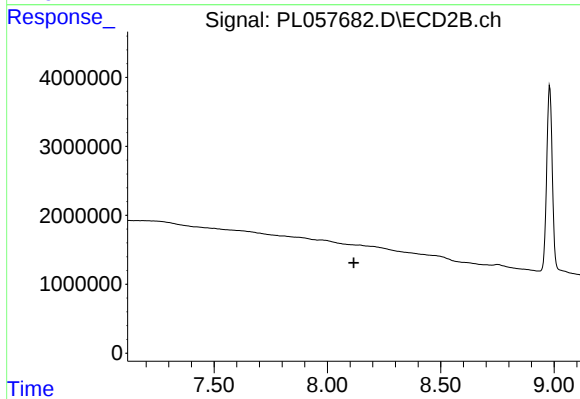

#22 Mirex


R.T.: 0.000 min
Exp R.T. : 8.116 min
Response: 0
Conc: N.D.

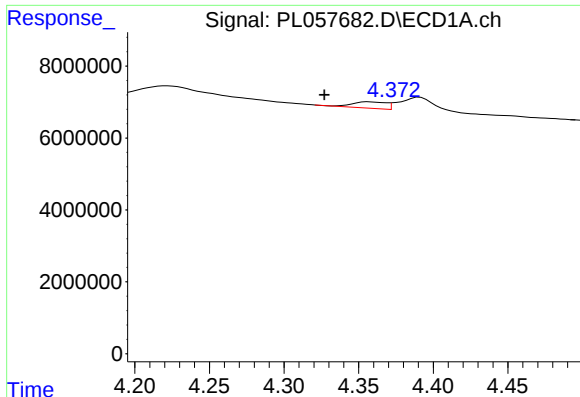

#23 Chlordane-1


R.T.: 4.357 min
Delta R.T.: 0.030 min
Response: 2833290
Conc: 8.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

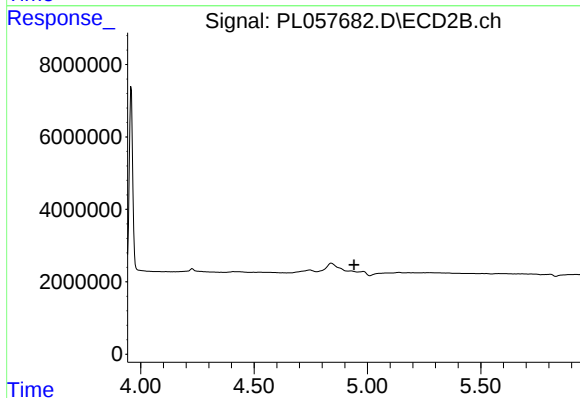


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.941 min
Response: 0
Conc: N.D.

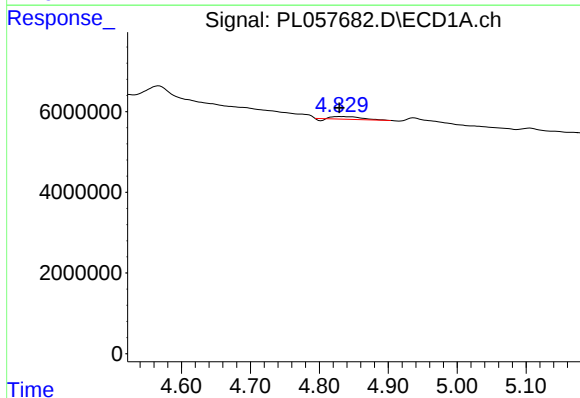


#24 Chlordane-2

R.T.: 4.830 min
Delta R.T.: 0.001 min
Response: 1791669
Conc: 4.93 ng/ml

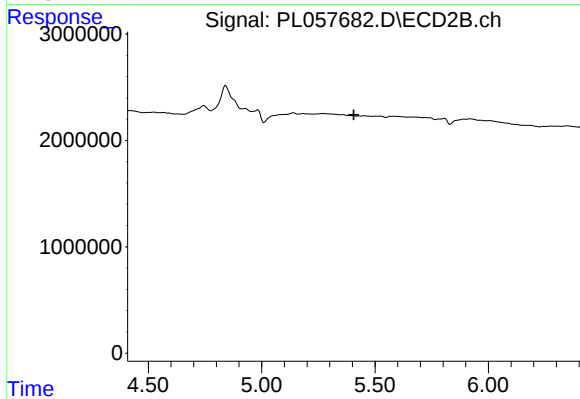

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.406 min
Response: 0
Conc: N.D.

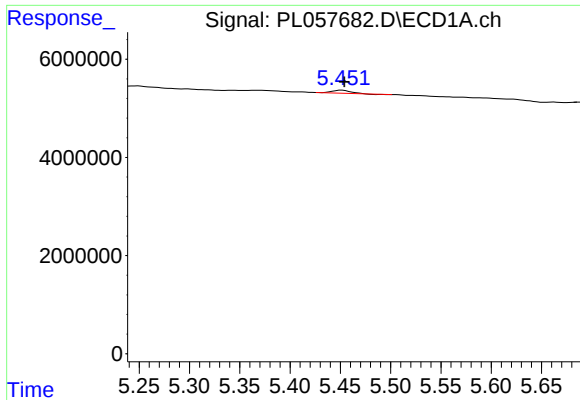

#26 Chlordane-4


R.T.: 5.452 min
Delta R.T.: -0.002 min
Response: 786433
Conc: 0.82 ng/ml

Instrument :
ECD_L
ClientSampleId :

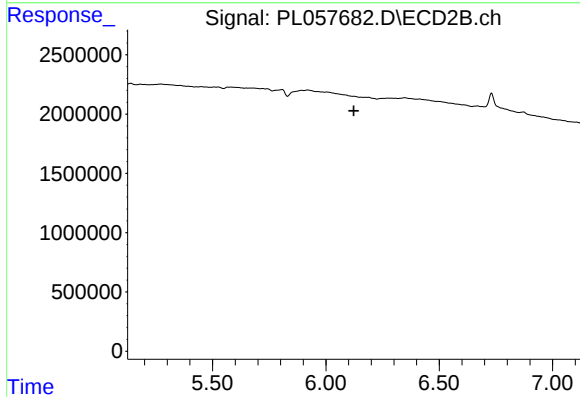


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.122 min
Response: 0
Conc: N.D.

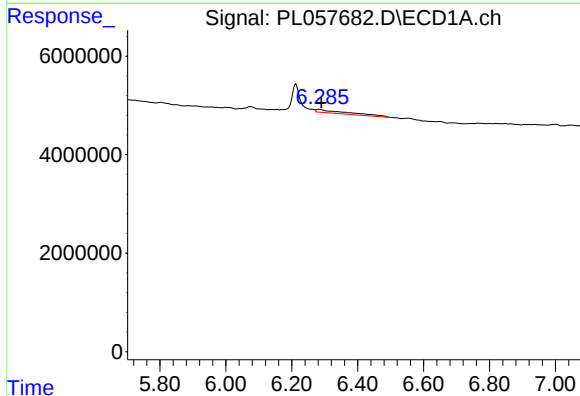


#27 Chlordane-5

R.T.: 6.284 min
Delta R.T.: -0.006 min
Response: 4342589
Conc: 11.93 ng/ml

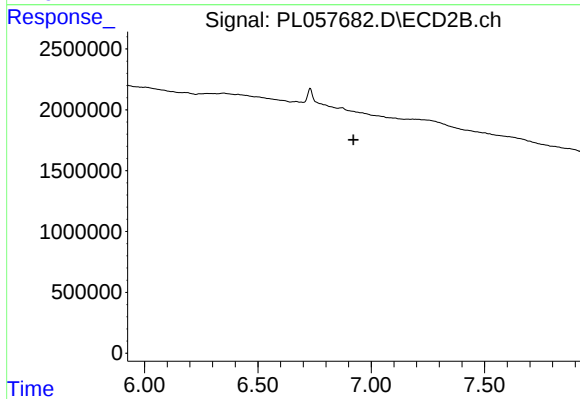

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 6.922 min
Response: 0
Conc: N.D.

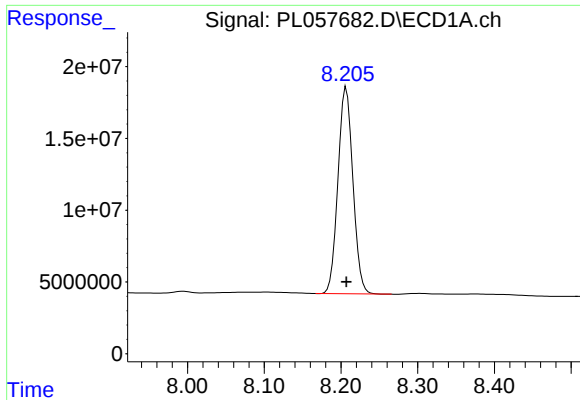

#28 Decachlorobiphenyl

R.T.: 8.207 min
Delta R.T.: 0.000 min
Response: 195106746
Conc: 18.44 ng/ml

Instrument :
ECD_L
ClientSampleId :

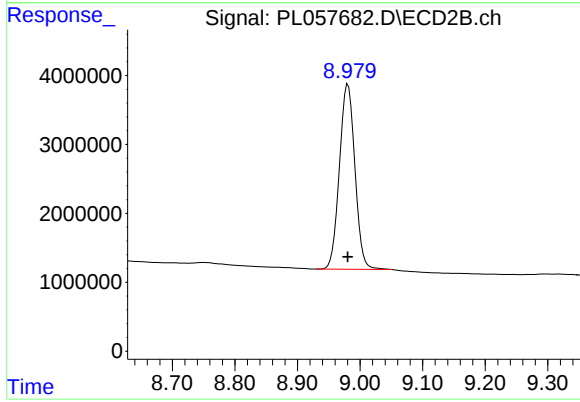

#28 Decachlorobiphenyl

R.T.: 8.981 min
Delta R.T.: 0.000 min
Response: 46361555
Conc: 20.91 ng/ml