

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL033022\
 Data File : PL073744.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Mar 2022 09:24
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 31 00:38:25 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 04:12:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.642	5.490	7156826	37623989	22.345	22.924
28)	SA Decachlor...	10.415	11.332	11230475	36776943	22.086	20.567
Target Compounds							
2)	A alpha-BHC	5.379f	0.000	20224	0	0.049	N.D. #
6)	B beta-BHC	0.000	6.682	0	518993	N.D.	0.498 #
7)	B delta-BHC	0.000	6.957	0	2559208	N.D.	1.188 #
10)	B gamma-Chl...	0.000	8.202	0	988836	N.D.	0.484 #
13)	MA Dieldrin	7.774	0.000	49438	0	0.119	N.D. #
14)	MA Endrin	8.090f	0.000	184610	0	0.476	N.D. #
15)	B Endosulfa...	8.353f	9.054	34369	303501	0.088	0.198 #
16)	A 4,4'-DDD	0.000	9.007f	0	534449	N.D.	0.366 #
23)	Chlordane-1	0.000	6.854	0	844659	N.D.	12.364 #
25)	Chlordane-3	0.000	8.202	0	988836	N.D.	3.647 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL033022\
Data File : PL073744.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Mar 2022 09:24
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 31 00:38:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 04:12:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

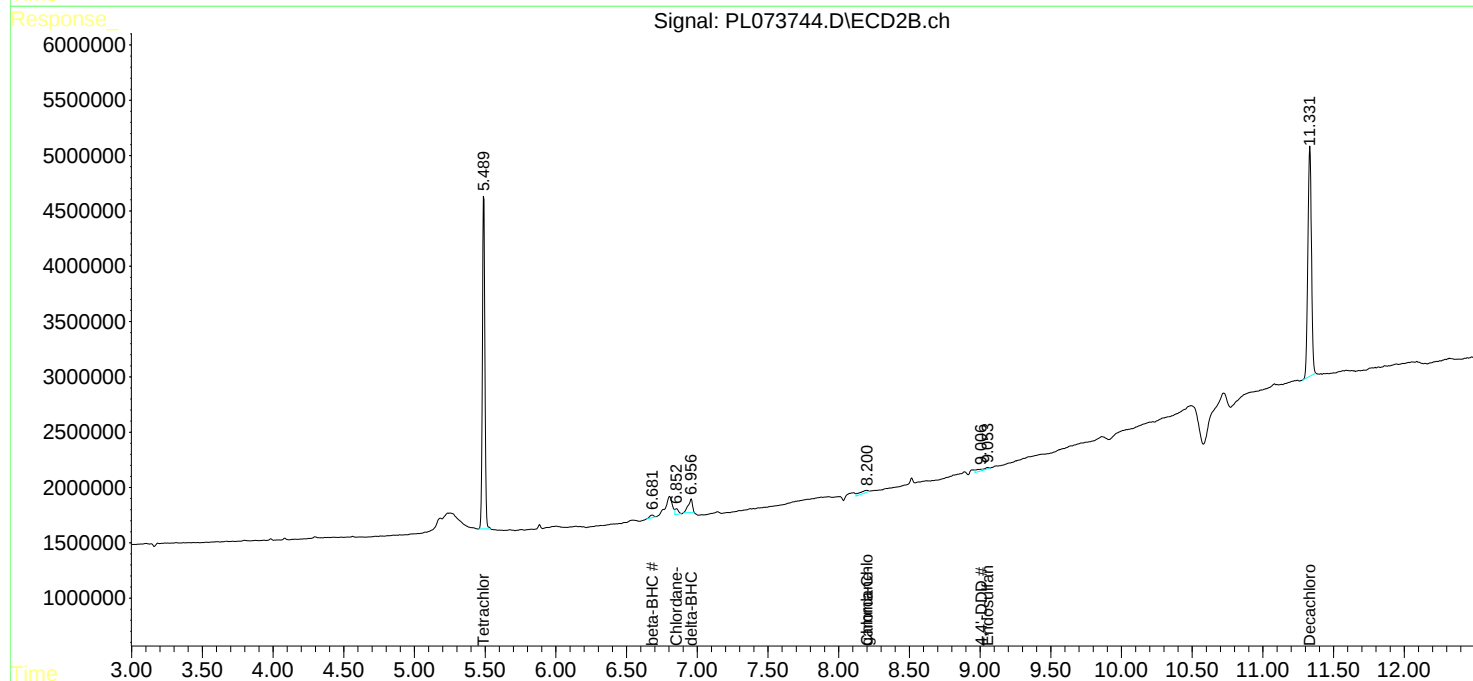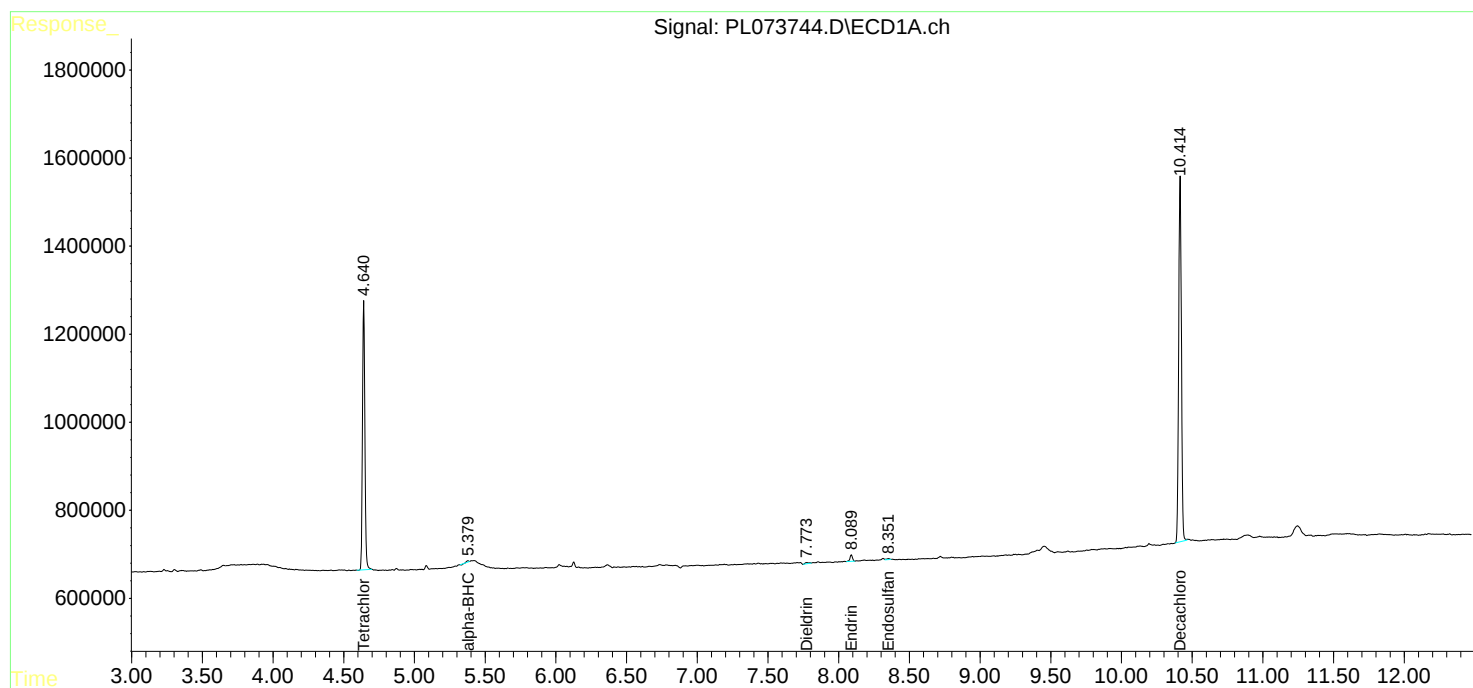


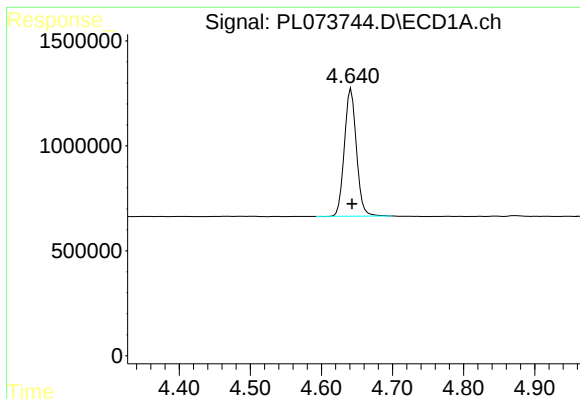

#1 Tetrachloro-m-xylene


R.T.: 4.642 min
Delta R.T.: -0.001 min
Response: 7156826
Conc: 22.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

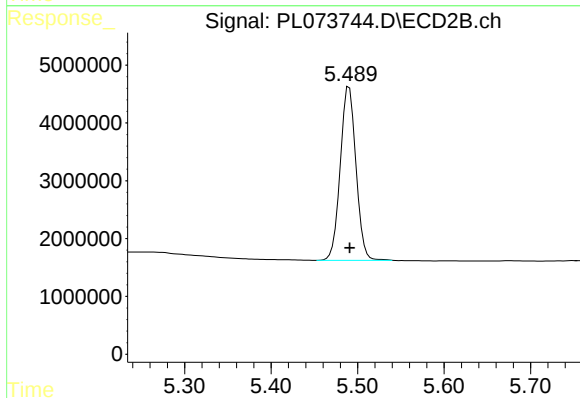


#1 Tetrachloro-m-xylene

R.T.: 5.490 min
Delta R.T.: 0.000 min
Response: 37623989
Conc: 22.92 ng/ml

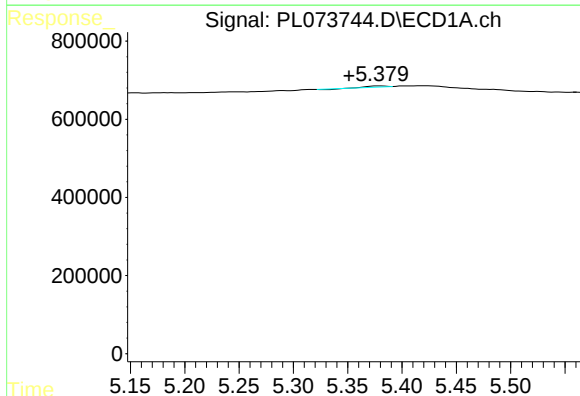


#2 alpha-BHC

R.T.: 5.379 min
Delta R.T.: 0.028 min
Response: 20224
Conc: 0.05 ng/ml

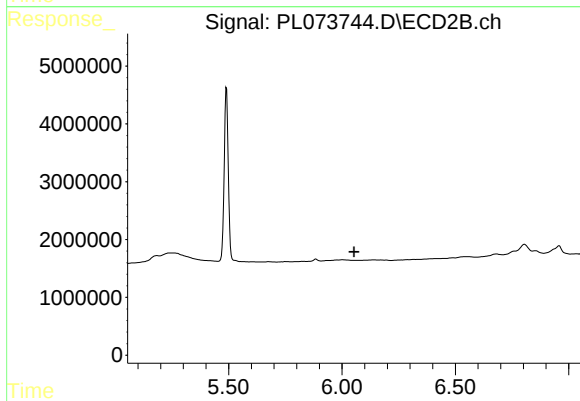

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 6.054 min
Response: 0
Conc: N.D.

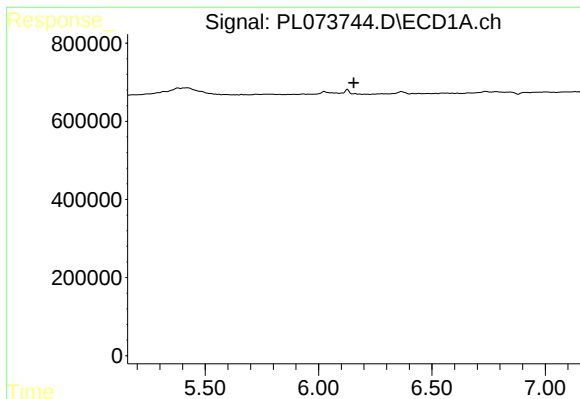

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 6.155 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

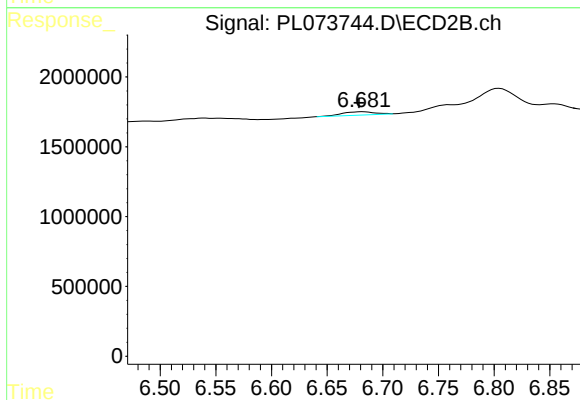


#6 beta-BHC

R.T.: 6.682 min
Delta R.T.: 0.004 min
Response: 518993
Conc: 0.50 ng/ml

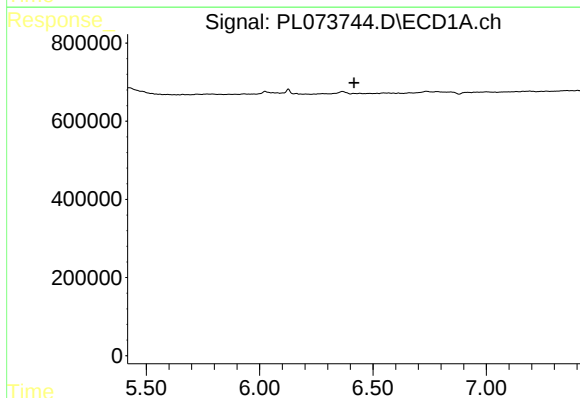


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 6.416 min
Response: 0
Conc: N.D.

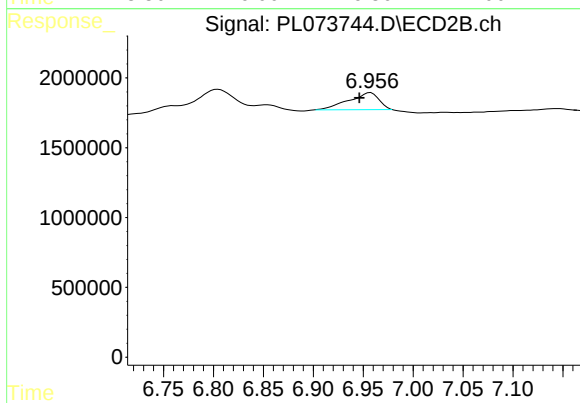

#7 delta-BHC


R.T.: 6.957 min
Delta R.T.: 0.011 min
Response: 2559208
Conc: 1.19 ng/ml

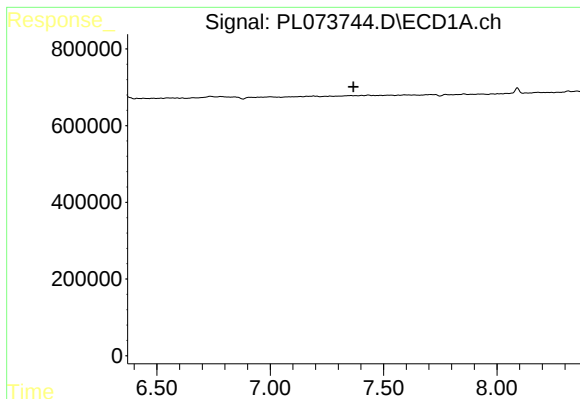

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.368 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

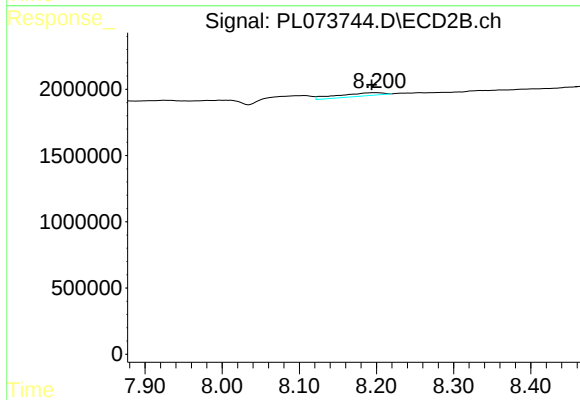


#10 gamma-Chlordane

R.T.: 8.202 min
Delta R.T.: 0.008 min
Response: 988836
Conc: 0.48 ng/ml

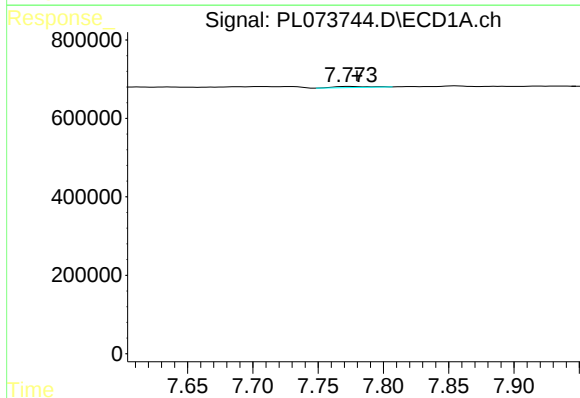


#13 Dieldrin

R.T.: 7.774 min
Delta R.T.: -0.005 min
Response: 49438
Conc: 0.12 ng/ml

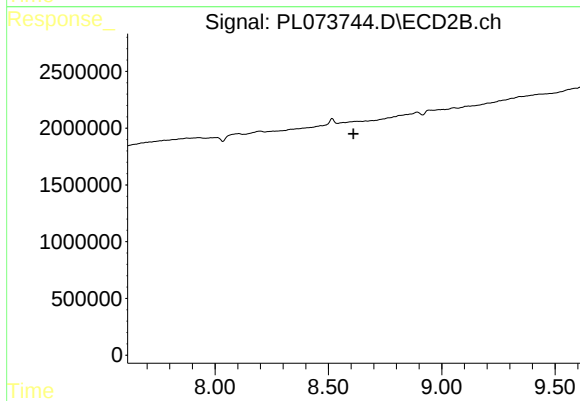

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 8.611 min
Response: 0
Conc: N.D.

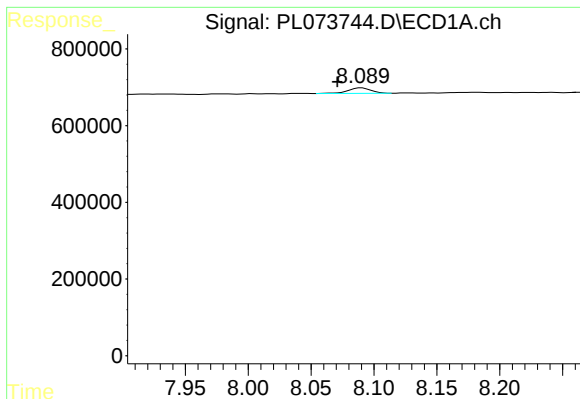

#14 Endrin


R.T.: 8.090 min
Delta R.T.: 0.019 min
Response: 184610
Conc: 0.48 ng/ml

Instrument :
ECD_L
ClientSampleId :

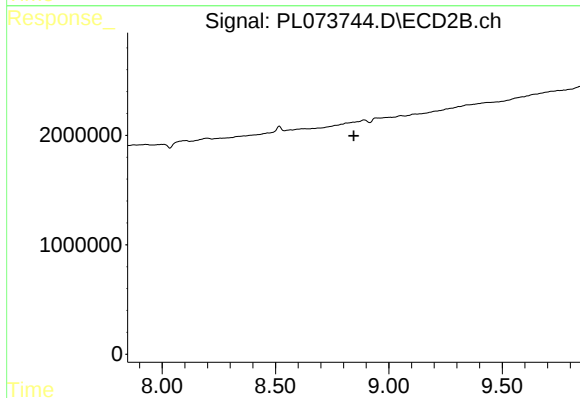


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 8.845 min
Response: 0
Conc: N.D.

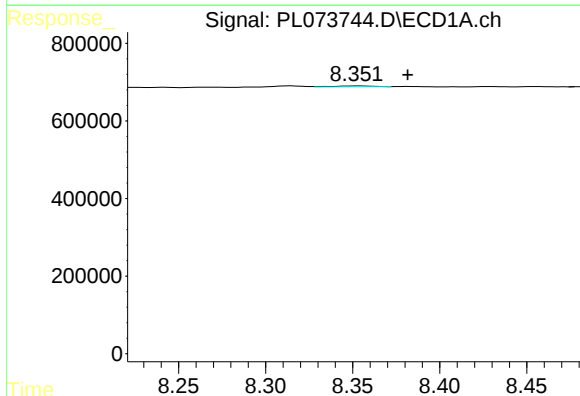


#15 Endosulfan II

R.T.: 8.353 min
Delta R.T.: -0.029 min
Response: 34369
Conc: 0.09 ng/ml

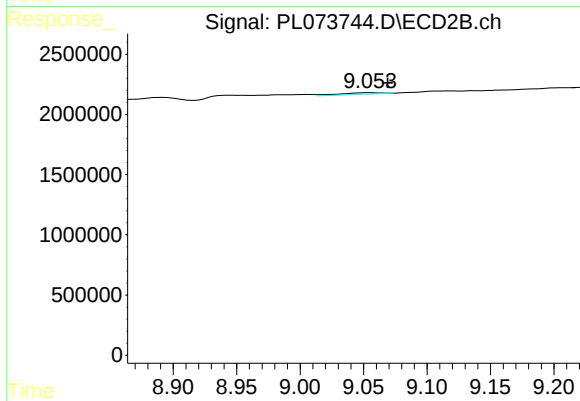

#15 Endosulfan II


R.T.: 9.054 min
Delta R.T.: -0.015 min
Response: 303501
Conc: 0.20 ng/ml

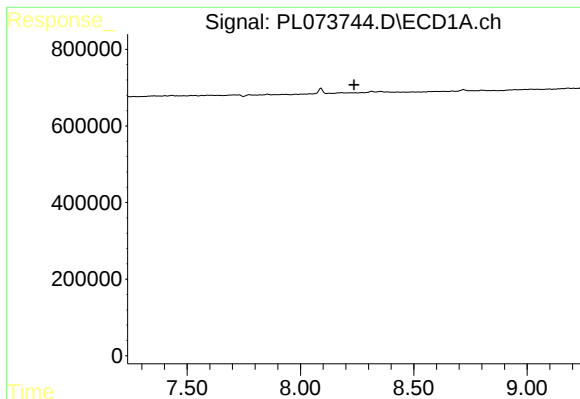

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 8.237 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

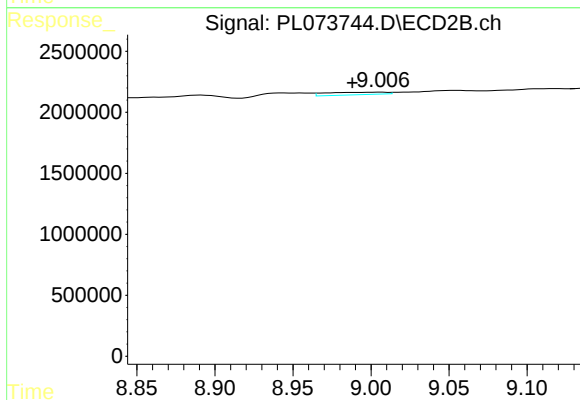


#16 4,4'-DDD

R.T.: 9.007 min
Delta R.T.: 0.019 min
Response: 534449
Conc: 0.37 ng/ml

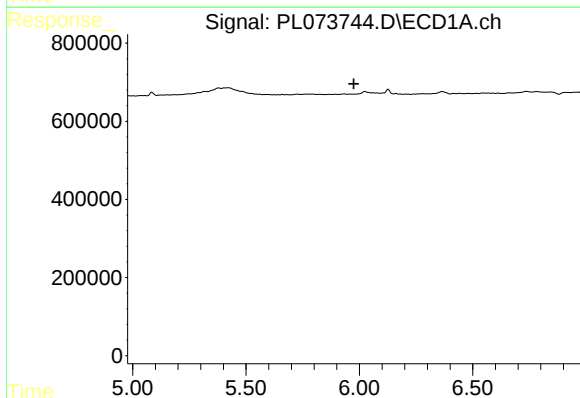


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.976 min
Response: 0
Conc: N.D.

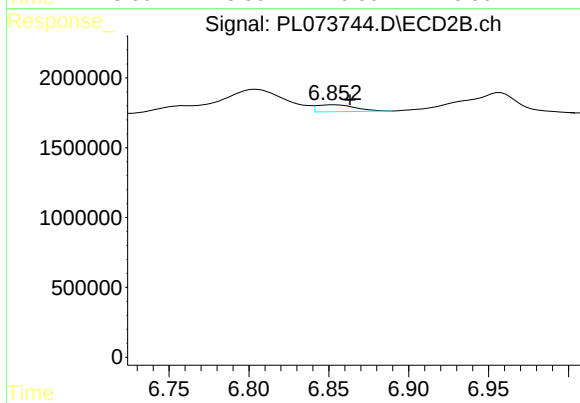

#23 Chlordane-1


R.T.: 6.854 min
Delta R.T.: -0.010 min
Response: 844659
Conc: 12.36 ng/ml

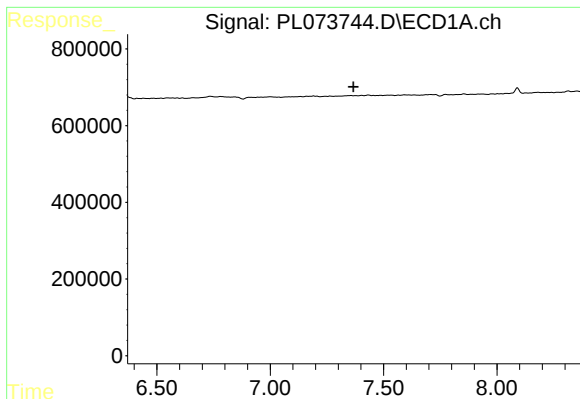

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.368 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

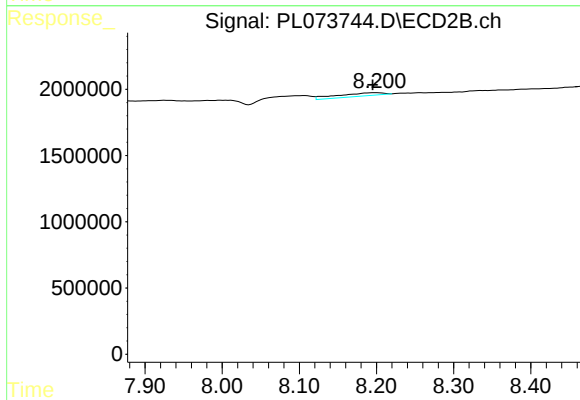


#25 Chlordane-3

R.T.: 8.202 min
Delta R.T.: 0.006 min
Response: 988836
Conc: 3.65 ng/ml

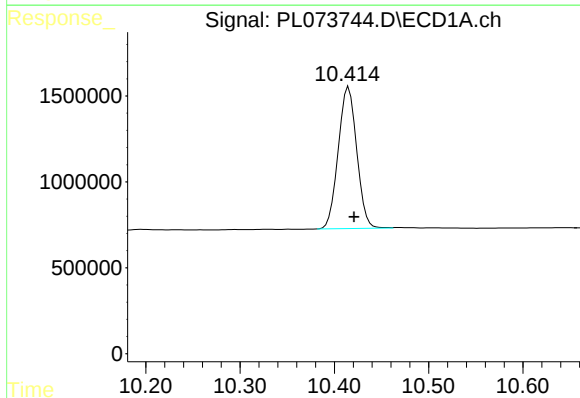

#28 Decachlorobiphenyl

R.T.: 10.415 min
Delta R.T.: -0.006 min
Response: 11230475
Conc: 22.09 ng/ml

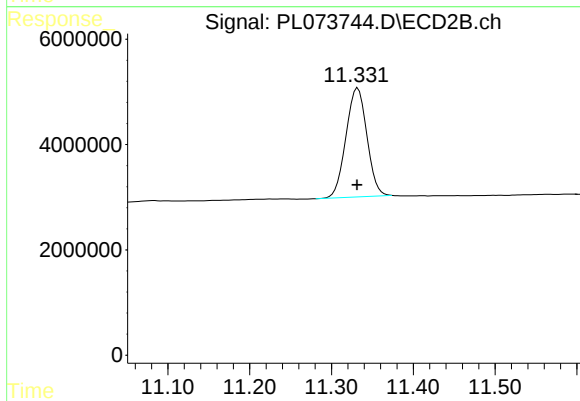

#28 Decachlorobiphenyl

R.T.: 11.332 min
Delta R.T.: 0.000 min
Response: 36776943
Conc: 20.57 ng/ml