

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL033022\
 Data File : PL073747.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Mar 2022 11:38
 Operator : AR\AJ
 Sample : N2149-01DL 5X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PILE-LINDEN-SWITCHDL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 31 01:50:21 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 04:12:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.649	5.487	682569	3366349	2.131	2.051
28)	SA Decachlor...	10.419	11.332	1838673	5173502	3.616	2.893
Target Compounds							
2)	A alpha-BHC	5.356	6.049	279471	1296206	0.678	0.576m
12)	B 4,4'-DDE	7.653	8.460	13527366	79158292	37.698	44.164
16)	A 4,4'-DDD	8.236	8.991	479967	3335650	1.478m	2.285m#
17)	MA 4,4'-DDT	8.498	9.306	6293821	29588249	16.642	18.102



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL033022\
Data File : PL073747.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Mar 2022 11:38
Operator : AR\AJ
Sample : N2149-01DL 5X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PILE-LINDEN-SWITCHDL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 31 01:50:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 04:12:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

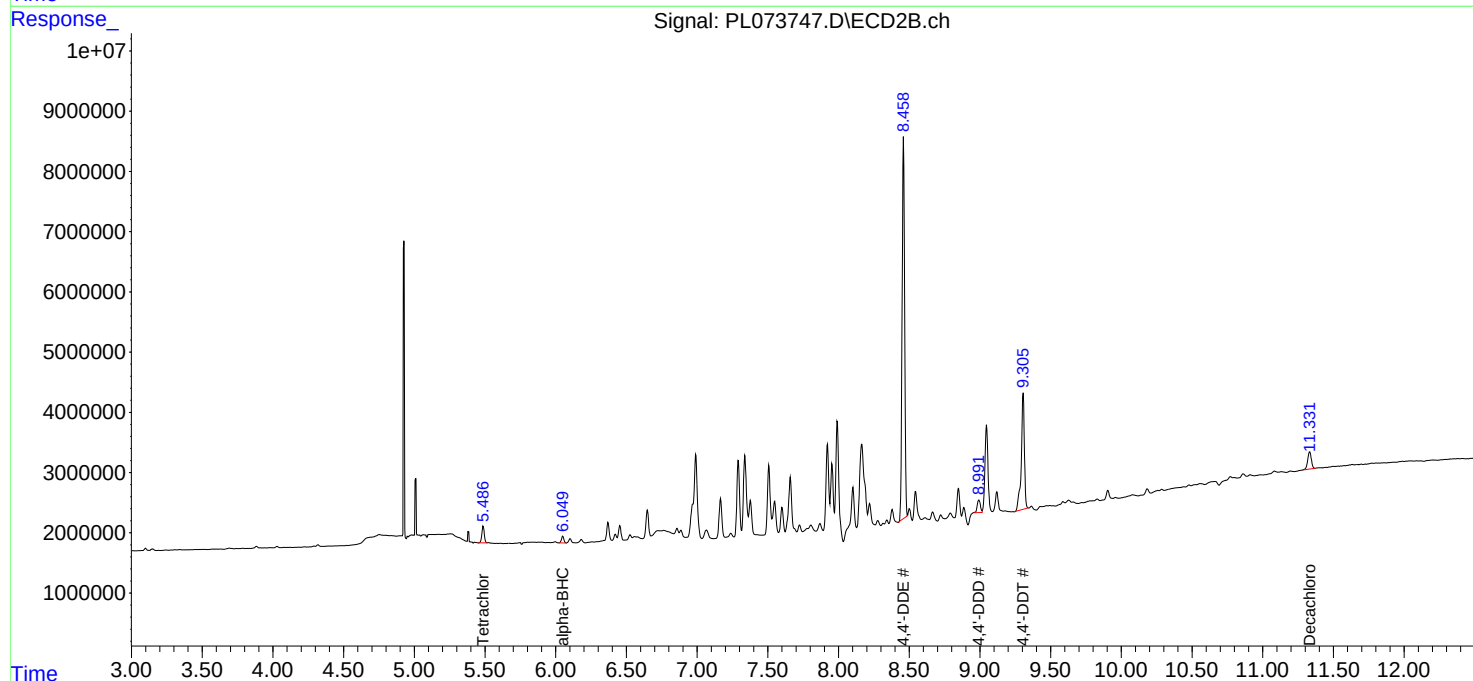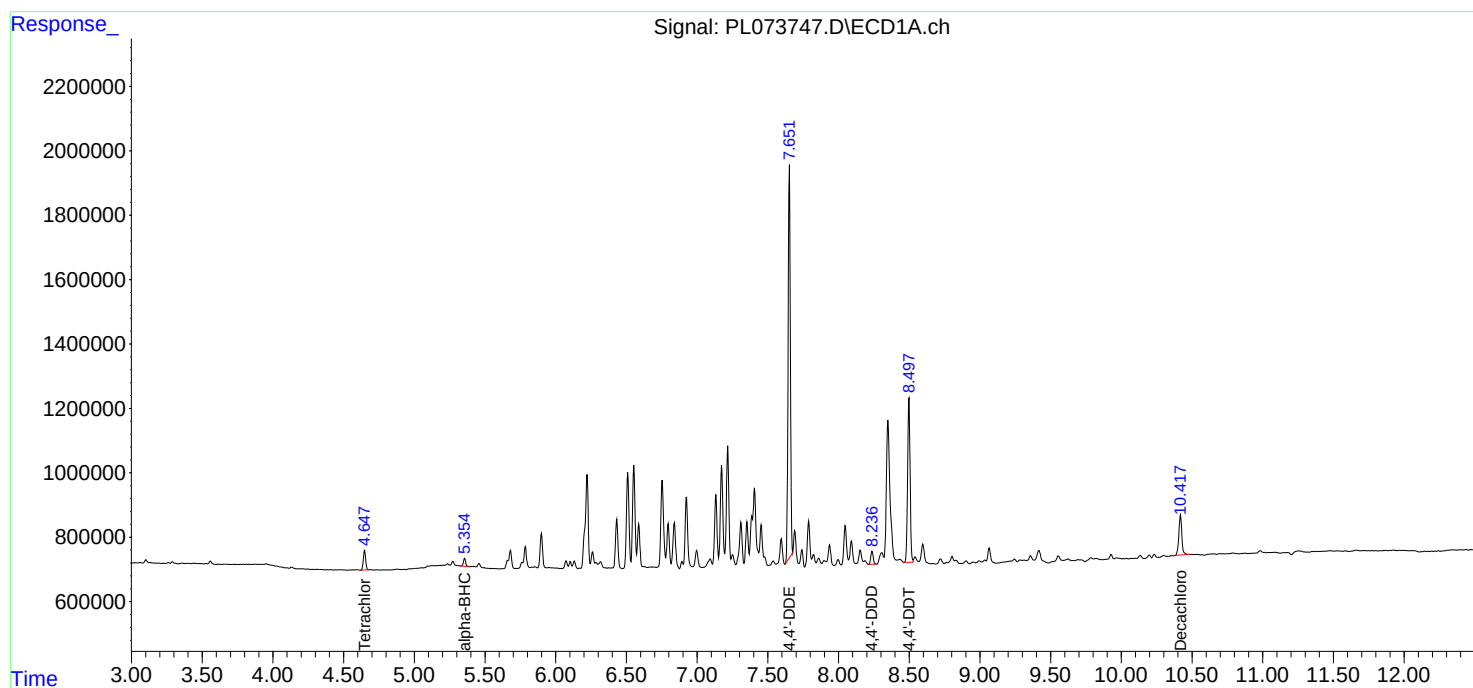


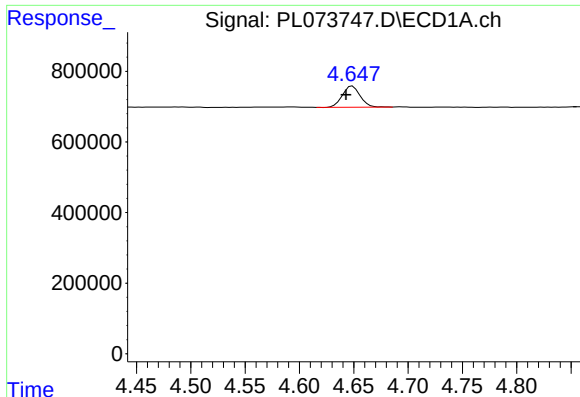

#1 Tetrachloro-m-xylene


R.T.: 4.649 min
Delta R.T.: 0.006 min
Response: 682569
Conc: 2.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
PILE-LINDEN-SWITCHDL

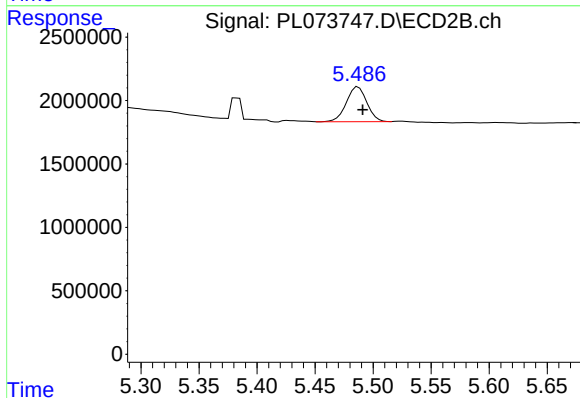


#1 Tetrachloro-m-xylene

R.T.: 5.487 min
Delta R.T.: -0.004 min
Response: 3366349
Conc: 2.05 ng/ml

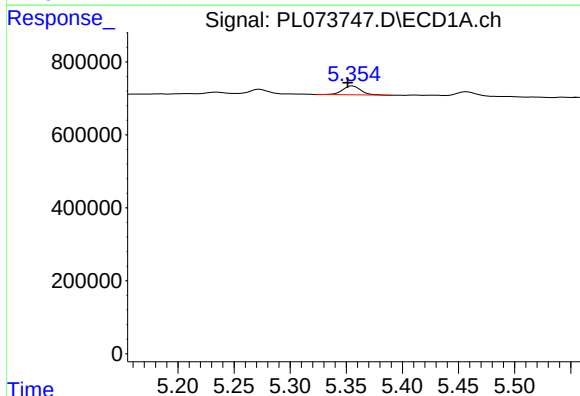


#2 alpha-BHC

R.T.: 5.356 min
Delta R.T.: 0.005 min
Response: 279471
Conc: 0.68 ng/ml

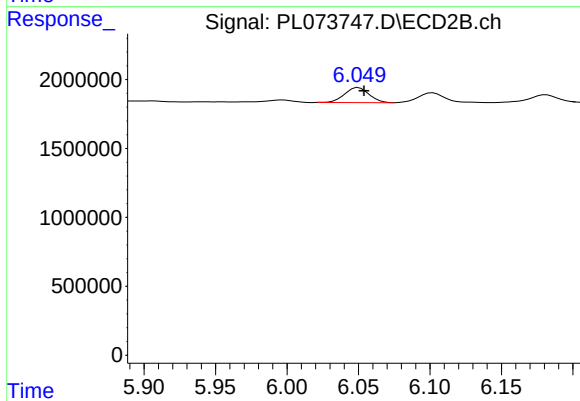

#2 alpha-BHC


R.T.: 6.049 min
Delta R.T.: -0.005 min
Response: 1296206
Conc: 0.58 ng/ml m

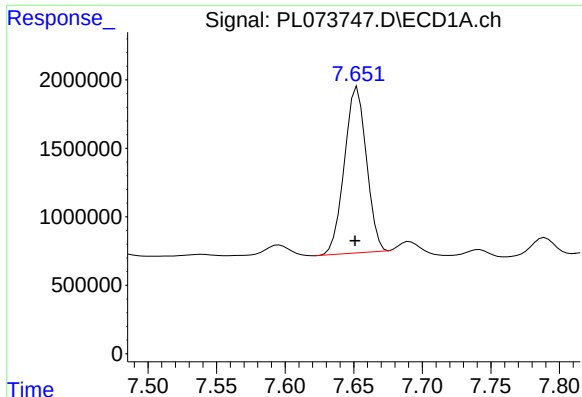

#12 4,4'-DDE


R.T.: 7.653 min
Delta R.T.: 0.002 min
Response: 13527366
Conc: 37.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
PILE-LINDEN-SWITCHDL

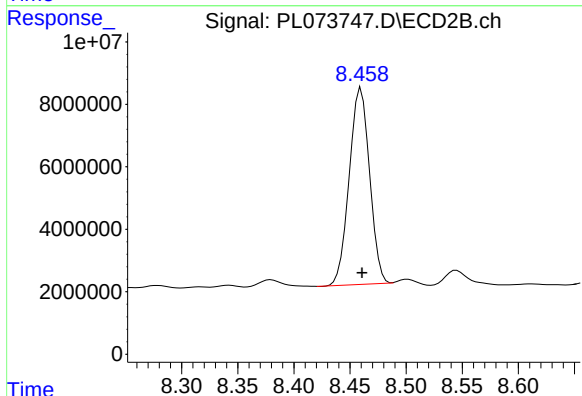


#12 4,4'-DDE

R.T.: 8.460 min
Delta R.T.: -0.001 min
Response: 79158292
Conc: 44.16 ng/ml

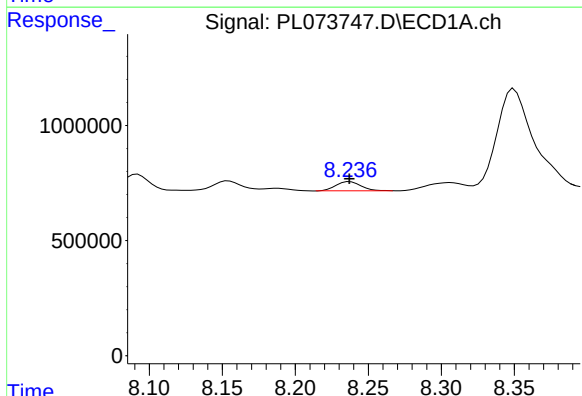


#16 4,4'-DDD

R.T.: 8.236 min
Delta R.T.: -0.001 min
Response: 479967
Conc: 1.48 ng/ml m

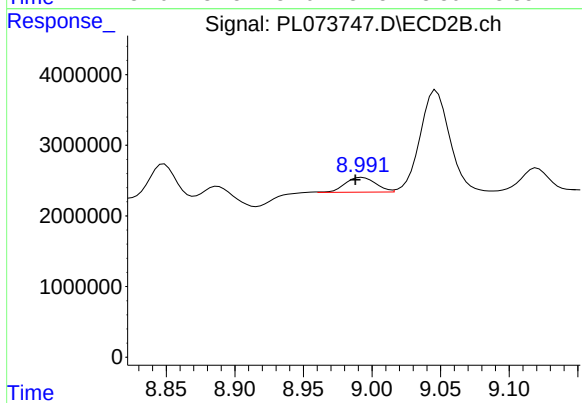

#16 4,4'-DDD


R.T.: 8.991 min
Delta R.T.: 0.003 min
Response: 3335650
Conc: 2.29 ng/ml m

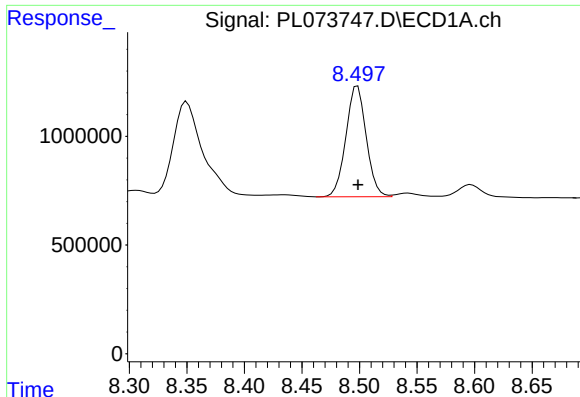

#17 4,4'-DDT


R.T.: 8.498 min
Delta R.T.: 0.000 min
Response: 6293821
Conc: 16.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
PILE-LINDEN-SWITCHDL

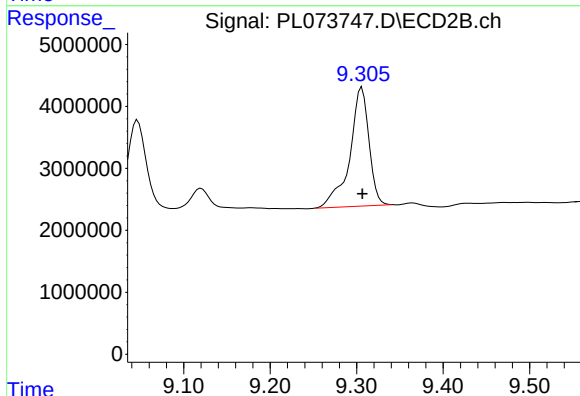


#17 4,4'-DDT

R.T.: 9.306 min
Delta R.T.: 0.000 min
Response: 29588249
Conc: 18.10 ng/ml

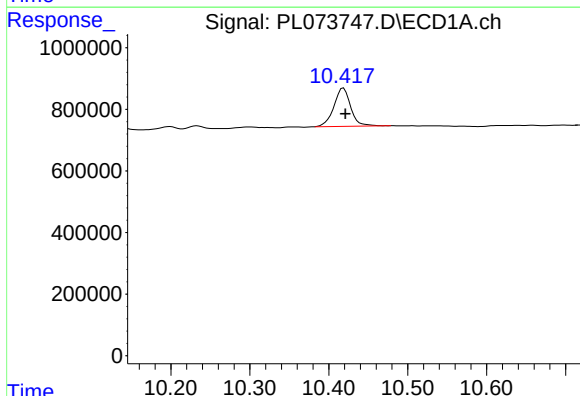

#28 Decachlorobiphenyl

R.T.: 10.419 min
Delta R.T.: -0.002 min
Response: 1838673
Conc: 3.62 ng/ml

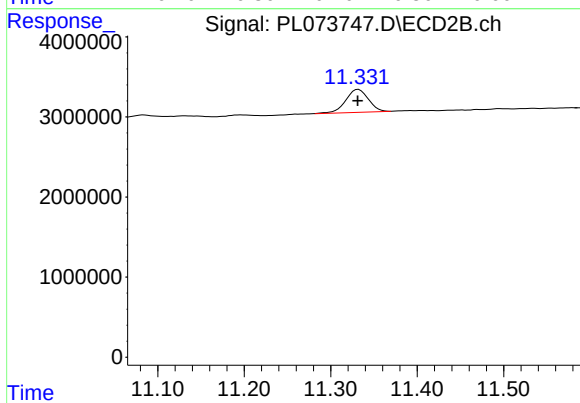

#28 Decachlorobiphenyl

R.T.: 11.332 min
Delta R.T.: 0.000 min
Response: 5173502
Conc: 2.89 ng/ml