

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL033121\
 Data File : PL065705.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Mar 2021 12:37
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 31 13:21:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 31 13:19:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.279	3.781	287.9E6	258.6E6	104.362	100.051
28)	SA Decachlor...	7.914	8.728	205.0E6	200.5E6	96.538	97.827
Target Compounds							
23)	Chlordane-1	4.114	4.745	88570237	107.0E6	1031.253	991.309
24)	Chlordane-2	4.601	5.208	106.5E6	103.7E6	965.241	972.987
25)	Chlordane-3	5.151	5.844	310.5E6	412.3E6	1078.157	1036.073
26)	Chlordane-4	5.206	5.914	275.0E6	485.6E6	1037.403	1024.505
27)	Chlordane-5	6.018	6.712	99785998	80756781	1022.513	1033.247



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL033121\
Data File : PL065705.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Mar 2021 12:37
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 31 13:21:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
Quant Title : GC Extractables
QLast Update : Wed Mar 31 13:19:51 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

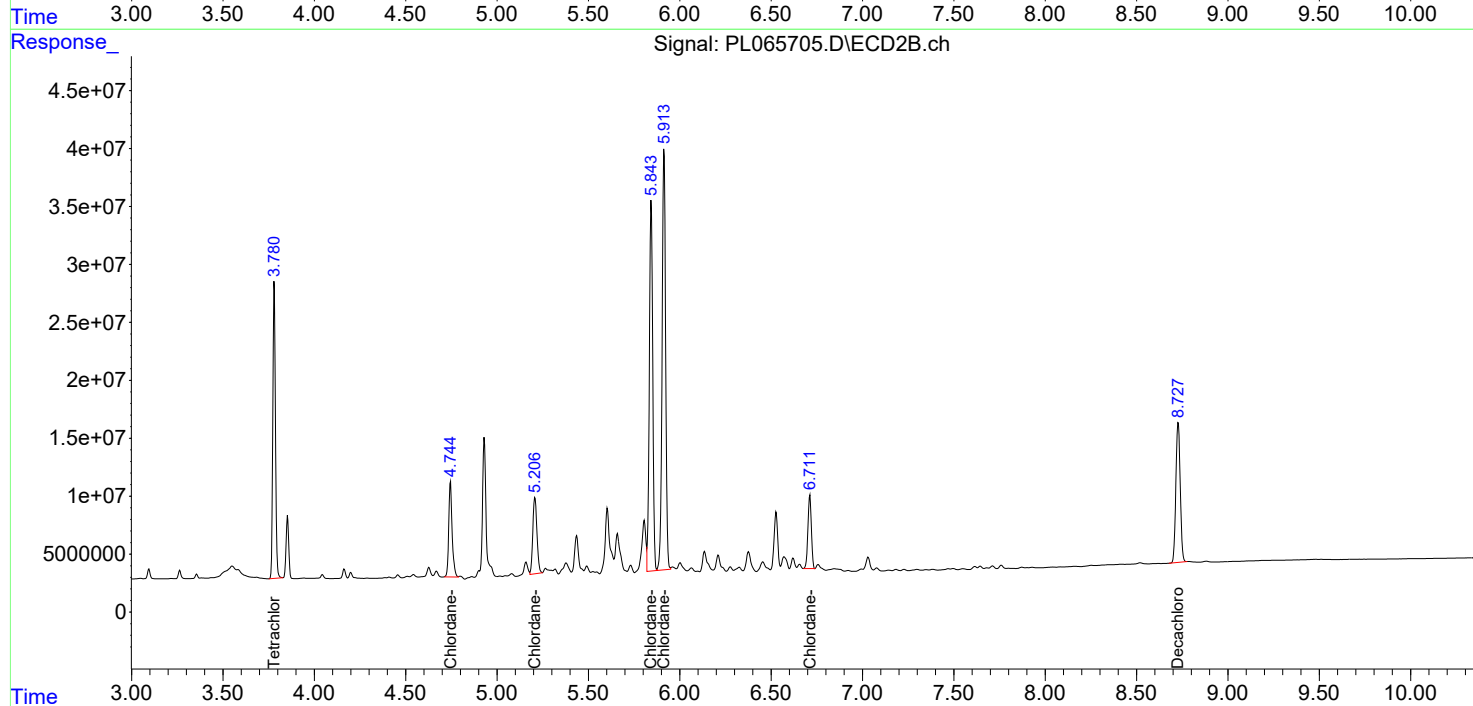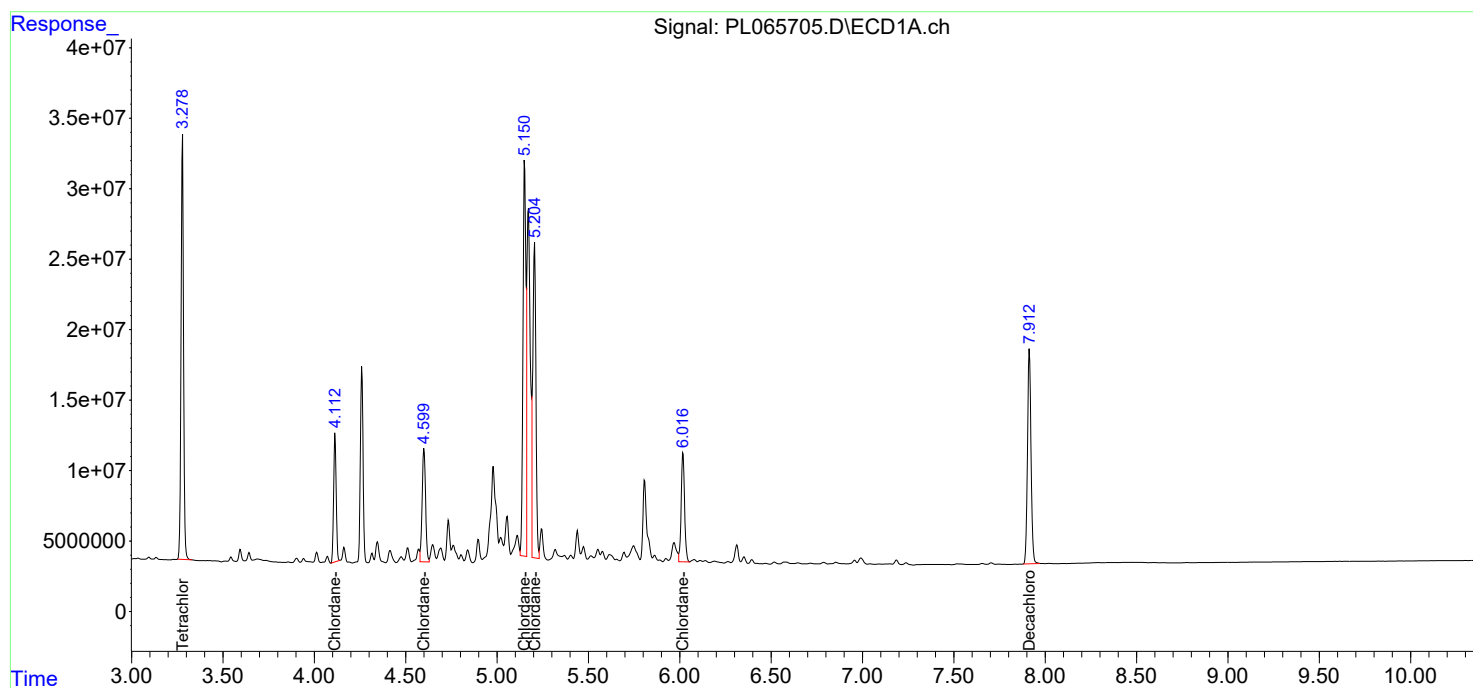


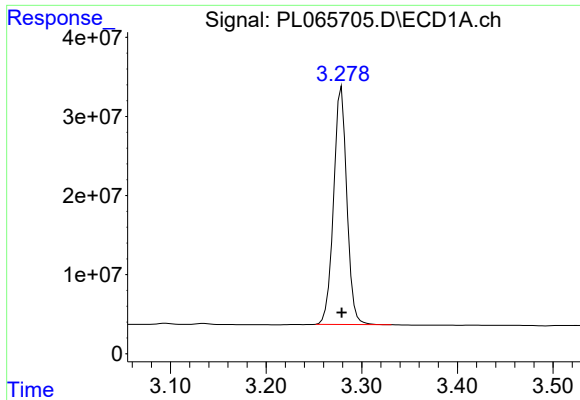

#1 Tetrachloro-m-xylene


R.T.: 3.279 min
Delta R.T.: 0.000 min
Response: 287868131
Conc: 104.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

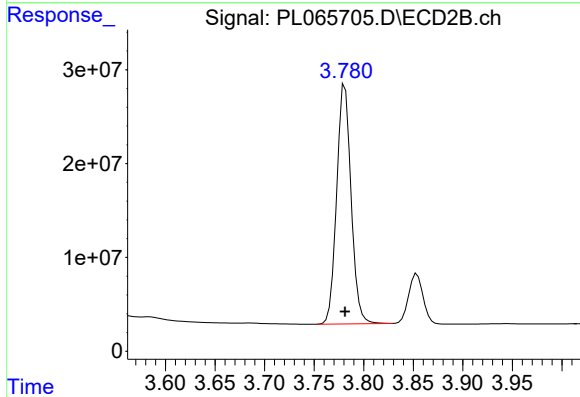


#1 Tetrachloro-m-xylene

R.T.: 3.781 min
Delta R.T.: 0.000 min
Response: 258625058
Conc: 100.05 ng/ml

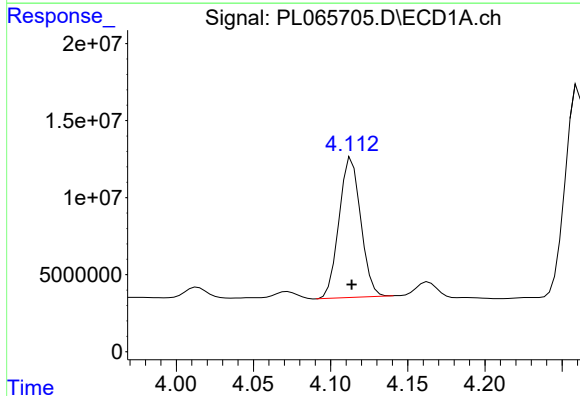


#23 Chlordane-1

R.T.: 4.114 min
Delta R.T.: 0.000 min
Response: 88570237
Conc: 1031.25 ng/ml

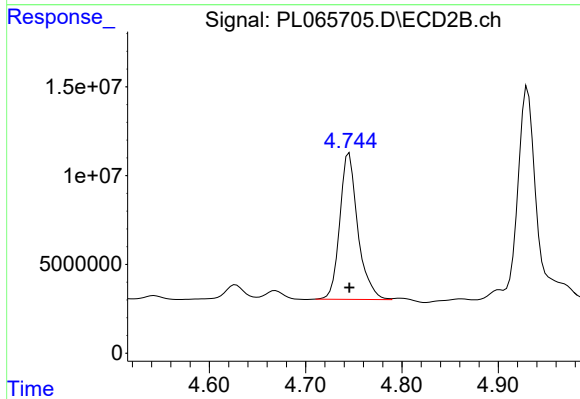

#23 Chlordane-1


R.T.: 4.745 min
Delta R.T.: 0.000 min
Response: 106985418
Conc: 991.31 ng/ml

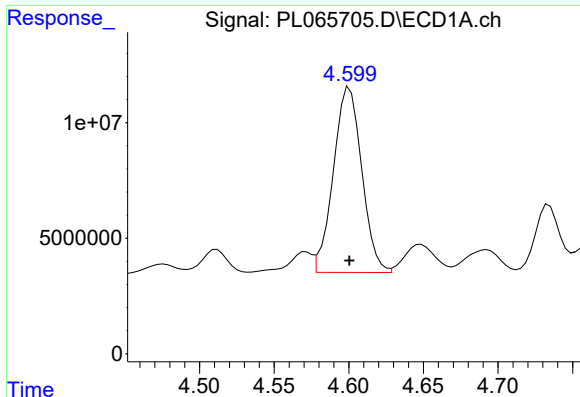

#24 Chlordane-2


R.T.: 4.601 min
Delta R.T.: 0.000 min
Response: 106464167
Conc: 965.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

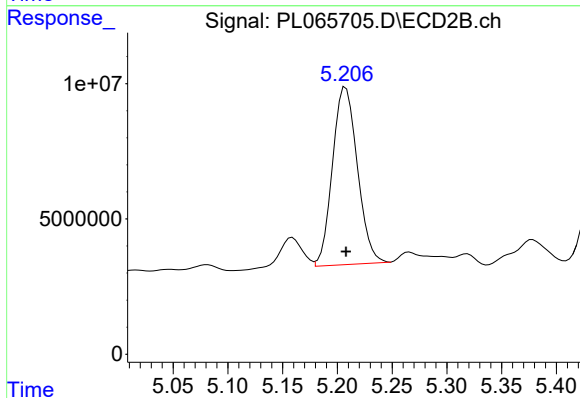


#24 Chlordane-2

R.T.: 5.208 min
Delta R.T.: 0.000 min
Response: 103737030
Conc: 972.99 ng/ml

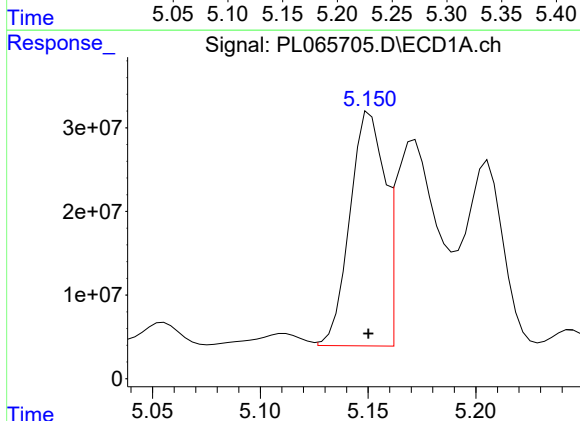


#25 Chlordane-3

R.T.: 5.151 min
Delta R.T.: 0.000 min
Response: 310457833
Conc: 1078.16 ng/ml

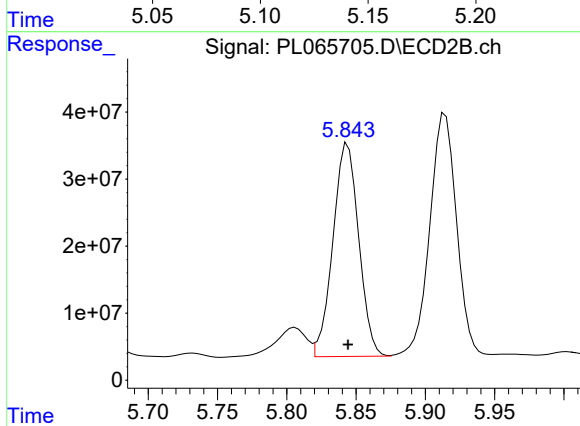

#25 Chlordane-3


R.T.: 5.844 min
Delta R.T.: 0.000 min
Response: 412349262
Conc: 1036.07 ng/ml

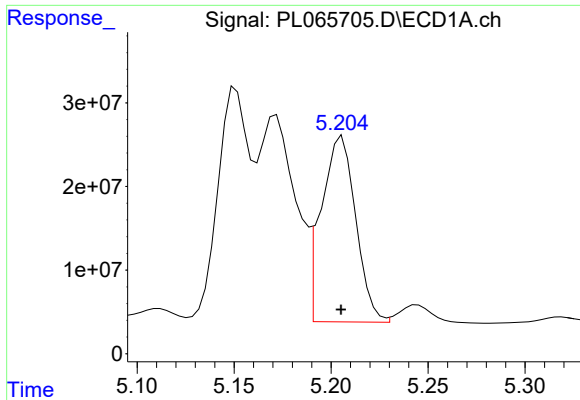

#26 Chlordane-4


R.T.: 5.206 min
Delta R.T.: 0.000 min
Response: 274956477
Conc: 1037.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

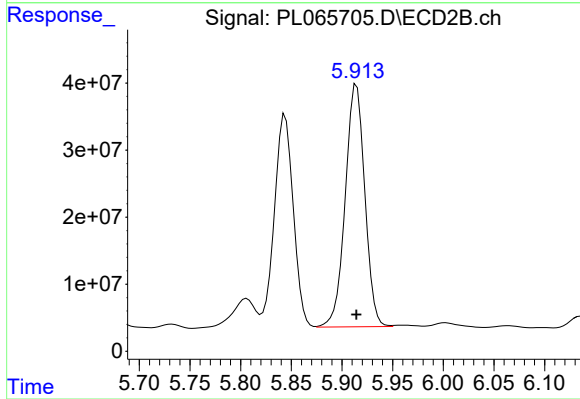


#26 Chlordane-4

R.T.: 5.914 min
Delta R.T.: 0.000 min
Response: 485589581
Conc: 1024.51 ng/ml

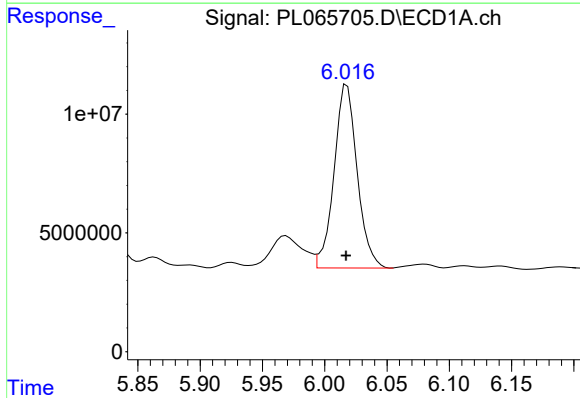


#27 Chlordane-5

R.T.: 6.018 min
Delta R.T.: 0.000 min
Response: 99785998
Conc: 1022.51 ng/ml

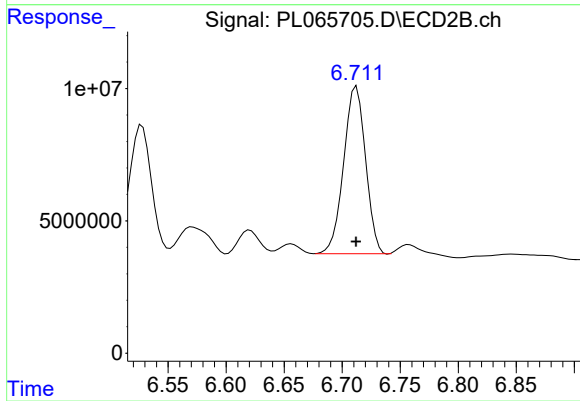

#27 Chlordane-5


R.T.: 6.712 min
Delta R.T.: 0.000 min
Response: 80756781
Conc: 1033.25 ng/ml

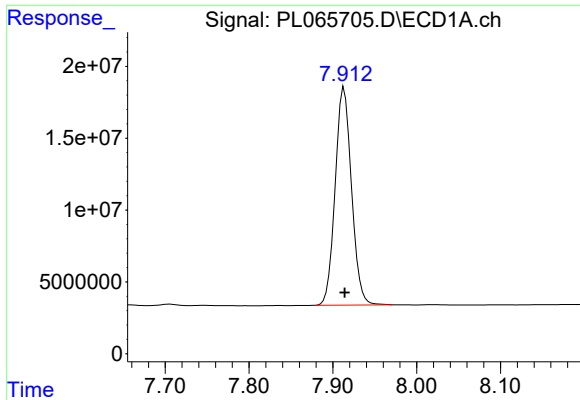

#28 Decachlorobiphenyl

R.T.: 7.914 min
Delta R.T.: 0.000 min
Response: 205027126
Conc: 96.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

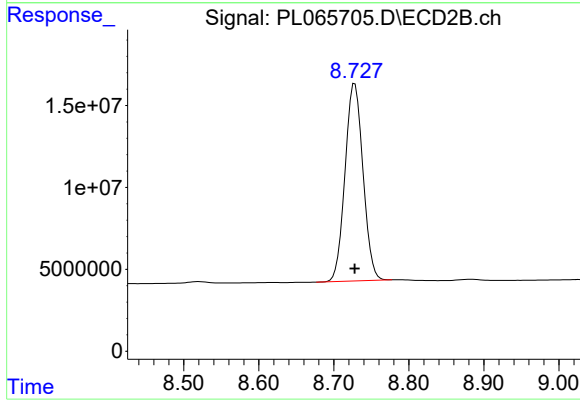

#28 Decachlorobiphenyl

R.T.: 8.728 min
Delta R.T.: 0.000 min
Response: 200517013
Conc: 97.83 ng/ml