

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL033121\
 Data File : PL065707.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Mar 2021 13:05
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 31 13:20:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 31 13:19:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.279	3.781	137.9E6	129.2E6	50.000	50.000
28)	SA Decachlor...	7.914	8.728	106.2E6	102.5E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.114	4.745	42943016	53961678	500.000	500.000
24)	Chlordane-2	4.600	5.208	55148997	53308533	500.000	500.000
25)	Chlordane-3	5.150	5.844	144.0E6	199.0E6	500.000	500.000
26)	Chlordane-4	5.205	5.914	132.5E6	237.0E6	500.000	500.000
27)	Chlordane-5	6.017	6.712	48794465	39079133	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL033121\
Data File : PL065707.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Mar 2021 13:05
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 31 13:20:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
Quant Title : GC Extractables
QLast Update : Wed Mar 31 13:19:51 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

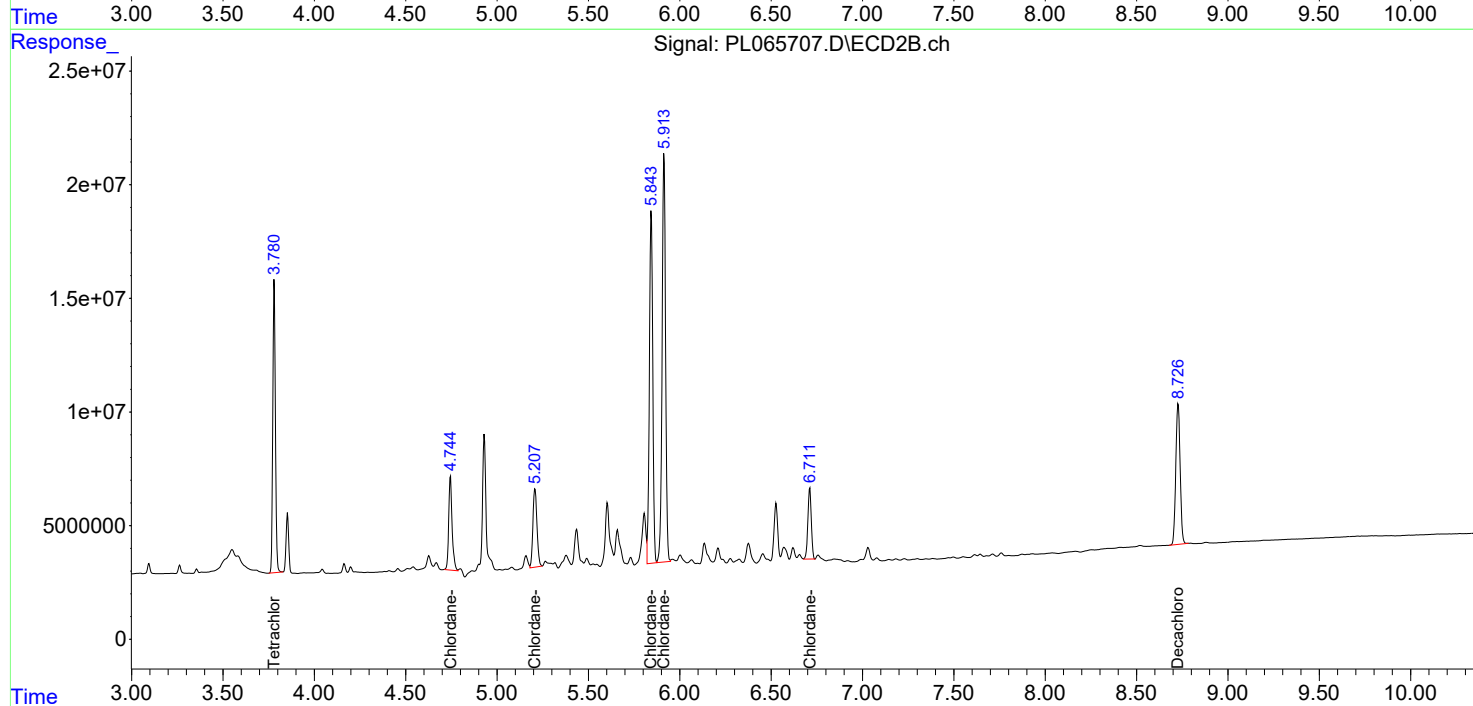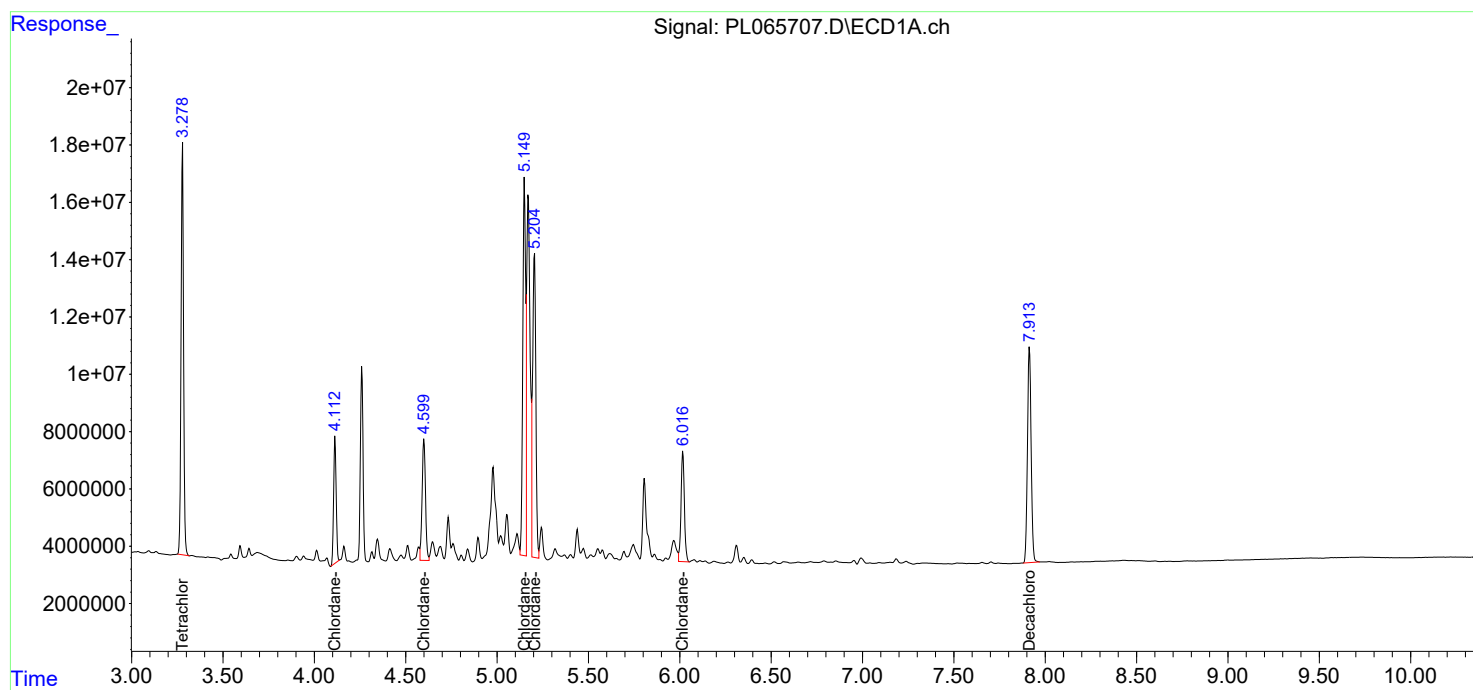


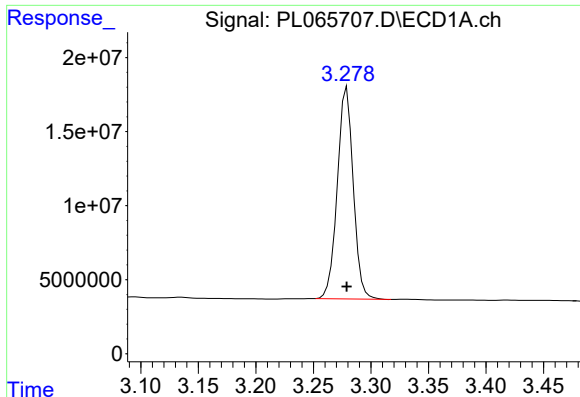

#1 Tetrachloro-m-xylene


R.T.: 3.279 min
Delta R.T.: 0.000 min
Response: 137918324
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

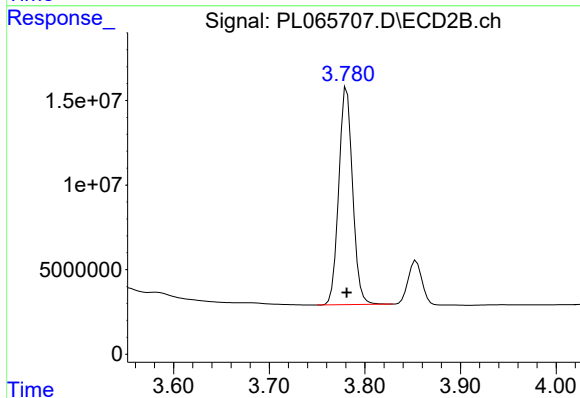


#1 Tetrachloro-m-xylene

R.T.: 3.781 min
Delta R.T.: 0.000 min
Response: 129247118
Conc: 50.00 ng/ml

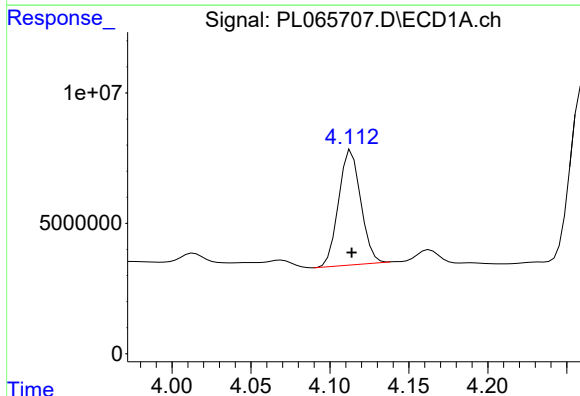


#23 Chlordane-1

R.T.: 4.114 min
Delta R.T.: 0.000 min
Response: 42943016
Conc: 500.00 ng/ml

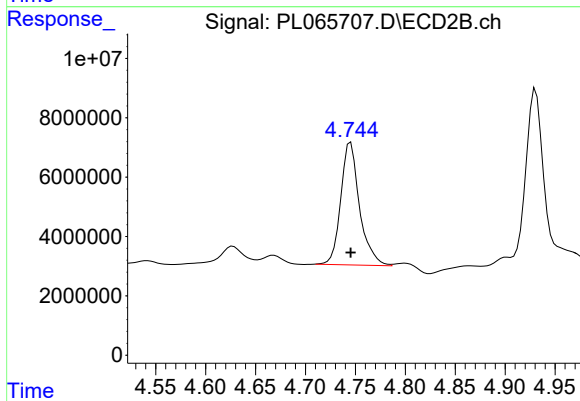

#23 Chlordane-1


R.T.: 4.745 min
Delta R.T.: 0.000 min
Response: 53961678
Conc: 500.00 ng/ml

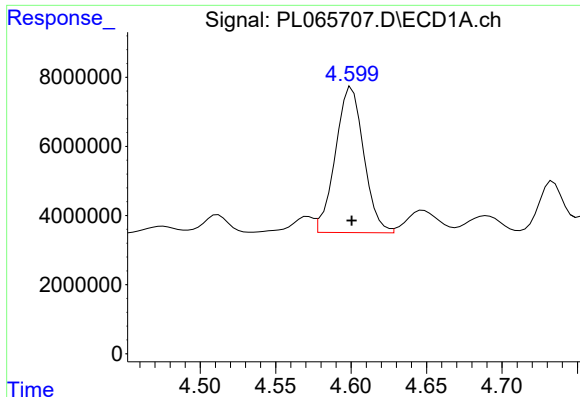

#24 Chlordane-2


R.T.: 4.600 min
Delta R.T.: 0.000 min
Response: 55148997
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

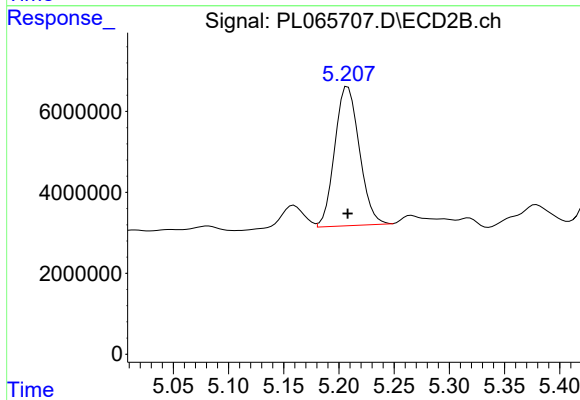


#24 Chlordane-2

R.T.: 5.208 min
Delta R.T.: 0.000 min
Response: 53308533
Conc: 500.00 ng/ml

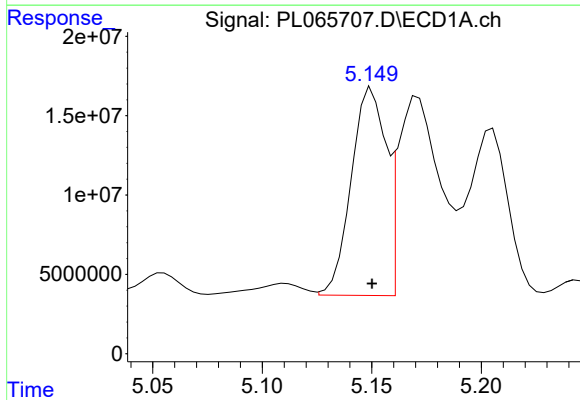


#25 Chlordane-3

R.T.: 5.150 min
Delta R.T.: 0.000 min
Response: 143976204
Conc: 500.00 ng/ml

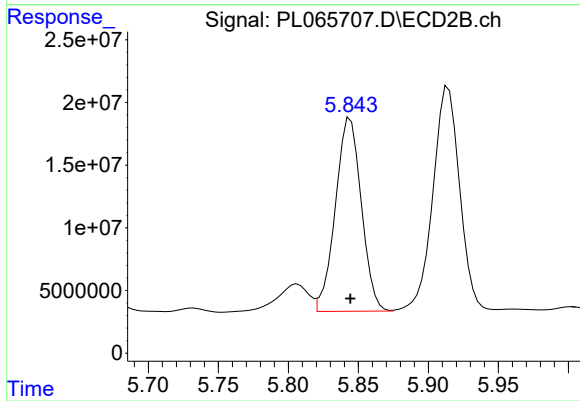

#25 Chlordane-3


R.T.: 5.844 min
Delta R.T.: 0.000 min
Response: 198996304
Conc: 500.00 ng/ml

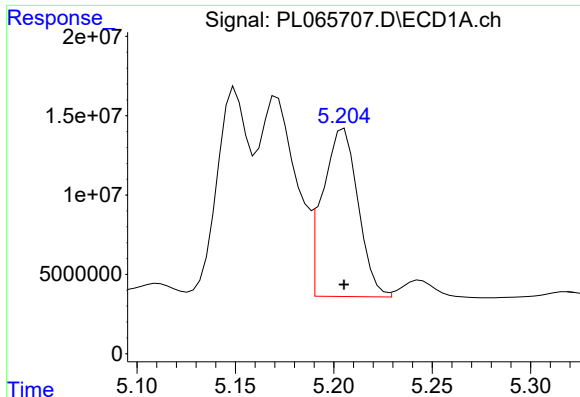

#26 Chlordane-4


R.T.: 5.205 min
Delta R.T.: 0.000 min
Response: 132521475
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

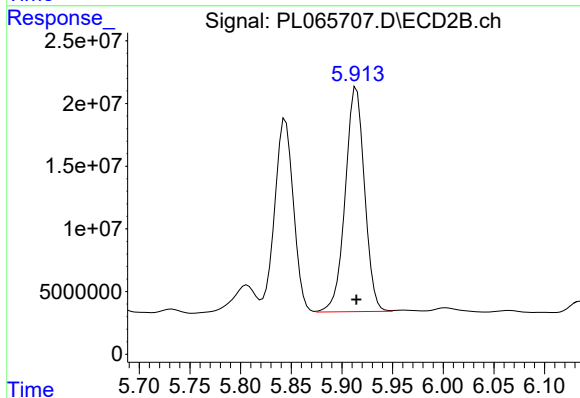


#26 Chlordane-4

R.T.: 5.914 min
Delta R.T.: 0.000 min
Response: 236987378
Conc: 500.00 ng/ml

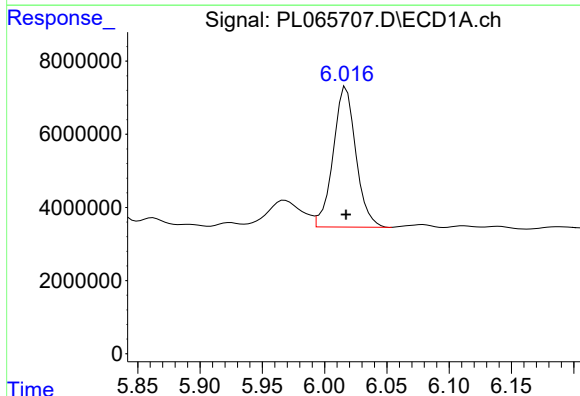


#27 Chlordane-5

R.T.: 6.017 min
Delta R.T.: 0.000 min
Response: 48794465
Conc: 500.00 ng/ml

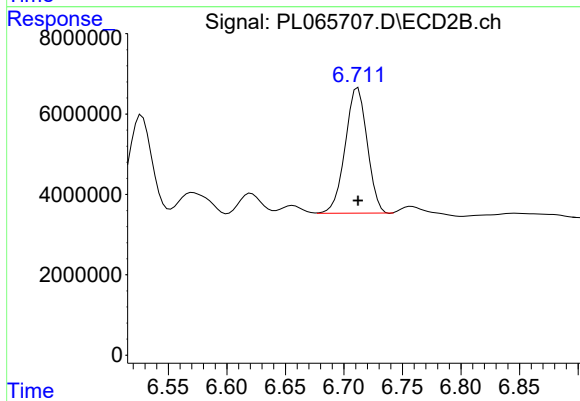

#27 Chlordane-5


R.T.: 6.712 min
Delta R.T.: 0.000 min
Response: 39079133
Conc: 500.00 ng/ml

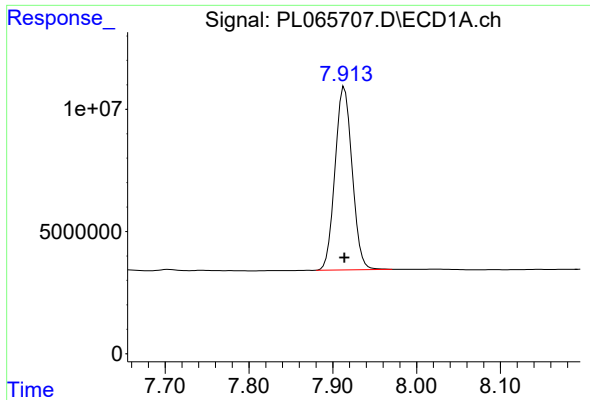

#28 Decachlorobiphenyl

R.T.: 7.914 min
Delta R.T.: 0.000 min
Response: 106189864
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

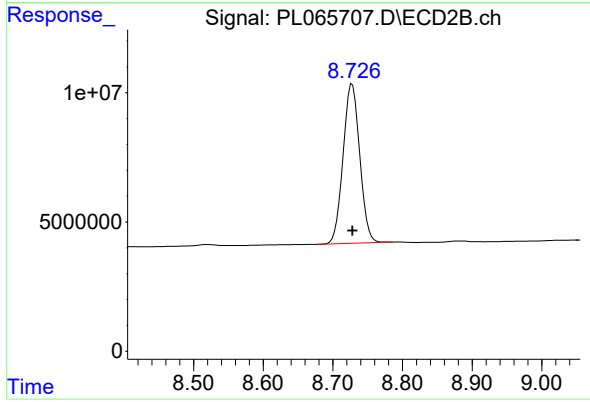

#28 Decachlorobiphenyl

R.T.: 8.728 min
Delta R.T.: 0.000 min
Response: 102485354
Conc: 50.00 ng/ml