

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL033121\
 Data File : PL065716.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Mar 2021 15:42
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL033121CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 31 15:56:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 31 15:55:13 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.280	3.781	157.1E6	138.7E6	54.458	51.229
28)	SA Decachlor...	7.914	8.726	124.1E6	106.3E6	53.987	49.022
Target Compounds							
23)	Chlordane-1	4.114	4.745	48029420	63267222	532.315	572.819
24)	Chlordane-2	4.600	5.208	63685895	55394760	554.110	484.058
25)	Chlordane-3	5.151	5.844	155.8E6	221.5E6	501.143	521.040
26)	Chlordane-4	5.205	5.914	146.4E6	254.1E6	512.650	502.232
27)	Chlordane-5	6.018	6.712	56302468	44716386	550.458	536.318



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL033121\
Data File : PL065716.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Mar 2021 15:42
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL033121CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 31 15:56:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
Quant Title : GC Extractables
QLast Update : Wed Mar 31 15:55:13 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

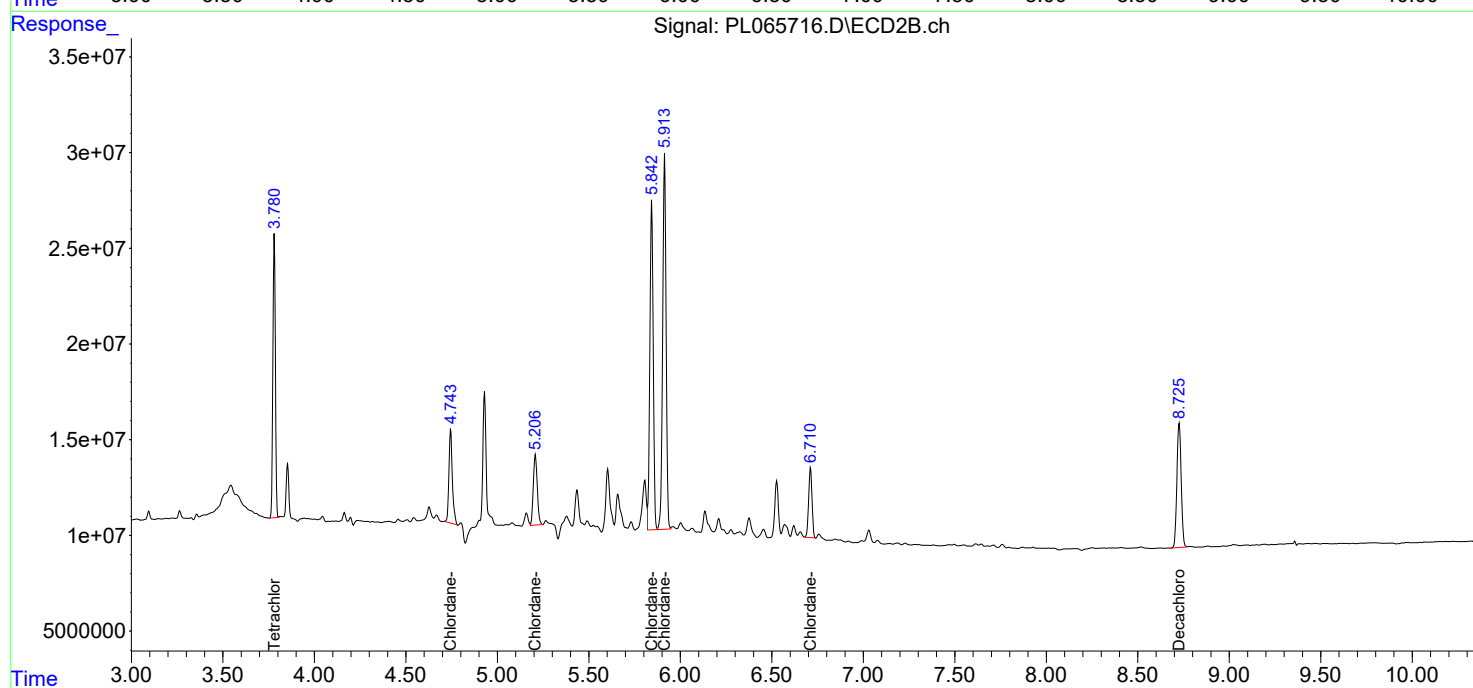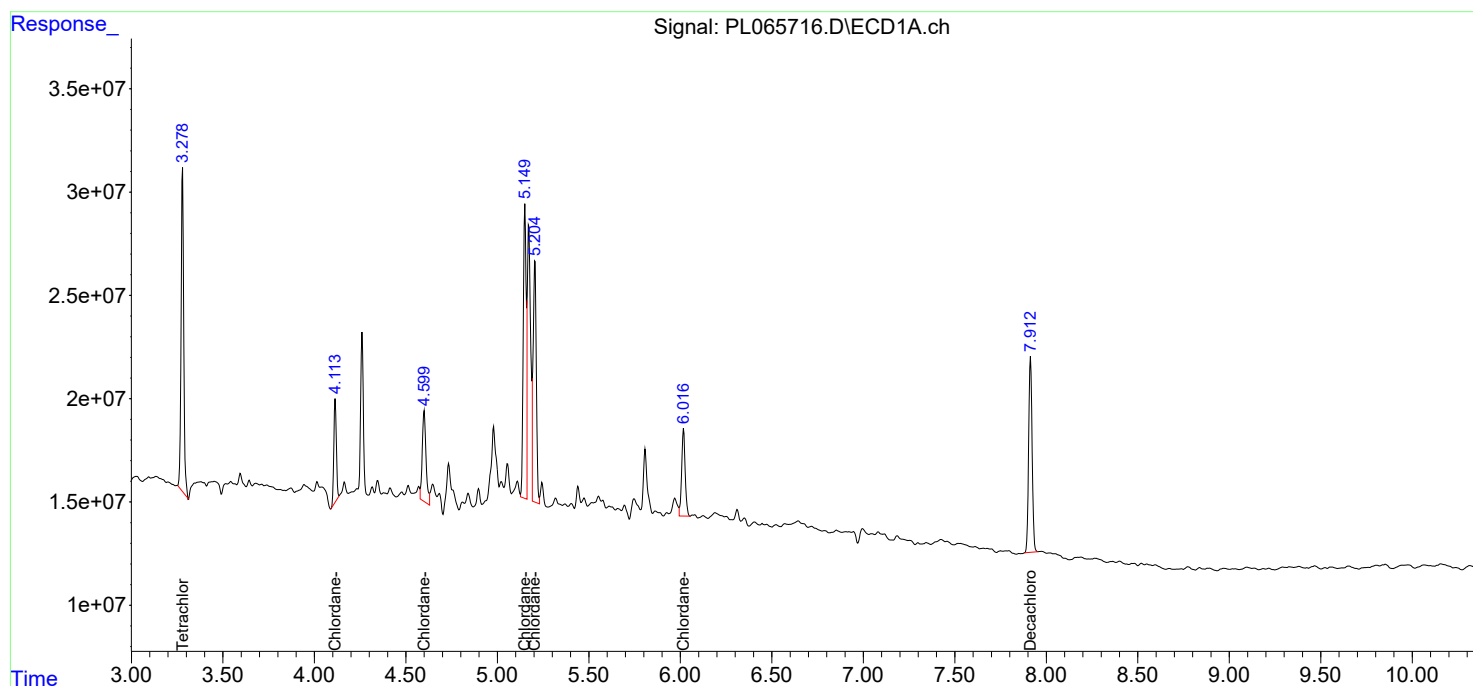


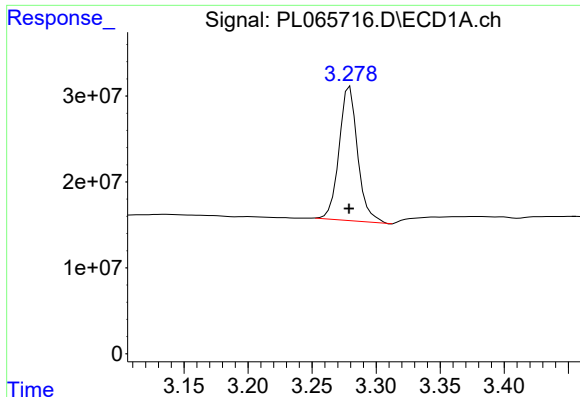

#1 Tetrachloro-m-xylene


R.T.: 3.280 min
Delta R.T.: 0.000 min
Response: 157110797
Conc: 54.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL033121CHLOR

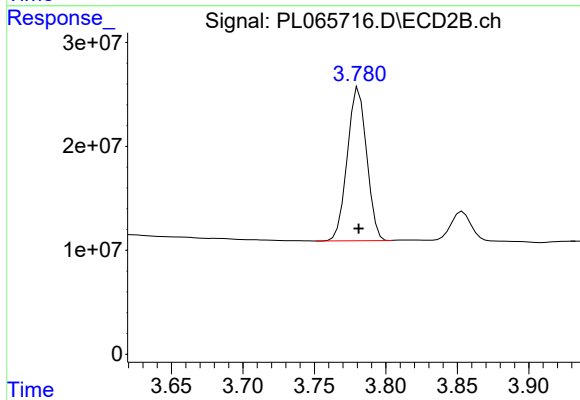


#1 Tetrachloro-m-xylene

R.T.: 3.781 min
Delta R.T.: 0.000 min
Response: 138709138
Conc: 51.23 ng/ml

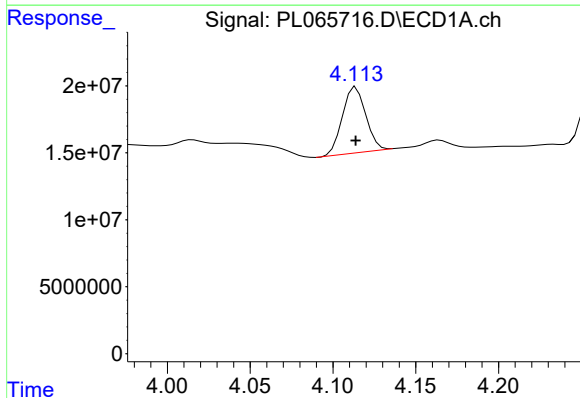


#23 Chlordane-1

R.T.: 4.114 min
Delta R.T.: 0.000 min
Response: 48029420
Conc: 532.32 ng/ml

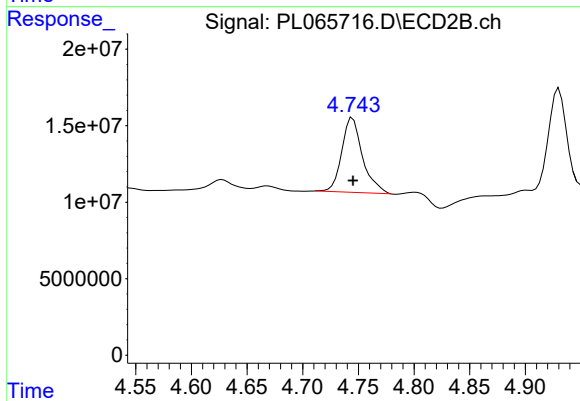

#23 Chlordane-1


R.T.: 4.745 min
Delta R.T.: 0.000 min
Response: 63267222
Conc: 572.82 ng/ml

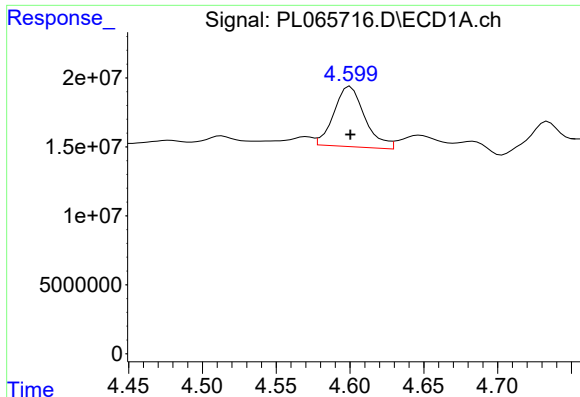

#24 Chlordane-2


R.T.: 4.600 min
Delta R.T.: 0.000 min
Response: 63685895
Conc: 554.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL033121CHLOR

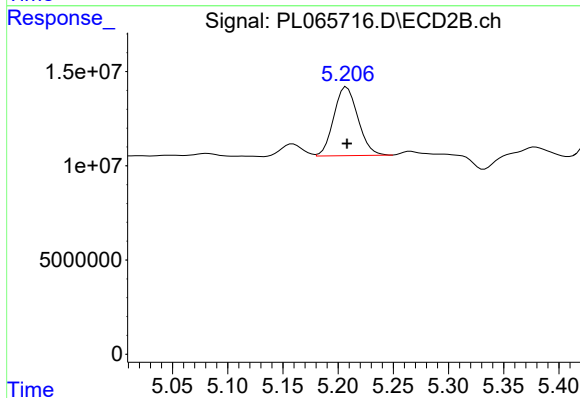


#24 Chlordane-2

R.T.: 5.208 min
Delta R.T.: 0.000 min
Response: 55394760
Conc: 484.06 ng/ml

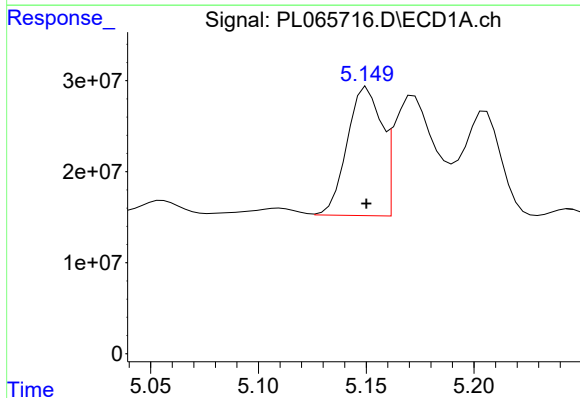


#25 Chlordane-3

R.T.: 5.151 min
Delta R.T.: 0.000 min
Response: 155760159
Conc: 501.14 ng/ml

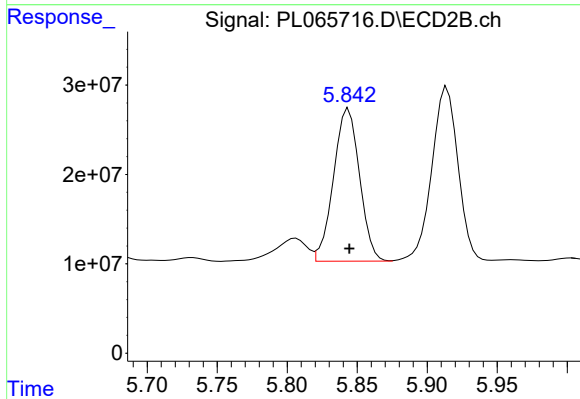

#25 Chlordane-3


R.T.: 5.844 min
Delta R.T.: 0.000 min
Response: 221463974
Conc: 521.04 ng/ml

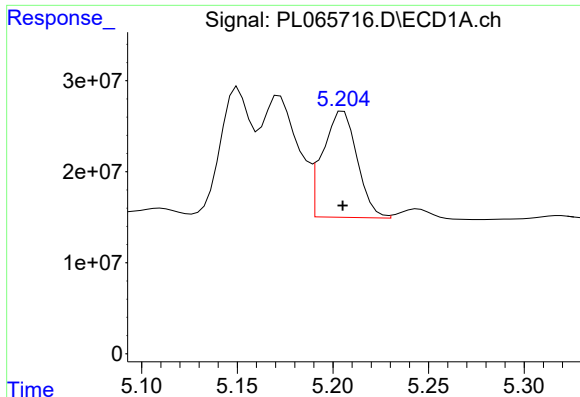

#26 Chlordane-4


R.T.: 5.205 min
Delta R.T.: 0.000 min
Response: 146368632
Conc: 512.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL033121CHLOR

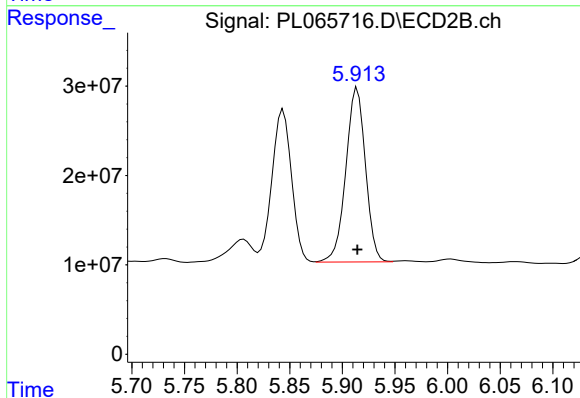


#26 Chlordane-4

R.T.: 5.914 min
Delta R.T.: 0.000 min
Response: 254070179
Conc: 502.23 ng/ml

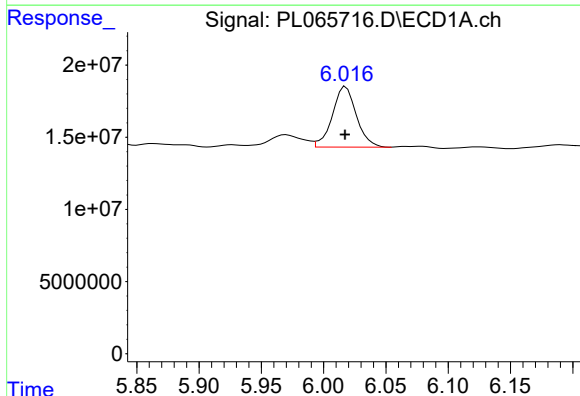


#27 Chlordane-5

R.T.: 6.018 min
Delta R.T.: 0.000 min
Response: 56302468
Conc: 550.46 ng/ml

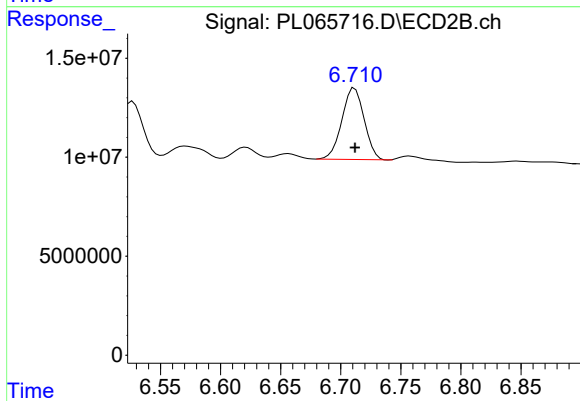

#27 Chlordane-5


R.T.: 6.712 min
Delta R.T.: 0.000 min
Response: 44716386
Conc: 536.32 ng/ml

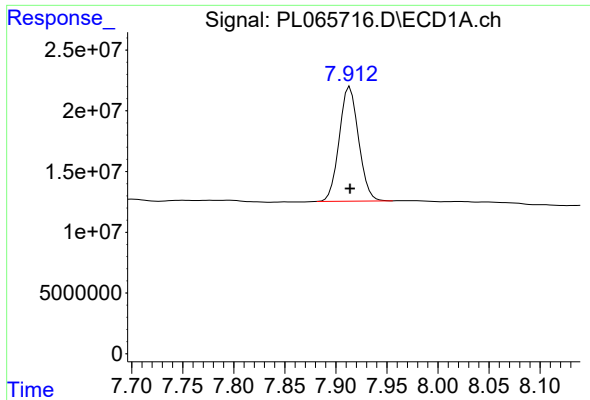

#28 Decachlorobiphenyl

R.T.: 7.914 min
Delta R.T.: 0.000 min
Response: 124079025
Conc: 53.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL033121CHLOR

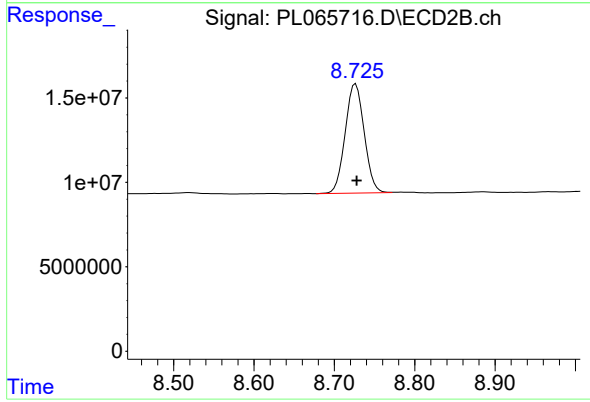

#28 Decachlorobiphenyl

R.T.: 8.726 min
Delta R.T.: -0.001 min
Response: 106258132
Conc: 49.02 ng/ml