

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL033121\
 Data File : PL065706.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Mar 2021 12:51
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 31 13:21:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 31 13:19:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.279	3.781	216.6E6	196.2E6	78.515	75.886
28)	SA Decachlor...	7.914	8.727	157.3E6	153.9E6	74.050	75.077
Target Compounds							
23)	Chlordane-1	4.113	4.745	66867688	79921091	778.563	740.536
24)	Chlordane-2	4.599	5.208	81958196	79876614	743.062	749.192
25)	Chlordane-3	5.150	5.844	227.9E6	309.2E6	791.523	776.947
26)	Chlordane-4	5.205	5.915	207.4E6	365.8E6	782.650	771.852
27)	Chlordane-5	6.017	6.712	75366310	60245003	772.283	770.808



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL033121\
Data File : PL065706.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Mar 2021 12:51
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 31 13:21:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
Quant Title : GC Extractables
QLast Update : Wed Mar 31 13:19:51 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

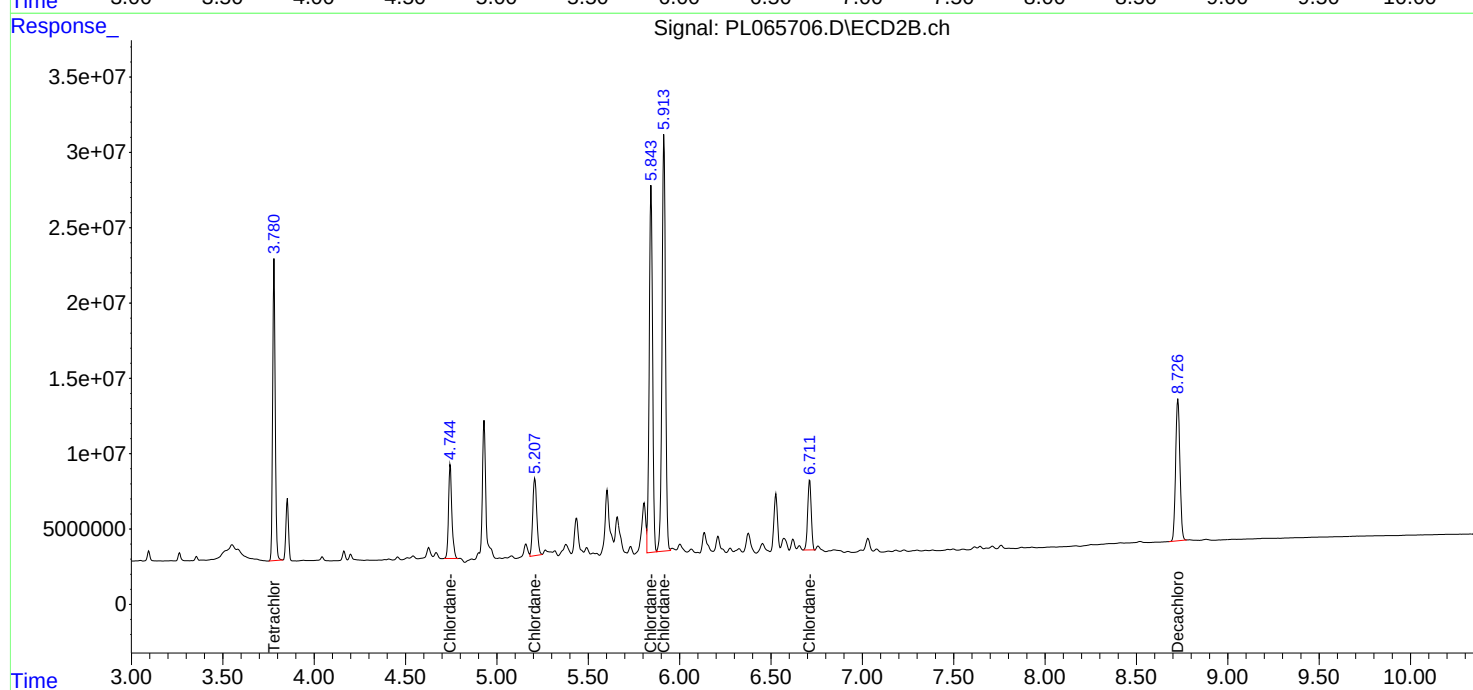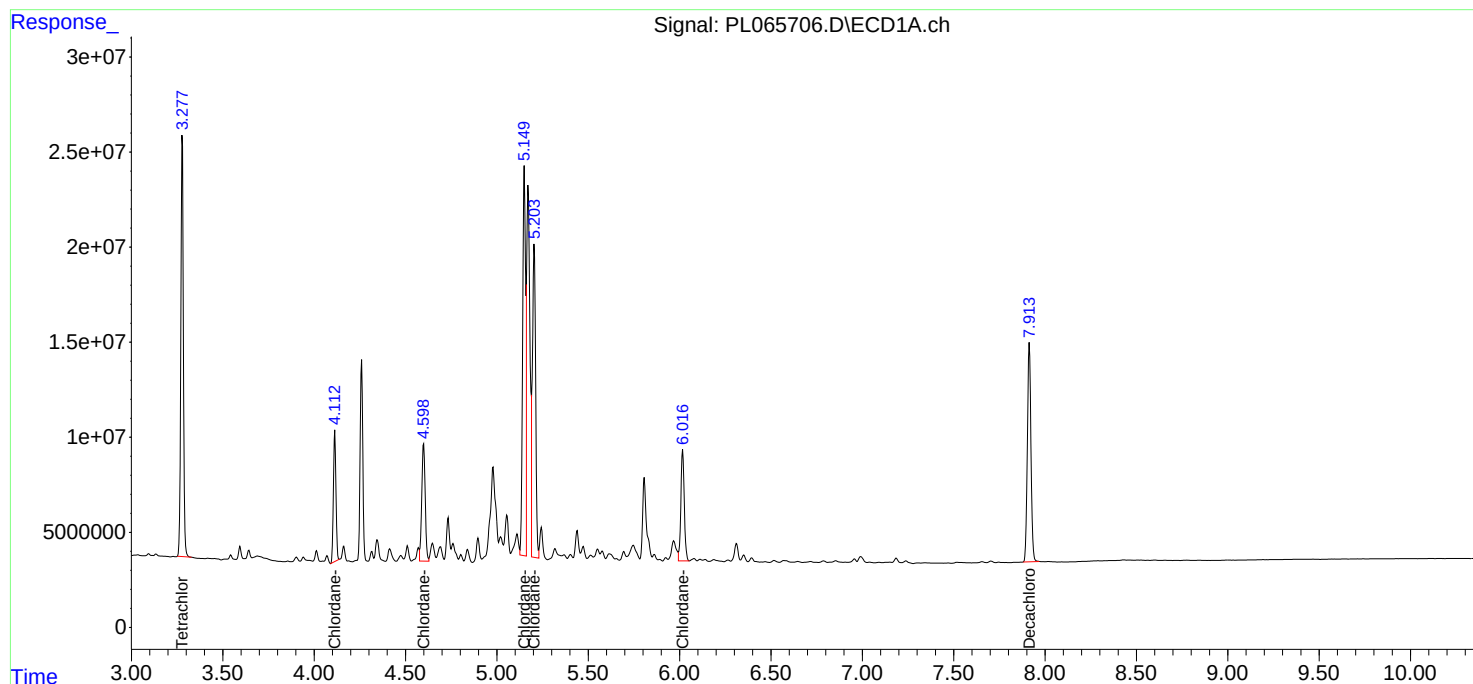


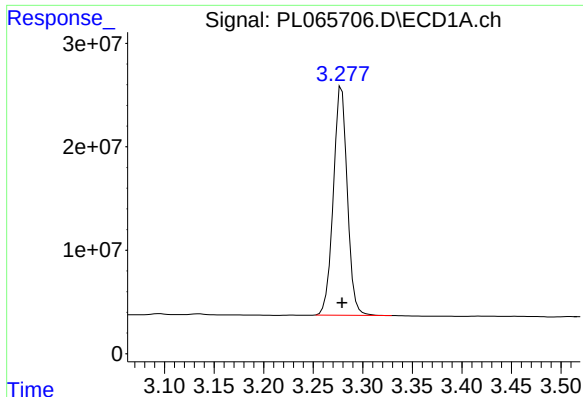

#1 Tetrachloro-m-xylene


R.T.: 3.279 min
Delta R.T.: 0.000 min
Response: 216573431
Conc: 78.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

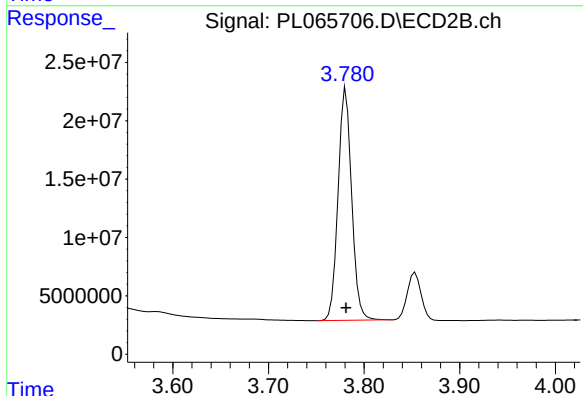


#1 Tetrachloro-m-xylene

R.T.: 3.781 min
Delta R.T.: 0.000 min
Response: 196161135
Conc: 75.89 ng/ml

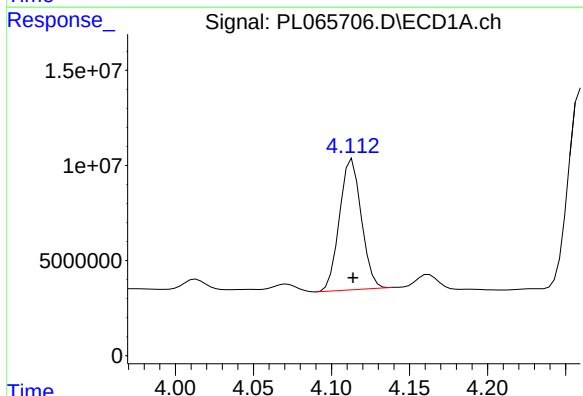


#23 Chlordane-1

R.T.: 4.113 min
Delta R.T.: 0.000 min
Response: 66867688
Conc: 778.56 ng/ml

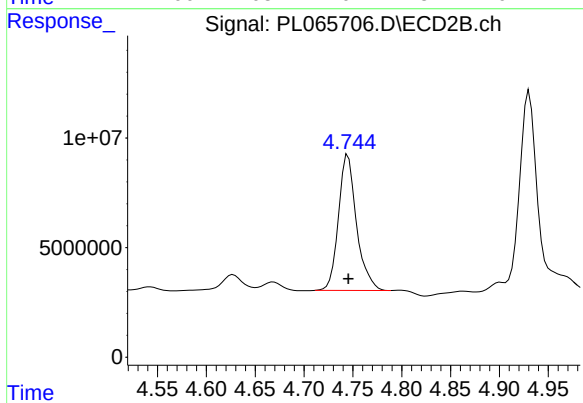

#23 Chlordane-1


R.T.: 4.745 min
Delta R.T.: 0.000 min
Response: 79921091
Conc: 740.54 ng/ml

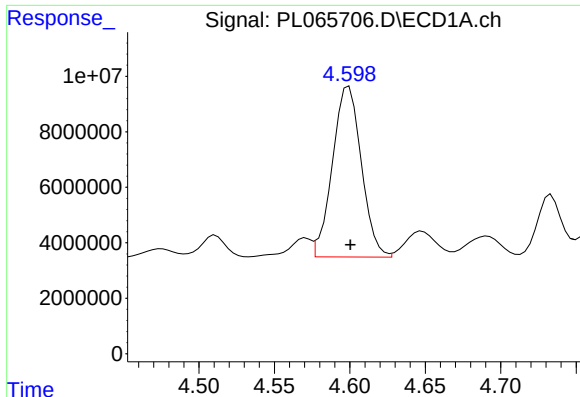

#24 Chlordane-2


R.T.: 4.599 min
Delta R.T.: 0.000 min
Response: 81958196
Conc: 743.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

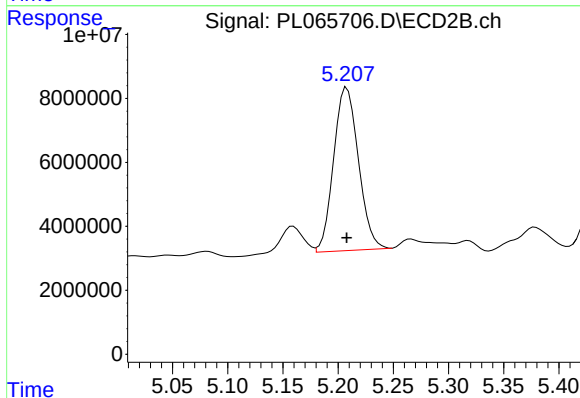


#24 Chlordane-2

R.T.: 5.208 min
Delta R.T.: 0.000 min
Response: 79876614
Conc: 749.19 ng/ml

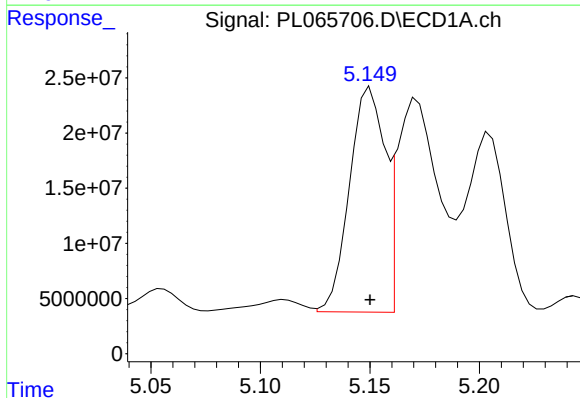


#25 Chlordane-3

R.T.: 5.150 min
Delta R.T.: 0.000 min
Response: 227920930
Conc: 791.52 ng/ml

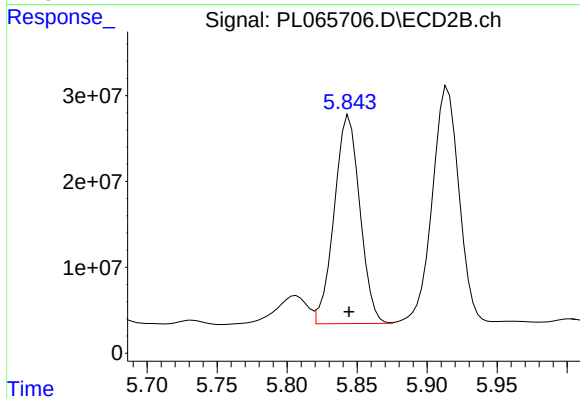

#25 Chlordane-3


R.T.: 5.844 min
Delta R.T.: 0.000 min
Response: 309219196
Conc: 776.95 ng/ml

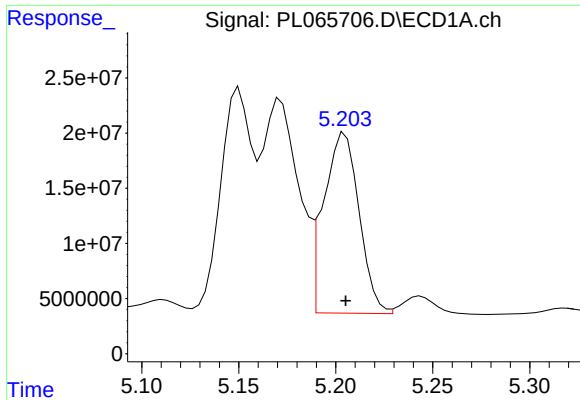

#26 Chlordane-4


R.T.: 5.205 min
Delta R.T.: 0.000 min
Response: 207435946
Conc: 782.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

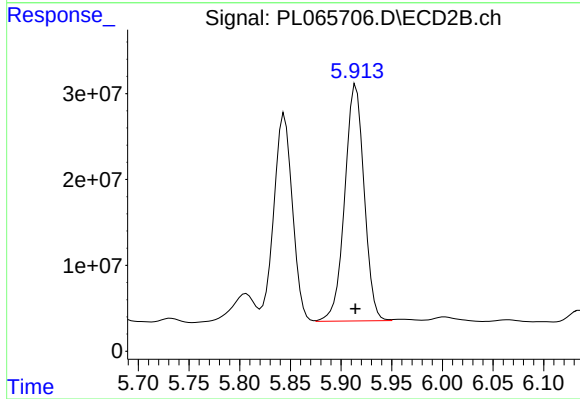


#26 Chlordane-4

R.T.: 5.915 min
Delta R.T.: 0.000 min
Response: 365838300
Conc: 771.85 ng/ml

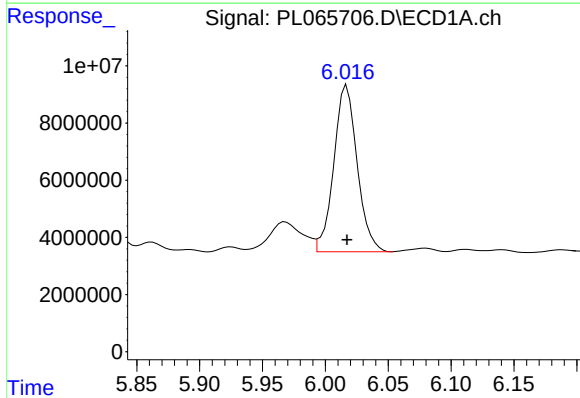


#27 Chlordane-5

R.T.: 6.017 min
Delta R.T.: 0.000 min
Response: 75366310
Conc: 772.28 ng/ml

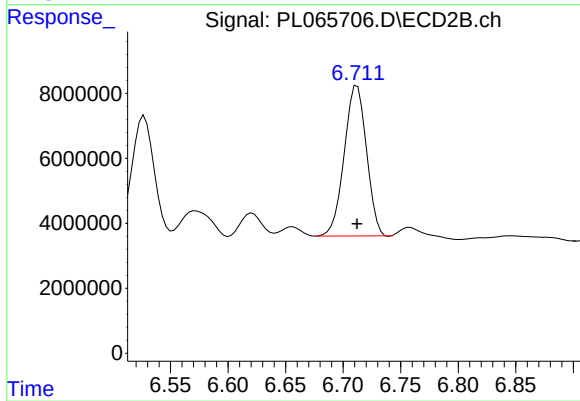

#27 Chlordane-5


R.T.: 6.712 min
Delta R.T.: 0.000 min
Response: 60245003
Conc: 770.81 ng/ml

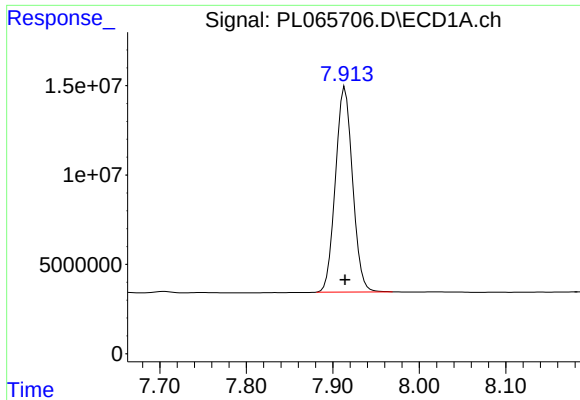

#28 Decachlorobiphenyl

R.T.: 7.914 min
Delta R.T.: 0.000 min
Response: 157267324
Conc: 74.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

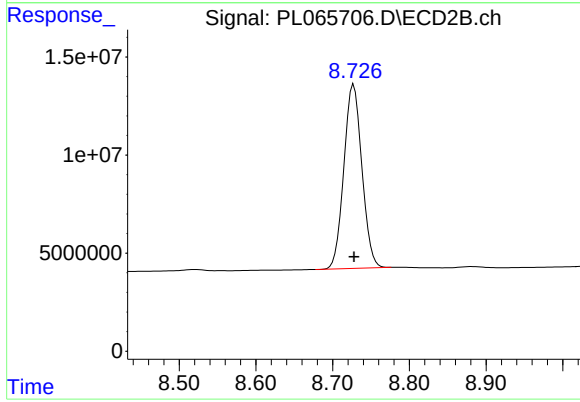

#28 Decachlorobiphenyl

R.T.: 8.727 min
Delta R.T.: 0.000 min
Response: 153886048
Conc: 75.08 ng/ml