

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL033121\
 Data File : PL065728.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Mar 2021 18:49
 Operator : AR\AJ
 Sample : M1836-09
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 B4-8-10

Manual Integrations
 APPROVED

Ankita
 4/1/2021 12:57:51 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 02:43:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 31 15:57:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.278	3.779	30354752	35882828	11.652m	13.072m
28)	SA Decachlor...	7.914	8.728	31507024	31841436	13.604	14.123
Target Compounds							
12)	B 4,4'-DDE	5.367	6.071	2289130	1653584	0.830m	0.633

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL033121\
Data File : PL065728.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Mar 2021 18:49
Operator : AR\AJ
Sample : M1836-09
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
B4-8-10


Manual Integrations
APPROVED

Ankita
4/1/2021 12:57:51 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 02:43:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
Quant Title : GC Extractables
QLast Update : Wed Mar 31 15:57:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

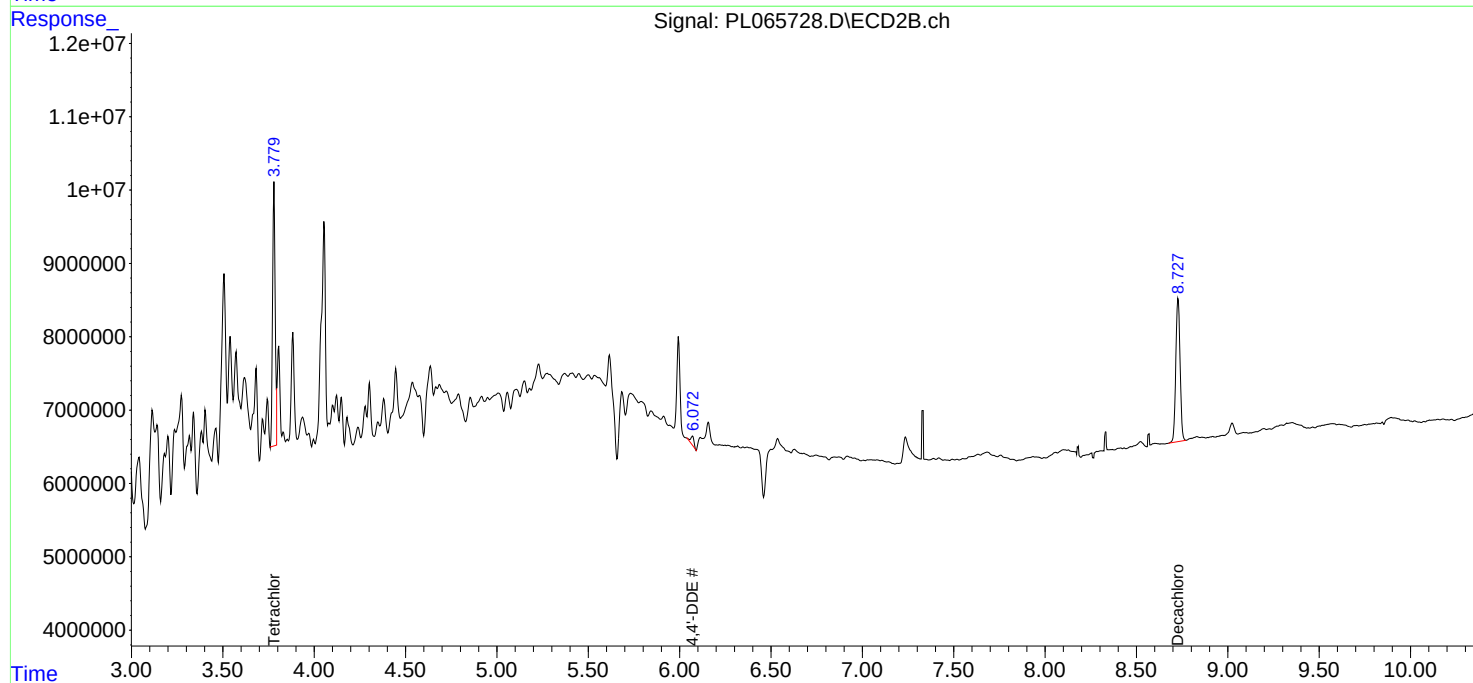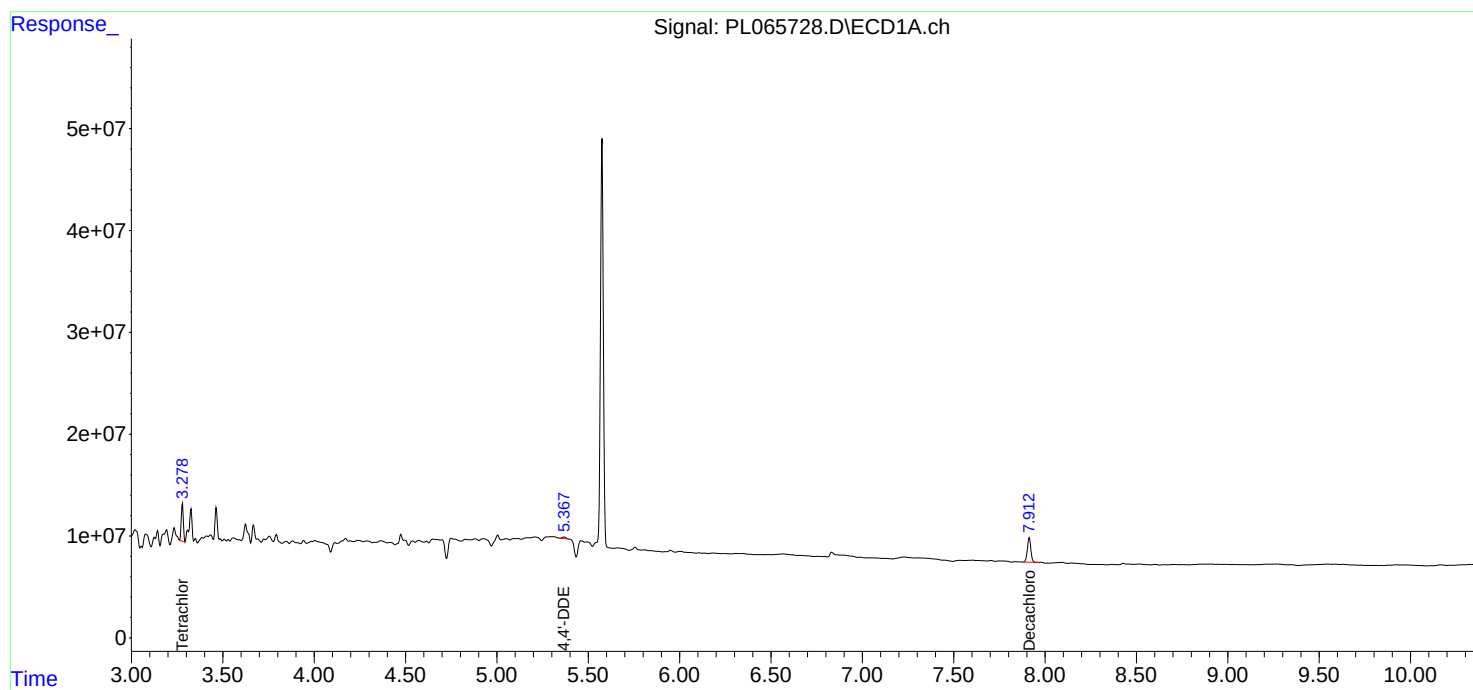

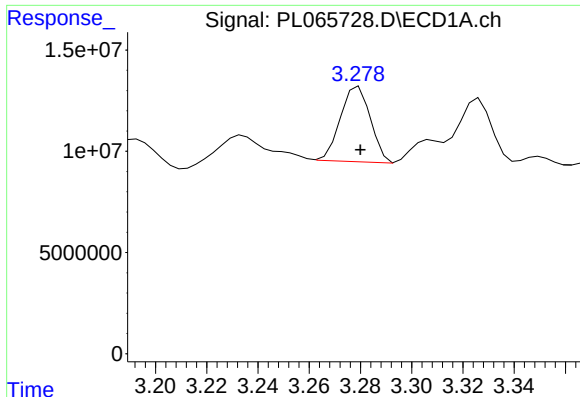


#1 Tetrachloro-m-xylene

R.T.: 3.278 min
Delta R.T.: -0.002 min
Response: 30354752
Conc: 11.65 ng/ml m

Instrument :
ECD_L
ClientSampleId :
B4-8-10


Manual Integrations
APPROVED

Ankita
4/1/2021 12:57:51 PM

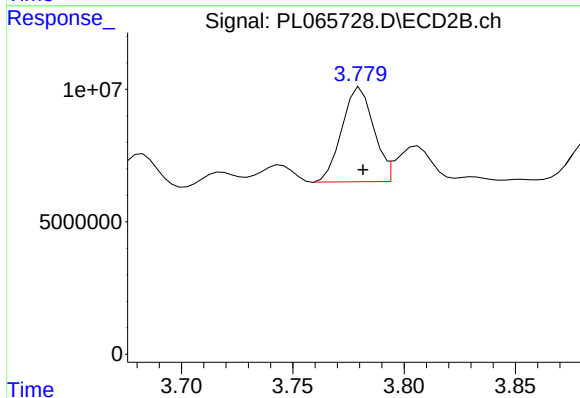


#1 Tetrachloro-m-xylene

R.T.: 3.779 min
Delta R.T.: -0.002 min
Response: 35882828
Conc: 13.07 ng/ml m

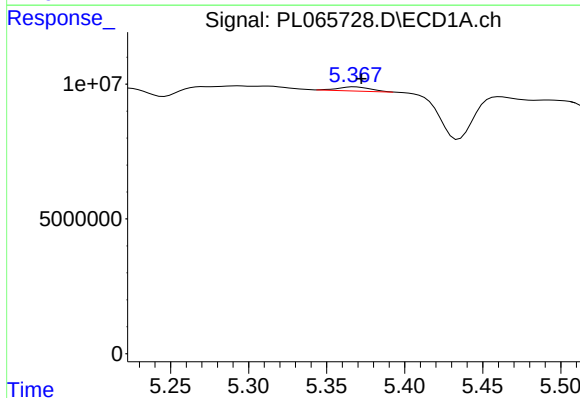


#12 4,4'-DDE

R.T.: 5.367 min
Delta R.T.: -0.005 min
Response: 2289130
Conc: 0.83 ng/ml m

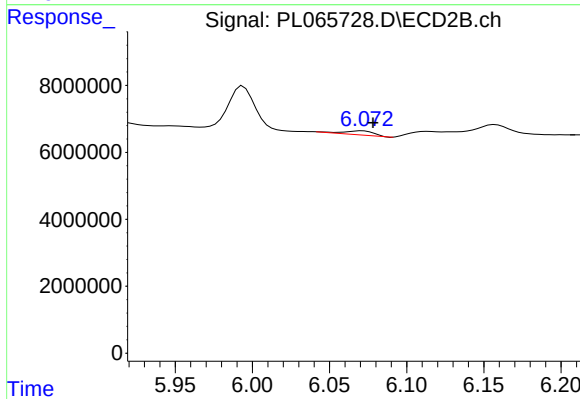

#12 4,4'-DDE

R.T.: 6.071 min
Delta R.T.: -0.007 min
Response: 1653584
Conc: 0.63 ng/ml

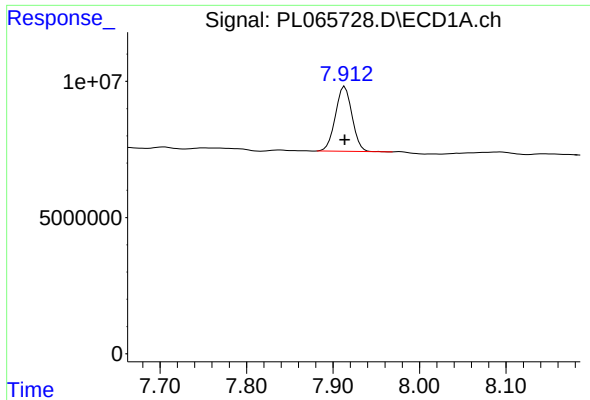


#28 Decachlorobiphenyl

R.T.: 7.914 min
Delta R.T.: 0.000 min
Response: 31507024
Conc: 13.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
B4-8-10

Manual Integrations
APPROVED

Ankita
4/1/2021 12:57:51 PM

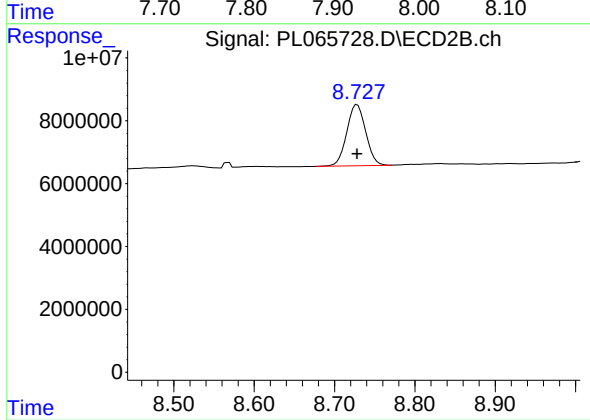

#28 Decachlorobiphenyl

R.T.: 8.728 min
Delta R.T.: 0.000 min
Response: 31841436
Conc: 14.12 ng/ml