

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL033121\
 Data File : PL065733.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Mar 2021 20:01
 Operator : AR\AJ
 Sample : M1836-05
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 B3-0-2

Manual Integrations
 APPROVED

Ankita
 4/1/2021 12:57:54 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 02:43:52 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 31 15:57:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.279	3.780	46227912	37731340	17.746	13.746m
28)	SA Decachlor...	7.913	8.729	36604541	40148717	15.805	17.808
Target Compounds							
8)	B Heptachlo...	4.928	5.616	9131891	7348213	2.904	2.366m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL033121\
Data File : PL065733.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Mar 2021 20:01
Operator : AR\AJ
Sample : M1836-05
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
B3-0-2


Manual Integrations
APPROVED

Ankita
4/1/2021 12:57:54 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 02:43:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
Quant Title : GC Extractables
QLast Update : Wed Mar 31 15:57:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

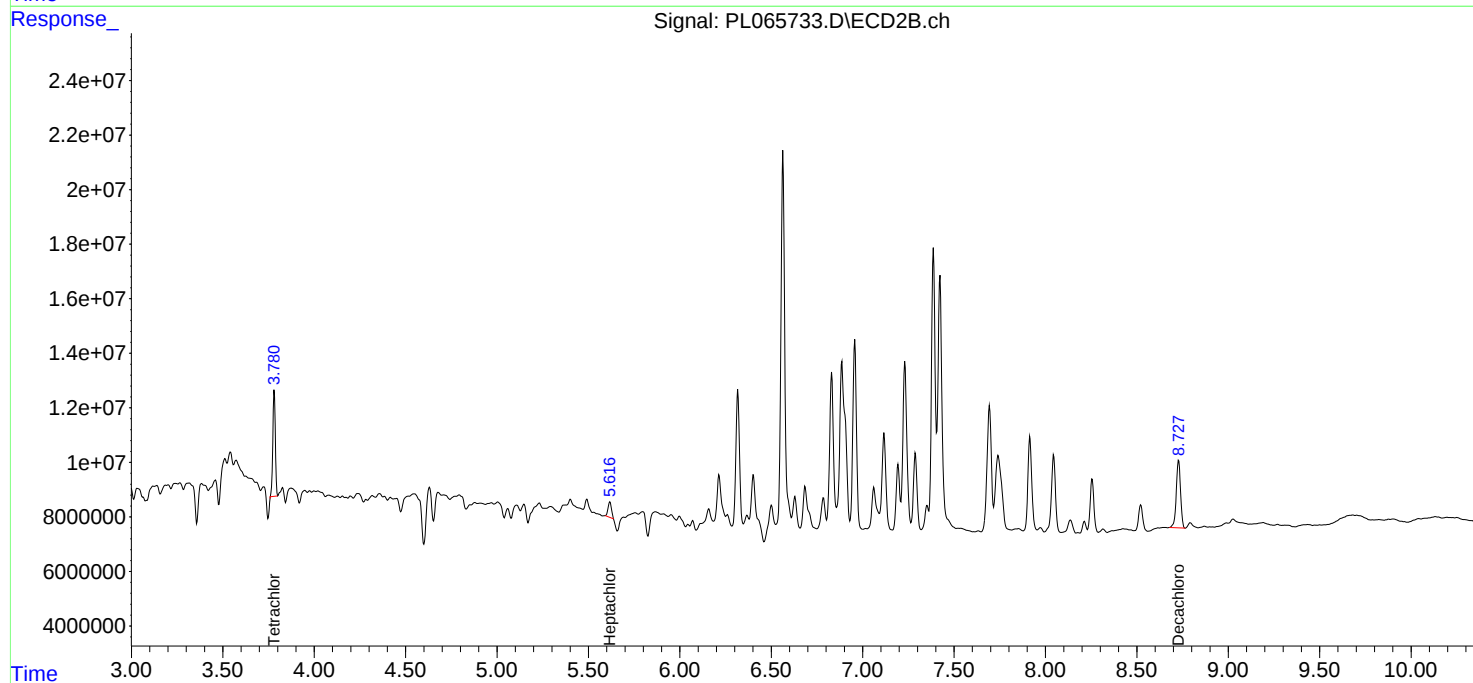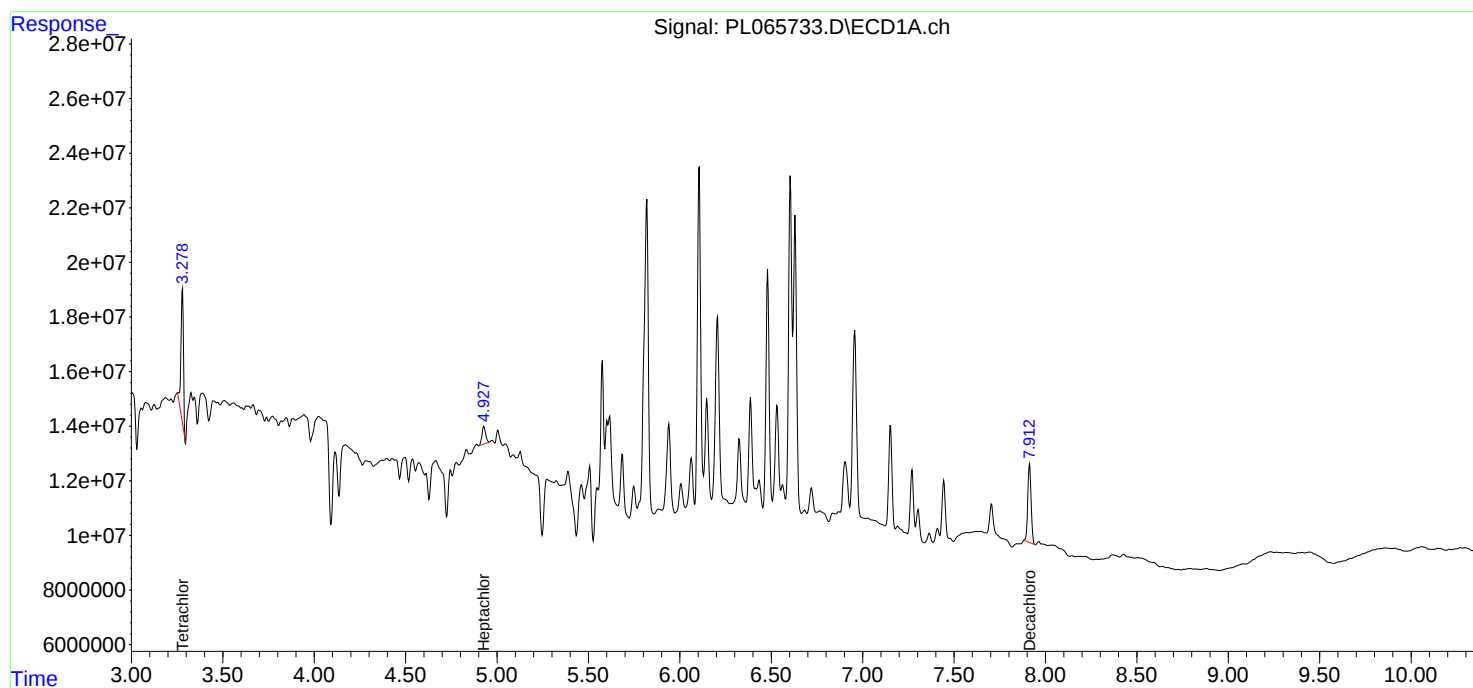

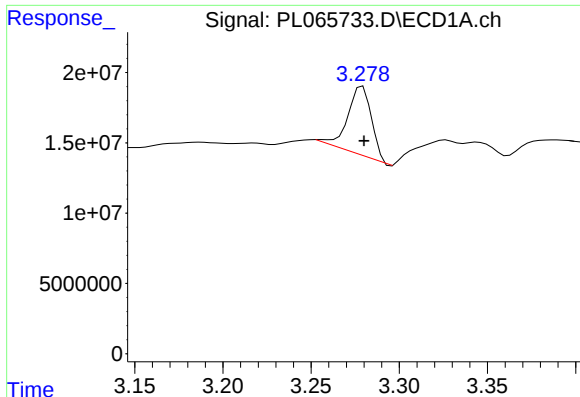


#1 Tetrachloro-m-xylene

R.T.: 3.279 min
Delta R.T.: 0.000 min
Response: 46227912
Conc: 17.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
B3-0-2


Manual Integrations
APPROVED

Ankita
4/1/2021 12:57:54 PM

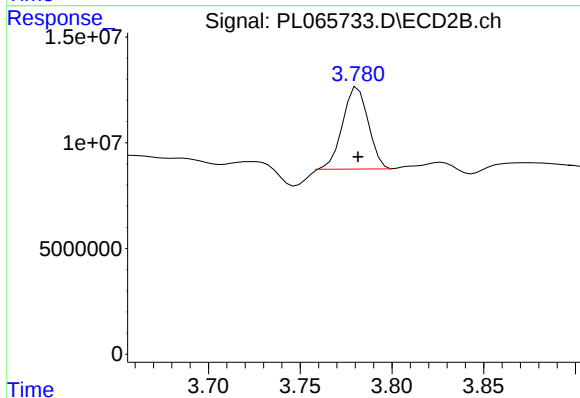


#1 Tetrachloro-m-xylene

R.T.: 3.780 min
Delta R.T.: -0.002 min
Response: 37731340
Conc: 13.75 ng/ml m

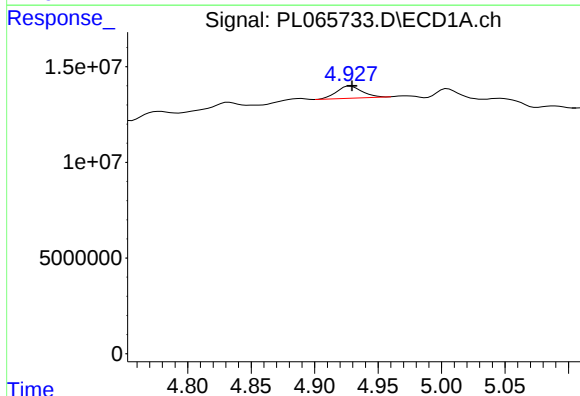


#8 Heptachlor epoxide

R.T.: 4.928 min
Delta R.T.: -0.001 min
Response: 9131891
Conc: 2.90 ng/ml

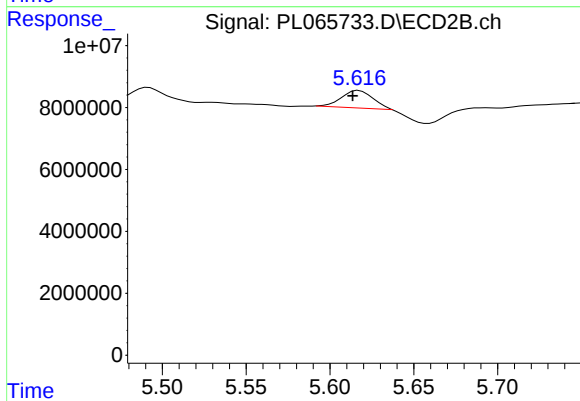

#8 Heptachlor epoxide

R.T.: 5.616 min
Delta R.T.: 0.002 min
Response: 7348213
Conc: 2.37 ng/ml m

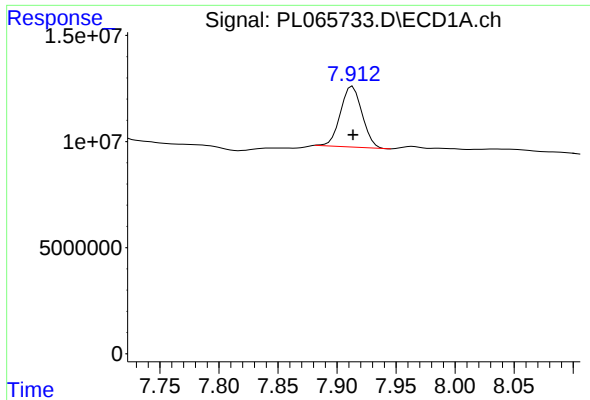


#28 Decachlorobiphenyl

R.T.: 7.913 min
Delta R.T.: 0.000 min
Response: 36604541
Conc: 15.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
B3-0-2

Manual Integrations
APPROVED

Ankita
4/1/2021 12:57:54 PM

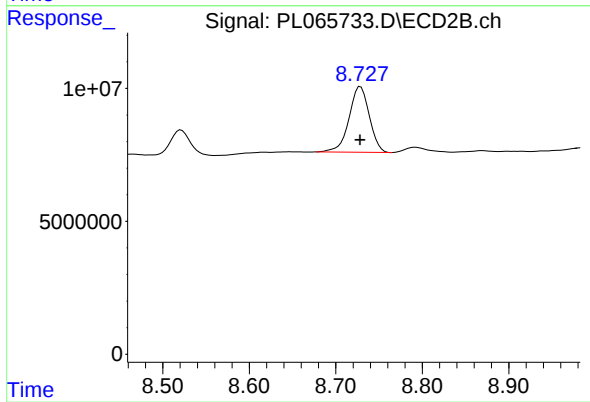

#28 Decachlorobiphenyl

R.T.: 8.729 min
Delta R.T.: 0.000 min
Response: 40148717
Conc: 17.81 ng/ml