

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL033121\
 Data File : PL065753.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Apr 2021 01:32
 Operator : AR\AJ
 Sample : M1874-01
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FS-SB18(9-10)

Manual Integrations
 APPROVED

Ankita
 4/1/2021 12:58:24 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 02:47:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 31 15:57:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.279	3.781	76769026	76358636	29.470	27.818m
28)	SA Decachlor...	7.911	8.729	47928356	45259907	20.694m	20.075

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL033121\
Data File : PL065753.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Apr 2021 01:32
Operator : AR\AJ
Sample : M1874-01
Misc :
ALS Vial : 50 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
FS-SB18(9-10)


Manual Integrations
APPROVED

Ankita
4/1/2021 12:58:24 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 02:47:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
Quant Title : GC Extractables
QLast Update : Wed Mar 31 15:57:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

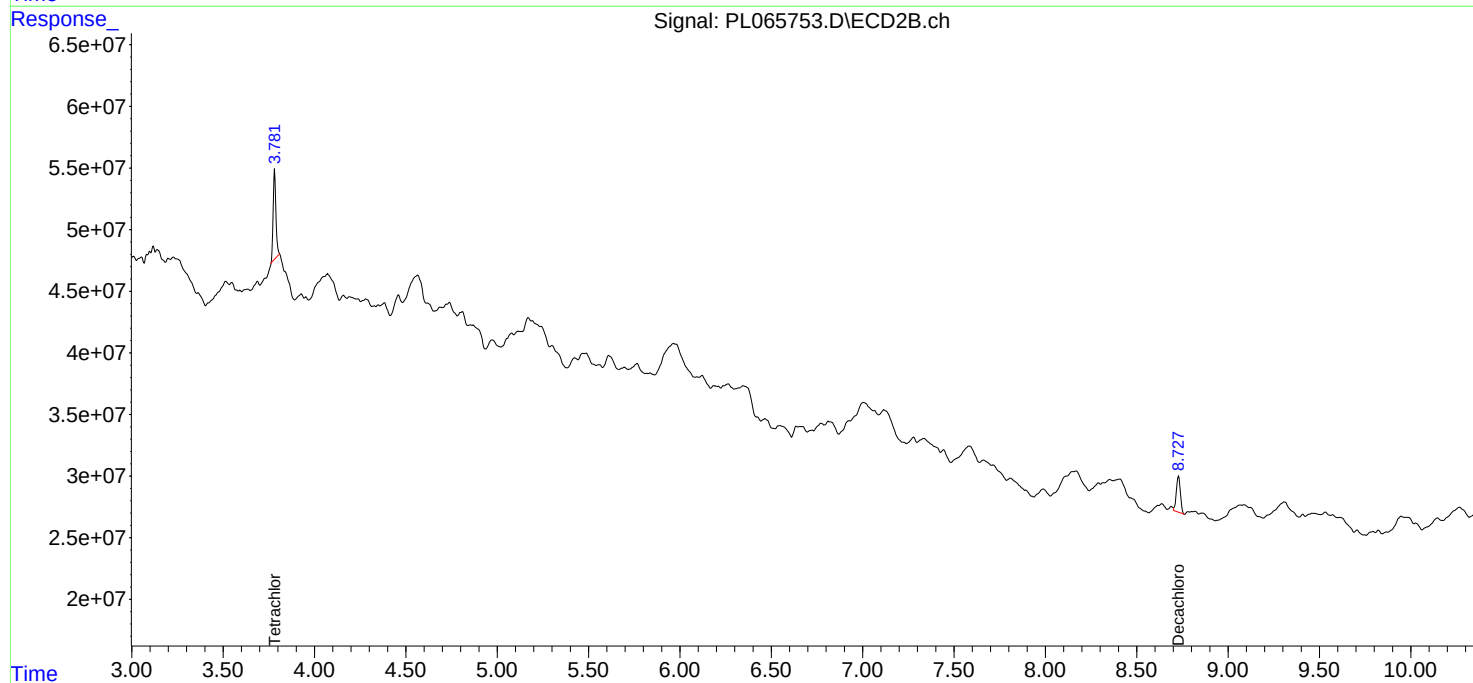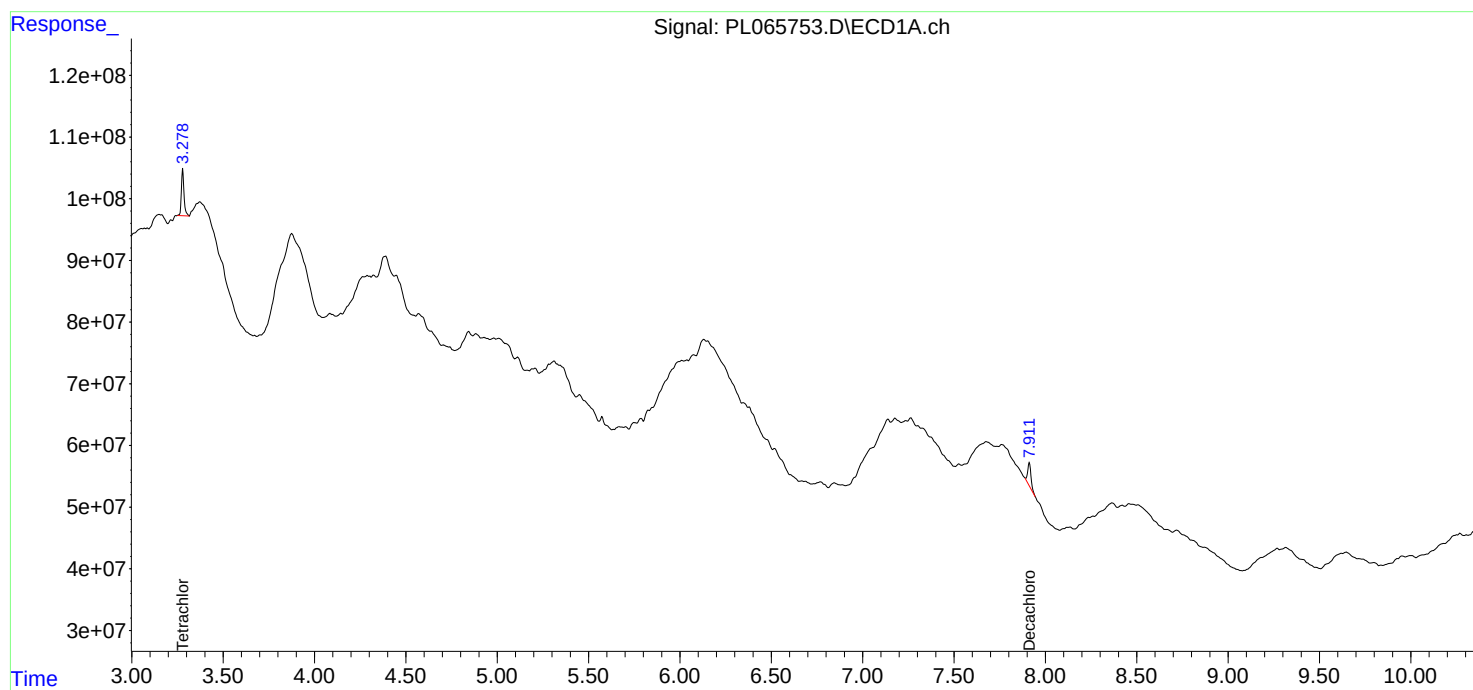

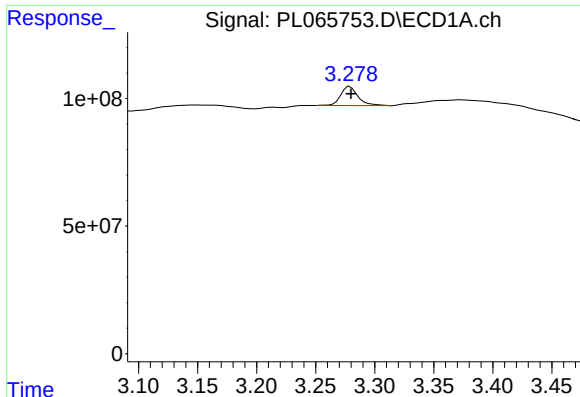


#1 Tetrachloro-m-xylene

R.T.: 3.279 min
Delta R.T.: 0.000 min
Response: 76769026
Conc: 29.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
FS-SB18(9-10)


Manual Integrations
APPROVED

Ankita
4/1/2021 12:58:24 PM

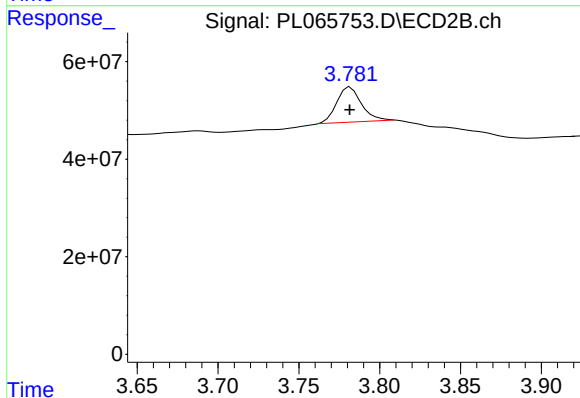


#1 Tetrachloro-m-xylene

R.T.: 3.781 min
Delta R.T.: -0.001 min
Response: 76358636
Conc: 27.82 ng/ml m

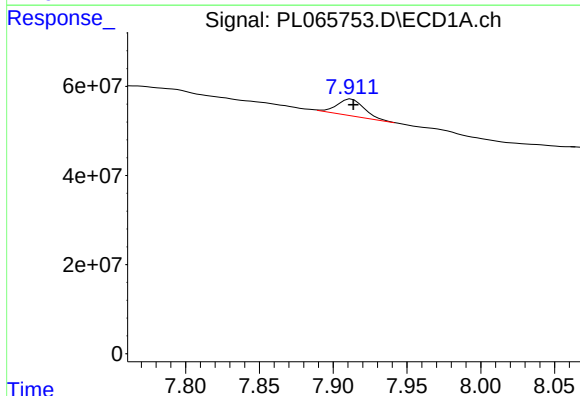

#28 Decachlorobiphenyl

R.T.: 7.911 min
Delta R.T.: -0.003 min
Response: 47928356
Conc: 20.69 ng/ml m

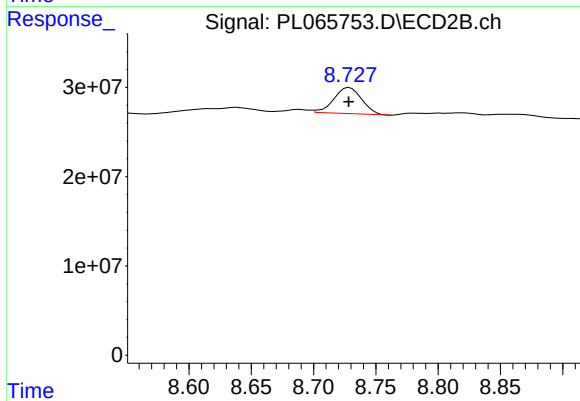

#28 Decachlorobiphenyl

R.T.: 8.729 min
Delta R.T.: 0.000 min
Response: 45259907
Conc: 20.08 ng/ml