

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL033121\
 Data File : PL065754.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Apr 2021 01:46
 Operator : AR\AJ
 Sample : M1874-02
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FS-SB18(24-25)

Manual Integrations
 APPROVED

Ankita
 4/1/2021 12:58:25 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 02:47:22 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 31 15:57:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.280	3.782	58341404	68672675	22.396	25.018
28) SA Decachlor...	7.913	8.728	46112157	47172536	19.910	20.924m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL033121\
Data File : PL065754.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Apr 2021 01:46
Operator : AR\AJ
Sample : M1874-02
Misc :
ALS Vial : 51 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
FS-SB18(24-25)


Manual Integrations
APPROVED

Ankita
4/1/2021 12:58:25 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 02:47:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
Quant Title : GC Extractables
QLast Update : Wed Mar 31 15:57:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

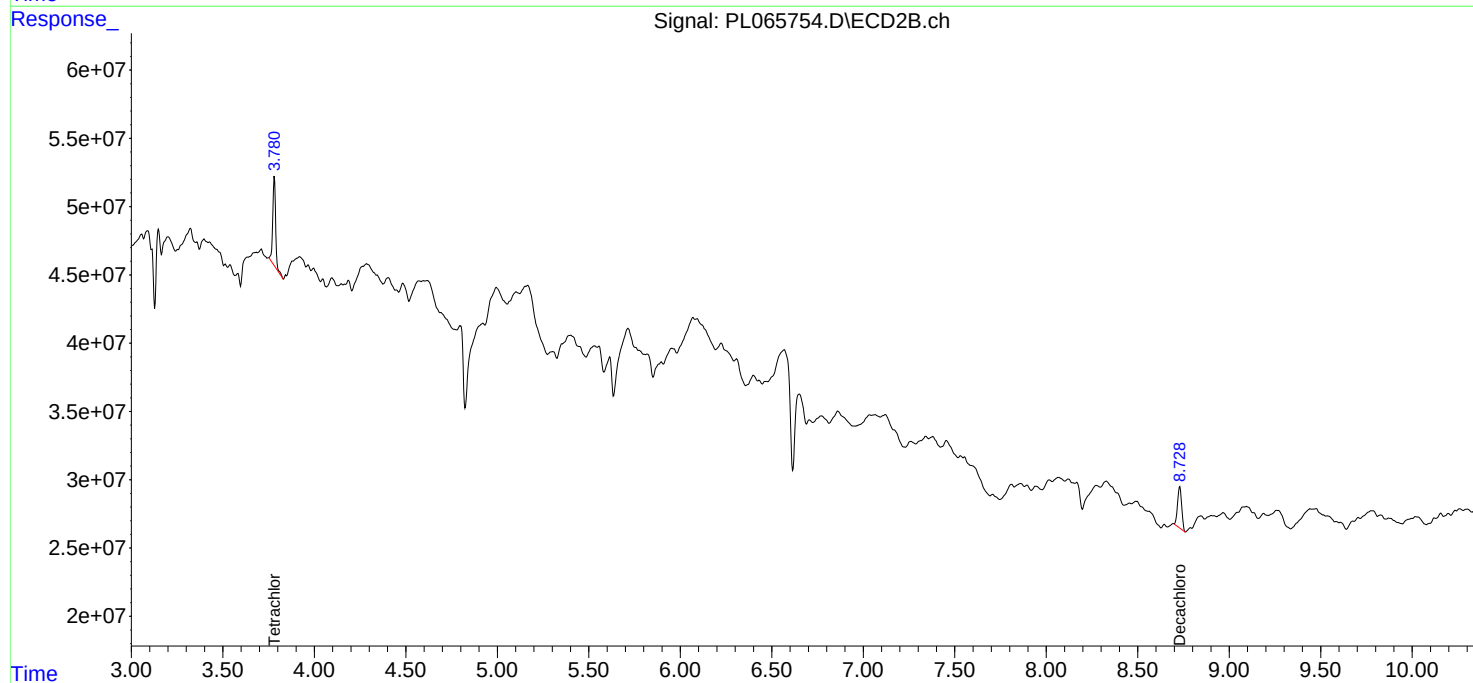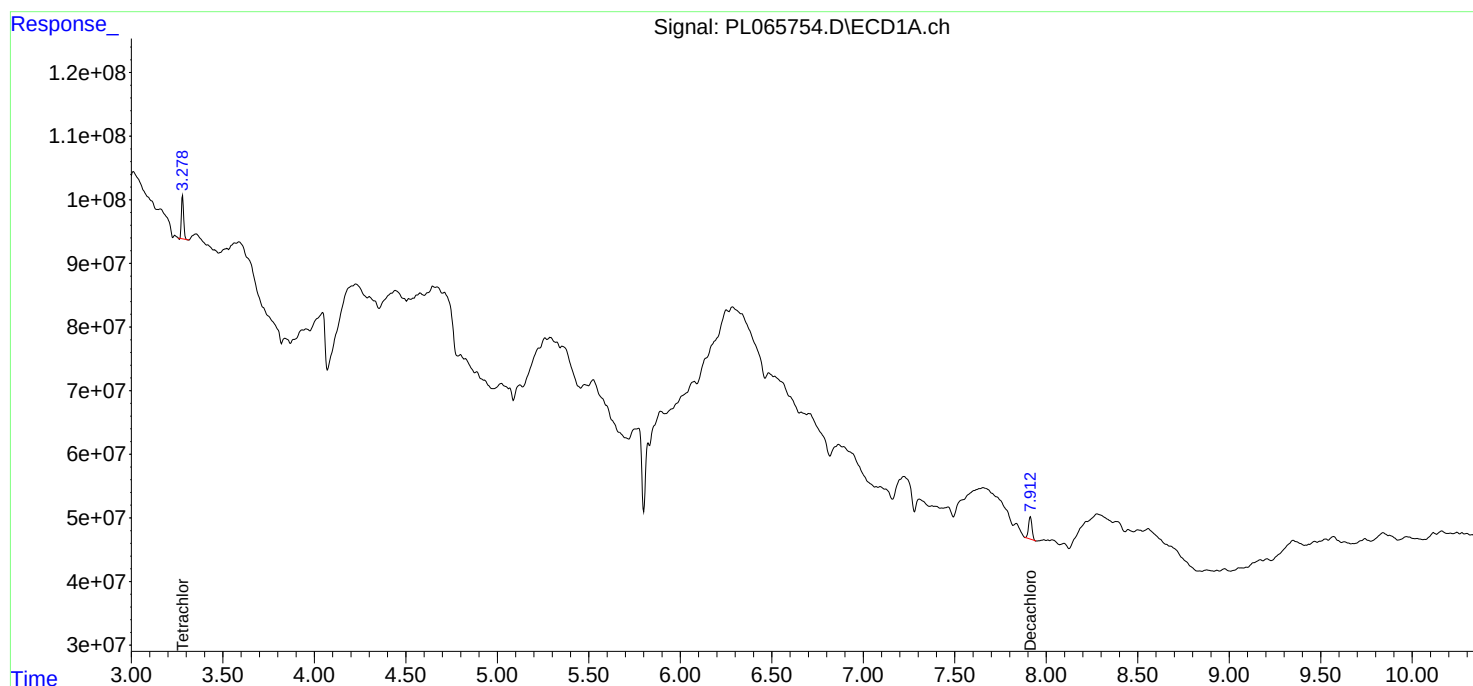

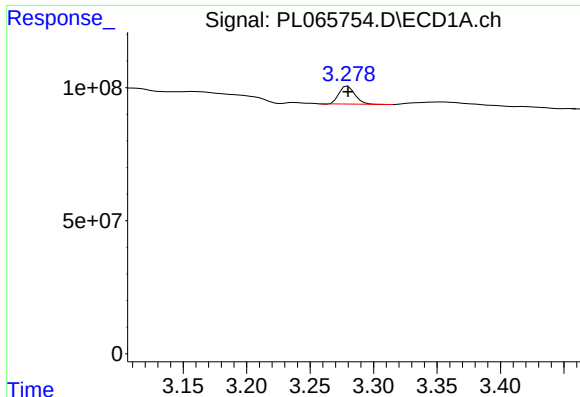


#1 Tetrachloro-m-xylene

R.T.: 3.280 min
Delta R.T.: 0.000 min
Response: 58341404
Conc: 22.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
FS-SB18(24-25)


Manual Integrations
APPROVED

Ankita
4/1/2021 12:58:25 PM

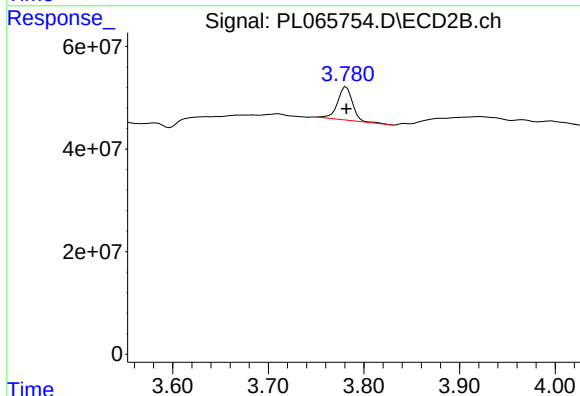


#1 Tetrachloro-m-xylene

R.T.: 3.782 min
Delta R.T.: 0.000 min
Response: 68672675
Conc: 25.02 ng/ml

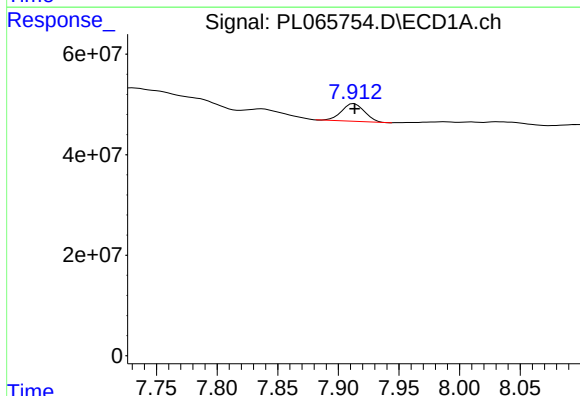

#28 Decachlorobiphenyl

R.T.: 7.913 min
Delta R.T.: 0.000 min
Response: 46112157
Conc: 19.91 ng/ml

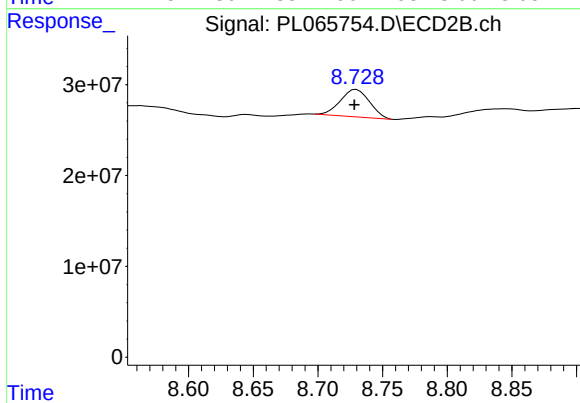

#28 Decachlorobiphenyl

R.T.: 8.728 min
Delta R.T.: 0.000 min
Response: 47172536
Conc: 20.92 ng/ml m