

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL033123\
 Data File : PL081814.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Mar 2023 13:41
 Operator : AR\AJ
 Sample : 02136-01 10X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SU-03-033023

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 04/03/2023
 Supervised By : Ankita Jodhani 04/03/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 31 22:13:12 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032223.M
 Quant Title : GC Extractables
 QLast Update : Thu Mar 23 01:07:33 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.328	2.656	4886903	4333519	2.101	2.171
28) SA Decachlor...	8.744	7.773	4130408	4856582	2.308m	2.449

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL033123\
Data File : PL081814.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Mar 2023 13:41
Operator : AR\AJ
Sample : 02136-01 10X
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SU-03-033023


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 04/03/2023
Supervised By : Ankita Jodhani 04/03/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 31 22:13:12 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032223.M
Quant Title : GC Extractables
QLast Update : Thu Mar 23 01:07:33 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

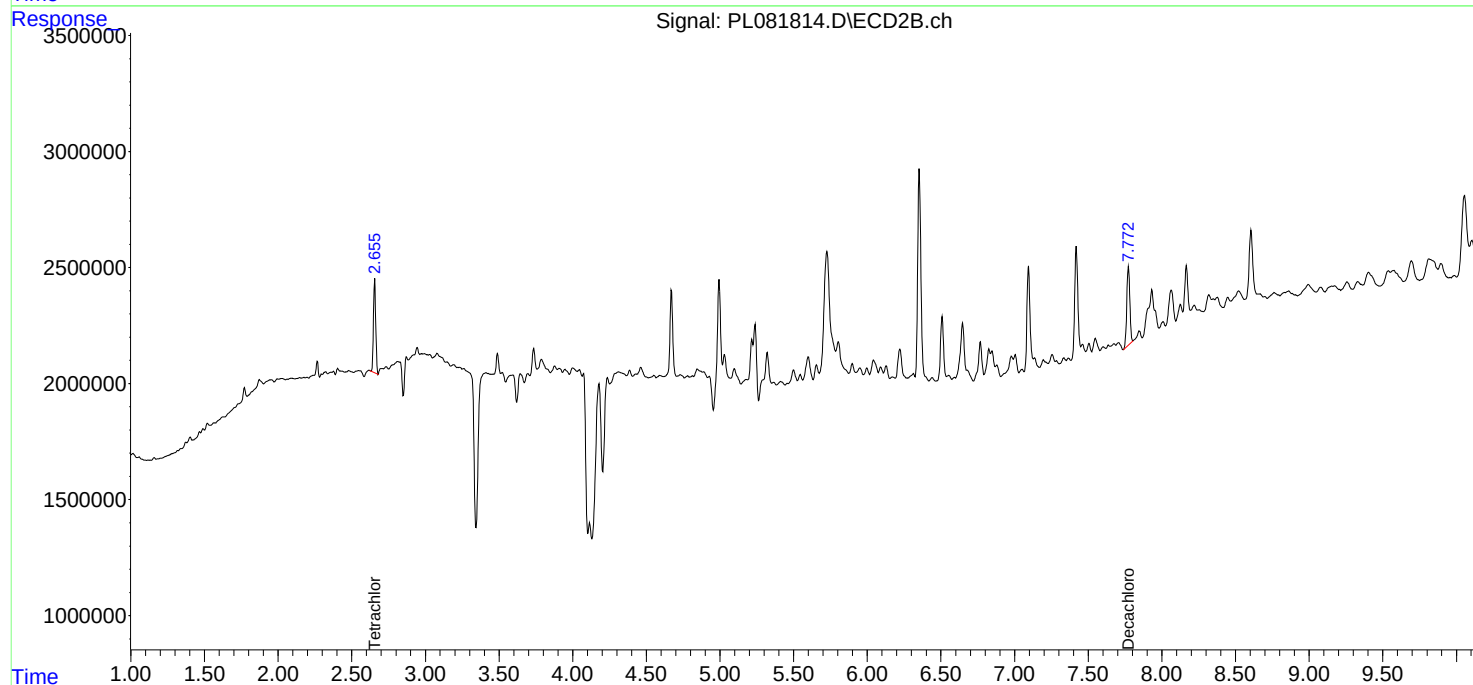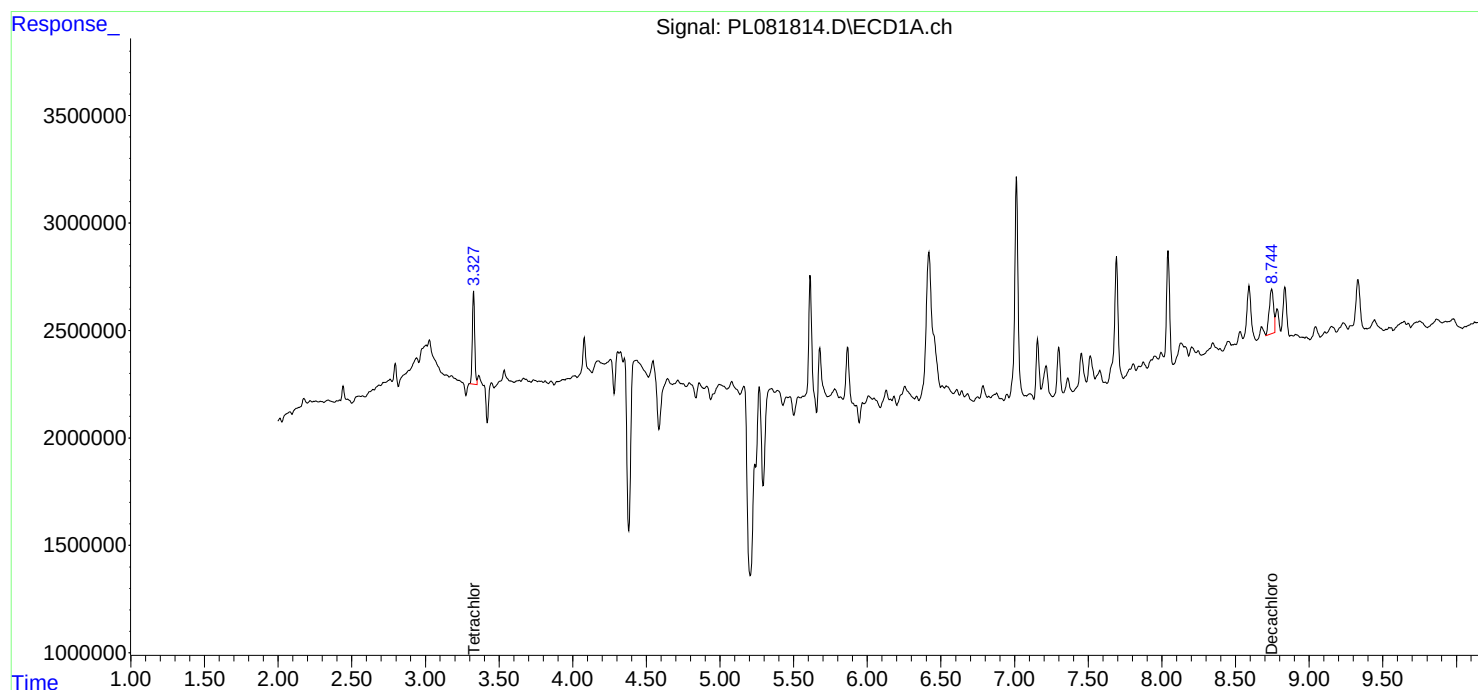

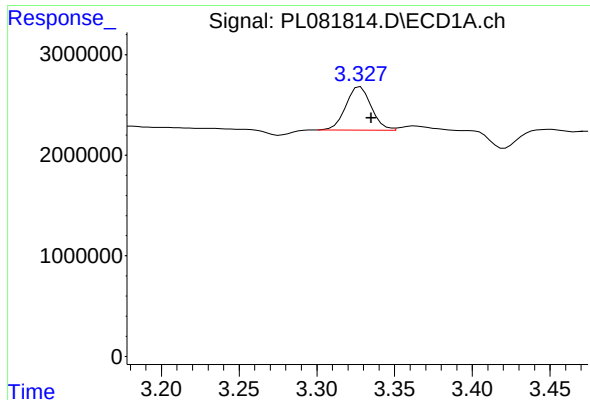


#1 Tetrachloro-m-xylene

R.T.: 3.328 min
Delta R.T.: -0.007 min
Response: 4886903
Conc: 2.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
SU-03-033023


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 04/03/2023
Supervised By :Ankita Jodhani 04/03/2023

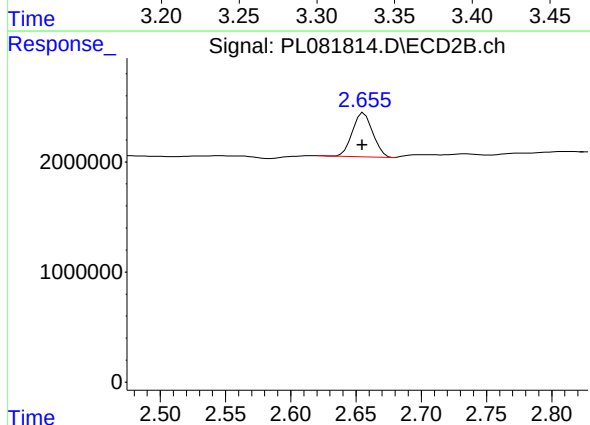


#1 Tetrachloro-m-xylene

R.T.: 2.656 min
Delta R.T.: 0.001 min
Response: 4333519
Conc: 2.17 ng/ml

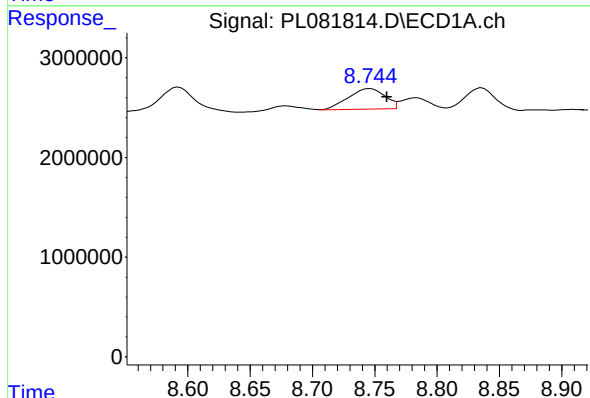

#28 Decachlorobiphenyl

R.T.: 8.744 min
Delta R.T.: -0.015 min
Response: 4130408
Conc: 2.31 ng/ml m

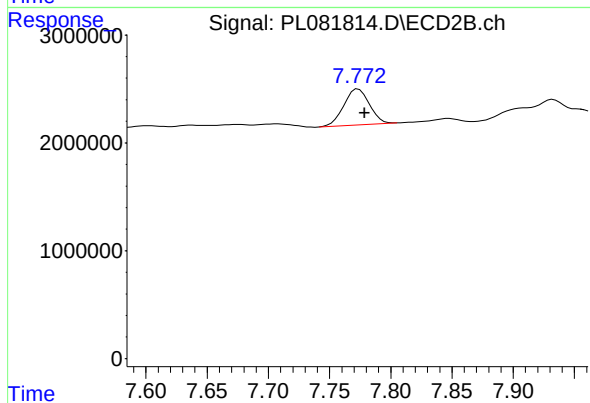

#28 Decachlorobiphenyl

R.T.: 7.773 min
Delta R.T.: -0.005 min
Response: 4856582
Conc: 2.45 ng/ml