

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL033125\
 Data File : PL094972.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Mar 2025 20:40
 Operator : AR\AJ
 Sample : Q1664-12
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 02:15:42 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 11 17:42:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.536	2.770	57165150	80498786	20.195	22.553
28)	SA Decachlor...	9.054	7.903	46869965	87703864	22.240	21.712
Target Compounds							
3)	MA gamma-BHC...	0.000	3.612	0	17649755	N.D.	3.434 #
6)	B beta-BHC	4.543f	0.000	457884	0	0.248	N.D. #
7)	B delta-BHC	4.762	0.000	6477498	0	1.663	N.D. #
9)	A Endosulfan I	0.000	5.123f	0	24391133	N.D.	5.558 #
10)	B gamma-Chl...	5.919f	0.000	5591251	0	1.659	N.D. #
13)	MA Dieldrin	0.000	5.368	0	40622298	N.D.	8.373 #
23)	Chlordane-1	0.000	3.781	0	11359677	N.D.	75.214 #
25)	Chlordane-3	5.919f	0.000	5591251	0	11.187	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL033125\
Data File : PL094972.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Mar 2025 20:40
Operator : AR\AJ
Sample : Q1664-12
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 02:15:42 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
Quant Title : GC Extractables
QLast Update : Tue Mar 11 17:42:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

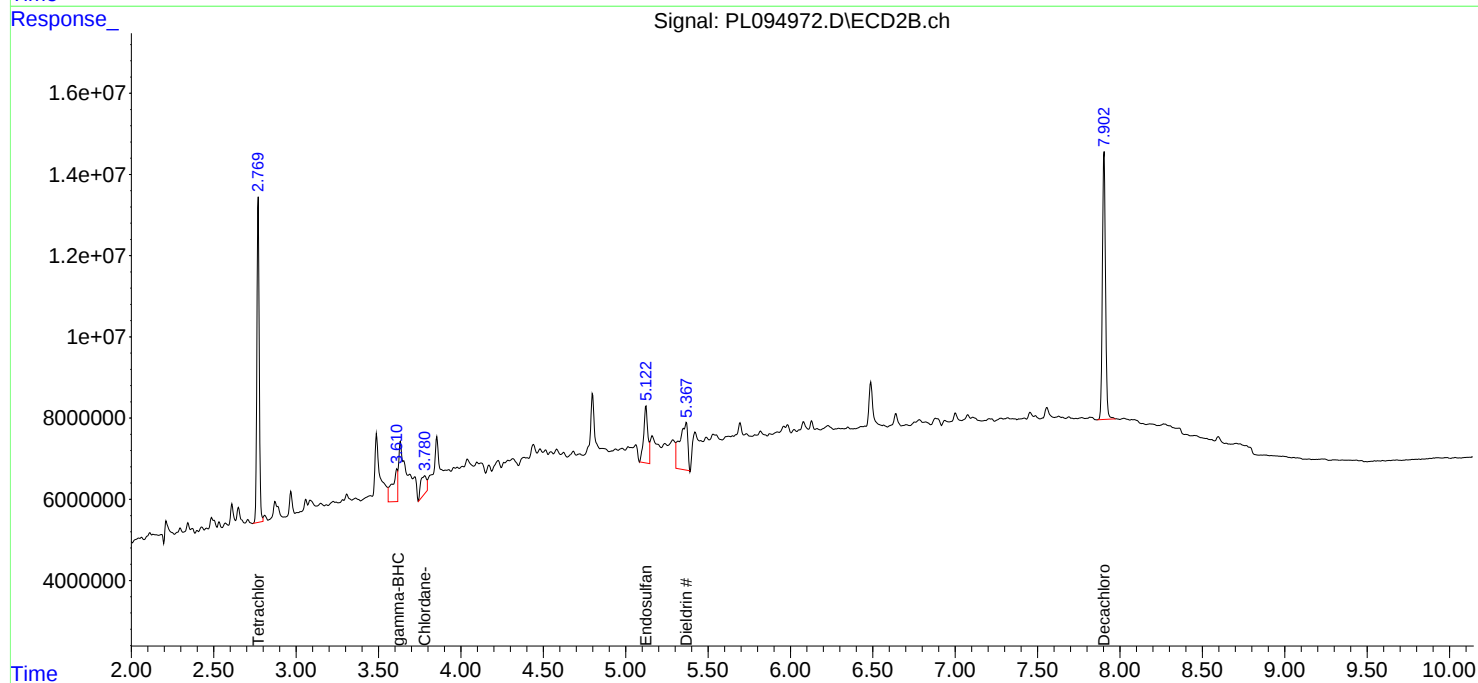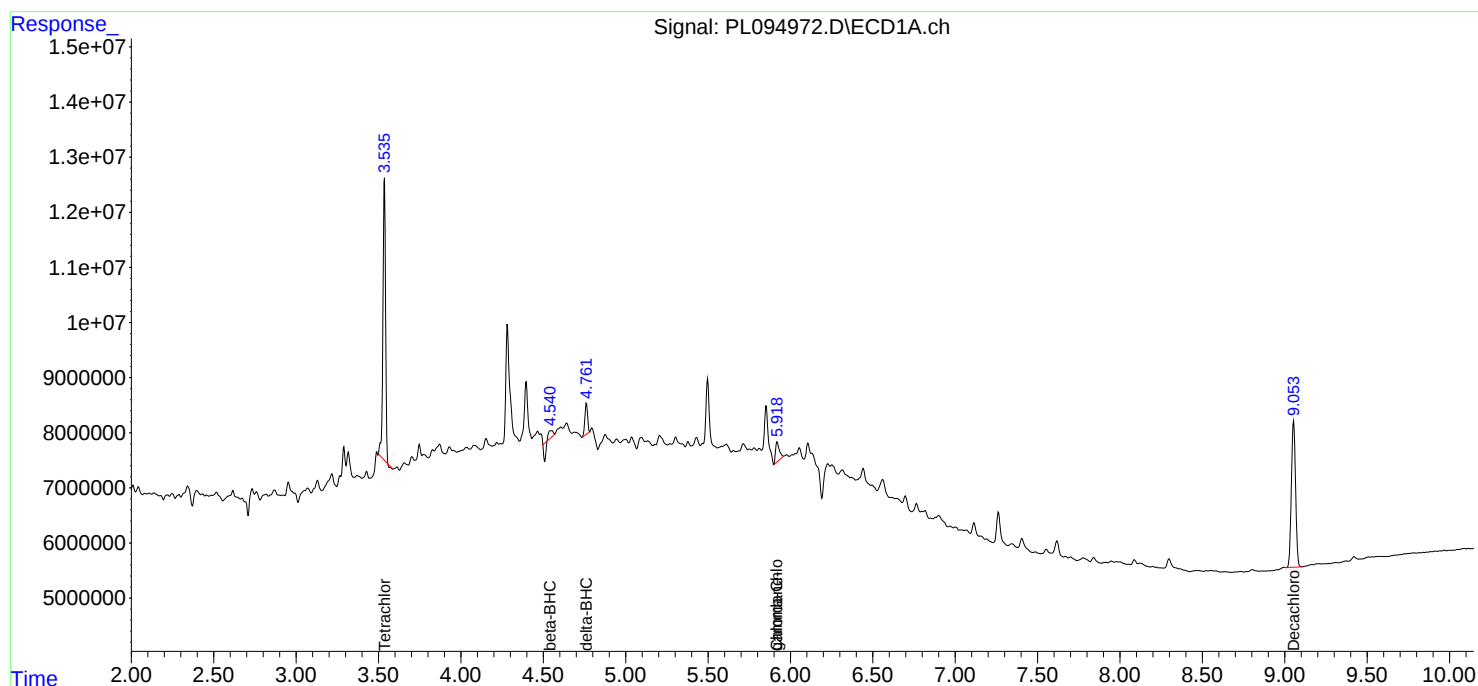


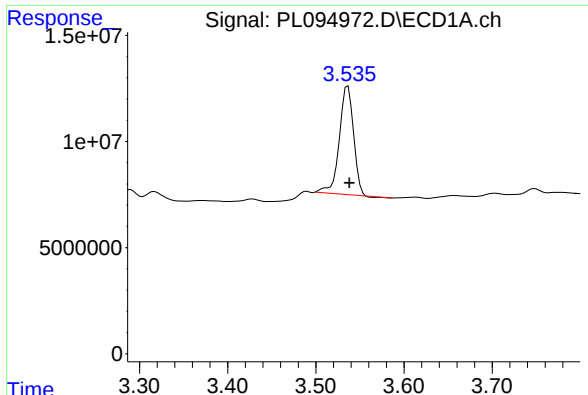

#1 Tetrachloro-m-xylene


R.T.: 3.536 min
Delta R.T.: -0.002 min
Response: 57165150
Conc: 20.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

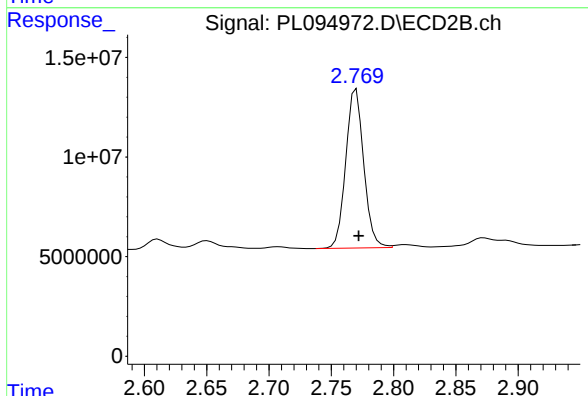


#1 Tetrachloro-m-xylene

R.T.: 2.770 min
Delta R.T.: -0.002 min
Response: 80498786
Conc: 22.55 ng/ml

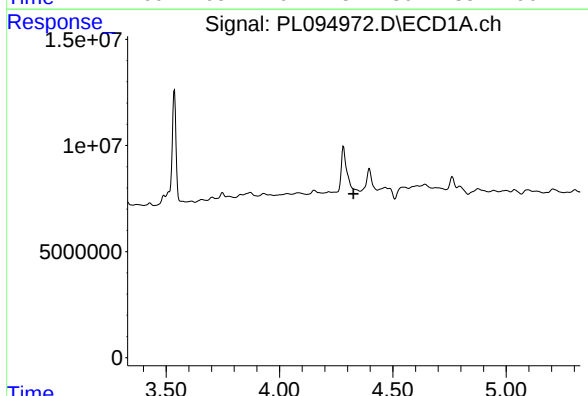


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.327 min
Response: 0
Conc: N.D.

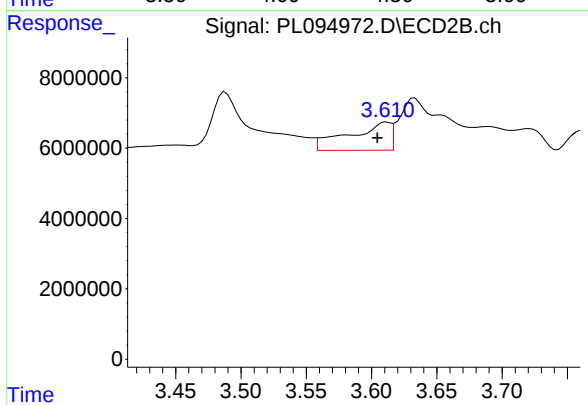

#3 gamma-BHC (Lindane)


R.T.: 3.612 min
Delta R.T.: 0.007 min
Response: 17649755
Conc: 3.43 ng/ml

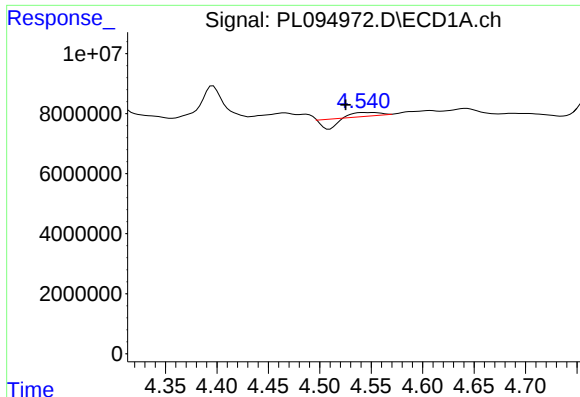

#6 beta-BHC


R.T.: 4.543 min
Delta R.T.: 0.017 min
Response: 457884
Conc: 0.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

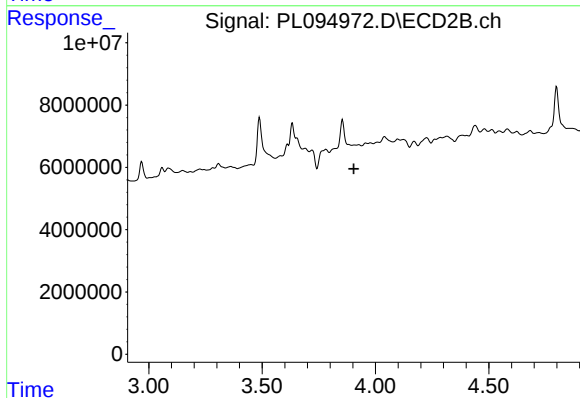


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 3.905 min
Response: 0
Conc: N.D.

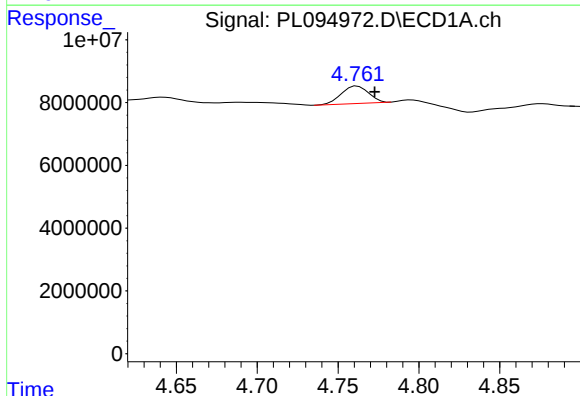


#7 delta-BHC

R.T.: 4.762 min
Delta R.T.: -0.011 min
Response: 6477498
Conc: 1.66 ng/ml

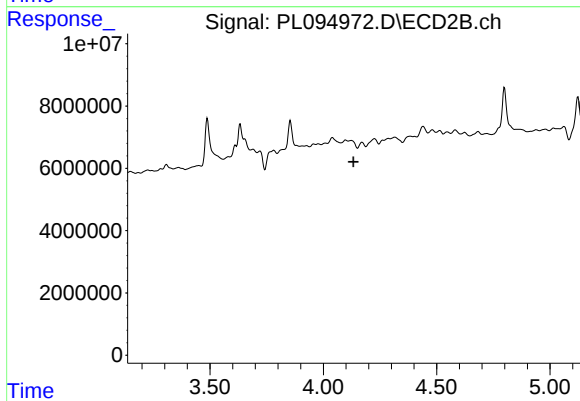

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.133 min
Response: 0
Conc: N.D.

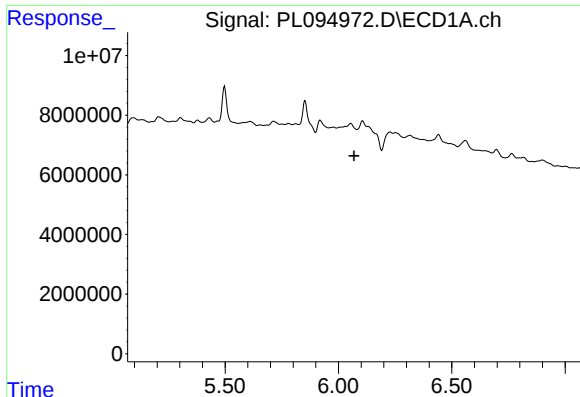

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.069 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

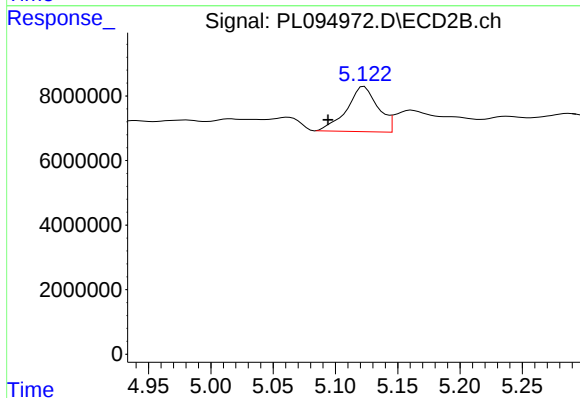


#9 Endosulfan I

R.T.: 5.123 min
Delta R.T.: 0.029 min
Response: 24391133
Conc: 5.56 ng/ml

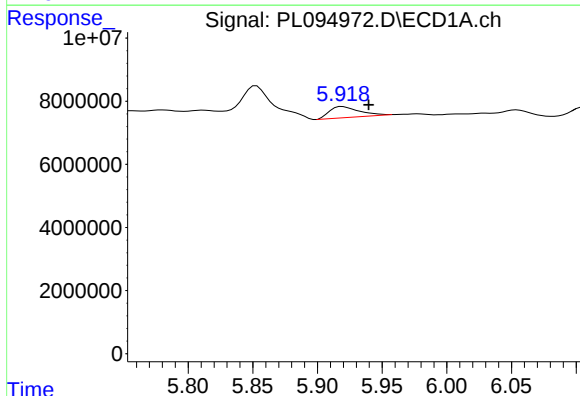


#10 gamma-Chlordane

R.T.: 5.919 min
Delta R.T.: -0.020 min
Response: 5591251
Conc: 1.66 ng/ml

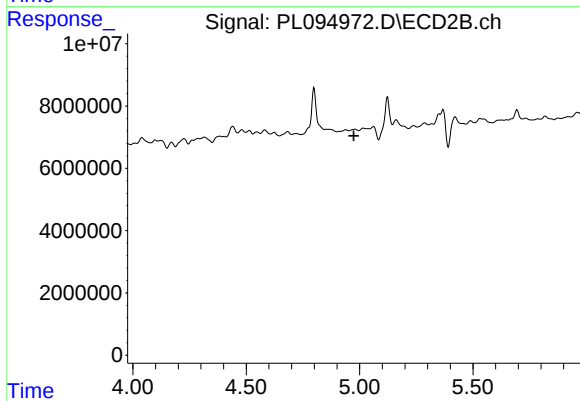

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 4.974 min
Response: 0
Conc: N.D.

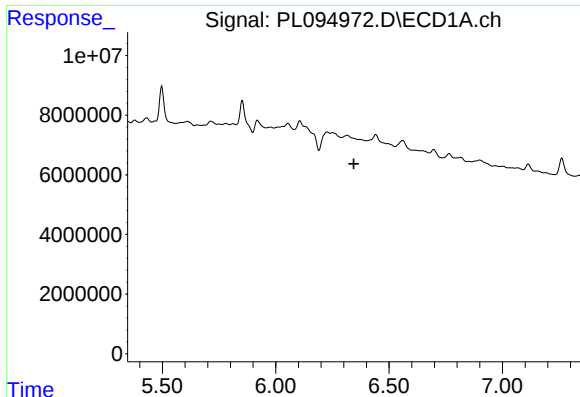

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.344 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

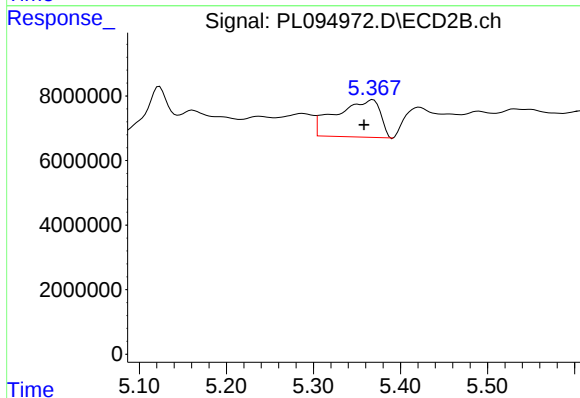


#13 Dieldrin

R.T.: 5.368 min
Delta R.T.: 0.010 min
Response: 40622298
Conc: 8.37 ng/ml

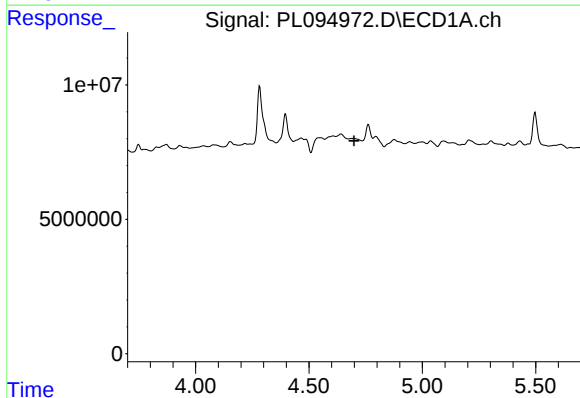


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.700 min
Response: 0
Conc: N.D.

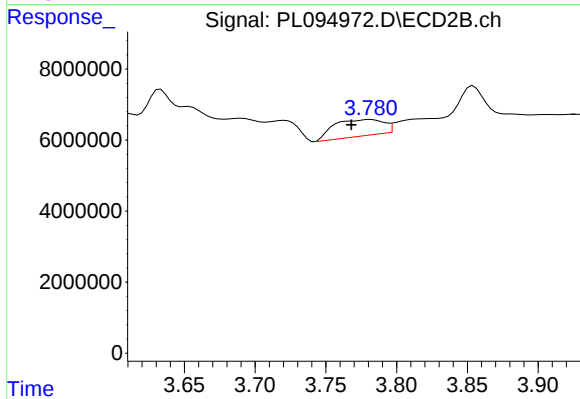

#23 Chlordane-1


R.T.: 3.781 min
Delta R.T.: 0.013 min
Response: 11359677
Conc: 75.21 ng/ml

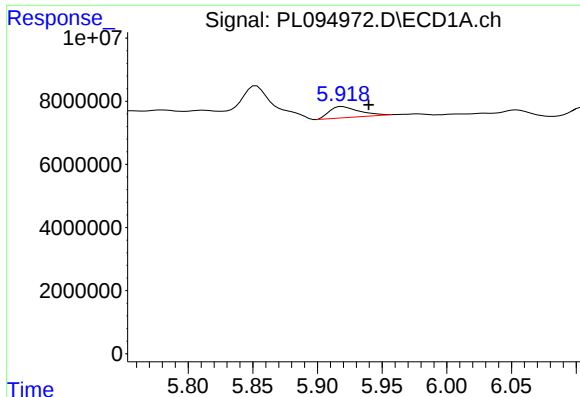

#25 Chlordane-3


R.T.: 5.919 min
Delta R.T.: -0.020 min
Response: 5591251
Conc: 11.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

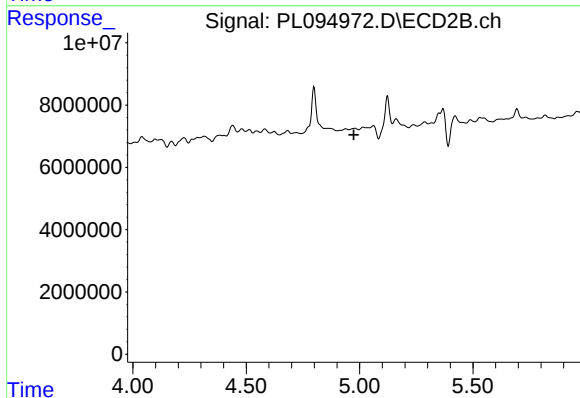


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 4.975 min
Response: 0
Conc: N.D.

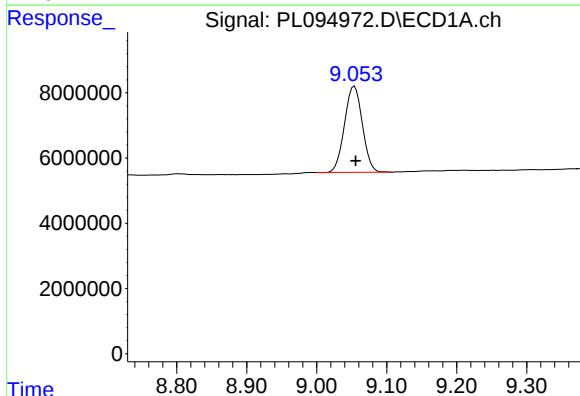

#28 Decachlorobiphenyl

R.T.: 9.054 min
Delta R.T.: -0.002 min
Response: 46869965
Conc: 22.24 ng/ml

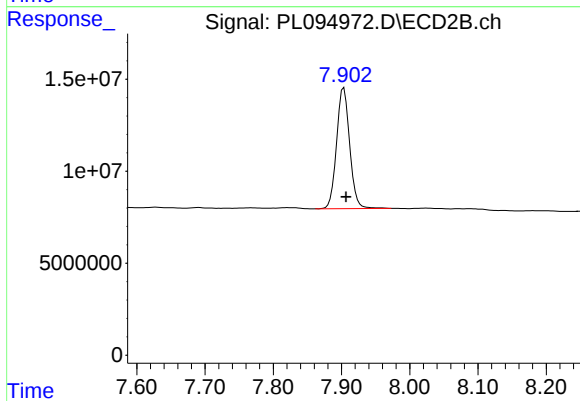

#28 Decachlorobiphenyl

R.T.: 7.903 min
Delta R.T.: -0.003 min
Response: 87703864
Conc: 21.71 ng/ml