

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040119\
 Data File : PL046865.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Apr 2019 06:24
 Operator : AJ\SJ
 Sample : K2180-07
 Misc :
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-6S

Manual Integrations
 APPROVED

Sohil
 4/2/2019 10:26:59 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 02 06:38:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.358	3.976	66609560	21592617	9.156	9.431
28) SA Decachlor...	8.033	9.027	100.3E6	31150373	11.919	13.436
Target Compounds						
12) B 4,4'-DDE	5.473	6.310	6505087	1345161	0.707m	0.542
17) MA 4,4'-DDT	6.217	7.096	3283433	1079650	0.433m	0.515m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040119\
Data File : PL046865.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Apr 2019 06:24
Operator : AJ\SJ
Sample : K2180-07
Misc :
ALS Vial : 71 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-6S


Manual Integrations
APPROVED

Sohil
4/2/2019 10:26:59 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 02 06:38:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

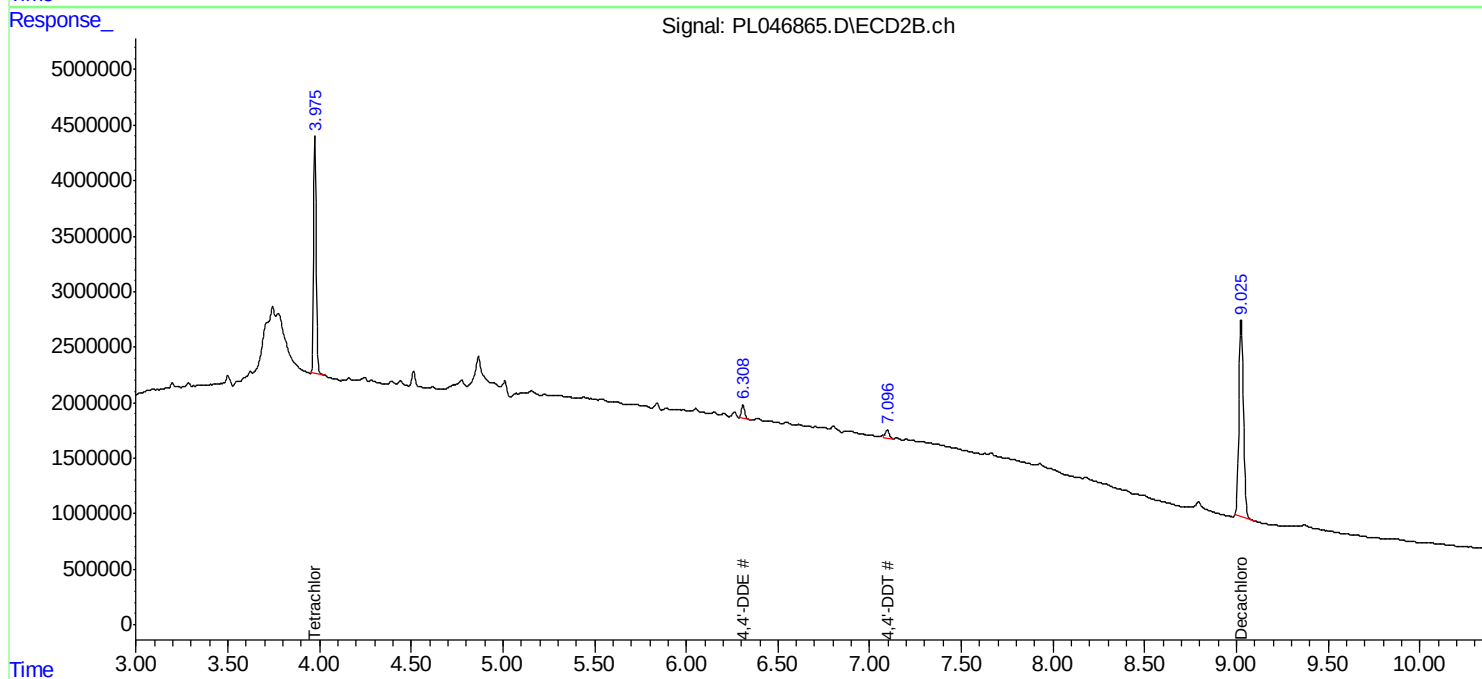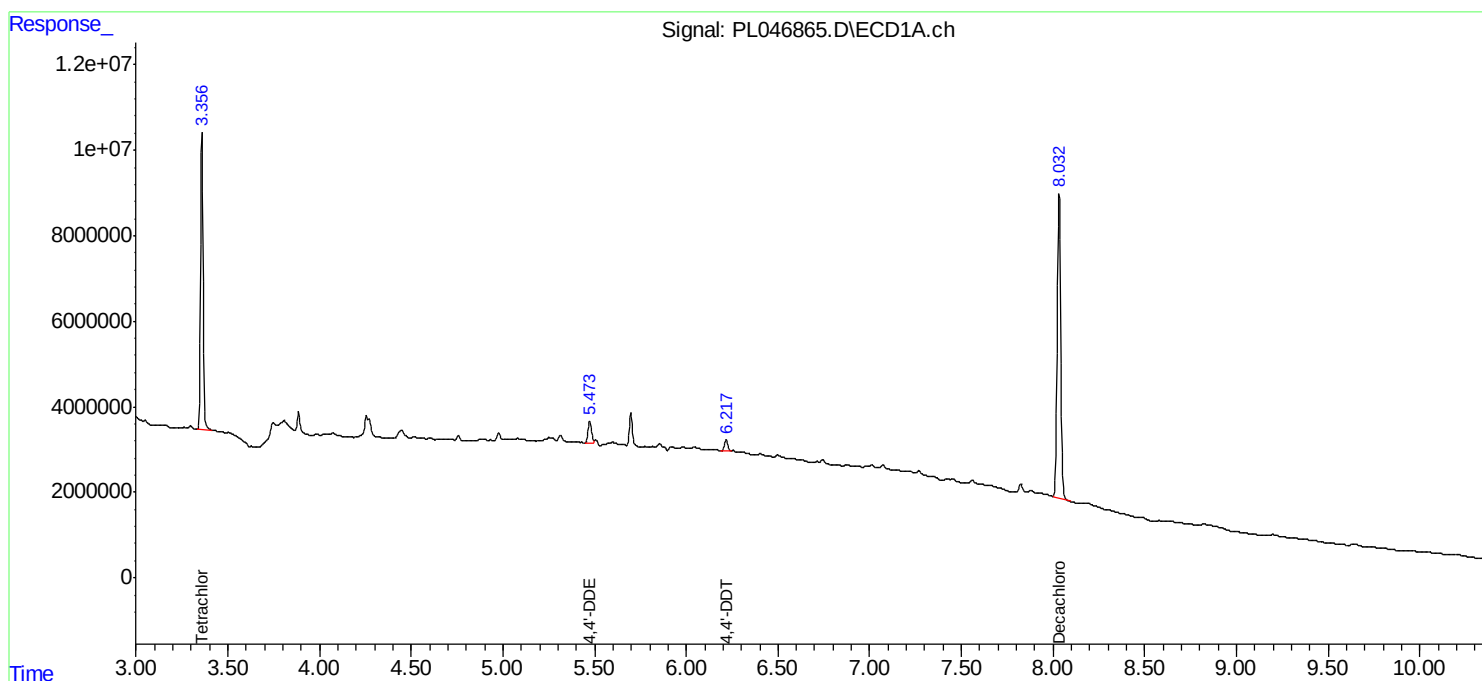

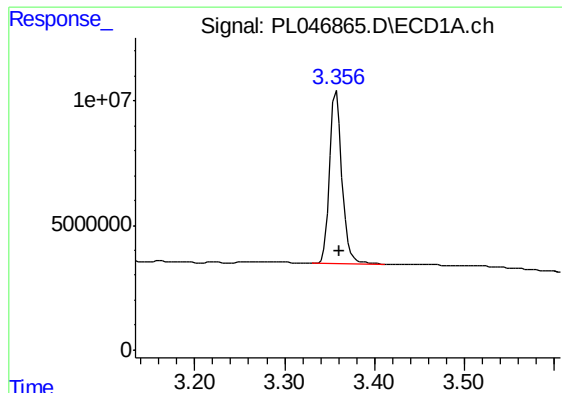


#1 Tetrachloro-m-xylene

R.T.: 3.358 min
Delta R.T.: -0.003 min
Response: 66609560
Conc: 9.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-6S


Manual Integrations
APPROVED

Sohil
4/2/2019 10:26:59 AM

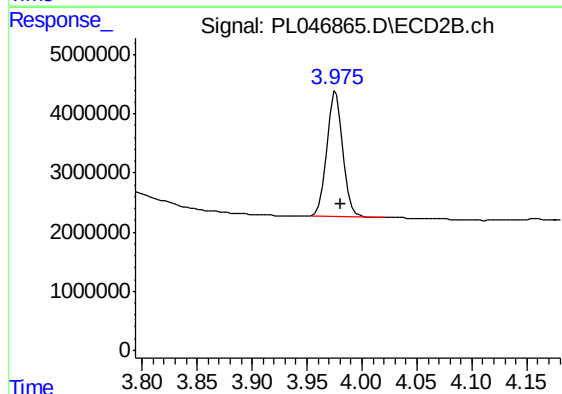


#1 Tetrachloro-m-xylene

R.T.: 3.976 min
Delta R.T.: -0.004 min
Response: 21592617
Conc: 9.43 ng/ml

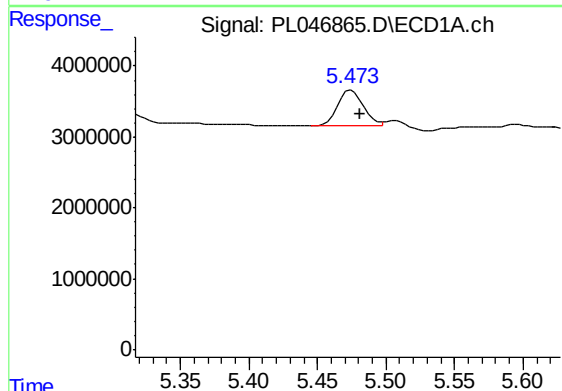


#12 4,4'-DDE

R.T.: 5.473 min
Delta R.T.: -0.007 min
Response: 6505087
Conc: 0.71 ng/ml m

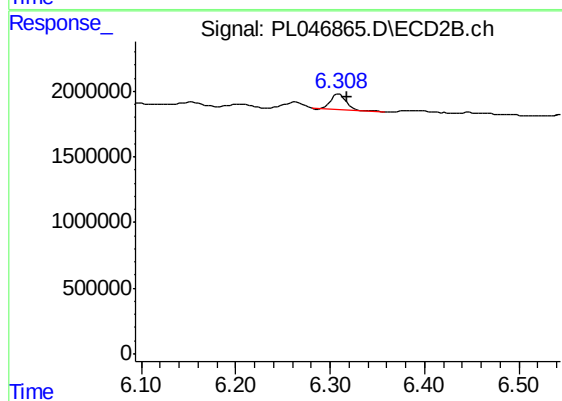

#12 4,4'-DDE

R.T.: 6.310 min
Delta R.T.: -0.008 min
Response: 1345161
Conc: 0.54 ng/ml

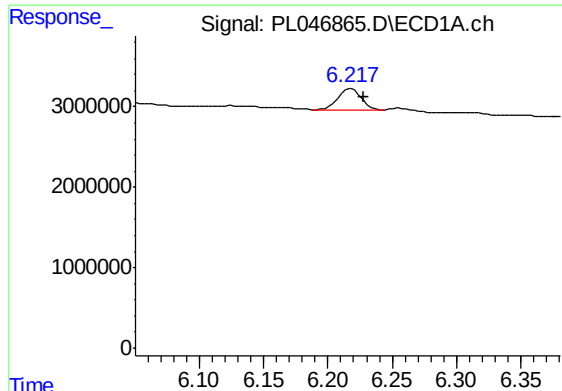


#17 4,4'-DDT

R.T.: 6.217 min
Delta R.T.: -0.011 min
Response: 3283433
Conc: 0.43 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TP-6S


Manual Integrations
APPROVED

Sohil
4/2/2019 10:26:59 AM

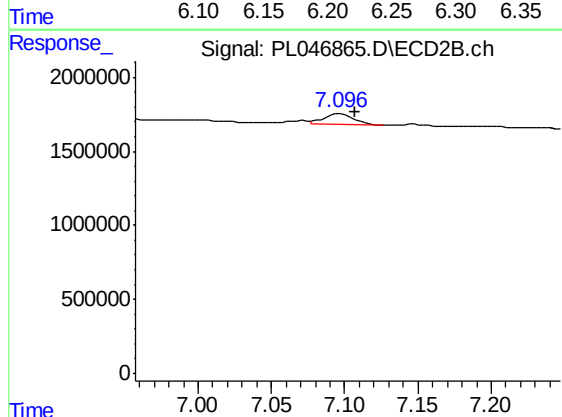


#17 4,4'-DDT

R.T.: 7.096 min
Delta R.T.: -0.011 min
Response: 1079650
Conc: 0.51 ng/ml m

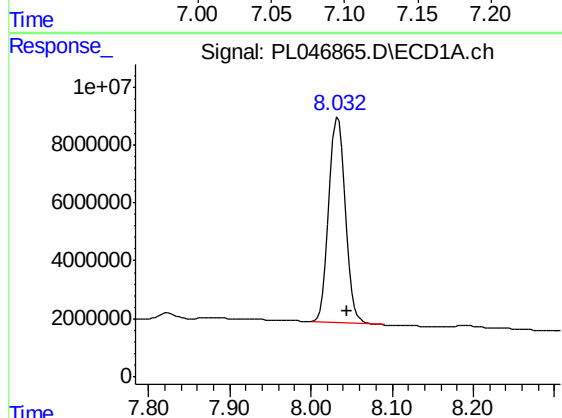

#28 Decachlorobiphenyl

R.T.: 8.033 min
Delta R.T.: -0.011 min
Response: 100254198
Conc: 11.92 ng/ml

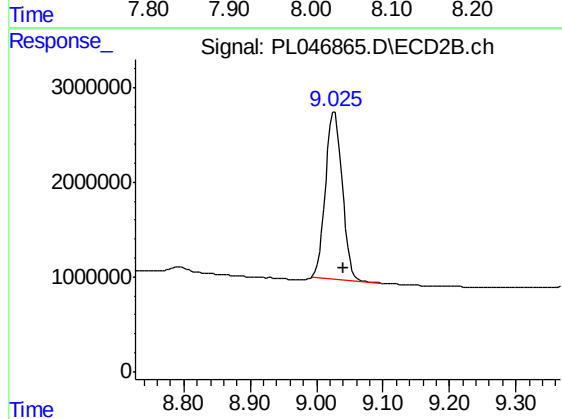

#28 Decachlorobiphenyl

R.T.: 9.027 min
Delta R.T.: -0.013 min
Response: 31150373
Conc: 13.44 ng/ml