

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040121\
 Data File : PL065781.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Apr 2021 15:54
 Operator : AR\AJ
 Sample : PB135458BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB135458BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 02 02:12:10 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 31 15:57:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.278	3.781	50117382	53253057	19.239	19.400
28)	SA Decachlor...	7.912	8.730	47314912	45065974	20.429	19.989
Target Compounds							
2)	A alpha-BHC	3.686f	0.000	1602180	0	0.392	N.D. #
5)	MB Aldrin	0.000	5.238	0	251846	N.D.	0.076 #
6)	B beta-BHC	0.000	4.631	0	4689083	N.D.	2.692 #
8)	B Heptachlo...	0.000	5.618	0	1734667	N.D.	0.559 #
14)	MA Endrin	5.755	0.000	667666	0	0.247	N.D. #
15)	B Endosulfa...	6.019	6.630f	957679	694128	0.386	0.294
21)	B Endrin ke...	0.000	7.440f	0	672488	N.D.	0.262 #
27)	Chlordane-5	6.019	0.000	957679	0	9.363	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040121\
Data File : PL065781.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Apr 2021 15:54
Operator : AR\AJ
Sample : PB135458BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB135458BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 02 02:12:10 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
Quant Title : GC Extractables
QLast Update : Wed Mar 31 15:57:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

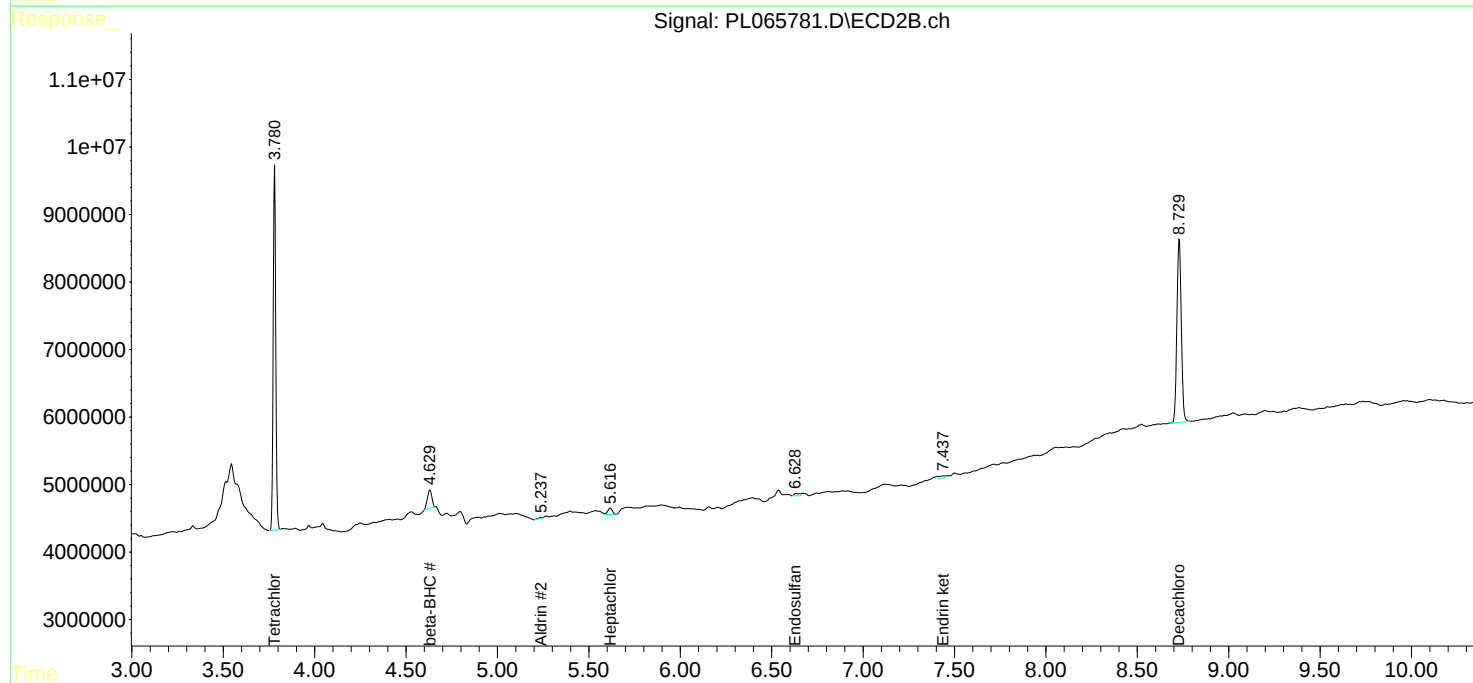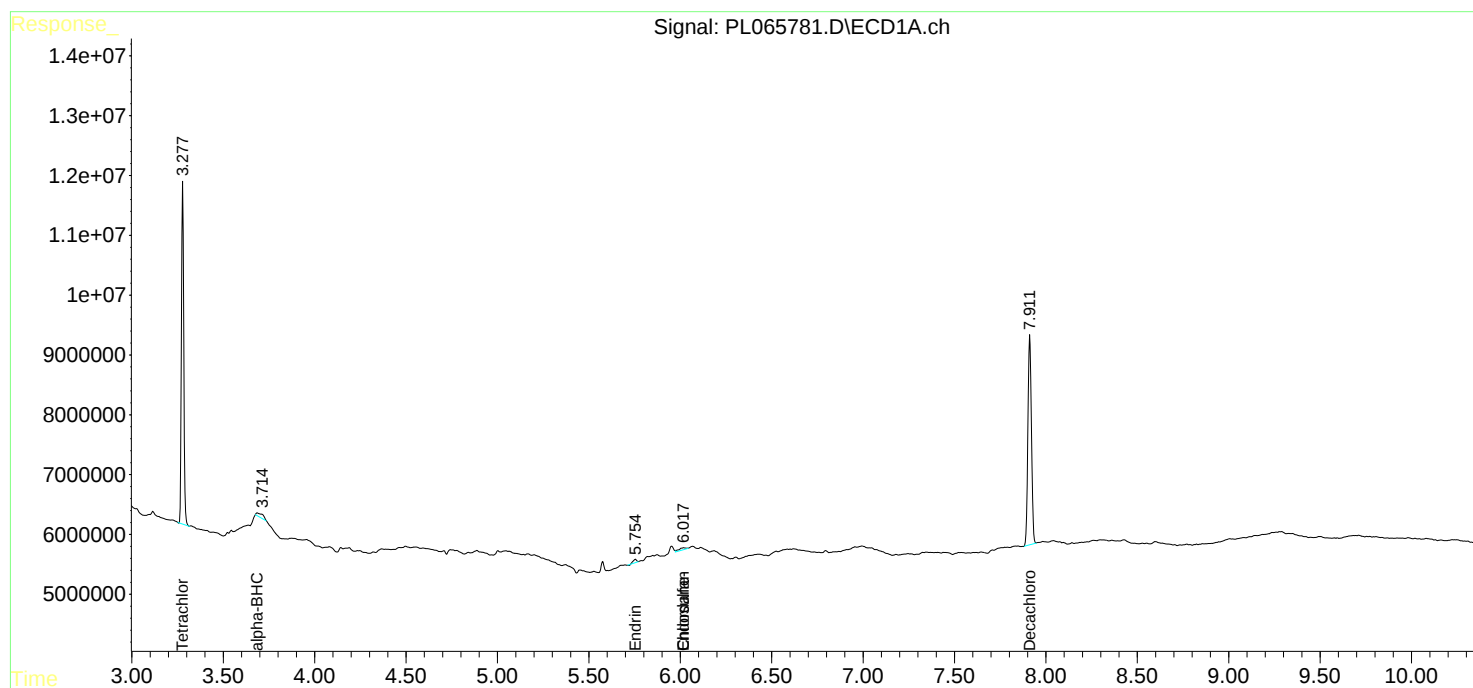


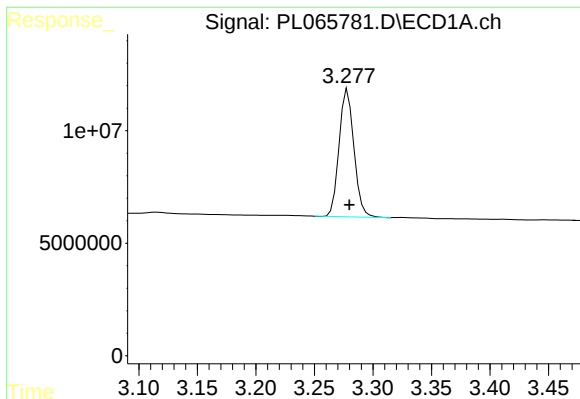

#1 Tetrachloro-m-xylene


R.T.: 3.278 min
Delta R.T.: -0.002 min
Response: 50117382
Conc: 19.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB135458BL

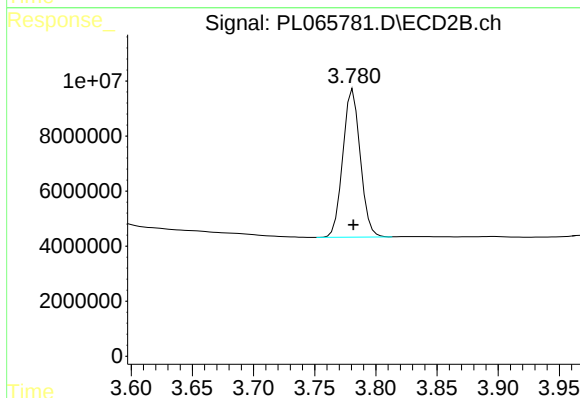


#1 Tetrachloro-m-xylene

R.T.: 3.781 min
Delta R.T.: 0.000 min
Response: 53253057
Conc: 19.40 ng/ml

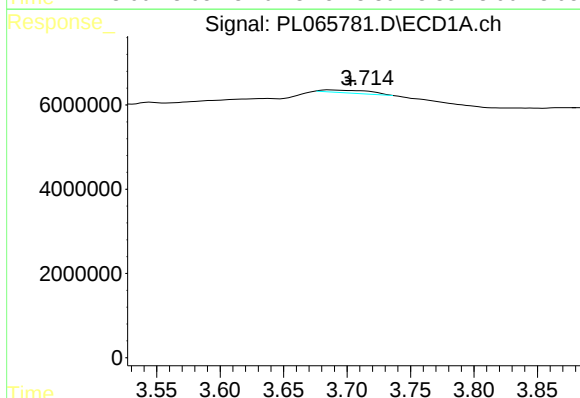


#2 alpha-BHC

R.T.: 3.686 min
Delta R.T.: -0.017 min
Response: 1602180
Conc: 0.39 ng/ml

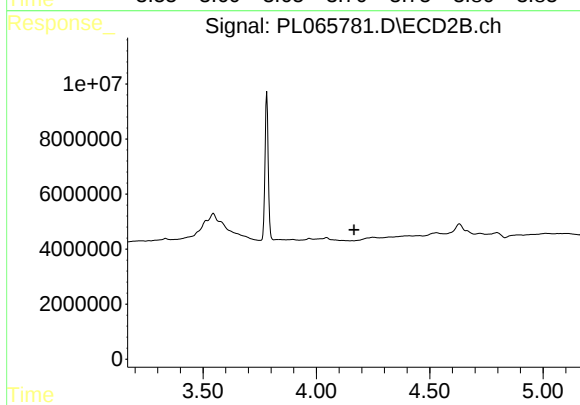

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.167 min
Response: 0
Conc: N.D.

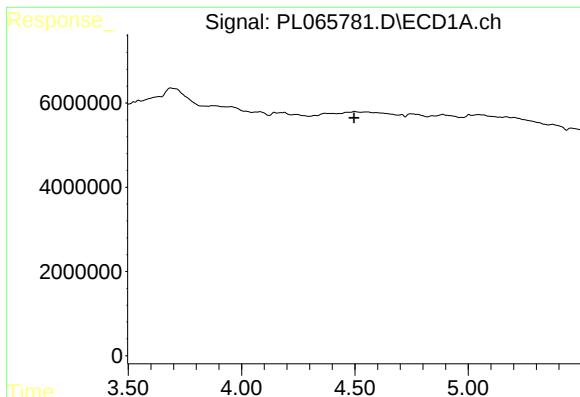

#5 Aldrin


R.T.: 0.000 min
Exp R.T. : 4.497 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB135458BL

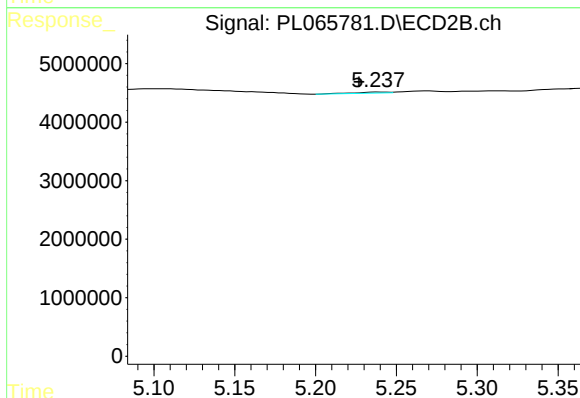


#5 Aldrin

R.T.: 5.238 min
Delta R.T.: 0.011 min
Response: 251846
Conc: 0.08 ng/ml

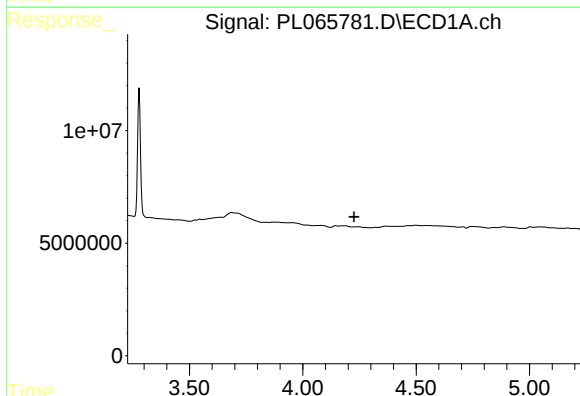


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.226 min
Response: 0
Conc: N.D.

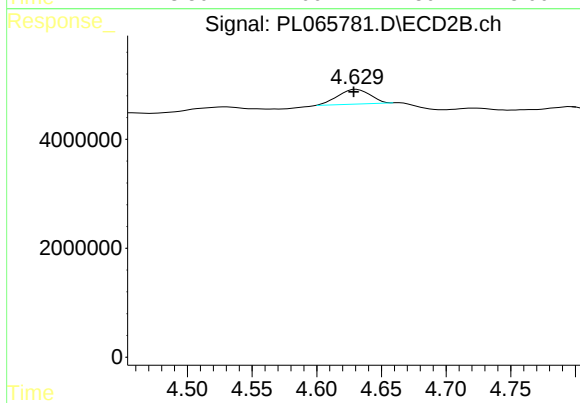

#6 beta-BHC


R.T.: 4.631 min
Delta R.T.: 0.002 min
Response: 4689083
Conc: 2.69 ng/ml

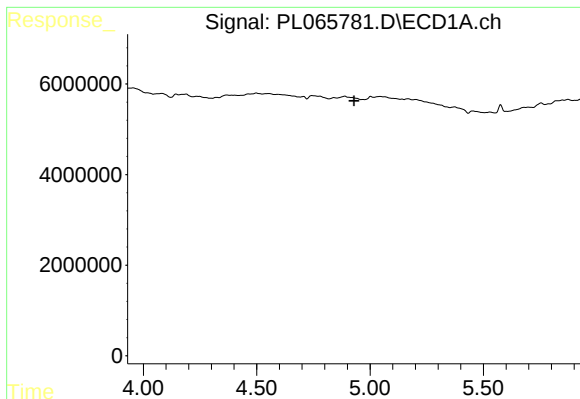

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.929 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB135458BL

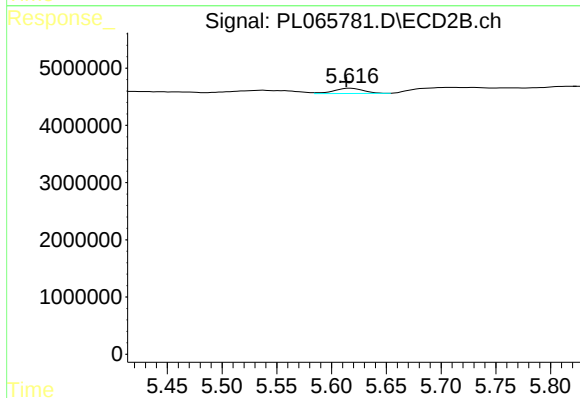


#8 Heptachlor epoxide

R.T.: 5.618 min
Delta R.T.: 0.004 min
Response: 1734667
Conc: 0.56 ng/ml

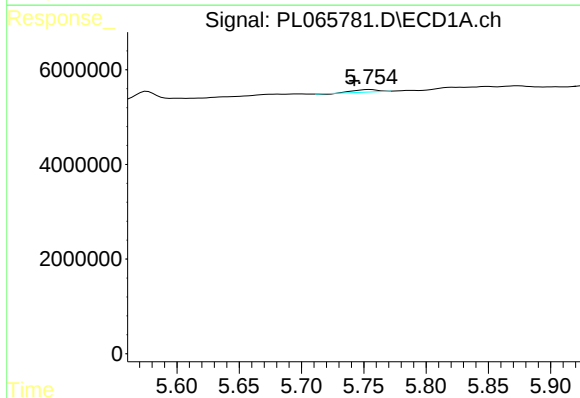


#14 Endrin

R.T.: 5.755 min
Delta R.T.: 0.013 min
Response: 667666
Conc: 0.25 ng/ml

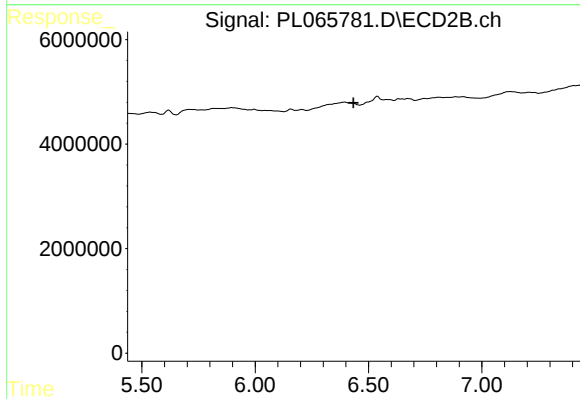

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

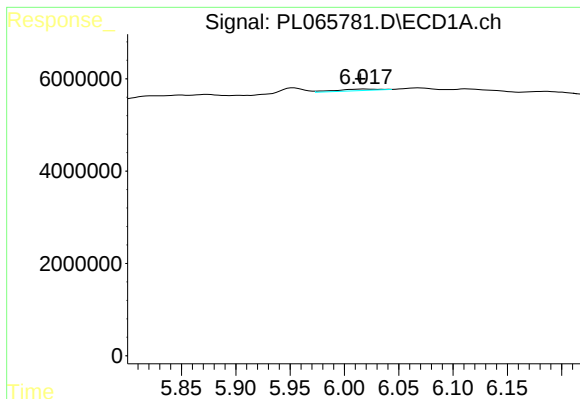

#15 Endosulfan II


R.T.: 6.019 min
Delta R.T.: 0.004 min
Response: 957679
Conc: 0.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB135458BL

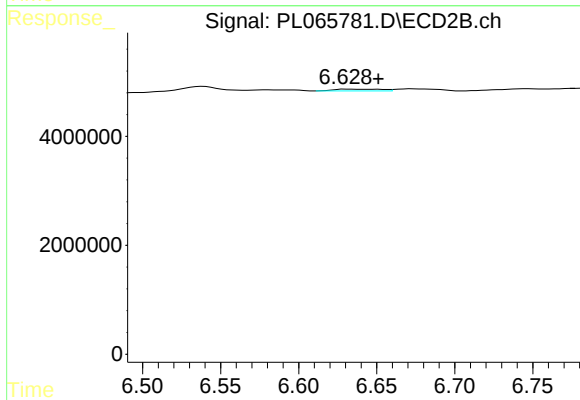


#15 Endosulfan II

R.T.: 6.630 min
Delta R.T.: -0.021 min
Response: 694128
Conc: 0.29 ng/ml

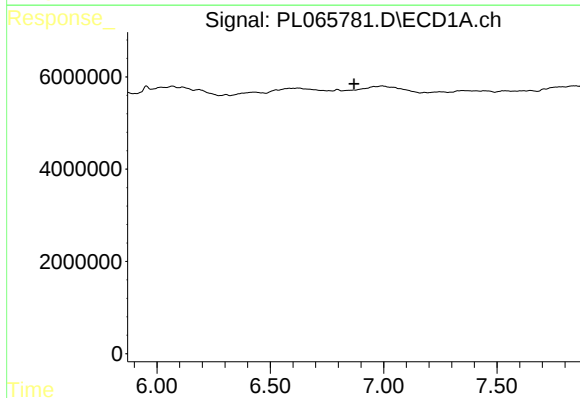


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 6.870 min
Response: 0
Conc: N.D.

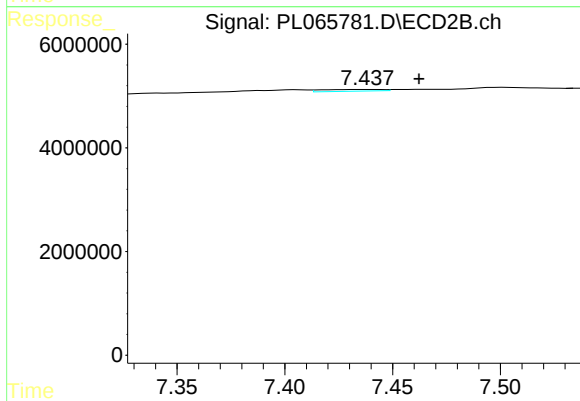

#21 Endrin ketone


R.T.: 7.440 min
Delta R.T.: -0.022 min
Response: 672488
Conc: 0.26 ng/ml

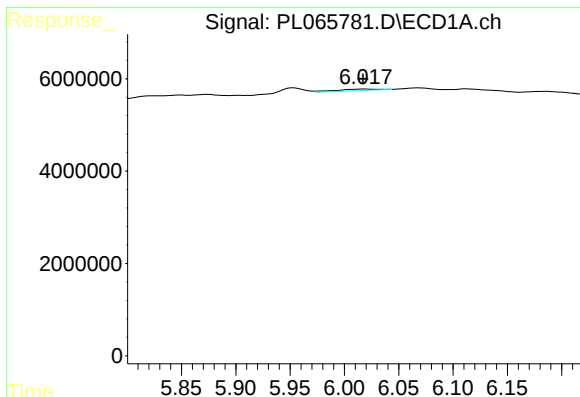

#27 Chlordane-5


R.T.: 6.019 min
Delta R.T.: 0.001 min
Response: 957679
Conc: 9.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB135458BL

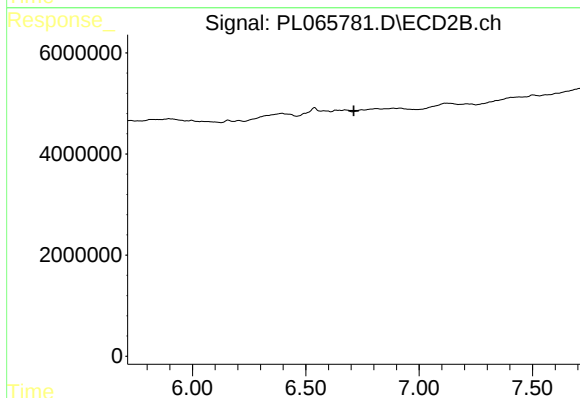


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.712 min
Response: 0
Conc: N.D.

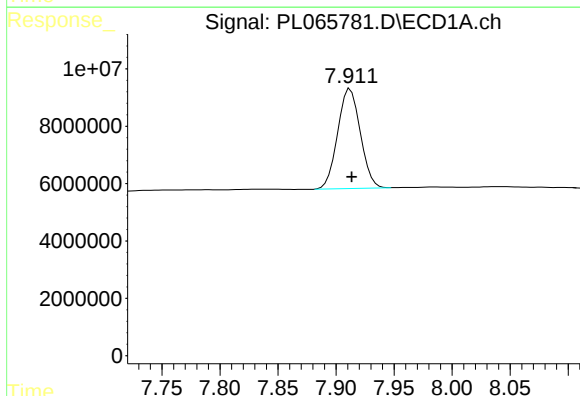

#28 Decachlorobiphenyl

R.T.: 7.912 min
Delta R.T.: -0.001 min
Response: 47314912
Conc: 20.43 ng/ml

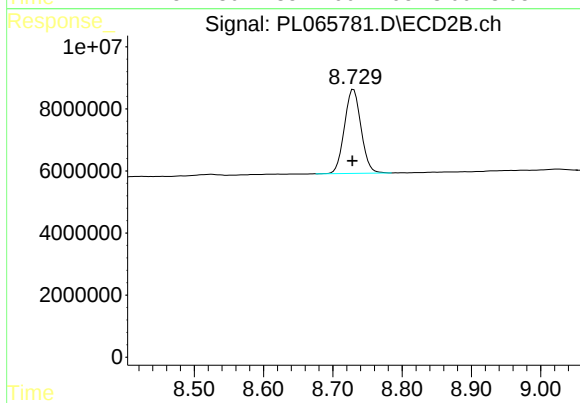

#28 Decachlorobiphenyl

R.T.: 8.730 min
Delta R.T.: 0.002 min
Response: 45065974
Conc: 19.99 ng/ml