

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040121\
 Data File : PL065809.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Apr 2021 22:35
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 02 02:21:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 31 15:57:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.278	3.780	59456588	61754706	22.824	22.497
28)	SA Decachlor...	7.910	8.727	53182480	50454311	22.963	22.379
Target Compounds							
4)	MA Heptachlor	4.233f	4.940	840879	863608	0.233	0.245
6)	B beta-BHC	4.233	4.631	840879	4024991	0.528	2.311 #
8)	B Heptachlo...	0.000	5.615	0	16452244	N.D.	5.298 #
13)	MA Dieldrin	0.000	6.227	0	225854	N.D.	0.080 #
14)	MA Endrin	5.754	0.000	1621646	0	0.601	N.D. #
15)	B Endosulfa...	6.003	0.000	358265	0	0.144	N.D. #
18)	B Endrin al...	6.182	0.000	870956	0	0.460	N.D. #
19)	B Endosulfa...	6.363f	0.000	323564	0	0.125	N.D. #
20)	A Methoxychlor	0.000	7.328	0	321328	N.D.	0.254 #
23)	Chlordane-1	4.142f	0.000	1029036	0	11.405	N.D. #
27)	Chlordane-5	6.003	6.687f	358265	2943626	3.503	35.305 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040121\
Data File : PL065809.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Apr 2021 22:35
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 02 02:21:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
Quant Title : GC Extractables
QLast Update : Wed Mar 31 15:57:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

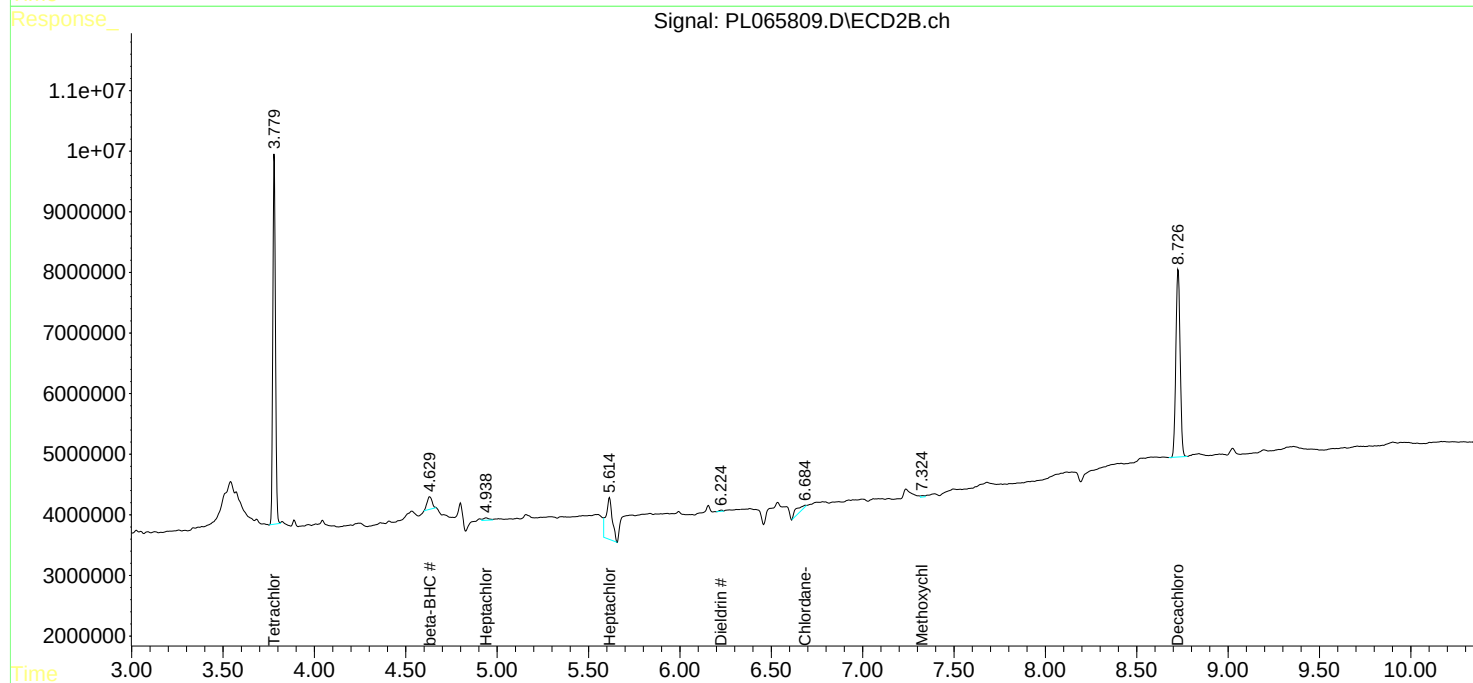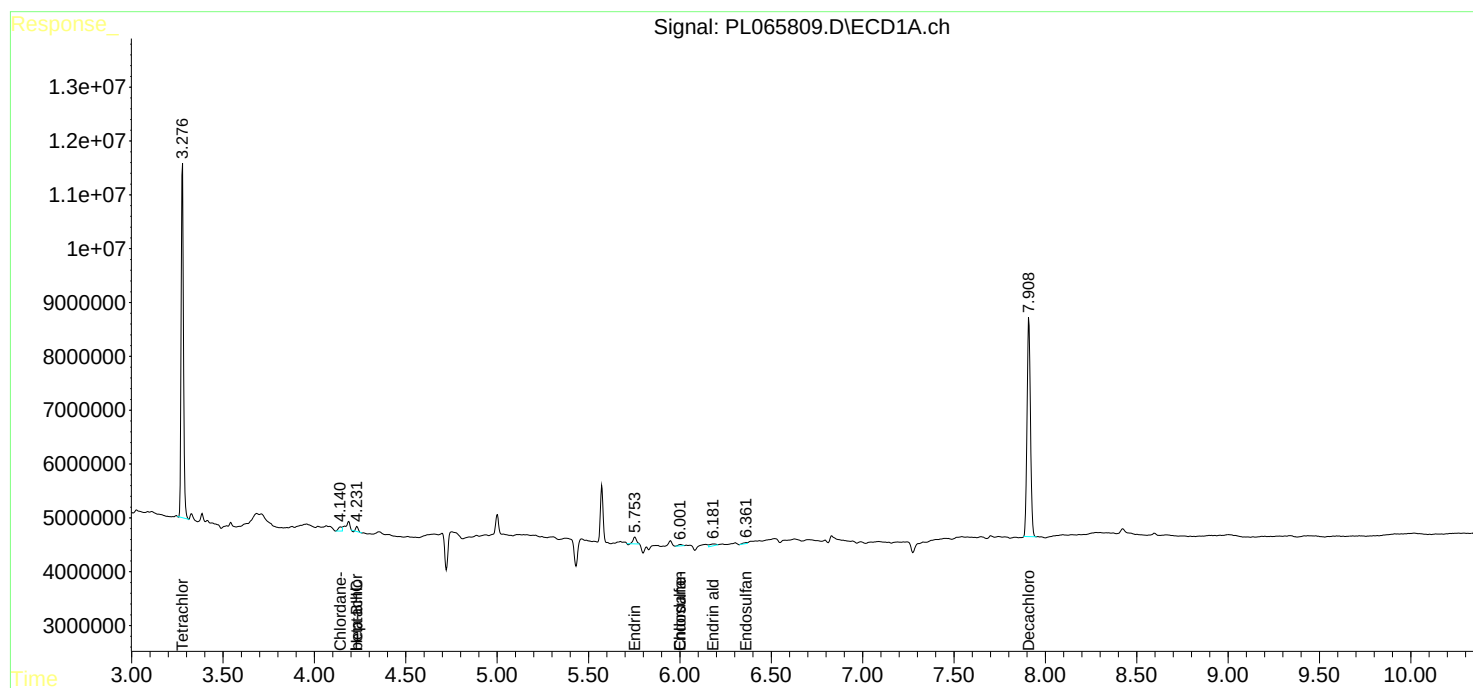


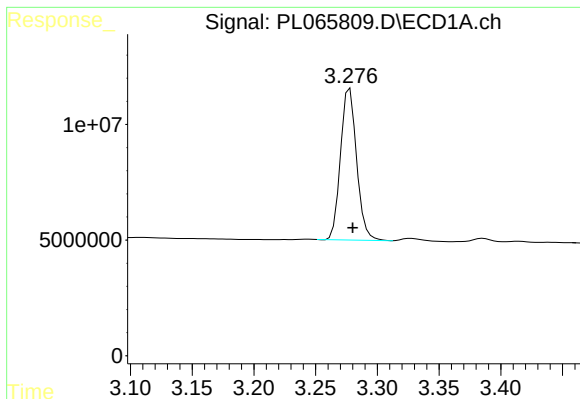

#1 Tetrachloro-m-xylene


R.T.: 3.278 min
Delta R.T.: -0.002 min
Response: 59456588
Conc: 22.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

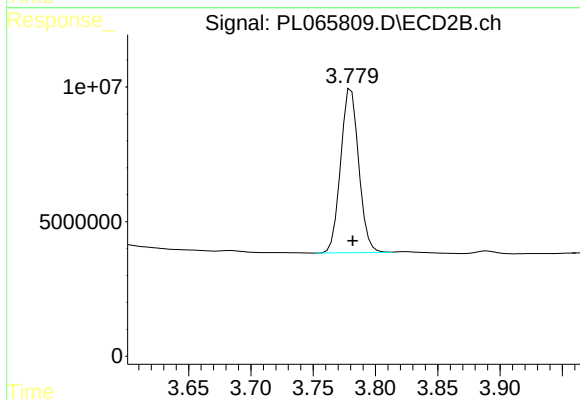


#1 Tetrachloro-m-xylene

R.T.: 3.780 min
Delta R.T.: -0.001 min
Response: 61754706
Conc: 22.50 ng/ml

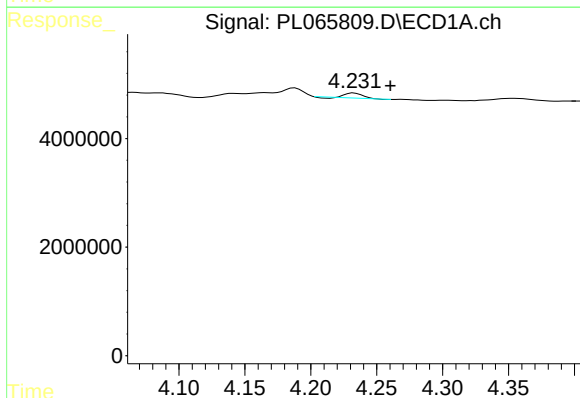


#4 Heptachlor

R.T.: 4.233 min
Delta R.T.: -0.027 min
Response: 840879
Conc: 0.23 ng/ml

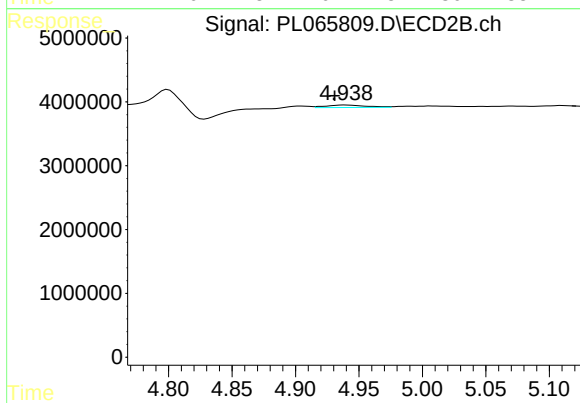

#4 Heptachlor


R.T.: 4.940 min
Delta R.T.: 0.009 min
Response: 863608
Conc: 0.24 ng/ml

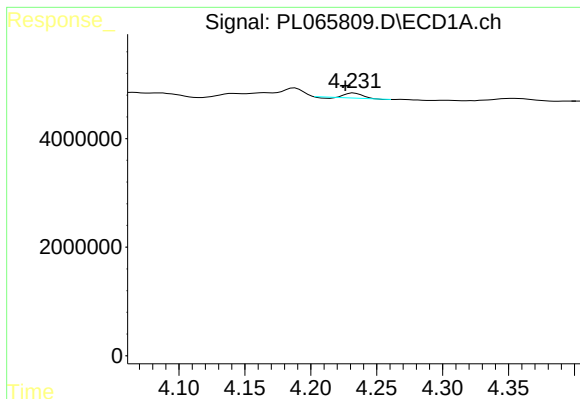

#6 beta-BHC


R.T.: 4.233 min
Delta R.T.: 0.007 min
Response: 840879
Conc: 0.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

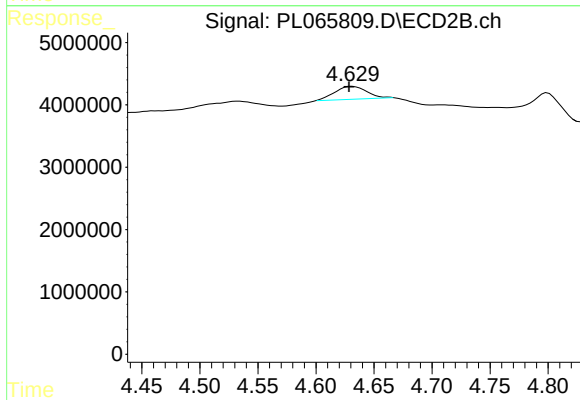


#6 beta-BHC

R.T.: 4.631 min
Delta R.T.: 0.002 min
Response: 4024991
Conc: 2.31 ng/ml

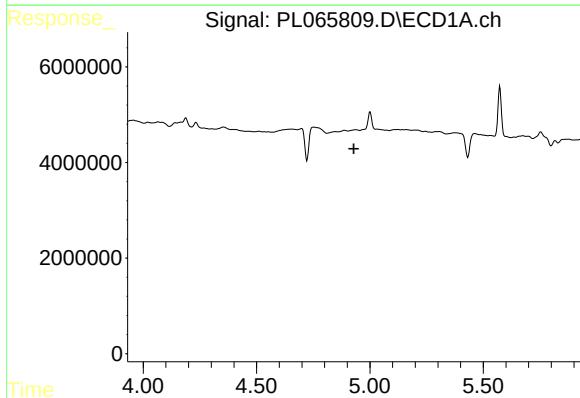


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.929 min
Response: 0
Conc: N.D.

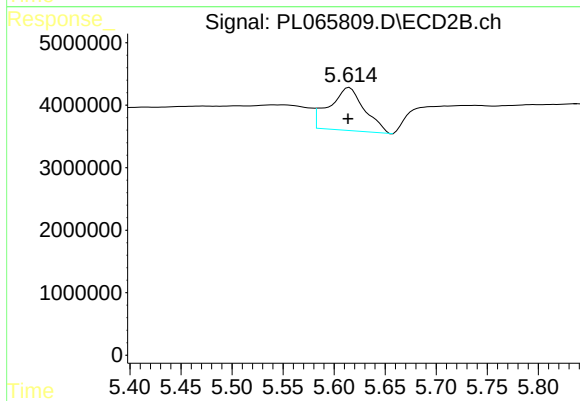

#8 Heptachlor epoxide


R.T.: 5.615 min
Delta R.T.: 0.001 min
Response: 16452244
Conc: 5.30 ng/ml

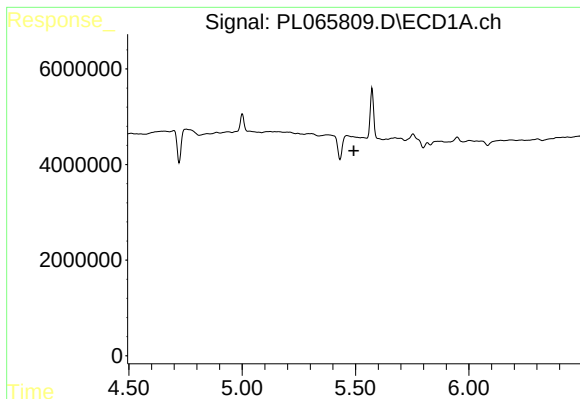

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 5.493 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

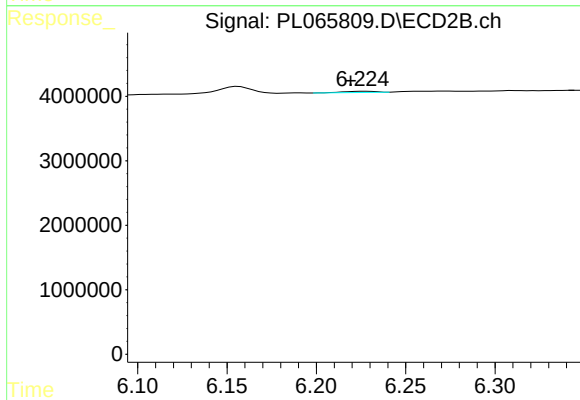


#13 Dieldrin

R.T.: 6.227 min
Delta R.T.: 0.008 min
Response: 225854
Conc: 0.08 ng/ml

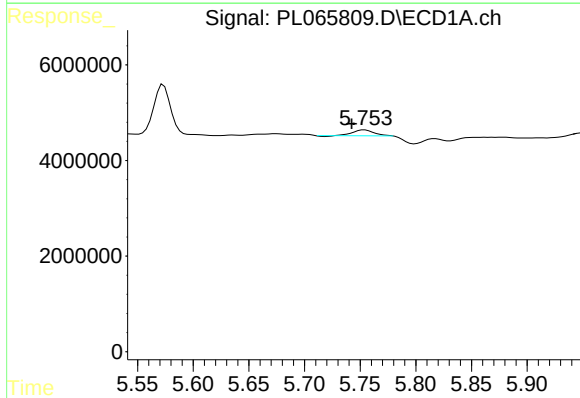


#14 Endrin

R.T.: 5.754 min
Delta R.T.: 0.012 min
Response: 1621646
Conc: 0.60 ng/ml

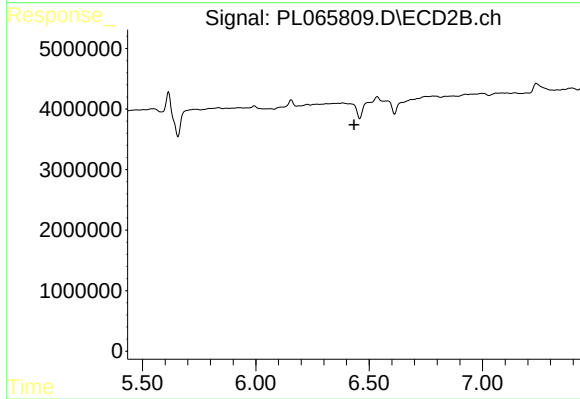

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

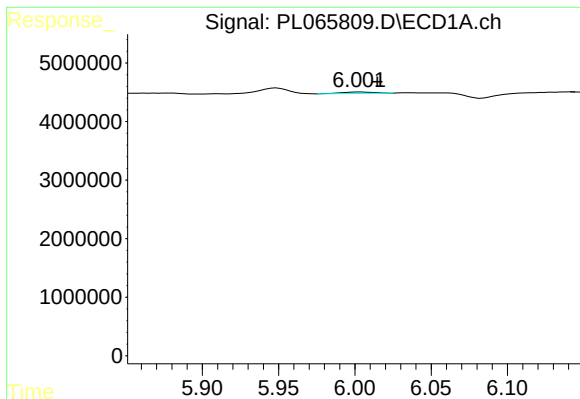

#15 Endosulfan II


R.T.: 6.003 min
Delta R.T.: -0.011 min
Response: 358265
Conc: 0.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

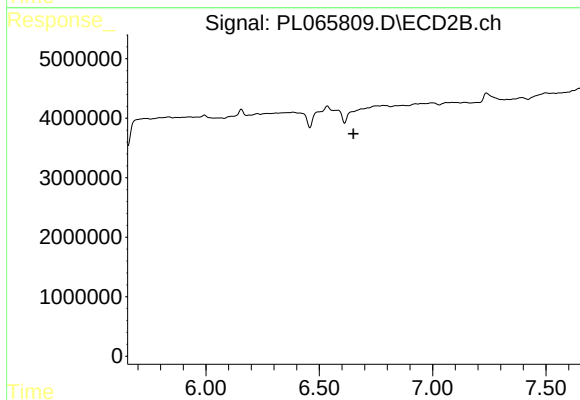


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.651 min
Response: 0
Conc: N.D.

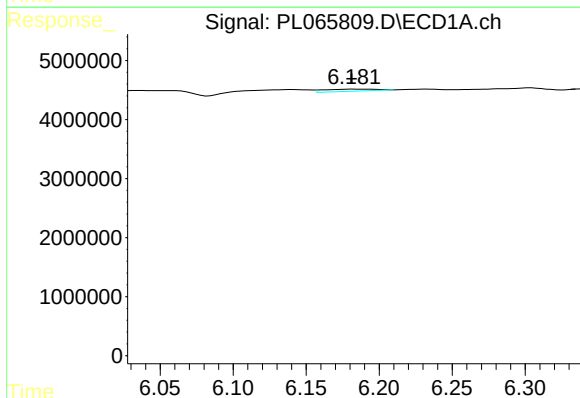


#18 Endrin aldehyde

R.T.: 6.182 min
Delta R.T.: 0.000 min
Response: 870956
Conc: 0.46 ng/ml

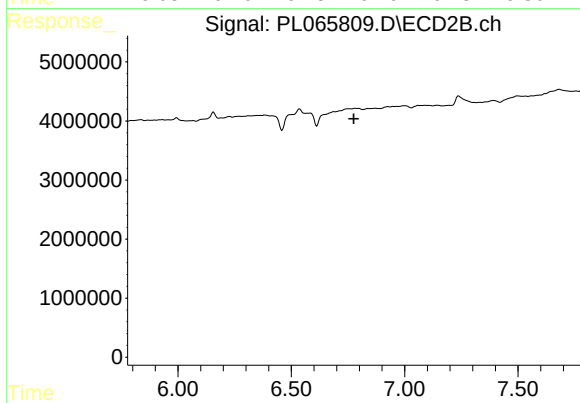

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 6.775 min
Response: 0
Conc: N.D.

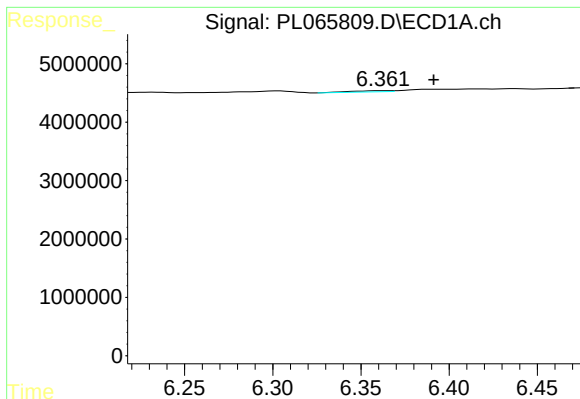

#19 Endosulfan Sulfate


R.T.: 6.363 min
Delta R.T.: -0.028 min
Response: 323564
Conc: 0.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

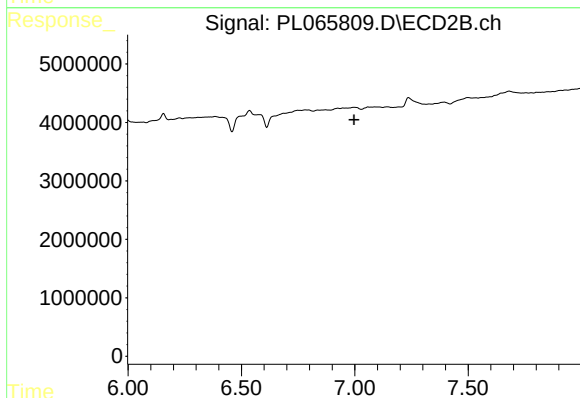


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 6.997 min
Response: 0
Conc: N.D.

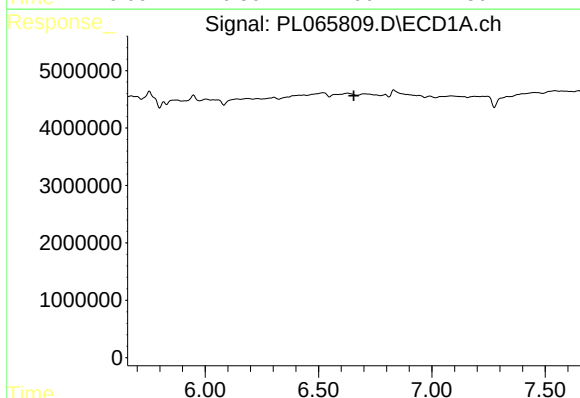


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.656 min
Response: 0
Conc: N.D.

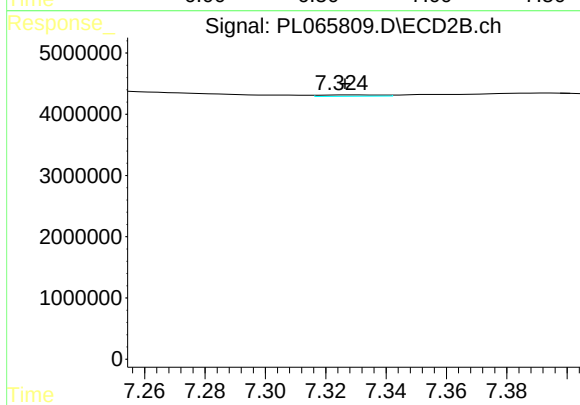

#20 Methoxychlor


R.T.: 7.328 min
Delta R.T.: 0.001 min
Response: 321328
Conc: 0.25 ng/ml

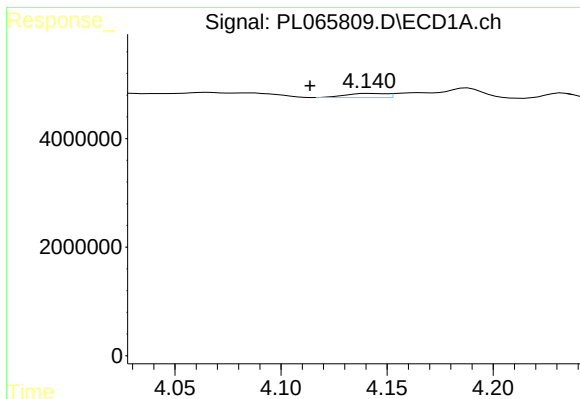

#23 Chlordane-1


R.T.: 4.142 min
Delta R.T.: 0.028 min
Response: 1029036
Conc: 11.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

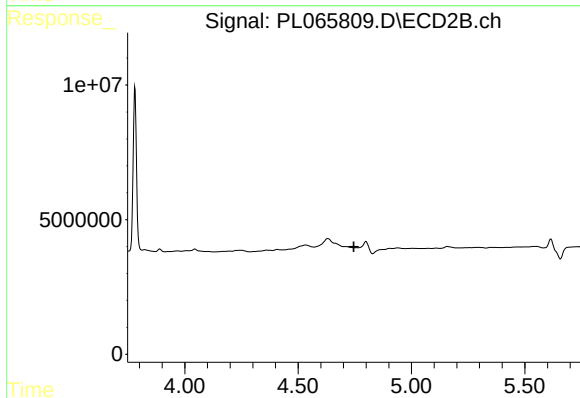


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.745 min
Response: 0
Conc: N.D.

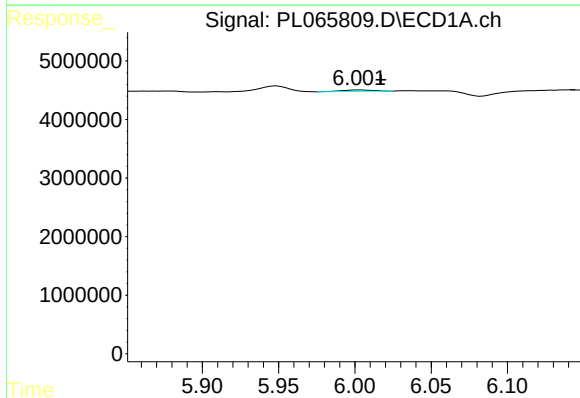


#27 Chlordane-5

R.T.: 6.003 min
Delta R.T.: -0.014 min
Response: 358265
Conc: 3.50 ng/ml

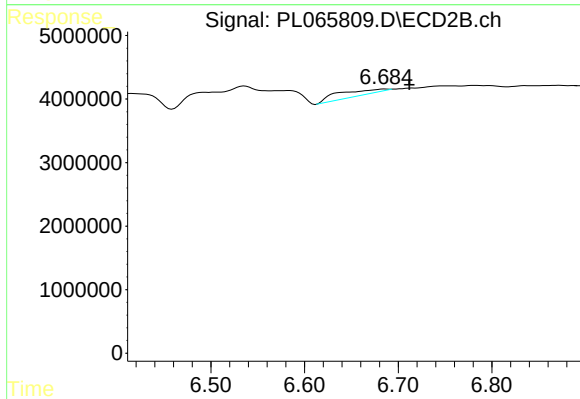

#27 Chlordane-5


R.T.: 6.687 min
Delta R.T.: -0.025 min
Response: 2943626
Conc: 35.31 ng/ml

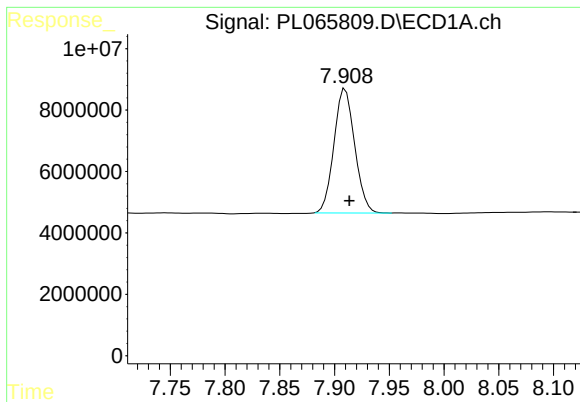

#28 Decachlorobiphenyl

R.T.: 7.910 min
Delta R.T.: -0.004 min
Response: 53182480
Conc: 22.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

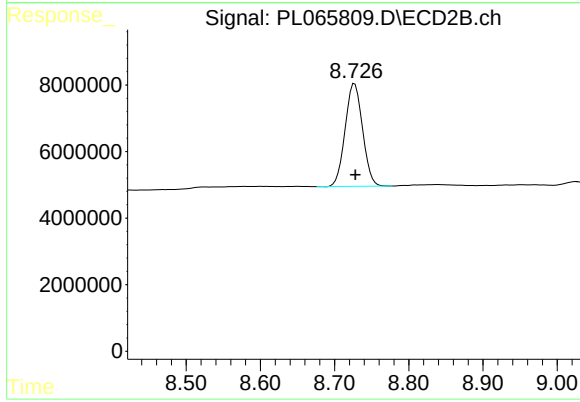

#28 Decachlorobiphenyl

R.T.: 8.727 min
Delta R.T.: -0.001 min
Response: 50454311
Conc: 22.38 ng/ml