

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040121\
 Data File : PL065769.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Apr 2021 12:19
 Operator : AR\AJ
 Sample : M1817-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PHC-326FB-002

Manual Integrations
 APPROVED

Ankita
 4/2/2021 11:30:52 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 02 02:08:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 31 15:57:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.279	3.781	37033526	40258335	14.216	14.666
28)	SA Decachlor...	7.914	8.730	33594565	32176155	14.505	14.272
Target Compounds							
12)	B 4,4'-DDE	5.371	6.074	2586235	3650906	0.937m	1.397 #
17)	MA 4,4'-DDT	6.109	6.859	1960436	1093021	0.931m	0.488m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040121\
Data File : PL065769.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Apr 2021 12:19
Operator : AR\AJ
Sample : M1817-01
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PHC-326FB-002


Manual Integrations
APPROVED

Ankita
4/2/2021 11:30:52 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 02 02:08:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
Quant Title : GC Extractables
QLast Update : Wed Mar 31 15:57:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

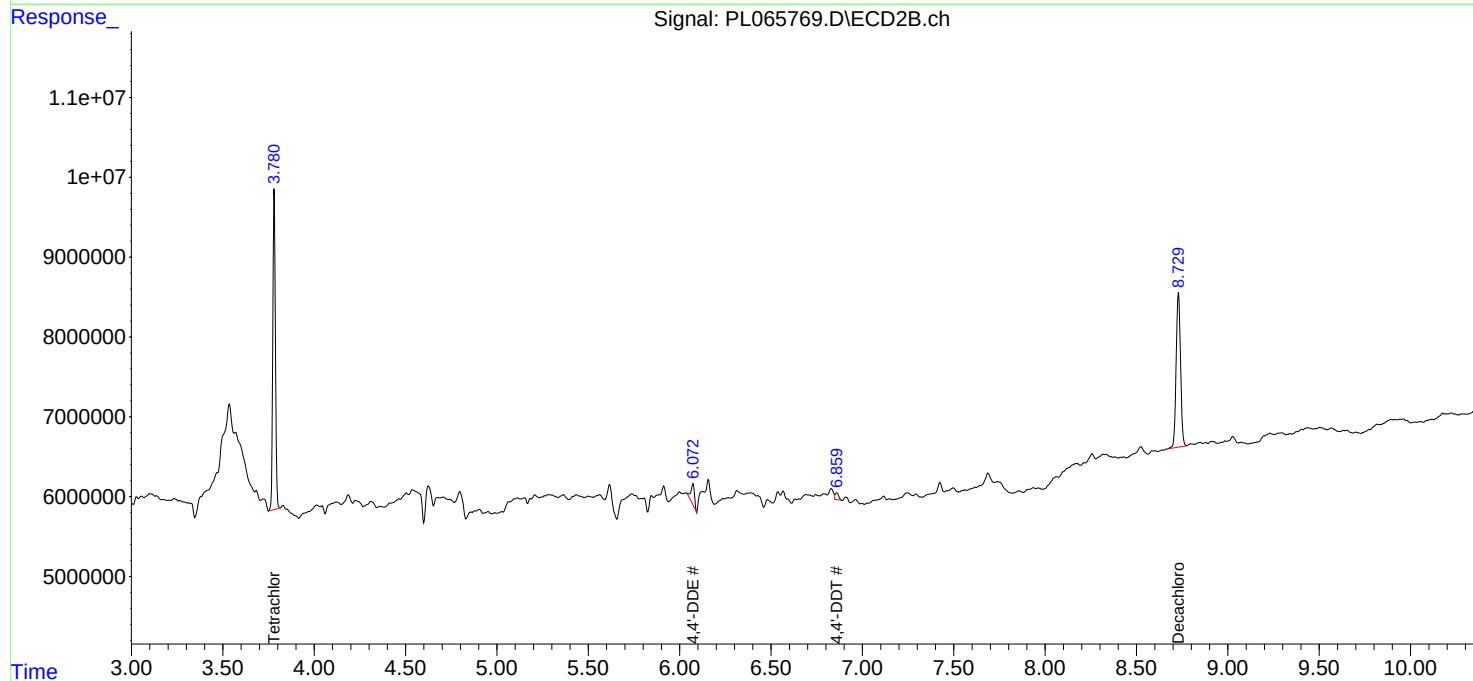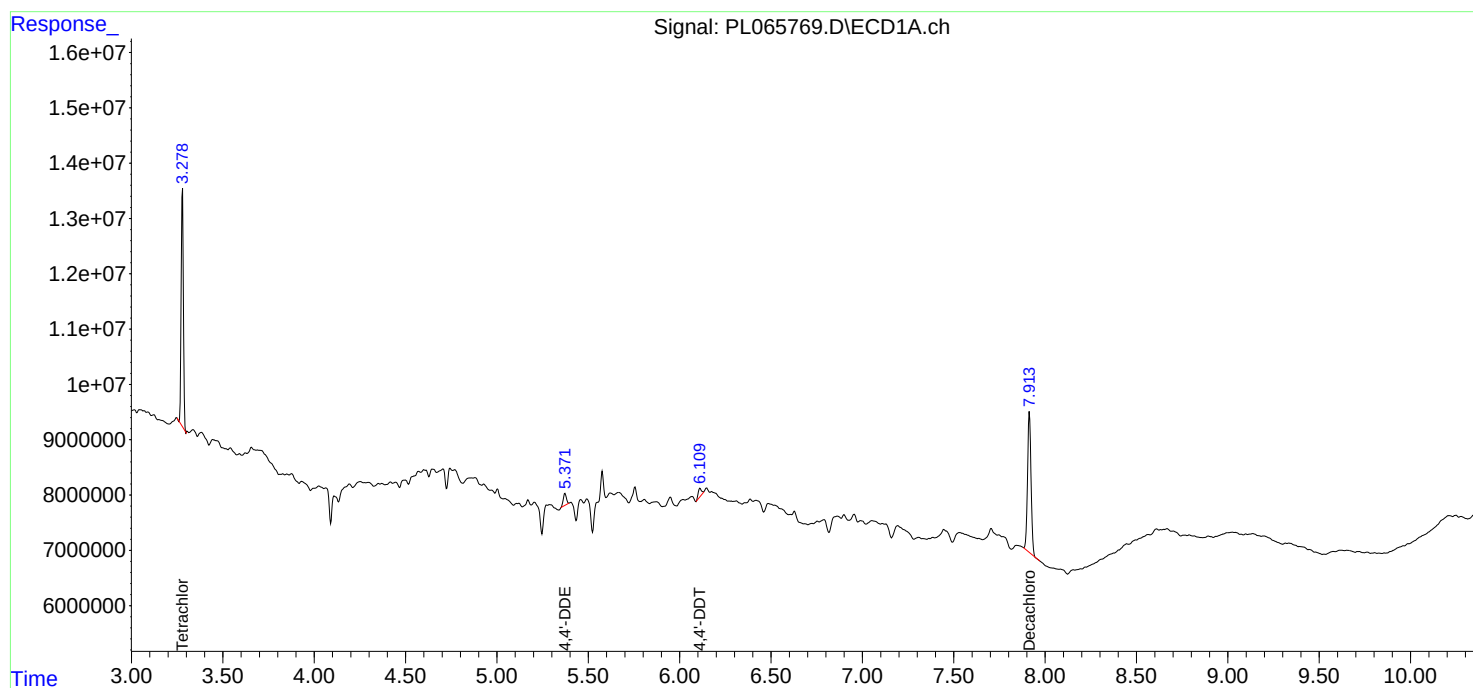

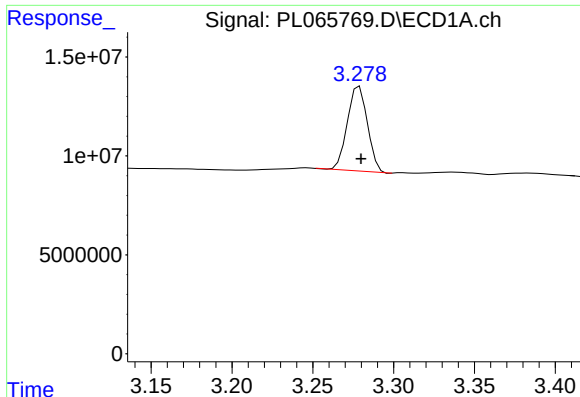


#1 Tetrachloro-m-xylene

R.T.: 3.279 min
Delta R.T.: -0.001 min
Response: 37033526
Conc: 14.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
PHC-326FB-002


Manual Integrations
APPROVED

Ankita
4/2/2021 11:30:52 AM

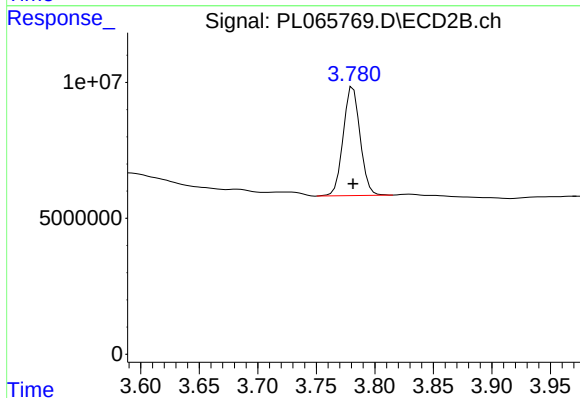


#1 Tetrachloro-m-xylene

R.T.: 3.781 min
Delta R.T.: 0.000 min
Response: 40258335
Conc: 14.67 ng/ml

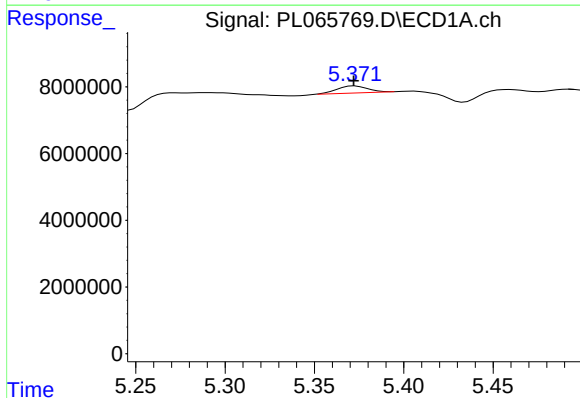


#12 4,4'-DDE

R.T.: 5.371 min
Delta R.T.: 0.000 min
Response: 2586235
Conc: 0.94 ng/ml m

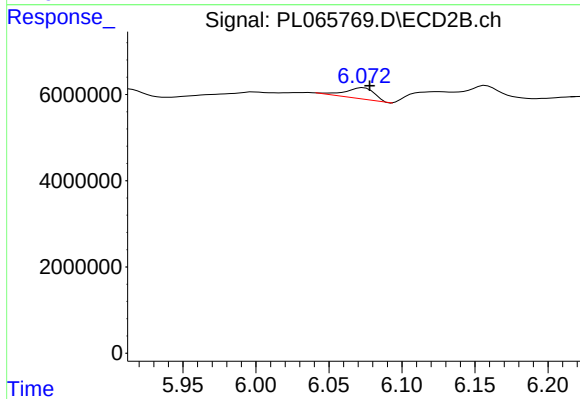

#12 4,4'-DDE

R.T.: 6.074 min
Delta R.T.: -0.004 min
Response: 3650906
Conc: 1.40 ng/ml

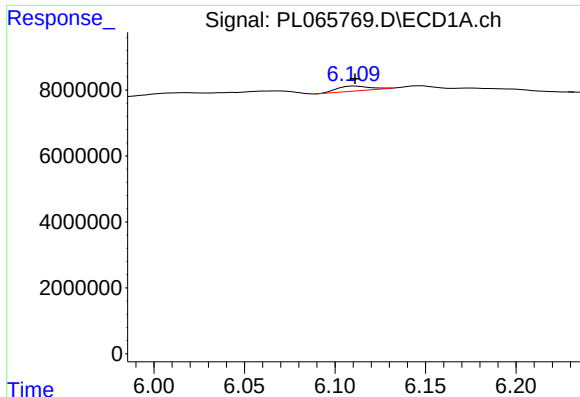


#17 4,4'-DDT

R.T.: 6.109 min
Delta R.T.: -0.002 min
Response: 1960436
Conc: 0.93 ng/ml m

Instrument :
ECD_L
ClientSampleId :
PHC-326FB-002


Manual Integrations
APPROVED

Ankita
4/2/2021 11:30:52 AM

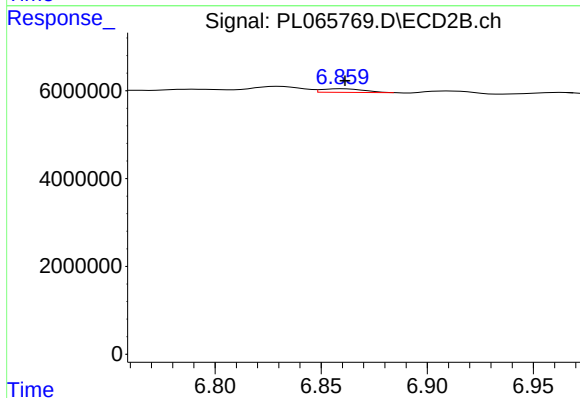


#17 4,4'-DDT

R.T.: 6.859 min
Delta R.T.: -0.003 min
Response: 1093021
Conc: 0.49 ng/ml m

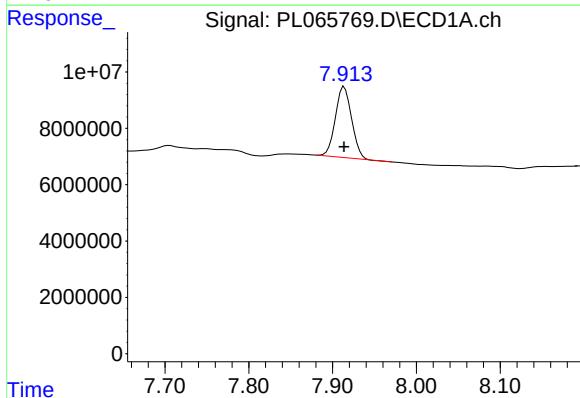

#28 Decachlorobiphenyl

R.T.: 7.914 min
Delta R.T.: 0.000 min
Response: 33594565
Conc: 14.51 ng/ml

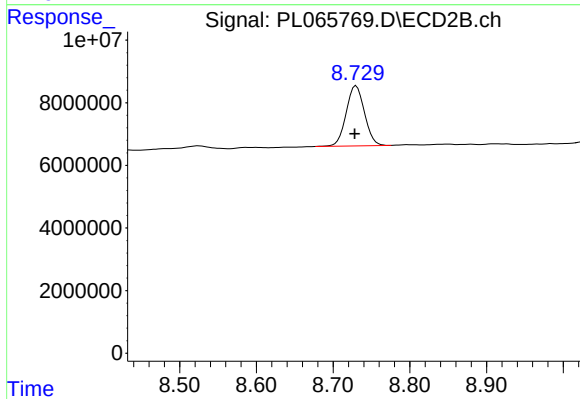

#28 Decachlorobiphenyl

R.T.: 8.730 min
Delta R.T.: 0.002 min
Response: 32176155
Conc: 14.27 ng/ml