

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040121\
 Data File : PL065783.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Apr 2021 16:23
 Operator : AR\AJ
 Sample : M1836-09
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 B4-8-10

Manual Integrations
 APPROVED

Ankita
 4/2/2021 11:31:25 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 02 02:12:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 31 15:57:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.277	3.780	30959204	34460455	11.884m	12.554
28)	SA Decachlor...	7.913	8.729	35645308	34793005	15.391	15.433

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040121\
Data File : PL065783.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Apr 2021 16:23
Operator : AR\AJ
Sample : M1836-09
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
B4-8-10


Manual Integrations
APPROVED

Ankita
4/2/2021 11:31:25 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 02 02:12:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
Quant Title : GC Extractables
QLast Update : Wed Mar 31 15:57:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

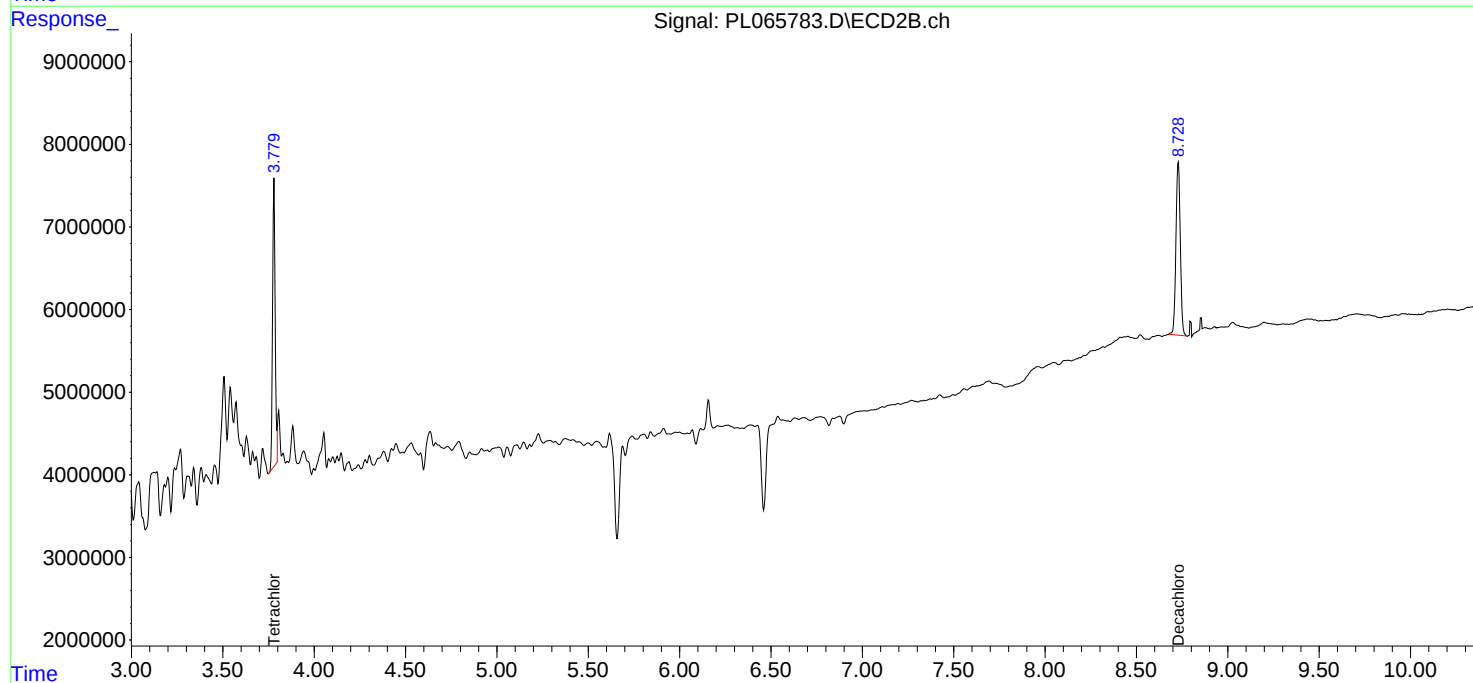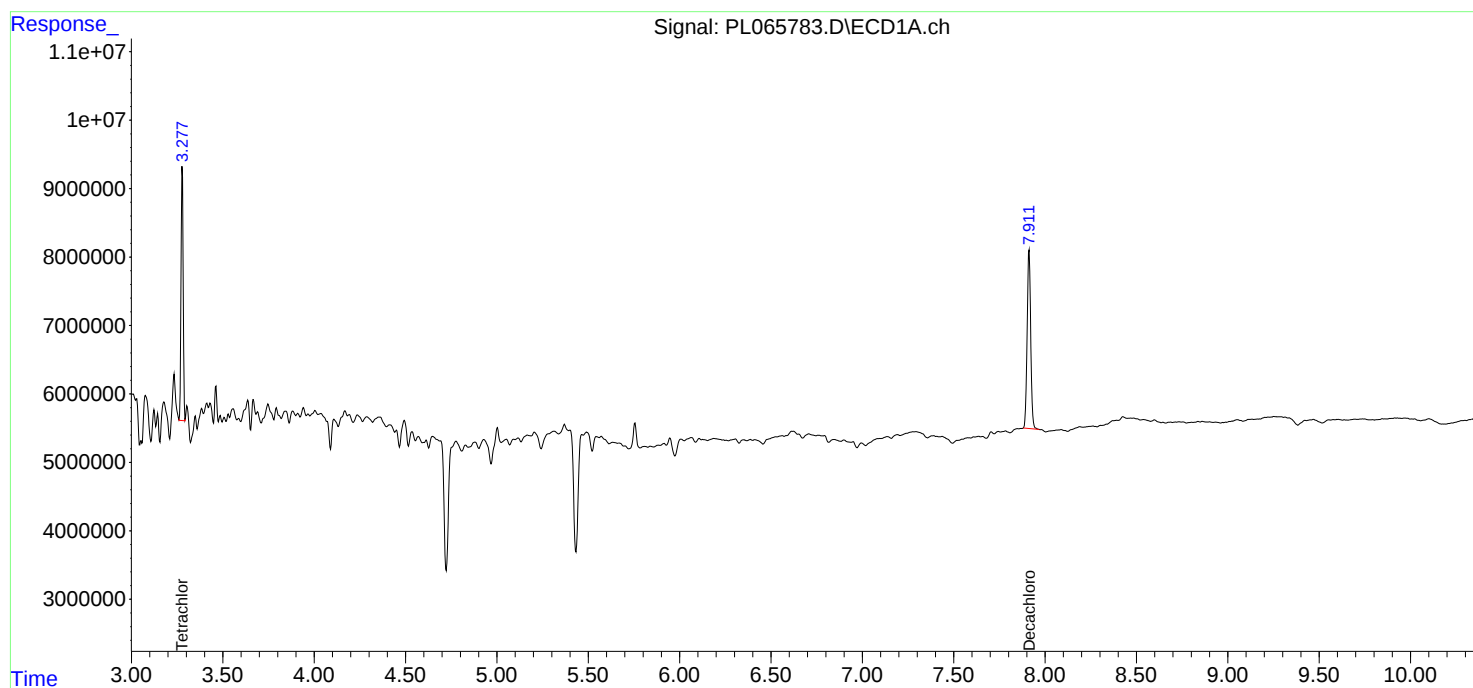

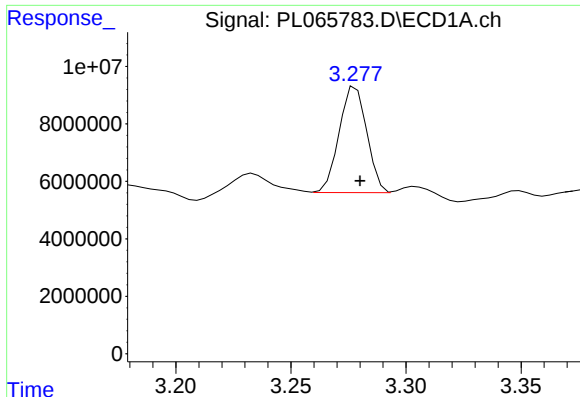


#1 Tetrachloro-m-xylene

R.T.: 3.277 min
Delta R.T.: -0.003 min
Response: 30959204
Conc: 11.88 ng/ml m

Instrument :
ECD_L
ClientSampleId :
B4-8-10


Manual Integrations
APPROVED

Ankita
4/2/2021 11:31:25 AM

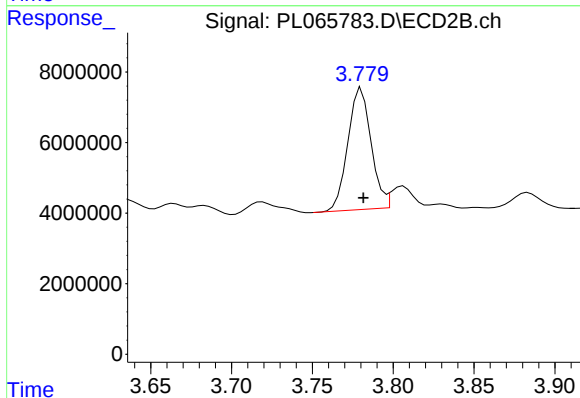


#1 Tetrachloro-m-xylene

R.T.: 3.780 min
Delta R.T.: -0.001 min
Response: 34460455
Conc: 12.55 ng/ml

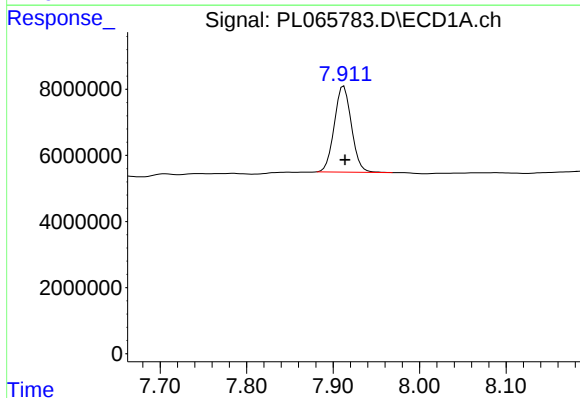

#28 Decachlorobiphenyl

R.T.: 7.913 min
Delta R.T.: -0.001 min
Response: 35645308
Conc: 15.39 ng/ml

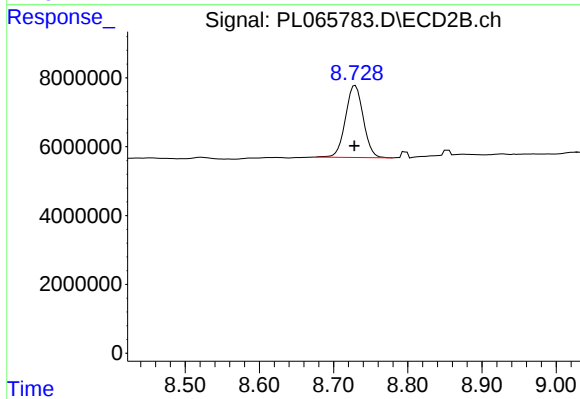

#28 Decachlorobiphenyl

R.T.: 8.729 min
Delta R.T.: 0.001 min
Response: 34793005
Conc: 15.43 ng/ml