

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040122\
 Data File : PL073778.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Apr 2022 16:19
 Operator : AR\AJ
 Sample : N2191-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BI-WEEKLY-DECANT

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 04/04/2022
 Supervised By :mohammad ahmed 04/04/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 23:40:09 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 04:12:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.639	5.490	4045720	31702210	12.632m	19.316 #
28) SA Decachlor...	10.413	11.335	6888456	13499549	13.547	7.549m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040122\
Data File : PL073778.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Apr 2022 16:19
Operator : AR\AJ
Sample : N2191-01
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
BI-WEEKLY-DECANT


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 04/04/2022
Supervised By : mohammad ahmed 04/04/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 23:40:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 04:12:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

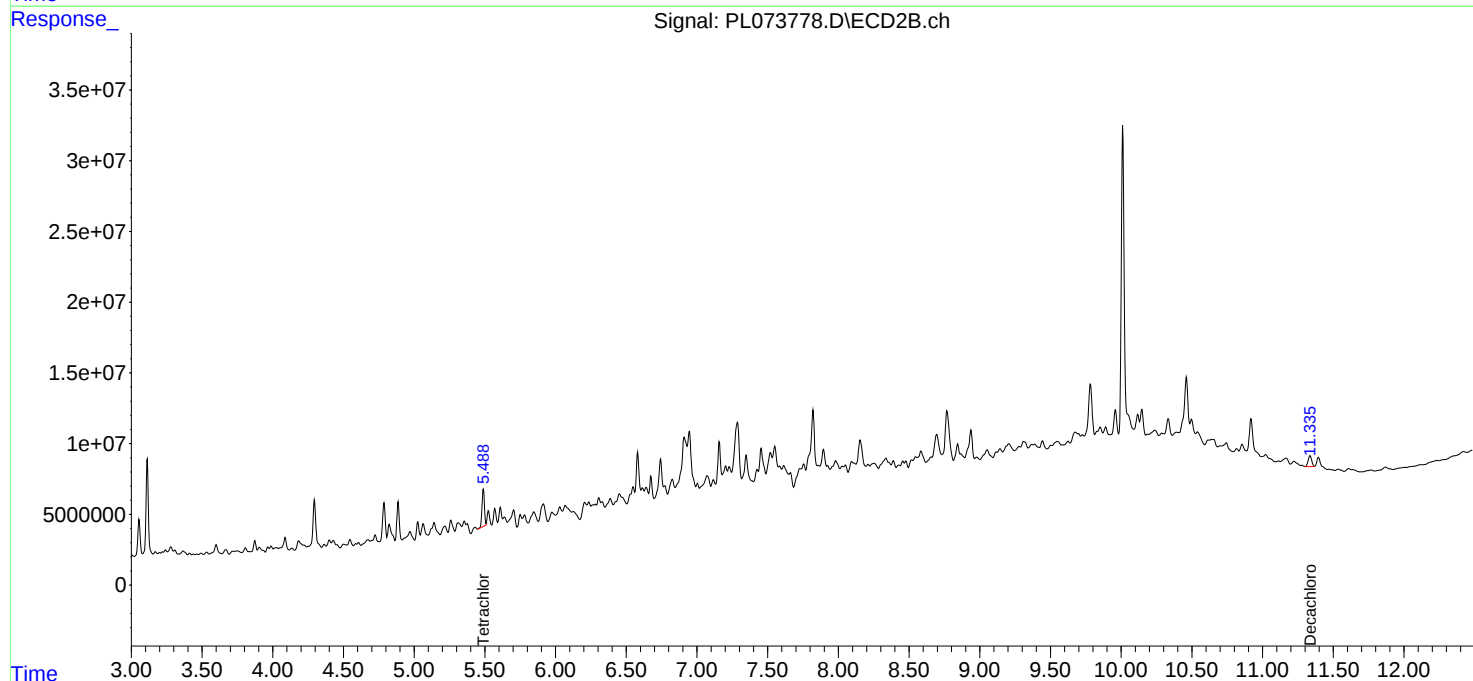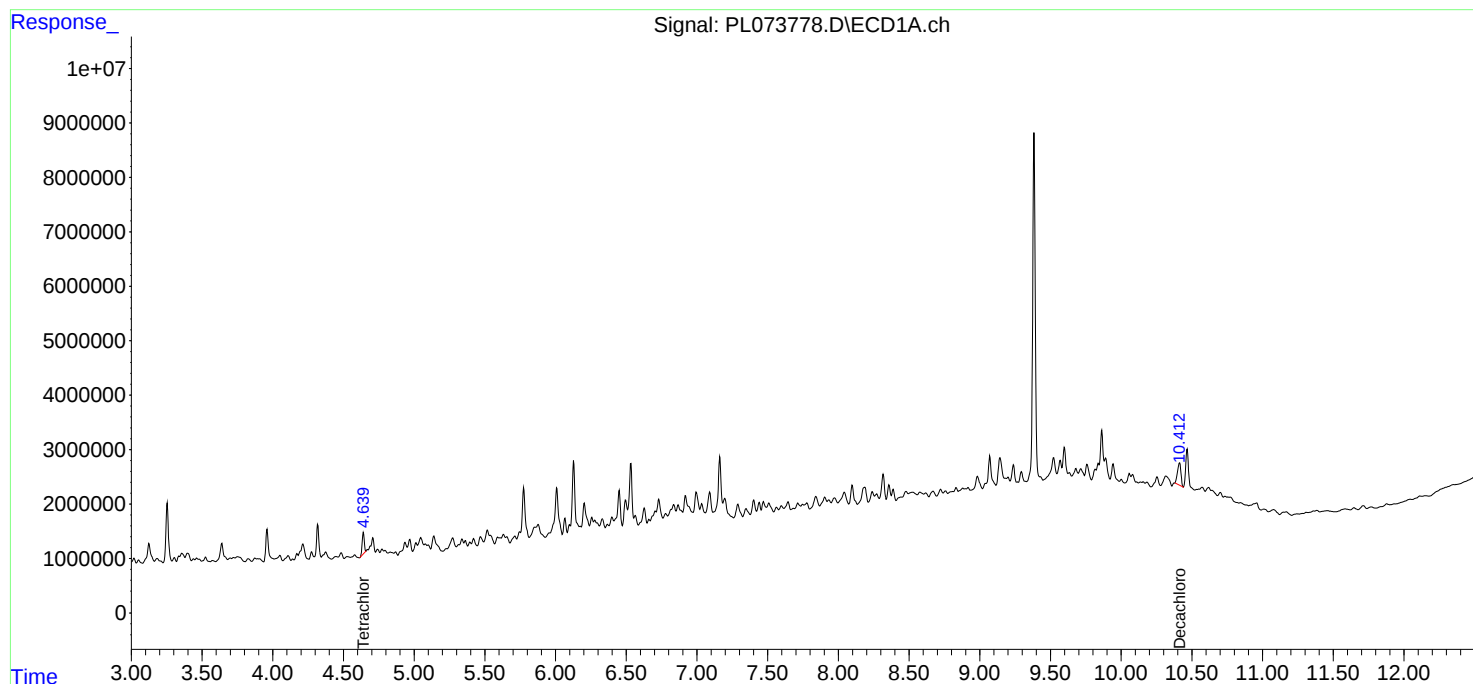

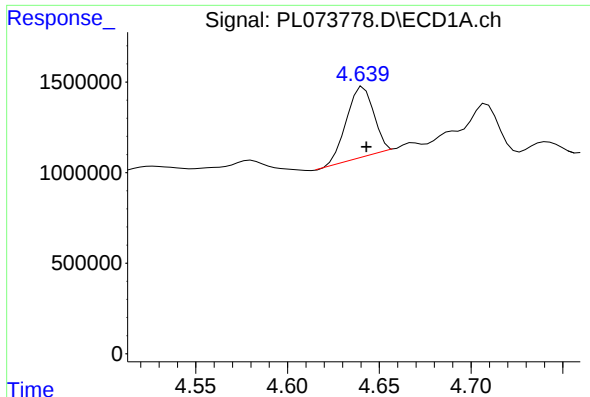


#1 Tetrachloro-m-xylene

R.T.: 4.639 min
Delta R.T.: -0.004 min
Response: 4045720
Conc: 12.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
BI-WEEKLY-DECANT


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 04/04/2022
Supervised By :mohammad ahmed 04/04/2022

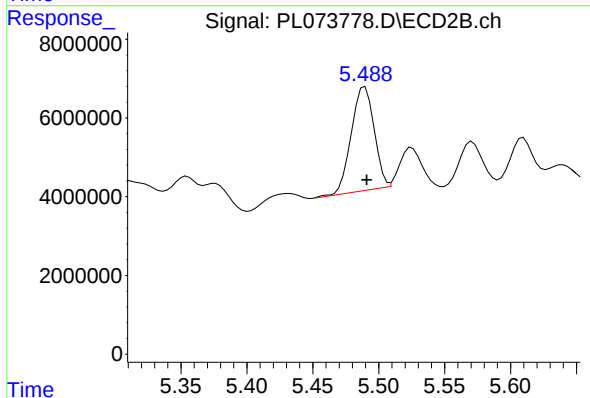


#1 Tetrachloro-m-xylene

R.T.: 5.490 min
Delta R.T.: -0.001 min
Response: 31702210
Conc: 19.32 ng/ml

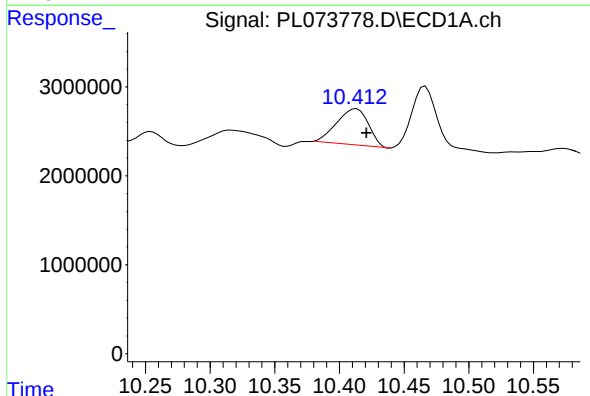

#28 Decachlorobiphenyl

R.T.: 10.413 min
Delta R.T.: -0.008 min
Response: 6888456
Conc: 13.55 ng/ml

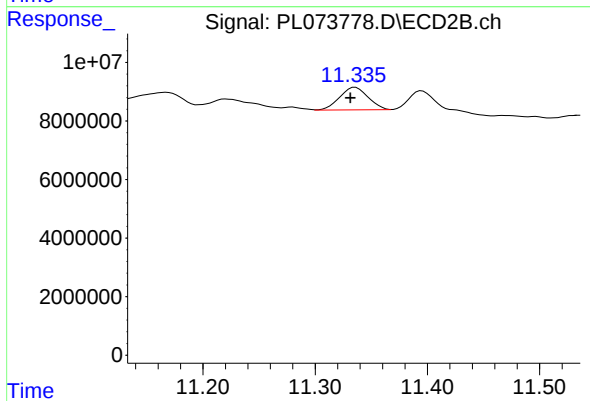

#28 Decachlorobiphenyl

R.T.: 11.335 min
Delta R.T.: 0.003 min
Response: 13499549
Conc: 7.55 ng/ml m