

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040122\
 Data File : PL073779.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Apr 2022 16:52
 Operator : AR\AJ
 Sample : PB143798BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB143798BL

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 04/04/2022
 Supervised By : mohammad ahmed 04/04/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 23:40:46 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 04:12:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.650	5.488	5537107	32263135	17.288m	19.658
28) SA Decachlor...	10.423	11.337	9364288	30980714	18.416	17.325

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040122\
Data File : PL073779.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Apr 2022 16:52
Operator : AR\AJ
Sample : PB143798BL
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PB143798BL


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 04/04/2022
Supervised By : mohammad ahmed 04/04/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 23:40:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 04:12:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

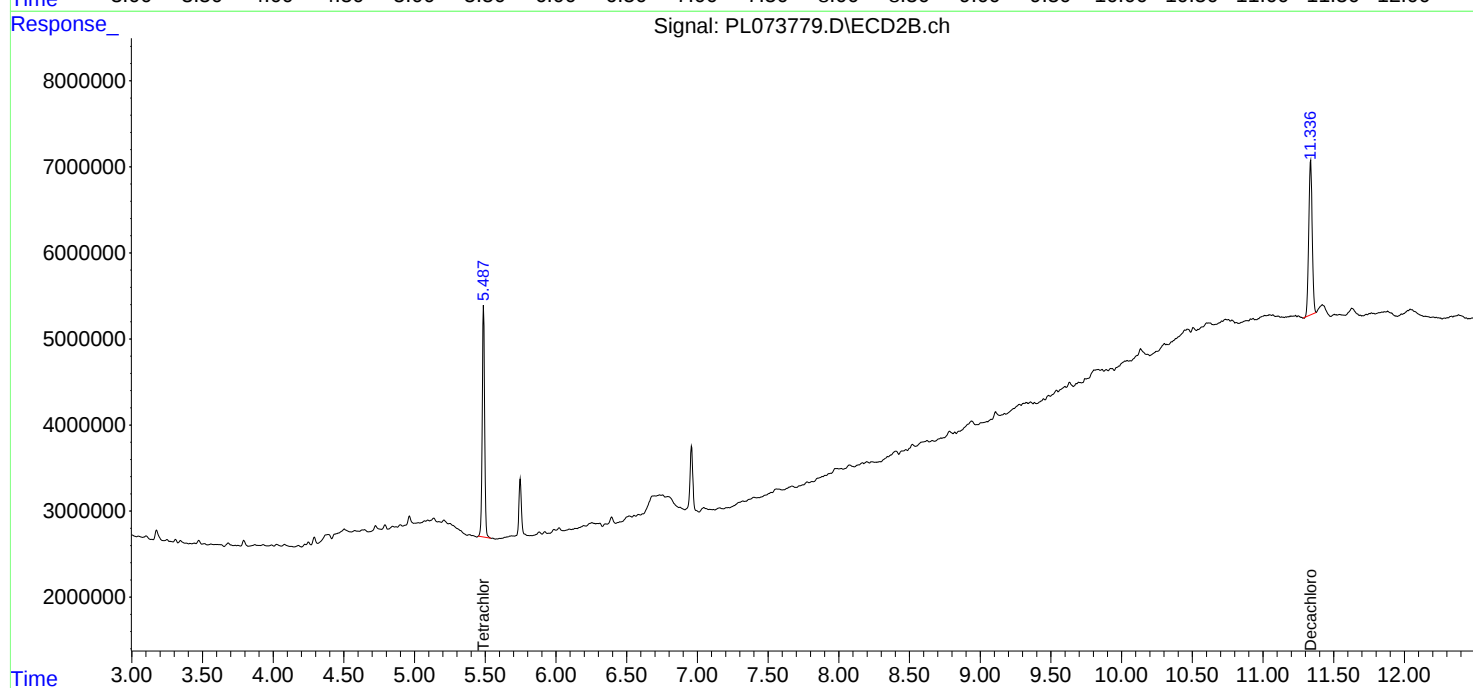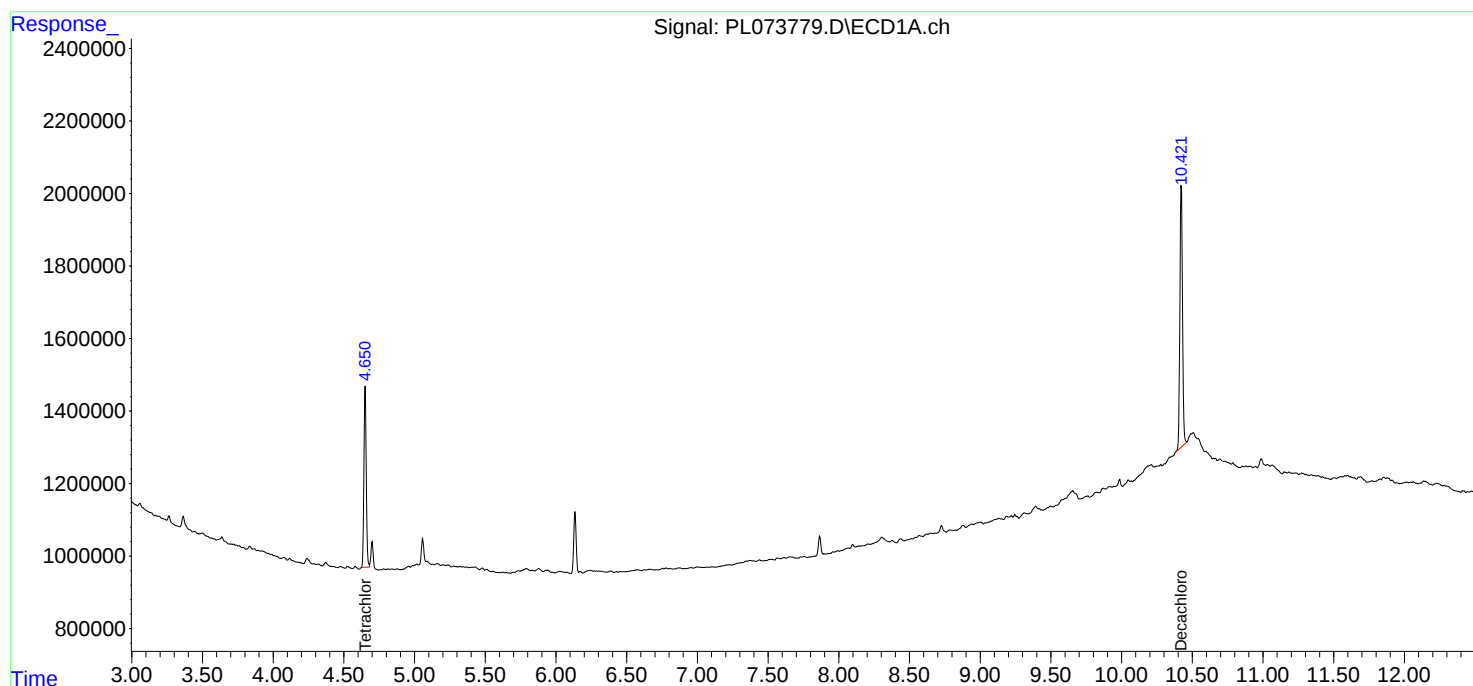

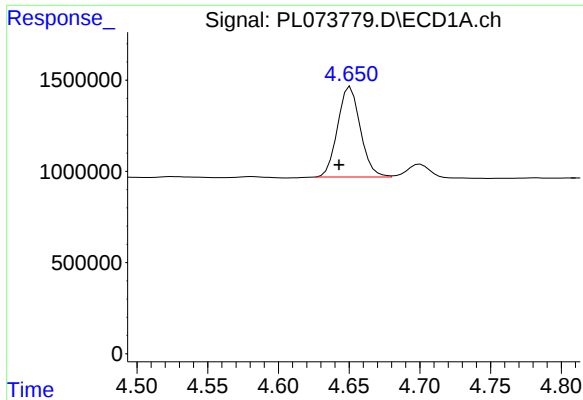


#1 Tetrachloro-m-xylene

R.T.: 4.650 min
Delta R.T.: 0.007 min
Response: 5537107
Conc: 17.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB143798BL


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 04/04/2022
Supervised By :mohammad ahmed 04/04/2022

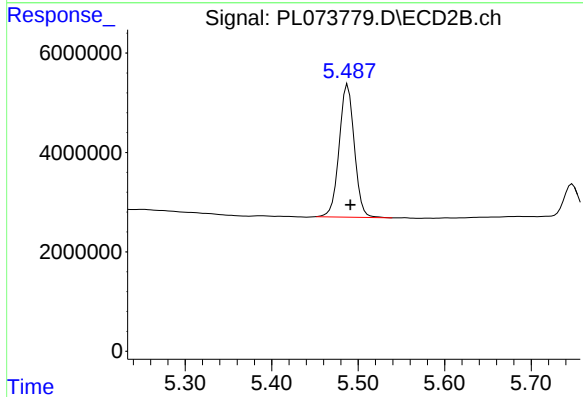


#1 Tetrachloro-m-xylene

R.T.: 5.488 min
Delta R.T.: -0.003 min
Response: 32263135
Conc: 19.66 ng/ml

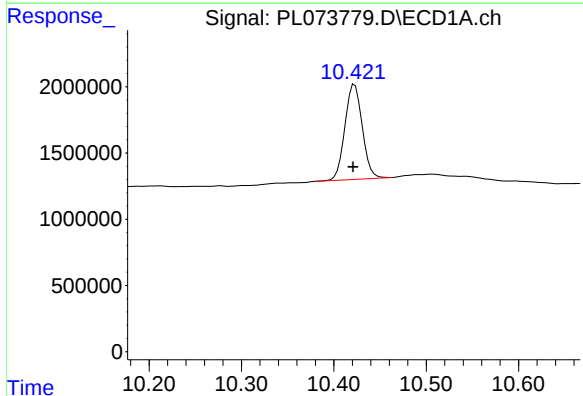

#28 Decachlorobiphenyl

R.T.: 10.423 min
Delta R.T.: 0.002 min
Response: 9364288
Conc: 18.42 ng/ml

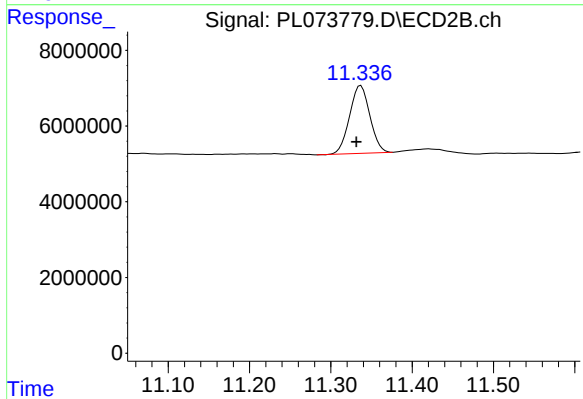

#28 Decachlorobiphenyl

R.T.: 11.337 min
Delta R.T.: 0.006 min
Response: 30980714
Conc: 17.33 ng/ml