

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040124\
 Data File : PL088849.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Apr 2024 15:15
 Operator : AR\AJ
 Sample : P1936-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TR-04-032924

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 02 01:14:28 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031324.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 13 15:45:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.633	2.851	26945277	15145171	10.168	11.364
28) SA Decachlor...	9.298	8.077	24484424	17968026	9.905	13.252 #
Target Compounds						
4) MA Heptachlor	5.035	4.048	26052174	12400676	6.860m	6.890m
10) B gamma-Chl...	6.075	5.105	127.0E6	27858513	38.117m	16.820m#
11) B alpha-Chl...	6.158	5.164	456.0E6	105.7E6	137.192	63.651 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040124\
Data File : PL088849.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Apr 2024 15:15
Operator : AR\AJ
Sample : P1936-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TR-04-032924

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 02 01:14:28 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031324.M
Quant Title : GC Extractables
QLast Update : Wed Mar 13 15:45:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

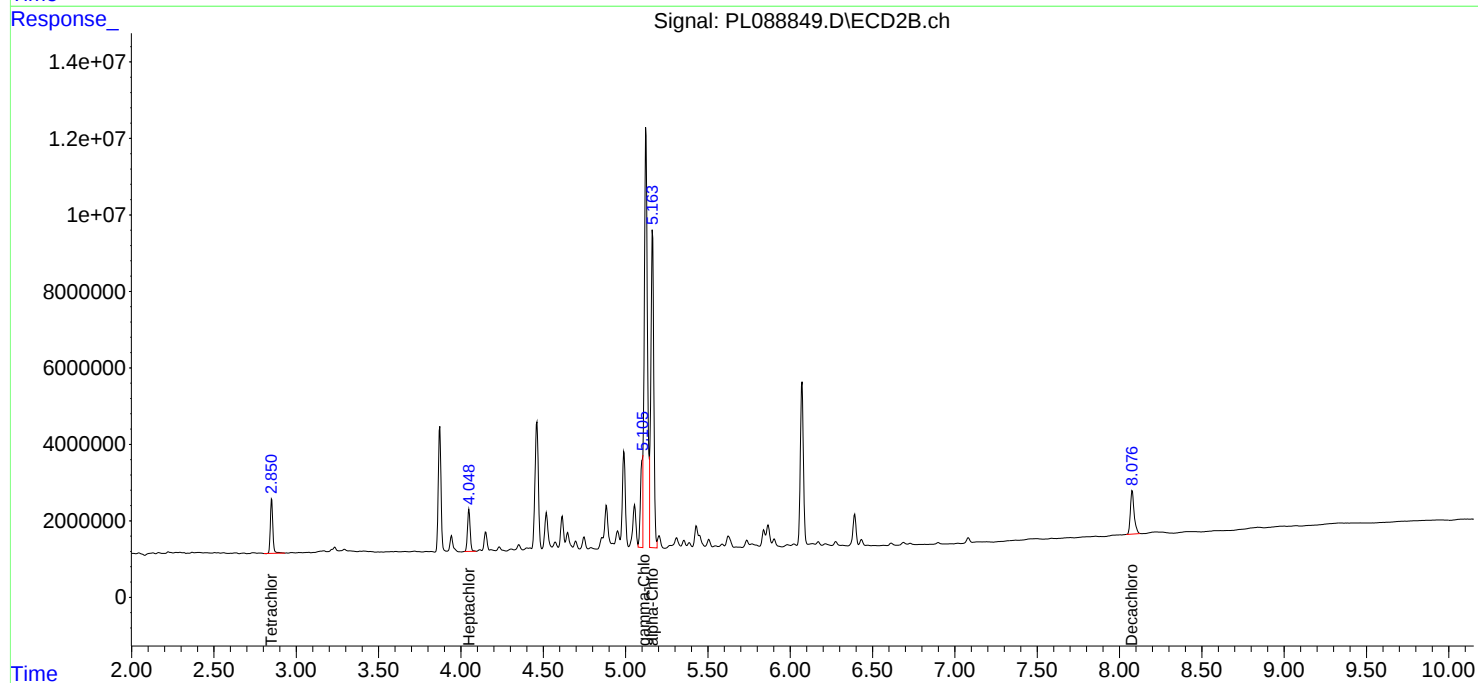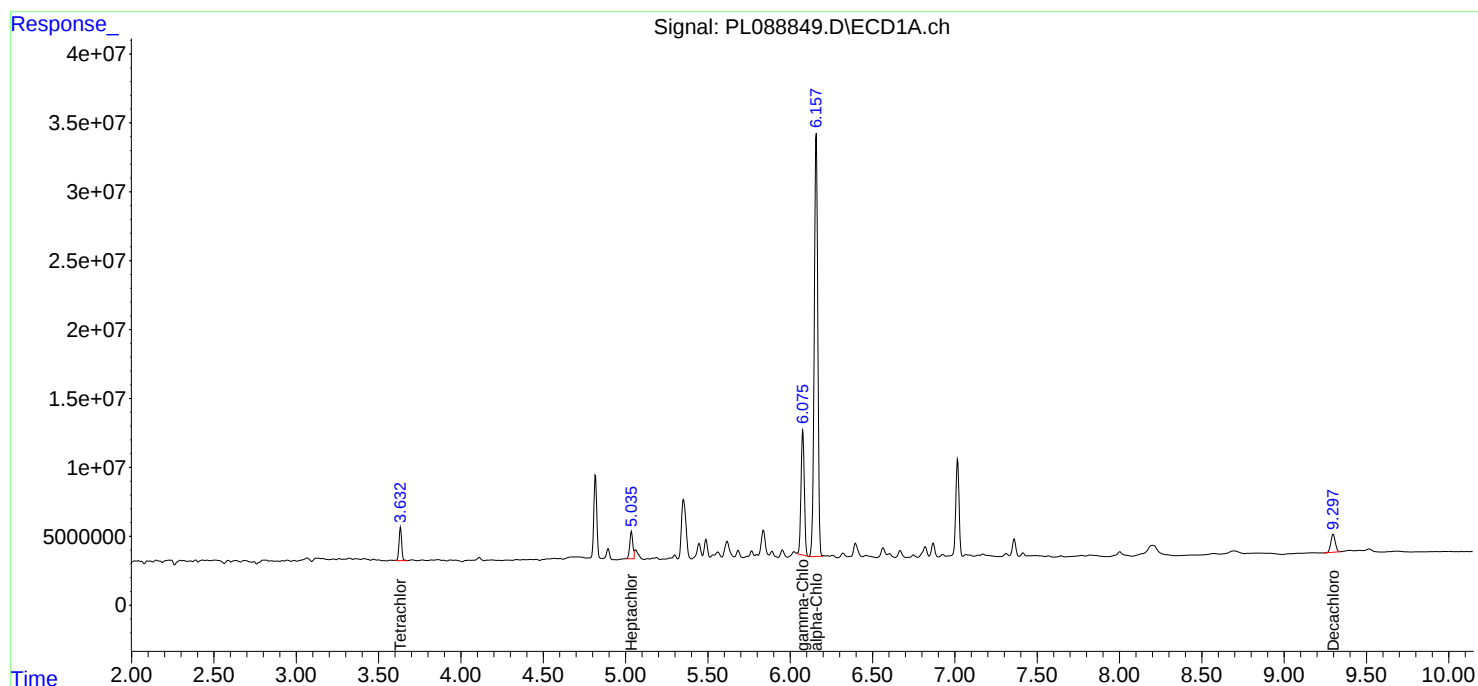


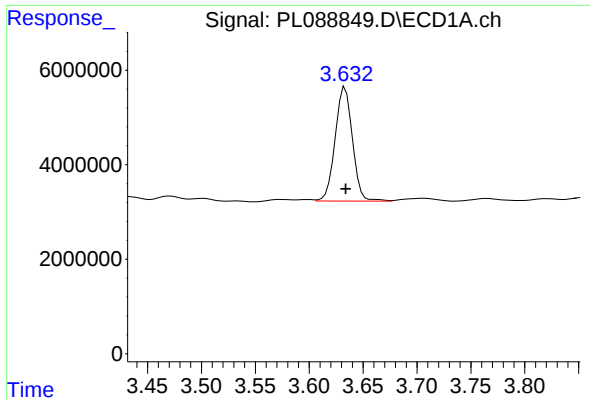

#1 Tetrachloro-m-xylene


R.T.: 3.633 min
Delta R.T.: 0.000 min
Response: 26945277
Conc: 10.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-04-032924

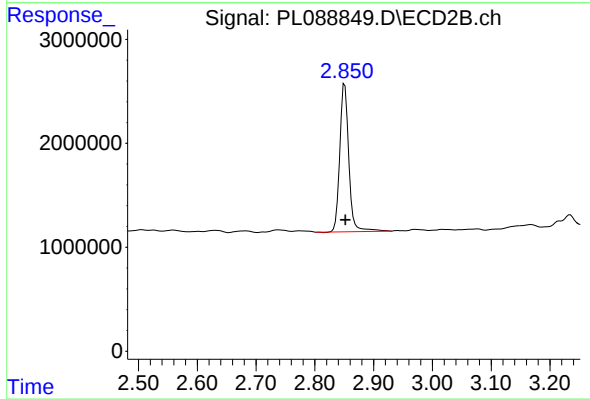


#1 Tetrachloro-m-xylene

R.T.: 2.851 min
Delta R.T.: -0.001 min
Response: 15145171
Conc: 11.36 ng/ml

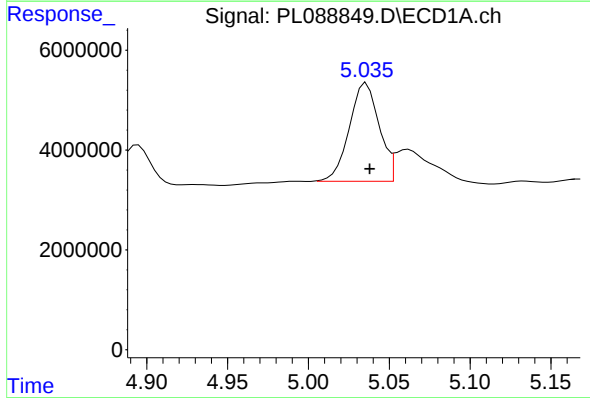


#4 Heptachlor

R.T.: 5.035 min
Delta R.T.: -0.003 min
Response: 26052174
Conc: 6.86 ng/ml m

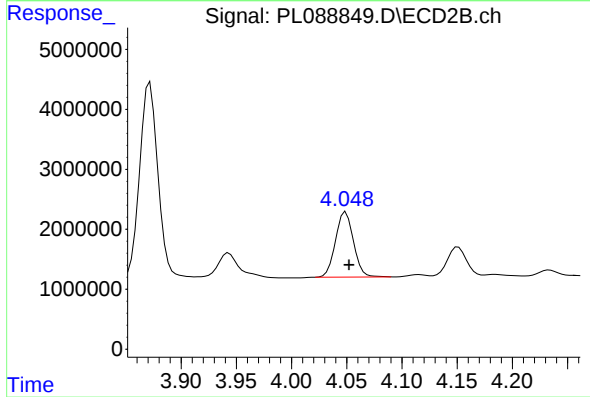

#4 Heptachlor


R.T.: 4.048 min
Delta R.T.: -0.004 min
Response: 12400676
Conc: 6.89 ng/ml m

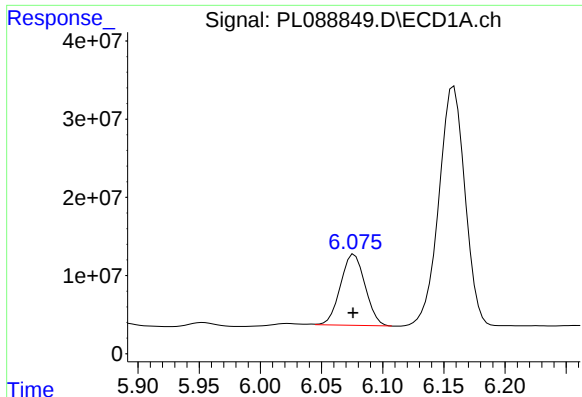

#10 gamma-Chlordane


R.T.: 6.075 min
Delta R.T.: 0.000 min
Response: 126961202
Conc: 38.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-04-032924

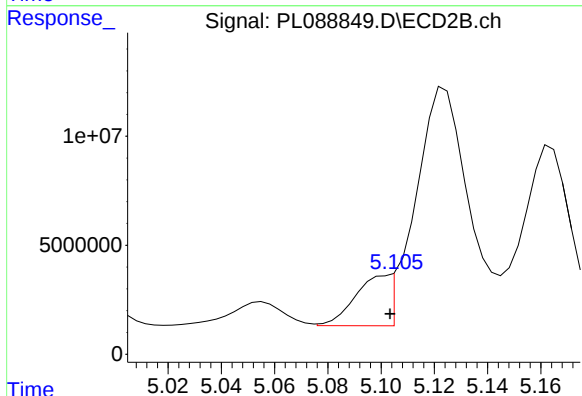


#10 gamma-Chlordane

R.T.: 5.105 min
Delta R.T.: 0.001 min
Response: 27858513
Conc: 16.82 ng/ml m

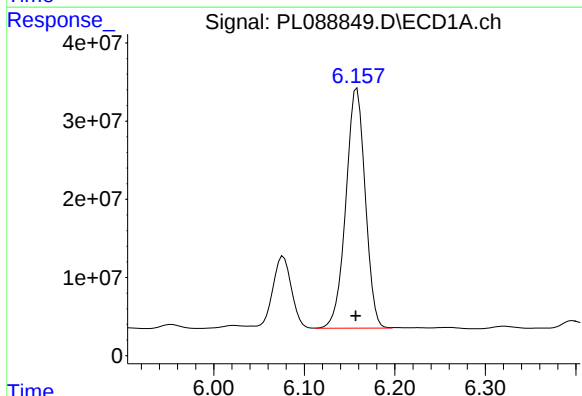


#11 alpha-Chlordane

R.T.: 6.158 min
Delta R.T.: 0.001 min
Response: 456032145
Conc: 137.19 ng/ml

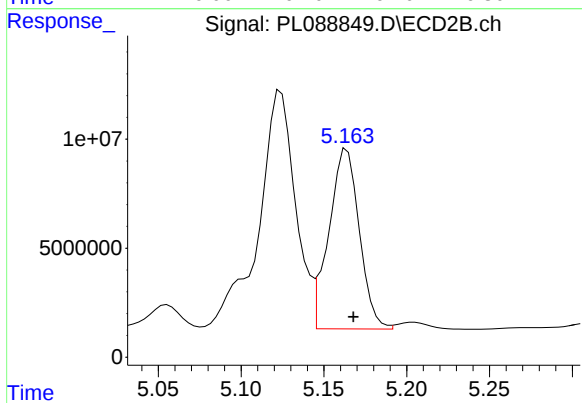

#11 alpha-Chlordane


R.T.: 5.164 min
Delta R.T.: -0.004 min
Response: 105656988
Conc: 63.65 ng/ml

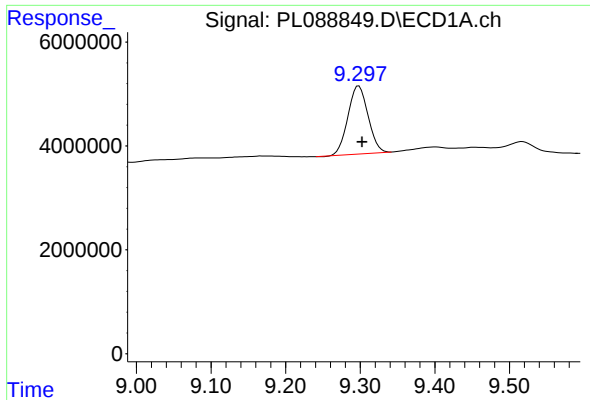

#28 Decachlorobiphenyl

R.T.: 9.298 min
Delta R.T.: -0.005 min
Response: 24484424
Conc: 9.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-04-032924

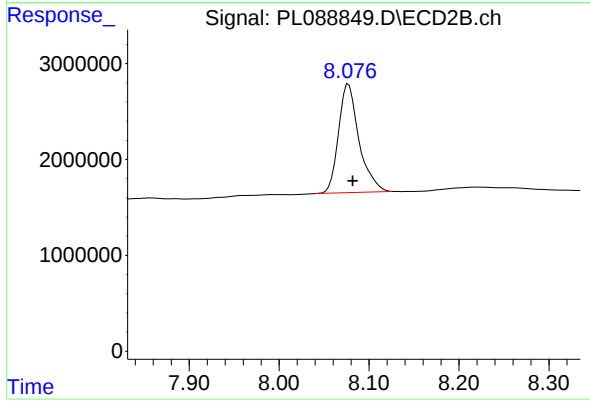

#28 Decachlorobiphenyl

R.T.: 8.077 min
Delta R.T.: -0.004 min
Response: 17968026
Conc: 13.25 ng/ml