

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040125\
 Data File : PL095002.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Apr 2025 19:52
 Operator : AR\AJ
 Sample : Q1692-01 10X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 NB-08-04012025

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 04/02/2025
 Supervised By :mohammad ahmed 04/03/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 02 01:28:21 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 11 17:42:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.535	2.768	4026003	5898333	1.422	1.653
28) SA Decachlor...	9.047	7.899	2988183	4348161	1.418m	1.076m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040125\
Data File : PL095002.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Apr 2025 19:52
Operator : AR\AJ
Sample : Q1692-01 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
NB-08-04012025


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 04/02/2025
Supervised By : mohammad ahmed 04/03/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 02 01:28:21 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
Quant Title : GC Extractables
QLast Update : Tue Mar 11 17:42:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

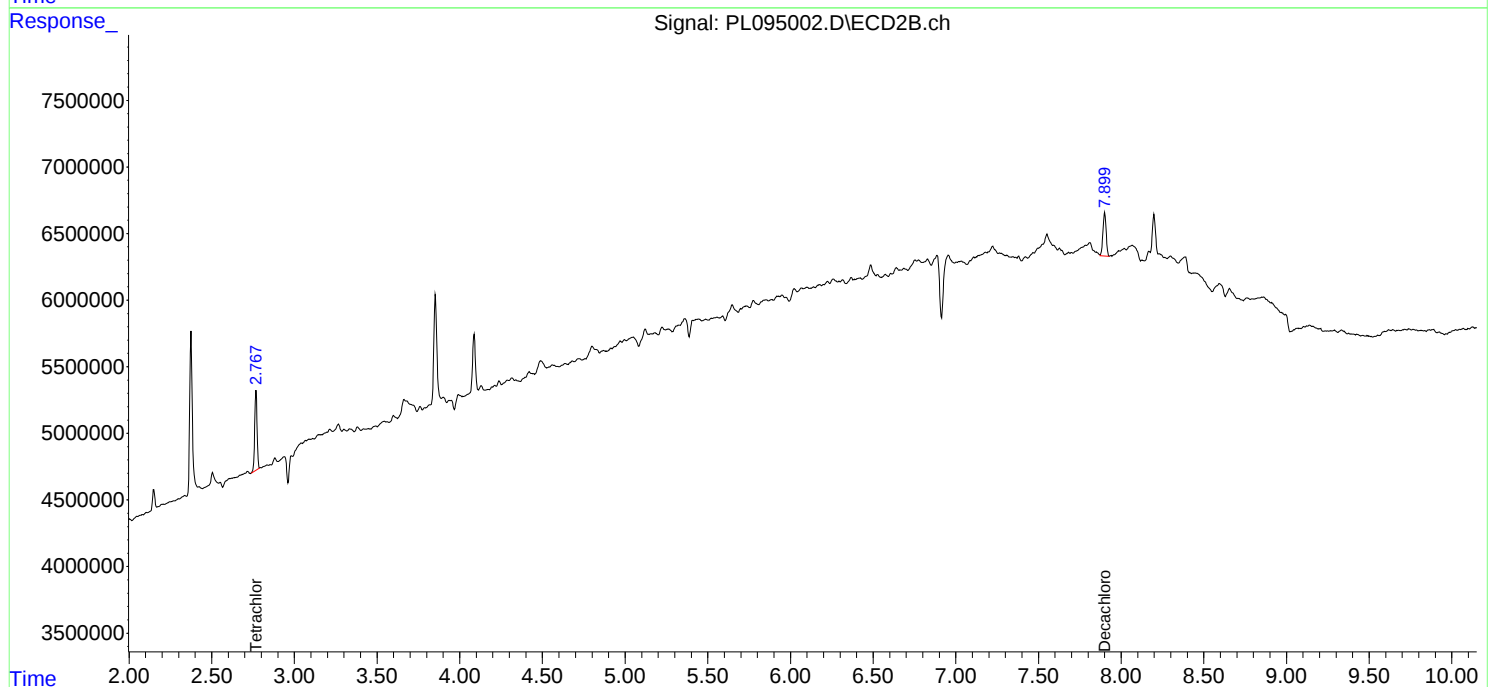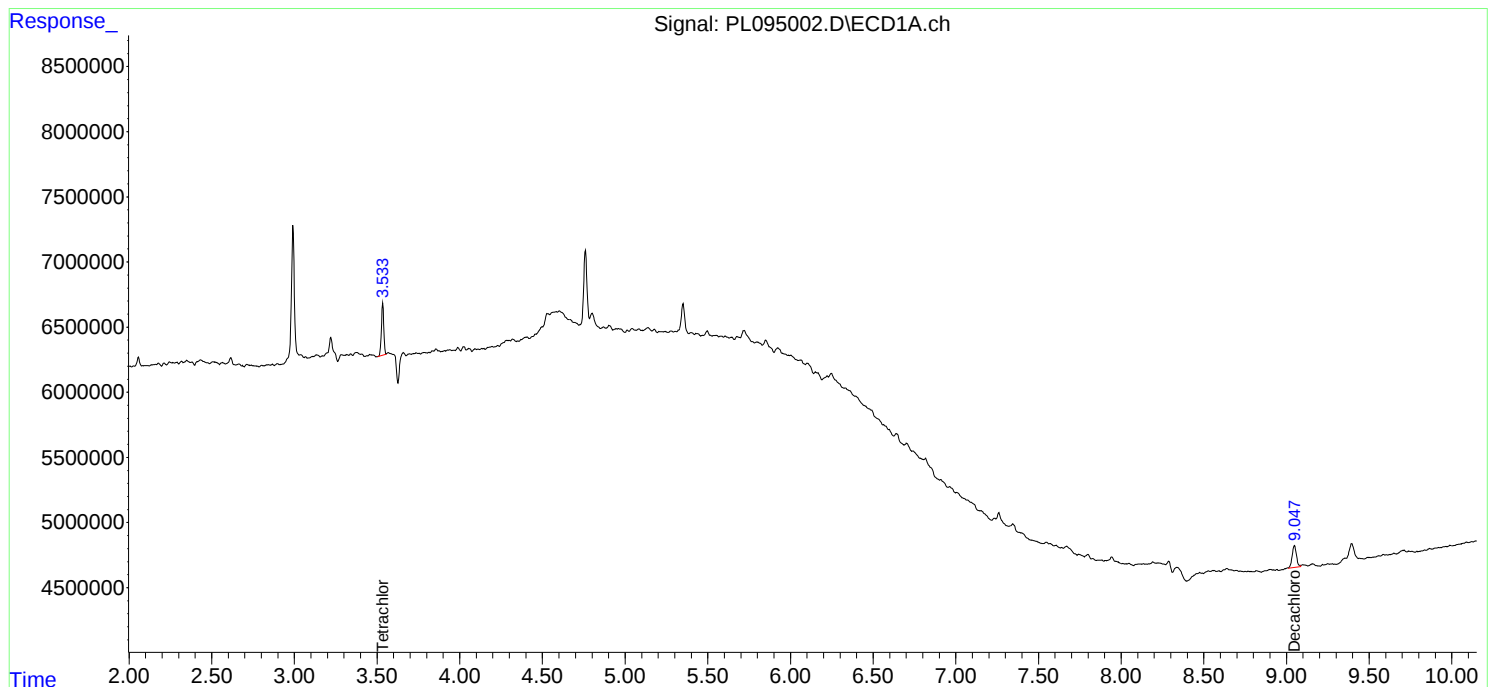

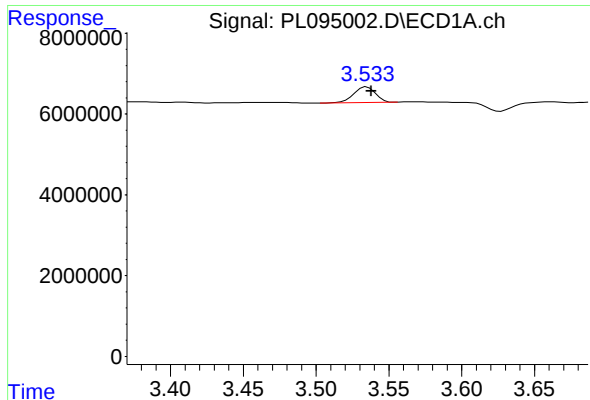


#1 Tetrachloro-m-xylene

R.T.: 3.535 min
Delta R.T.: -0.003 min
Response: 4026003
Conc: 1.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
NB-08-04012025


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 04/02/2025
Supervised By :mohammad ahmed 04/03/2025

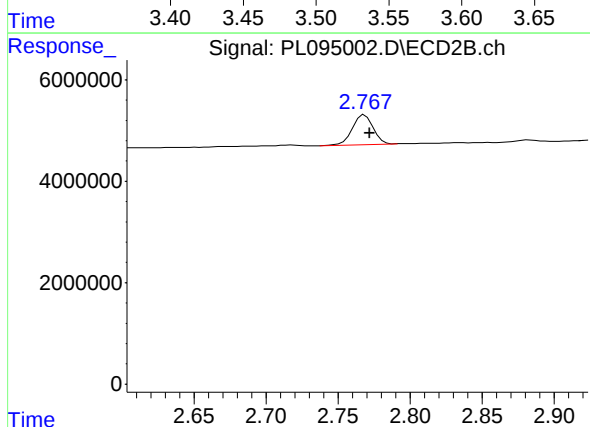


#1 Tetrachloro-m-xylene

R.T.: 2.768 min
Delta R.T.: -0.004 min
Response: 5898333
Conc: 1.65 ng/ml

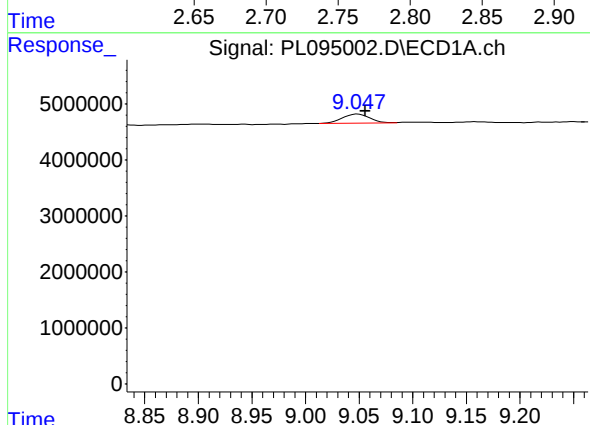

#28 Decachlorobiphenyl

R.T.: 9.047 min
Delta R.T.: -0.008 min
Response: 2988183
Conc: 1.42 ng/ml m

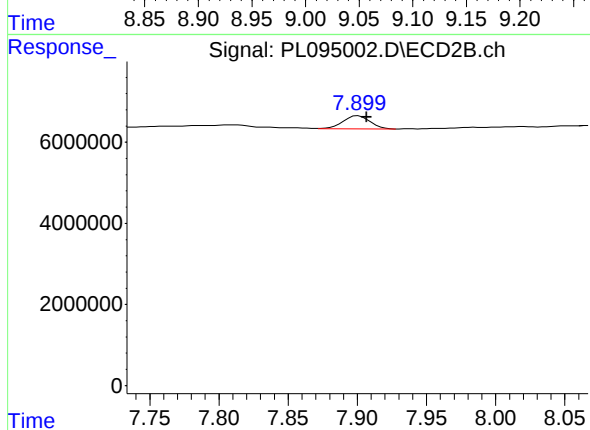

#28 Decachlorobiphenyl

R.T.: 7.899 min
Delta R.T.: -0.007 min
Response: 4348161
Conc: 1.08 ng/ml m