

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040219\
 Data File : PL046871.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Apr 2019 08:04
 Operator : AJ\SJ
 Sample : PSTDCCC050
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PSTDCCC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 01:08:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.358	3.976	369.7E6	115.5E6	50.823	50.452
28)	SA Decachlor...	8.033	9.027	412.9E6	120.5E6	49.089	51.994
Target Compounds							
2)	A alpha-BHC	3.787	4.366	603.4E6	166.8E6	51.744	51.924
3)	MA gamma-BHC...	4.064	4.650	555.4E6	156.0E6	51.695	52.123
4)	MA Heptachlor	4.351	5.156	570.9E6	156.6E6	51.783	50.898
5)	MB Aldrin	4.591	5.460	541.6E6	150.0E6	52.503	52.364
6)	B beta-BHC	4.317	4.823	226.5E6	69899360	50.315	52.727
7)	B delta-BHC	4.512	5.038	536.1E6	135.1E6	52.958	58.226
8)	B Heptachlor...	5.028	5.846	509.0E6	144.4E6	52.186	54.740
9)	A Endosulfan I	5.360	6.202	484.9E6	135.9E6	51.571	52.074
10)	B gamma-Chl...	5.250	6.080	530.6E6	152.8E6	51.650	53.826
11)	B alpha-Chl...	5.307	6.152	521.2E6	148.0E6	51.406	52.187
12)	B 4,4'-DDE	5.474	6.310	483.7E6	128.0E6	52.535	51.577
13)	MA Dieldrin	5.599	6.459	521.8E6	137.9E6	51.998	50.886
14)	MA Endrin	5.852	6.676	461.3E6	116.8E6	48.977	48.892
15)	B Endosulfa...	6.127	6.886	459.6E6	123.5E6	51.300	51.179
16)	A 4,4'-DDD	5.985	6.800	401.5E6	105.9E6	53.109	52.622
17)	MA 4,4'-DDT	6.220	7.098	395.1E6	104.1E6	52.167	49.628
18)	B Endrin al...	6.293	7.010	381.2E6	107.4E6	50.854	50.572
19)	B Endosulfa...	6.505	7.233	420.7E6	118.1E6	51.239	50.058
20)	A Methoxychlor	6.765	7.557	208.0E6	63436460	48.933	49.763
21)	B Endrin ke...	6.988	7.702	468.7E6	130.2E6	50.689	52.398
22)	Mirex	7.164	8.154	347.4E6	103.5E6	47.684	51.723
24)	Chlordane-2	0.000	5.460f	0	150.0E6	N.D.	1284.321 #
25)	Chlordane-3	5.250	6.080	530.6E6	152.8E6	476.421	400.671
26)	Chlordane-4	5.307	6.152	521.2E6	148.0E6	504.042	320.824 #
27)	Chlordane-5	6.127	0.000	459.6E6	0	1346.828	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040219\
Data File : PL046871.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Apr 2019 08:04
Operator : AJ\SJ
Sample : PSTDCCC050
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 01:08:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

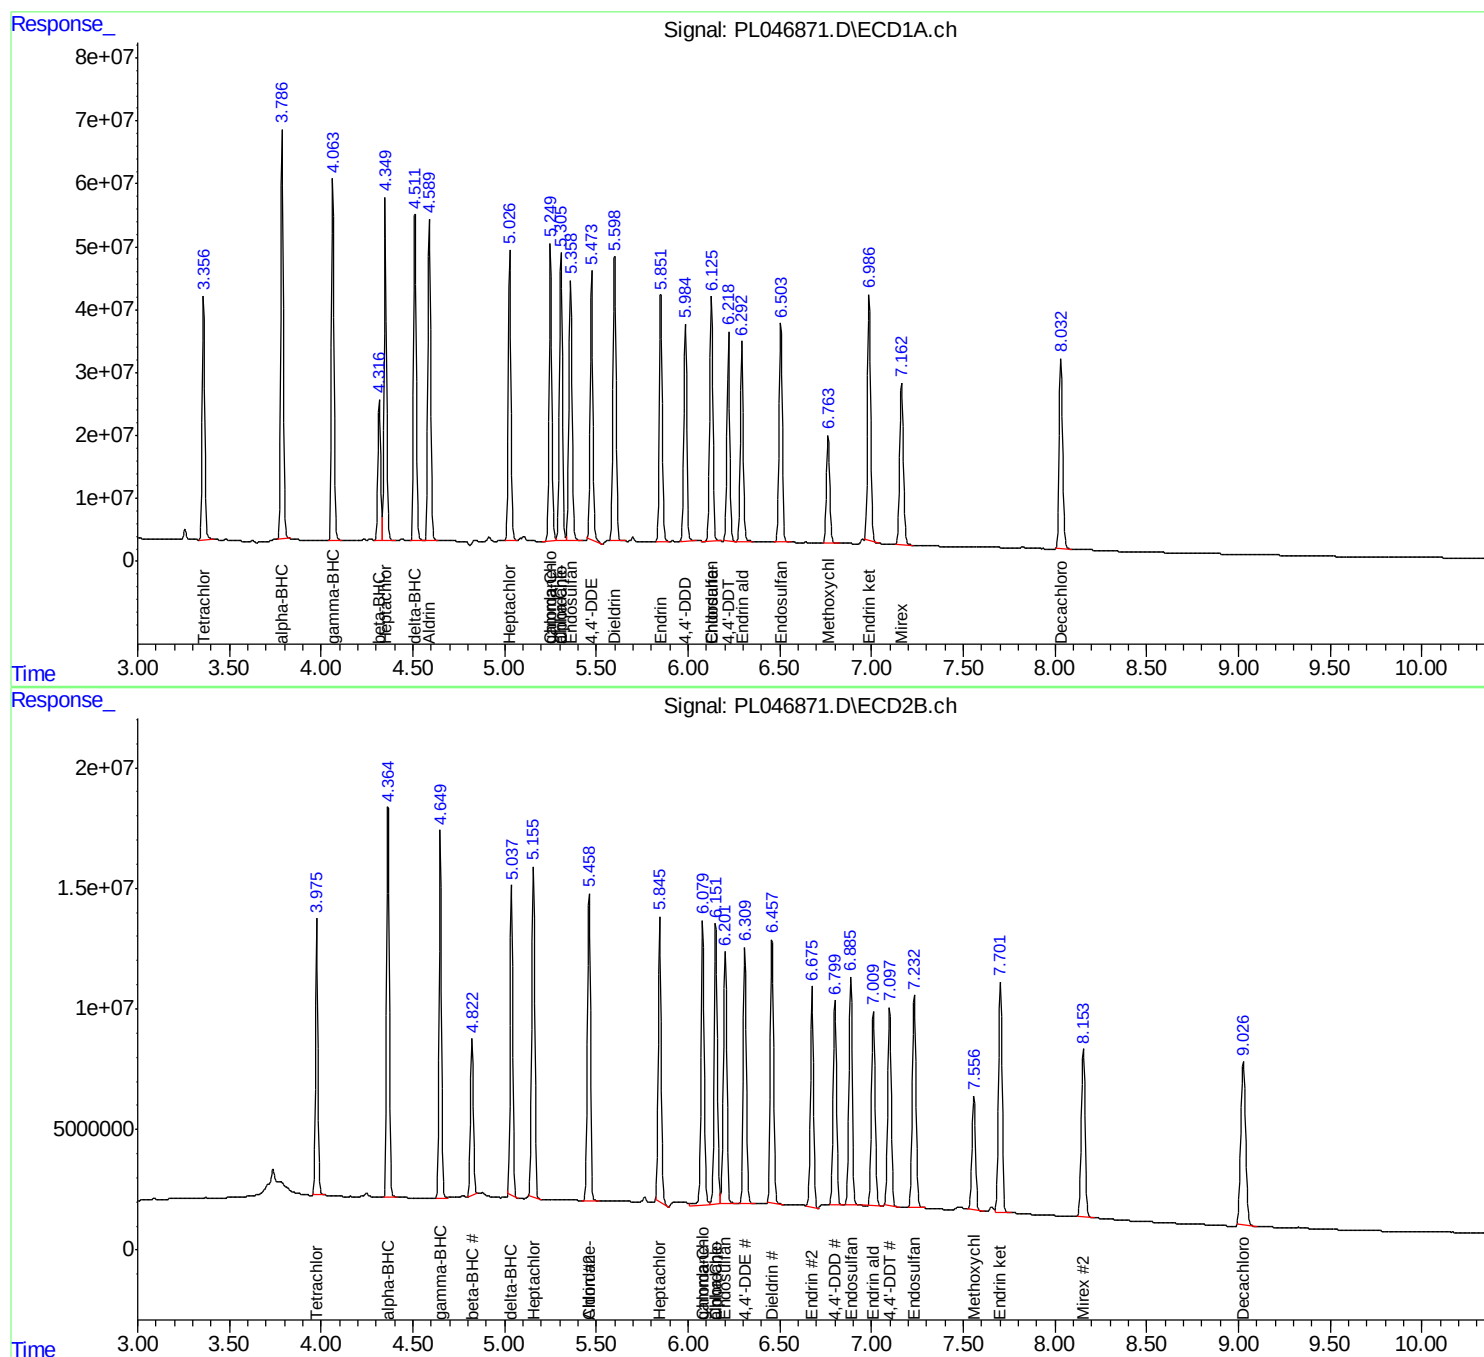


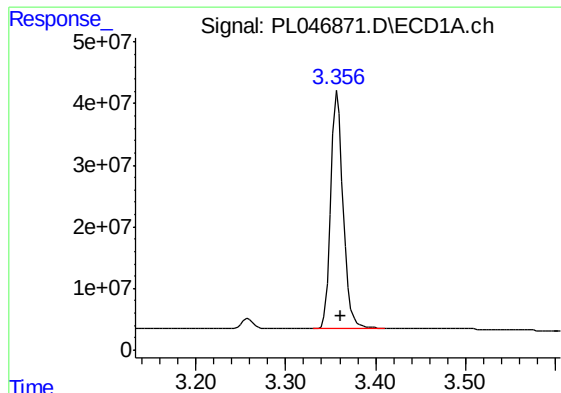

#1 Tetrachloro-m-xylene


R.T.: 3.358 min
Delta R.T.: -0.003 min
Response: 369720847
Conc: 50.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

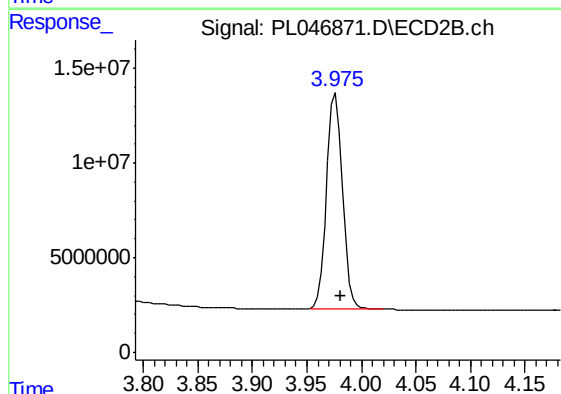


#1 Tetrachloro-m-xylene

R.T.: 3.976 min
Delta R.T.: -0.004 min
Response: 115516048
Conc: 50.45 ng/ml

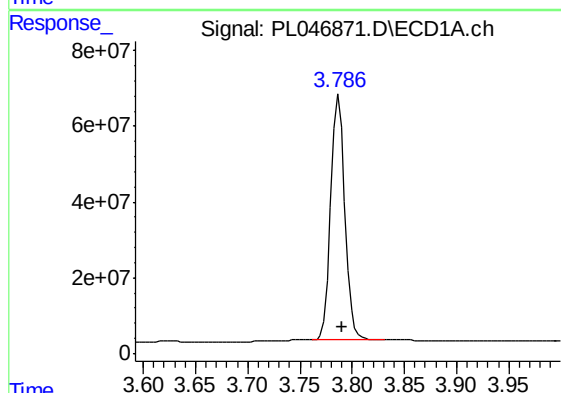


#2 alpha-BHC

R.T.: 3.787 min
Delta R.T.: -0.003 min
Response: 603441041
Conc: 51.74 ng/ml

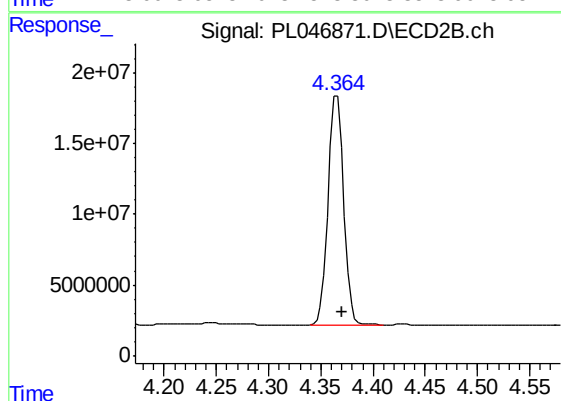

#2 alpha-BHC


R.T.: 4.366 min
Delta R.T.: -0.005 min
Response: 166847421
Conc: 51.92 ng/ml



#3 gamma-BHC (Lindane)


R.T.: 4.064 min
Delta R.T.: -0.004 min
Response: 555440190
Conc: 51.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

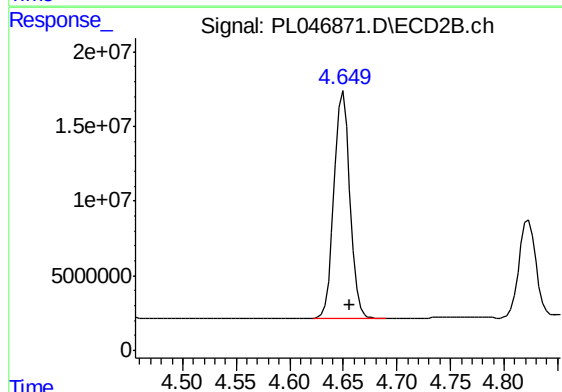


#3 gamma-BHC (Lindane)

R.T.: 4.650 min
Delta R.T.: -0.006 min
Response: 156004496
Conc: 52.12 ng/ml




#4 Heptachlor

R.T.: 4.351 min
Delta R.T.: -0.005 min
Response: 570911155
Conc: 51.78 ng/ml

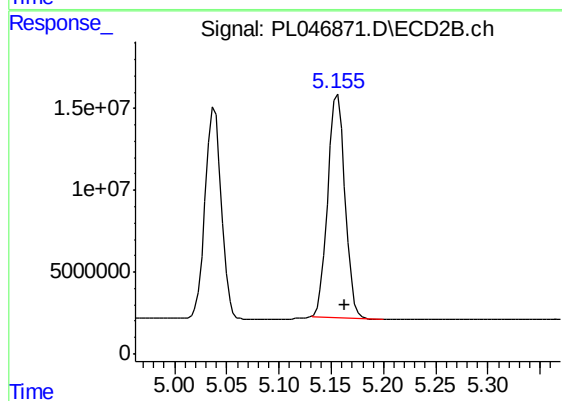

#4 Heptachlor


R.T.: 5.156 min
Delta R.T.: -0.006 min
Response: 156555802
Conc: 50.90 ng/ml



#5 Aldrin


R.T.: 4.591 min
Delta R.T.: -0.005 min
Response: 541562382
Conc: 52.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

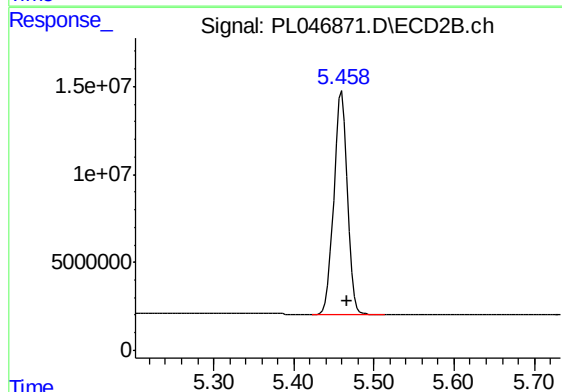


#5 Aldrin

R.T.: 5.460 min
Delta R.T.: -0.007 min
Response: 150020571
Conc: 52.36 ng/ml




#6 beta-BHC

R.T.: 4.317 min
Delta R.T.: -0.004 min
Response: 226540188
Conc: 50.32 ng/ml

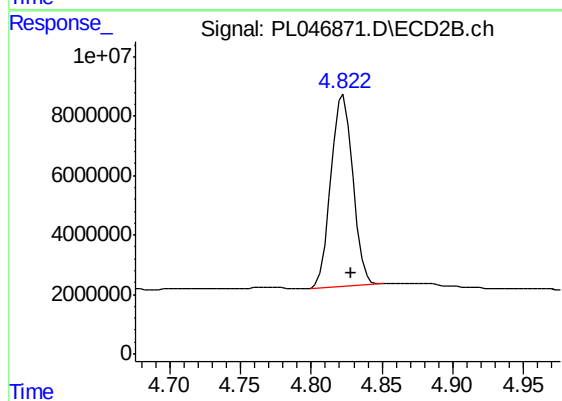

#6 beta-BHC


R.T.: 4.823 min
Delta R.T.: -0.005 min
Response: 69899360
Conc: 52.73 ng/ml



#7 delta-BHC


R.T.: 4.512 min
Delta R.T.: -0.005 min
Response: 536096816
Conc: 52.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

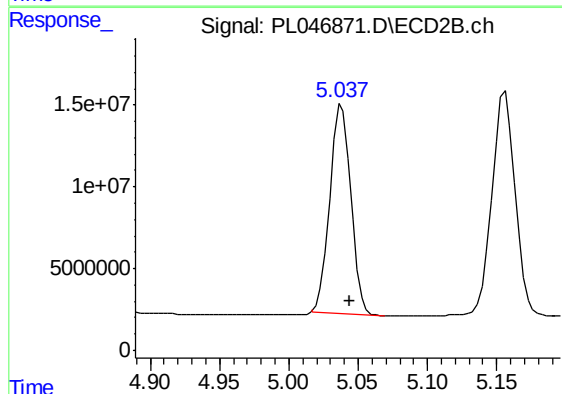


#7 delta-BHC

R.T.: 5.038 min
Delta R.T.: -0.006 min
Response: 135094858
Conc: 58.23 ng/ml

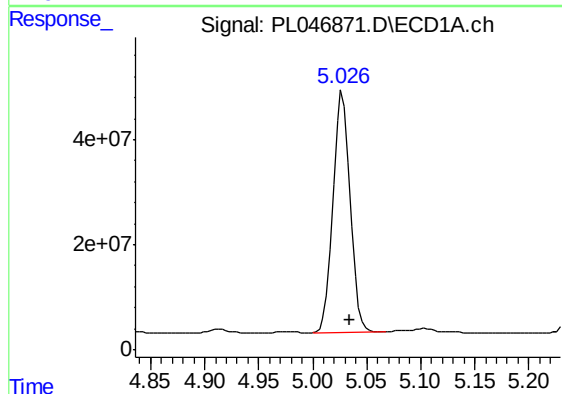


#8 Heptachlor epoxide

R.T.: 5.028 min
Delta R.T.: -0.006 min
Response: 508994590
Conc: 52.19 ng/ml

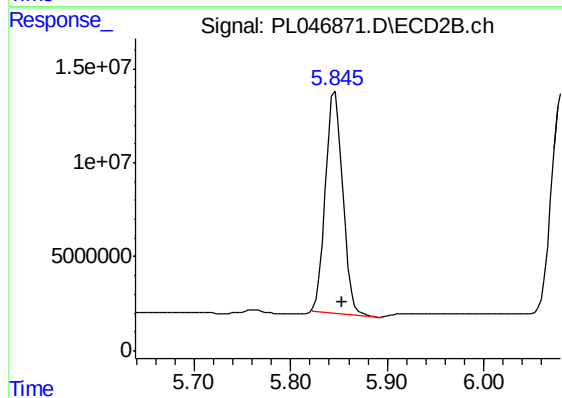

#8 Heptachlor epoxide


R.T.: 5.846 min
Delta R.T.: -0.007 min
Response: 144359418
Conc: 54.74 ng/ml



#9 Endosulfan I


R.T.: 5.360 min
Delta R.T.: -0.007 min
Response: 484886244
Conc: 51.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

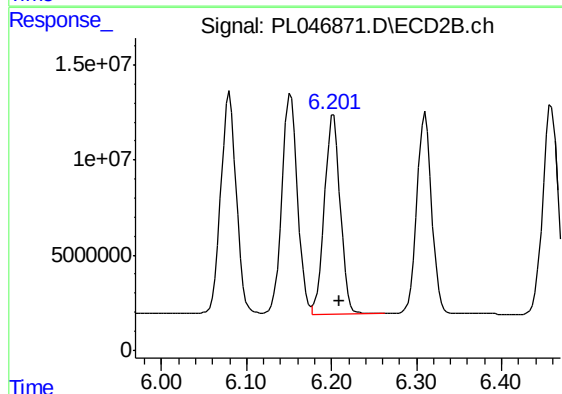


#9 Endosulfan I

R.T.: 6.202 min
Delta R.T.: -0.008 min
Response: 135906011
Conc: 52.07 ng/ml




#10 gamma-Chlordane

R.T.: 5.250 min
Delta R.T.: -0.006 min
Response: 530577156
Conc: 51.65 ng/ml

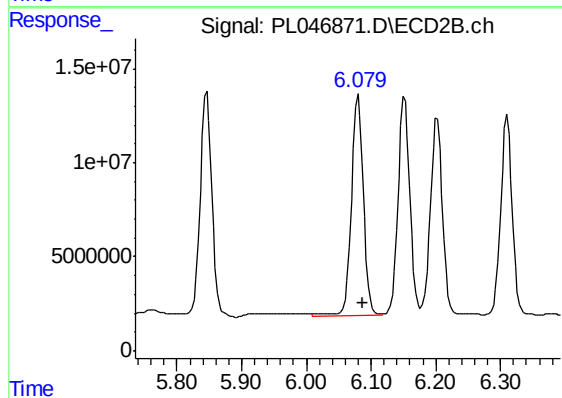

#10 gamma-Chlordane


R.T.: 6.080 min
Delta R.T.: -0.007 min
Response: 152762801
Conc: 53.83 ng/ml

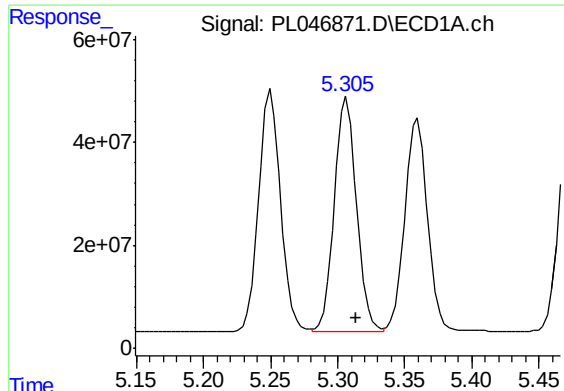

#11 alpha-Chlordane


R.T.: 5.307 min
Delta R.T.: -0.007 min
Response: 521209398
Conc: 51.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

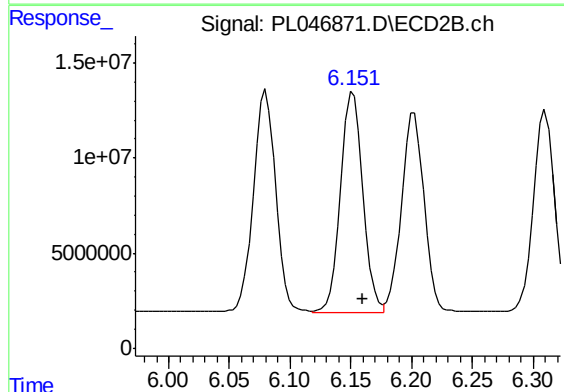


#11 alpha-Chlordane

R.T.: 6.152 min
Delta R.T.: -0.008 min
Response: 148036063
Conc: 52.19 ng/ml

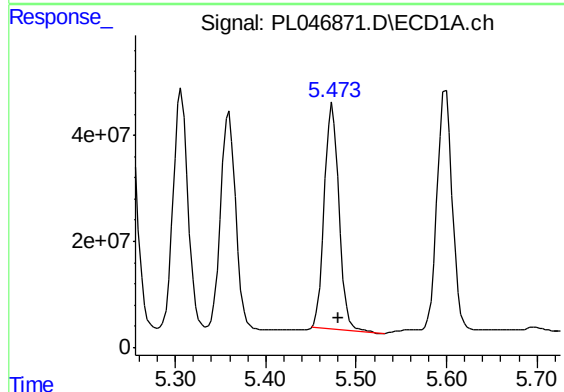


#12 4,4'-DDE

R.T.: 5.474 min
Delta R.T.: -0.007 min
Response: 483690682
Conc: 52.54 ng/ml

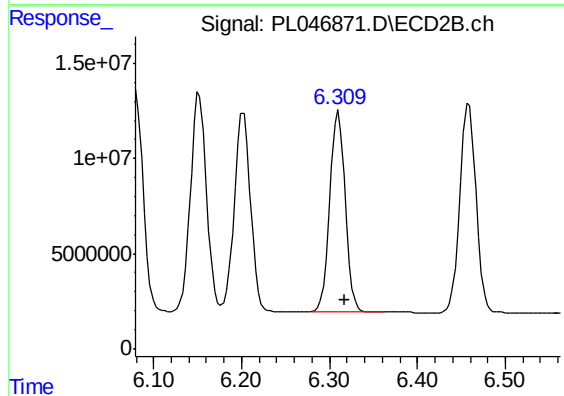

#12 4,4'-DDE


R.T.: 6.310 min
Delta R.T.: -0.008 min
Response: 128031194
Conc: 51.58 ng/ml

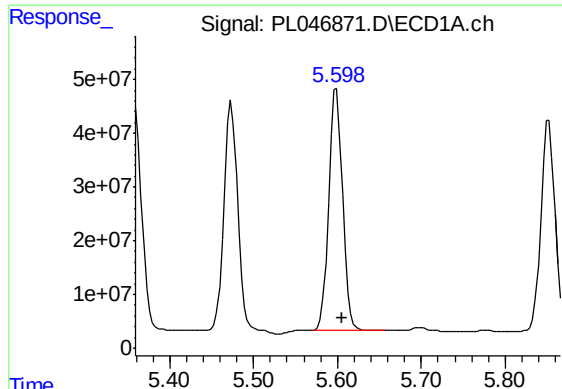

#13 Dielddrin


R.T.: 5.599 min
Delta R.T.: -0.007 min
Response: 521831085
Conc: 52.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

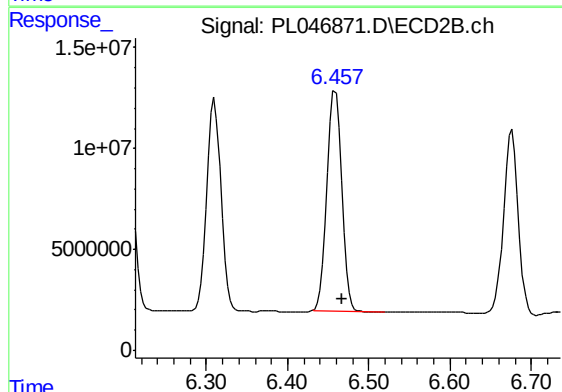


#13 Dielddrin

R.T.: 6.459 min
Delta R.T.: -0.008 min
Response: 137934807
Conc: 50.89 ng/ml




#14 Endrin

R.T.: 5.852 min
Delta R.T.: -0.007 min
Response: 461327463
Conc: 48.98 ng/ml

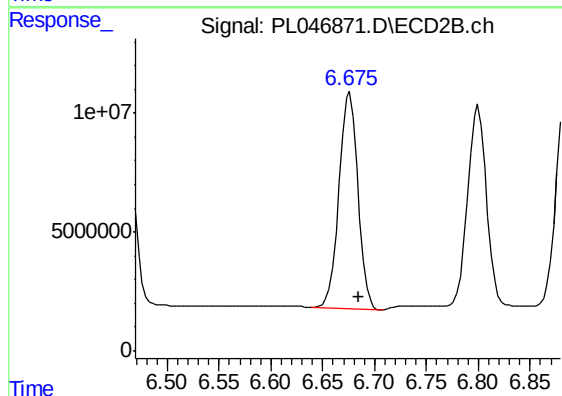

#14 Endrin


R.T.: 6.676 min
Delta R.T.: -0.008 min
Response: 116840691
Conc: 48.89 ng/ml



#15 Endosulfan II


R.T.: 6.127 min
Delta R.T.: -0.007 min
Response: 459627892
Conc: 51.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

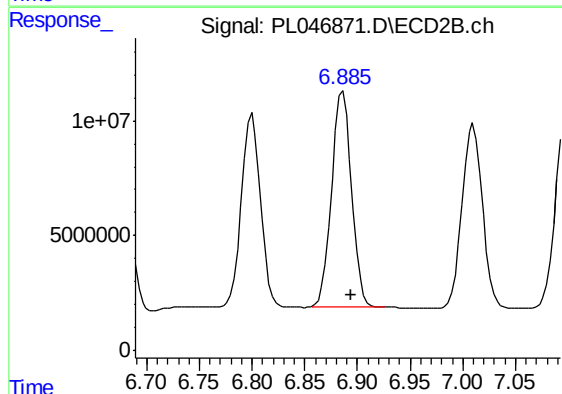


#15 Endosulfan II

R.T.: 6.886 min
Delta R.T.: -0.008 min
Response: 123489465
Conc: 51.18 ng/ml




#16 4,4'-DDD

R.T.: 5.985 min
Delta R.T.: -0.008 min
Response: 401457024
Conc: 53.11 ng/ml

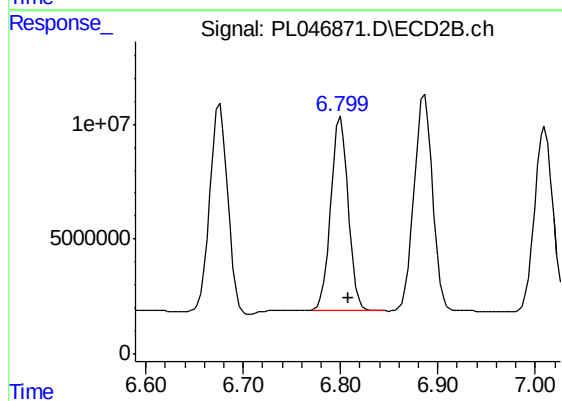

#16 4,4'-DDD


R.T.: 6.800 min
Delta R.T.: -0.008 min
Response: 105876764
Conc: 52.62 ng/ml



#17 4,4'-DDT


R.T.: 6.220 min
Delta R.T.: -0.008 min
Response: 395130001
Conc: 52.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

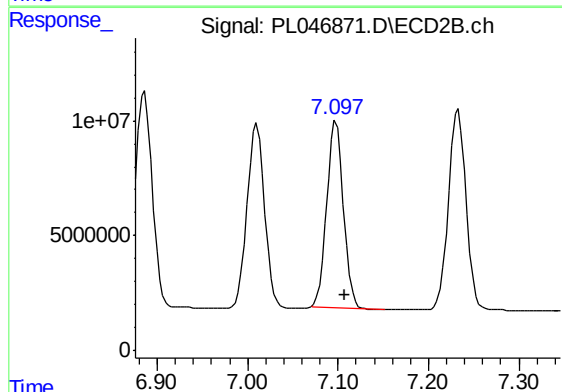


#17 4,4'-DDT

R.T.: 7.098 min
Delta R.T.: -0.009 min
Response: 104068539
Conc: 49.63 ng/ml




#18 Endrin aldehyde

R.T.: 6.293 min
Delta R.T.: -0.008 min
Response: 381161915
Conc: 50.85 ng/ml

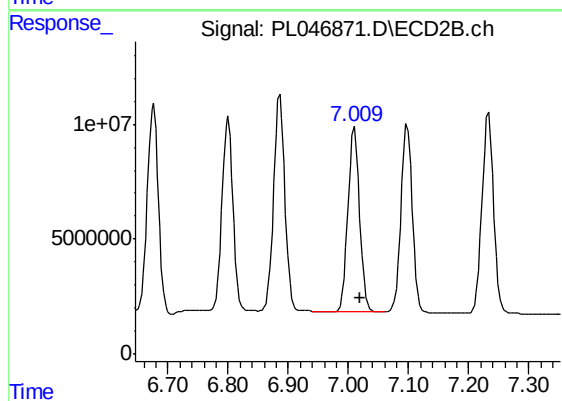

#18 Endrin aldehyde


R.T.: 7.010 min
Delta R.T.: -0.009 min
Response: 107414334
Conc: 50.57 ng/ml

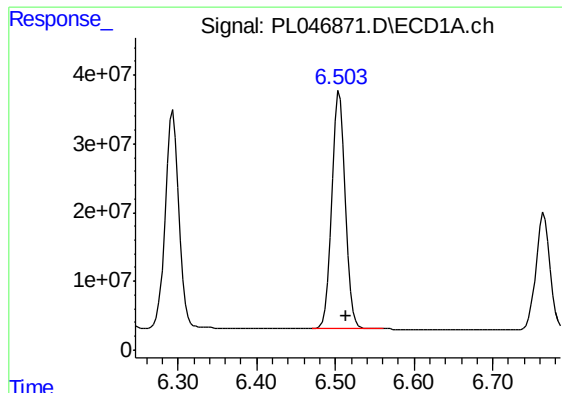

#19 Endosulfan Sulfate


R.T.: 6.505 min
Delta R.T.: -0.008 min
Response: 420734776
Conc: 51.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

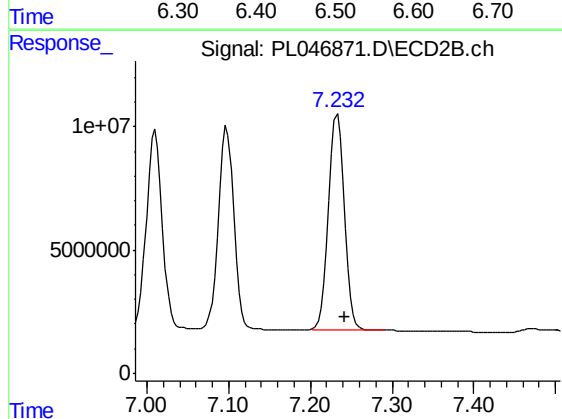


#19 Endosulfan Sulfate

R.T.: 7.233 min
Delta R.T.: -0.009 min
Response: 118086644
Conc: 50.06 ng/ml

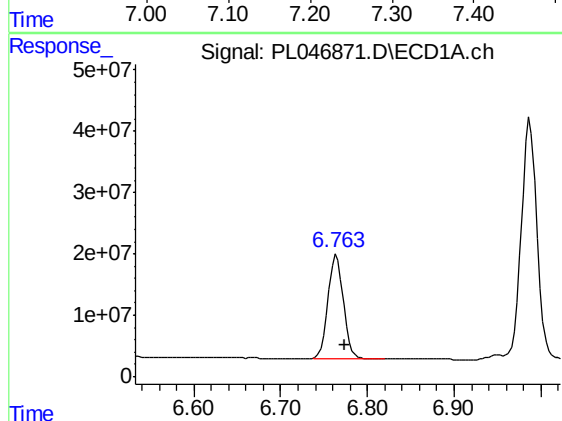


#20 Methoxychlor

R.T.: 6.765 min
Delta R.T.: -0.009 min
Response: 207957629
Conc: 48.93 ng/ml

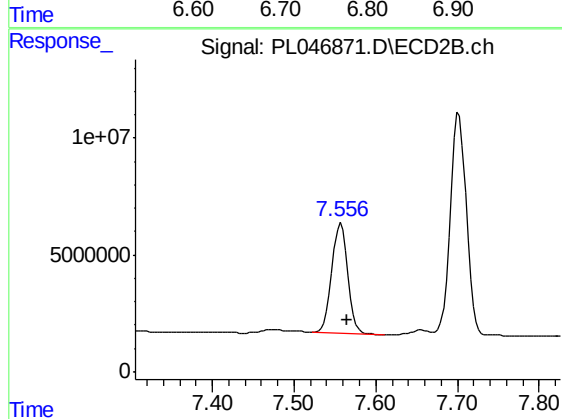

#20 Methoxychlor


R.T.: 7.557 min
Delta R.T.: -0.008 min
Response: 63436460
Conc: 49.76 ng/ml



#21 Endrin ketone


R.T.: 6.988 min
Delta R.T.: -0.008 min
Response: 468707254
Conc: 50.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

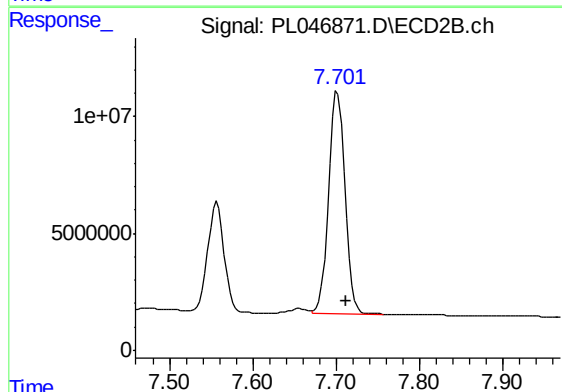


#21 Endrin ketone

R.T.: 7.702 min
Delta R.T.: -0.010 min
Response: 130184453
Conc: 52.40 ng/ml




#22 Mirex

R.T.: 7.164 min
Delta R.T.: -0.010 min
Response: 347401868
Conc: 47.68 ng/ml

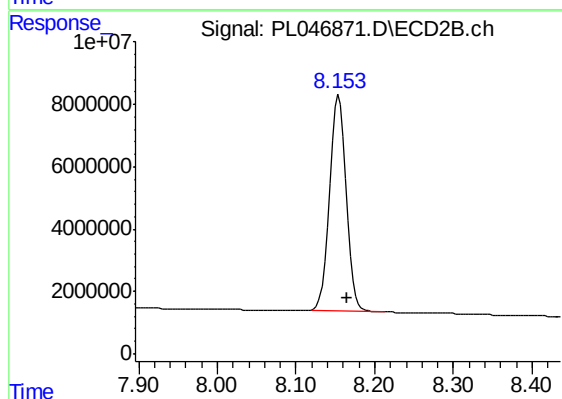

#22 Mirex


R.T.: 8.154 min
Delta R.T.: -0.011 min
Response: 103455102
Conc: 51.72 ng/ml

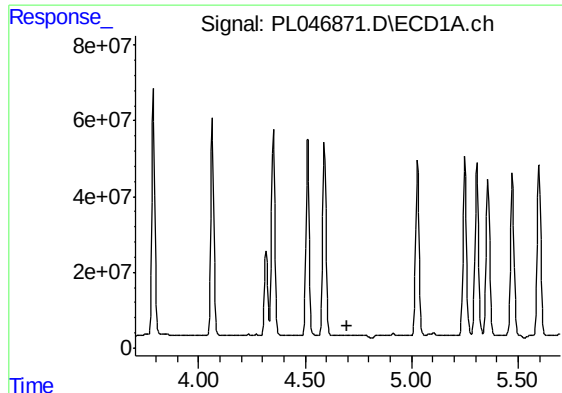

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.701 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

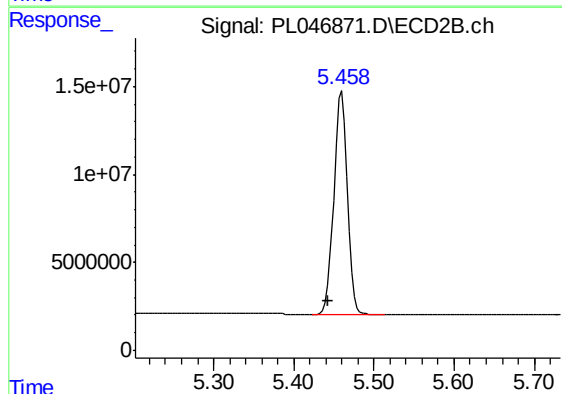


#24 Chlordane-2

R.T.: 5.460 min
Delta R.T.: 0.017 min
Response: 150020571
Conc: 1284.32 ng/ml

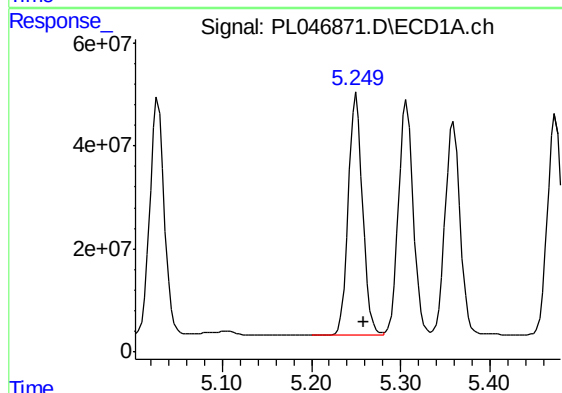


#25 Chlordane-3

R.T.: 5.250 min
Delta R.T.: -0.008 min
Response: 530577156
Conc: 476.42 ng/ml

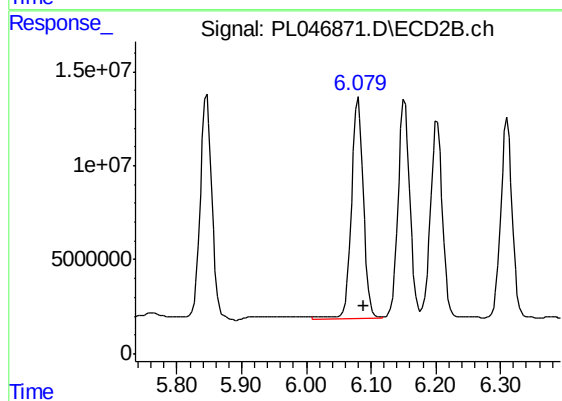

#25 Chlordane-3


R.T.: 6.080 min
Delta R.T.: -0.009 min
Response: 152762801
Conc: 400.67 ng/ml

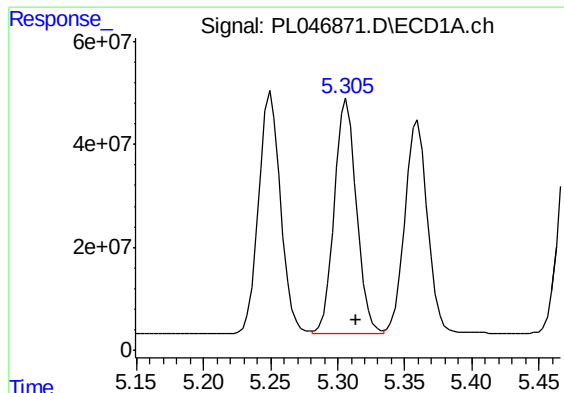

#26 Chlordane-4


R.T.: 5.307 min
Delta R.T.: -0.007 min
Response: 521209398
Conc: 504.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

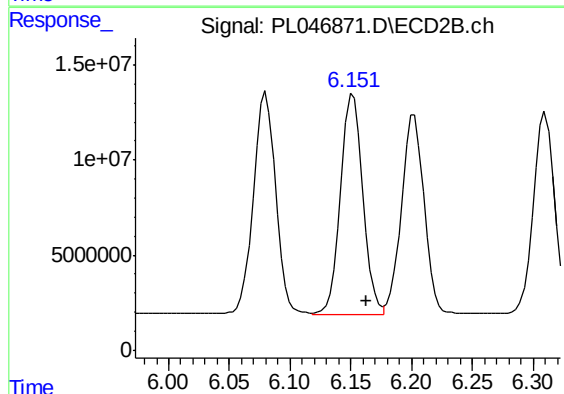


#26 Chlordane-4

R.T.: 6.152 min
Delta R.T.: -0.011 min
Response: 148036063
Conc: 320.82 ng/ml

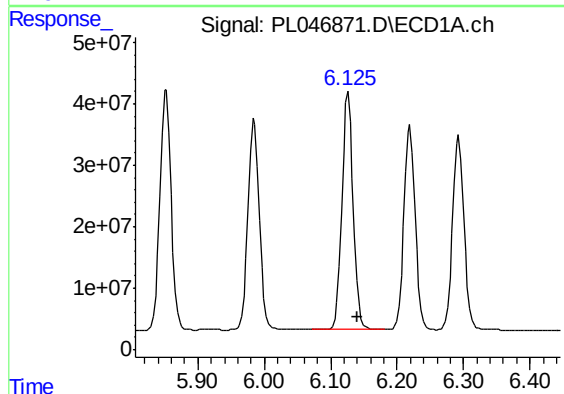


#27 Chlordane-5

R.T.: 6.127 min
Delta R.T.: -0.013 min
Response: 459627892
Conc: 1346.83 ng/ml

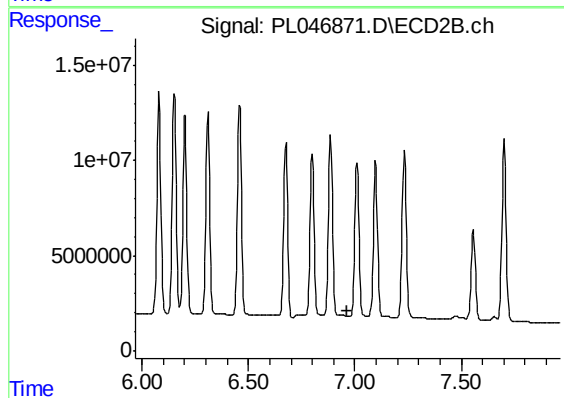

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 6.967 min
Response: 0
Conc: N.D.

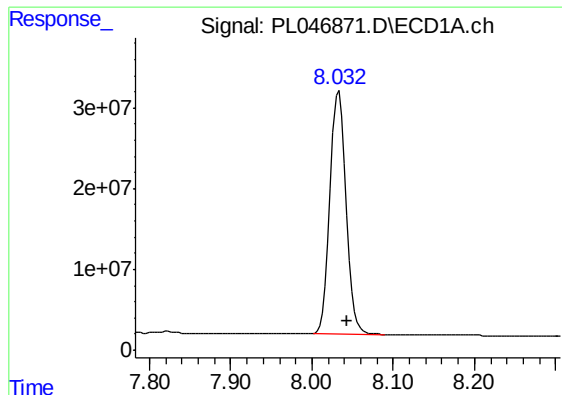

#28 Decachlorobiphenyl

R.T.: 8.033 min
Delta R.T.: -0.011 min
Response: 412892680
Conc: 49.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

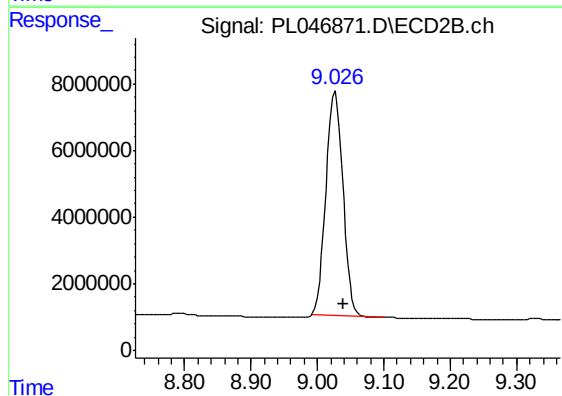

#28 Decachlorobiphenyl

R.T.: 9.027 min
Delta R.T.: -0.013 min
Response: 120547773
Conc: 51.99 ng/ml