

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040219\
 Data File : PL046892.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Apr 2019 13:58
 Operator : AJ\SJ
 Sample : K2182-07
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 S7C(2-10)COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 01:13:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.358	3.977	130.5E6	41891808	17.938	18.296
28)	SA Decachlor...	8.035	9.028	152.3E6	46762714	18.106	20.170
Target Compounds							
9)	A Endosulfan I	5.390f	0.000	12223057	0	1.300	N.D. #
10)	B gamma-Chl...	0.000	6.071f	0	1668870	N.D.	0.588 #
12)	B 4,4'-DDE	0.000	6.309	0	2023223	N.D.	0.815 #
13)	MA Dieldrin	5.609	0.000	17764326	0	1.770	N.D. #
16)	A 4,4'-DDD	0.000	6.805	0	6303969	N.D.	3.133 #
17)	MA 4,4'-DDT	6.217	0.000	34588242	0	4.567	N.D. #
19)	B Endosulfa...	6.527	0.000	12701266	0	1.547	N.D. #
25)	Chlordane-3	0.000	6.071f	0	1668870	N.D.	4.377 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040219\
Data File : PL046892.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Apr 2019 13:58
Operator : AJ\SJ
Sample : K2182-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
S7C(2-10)COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 01:13:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

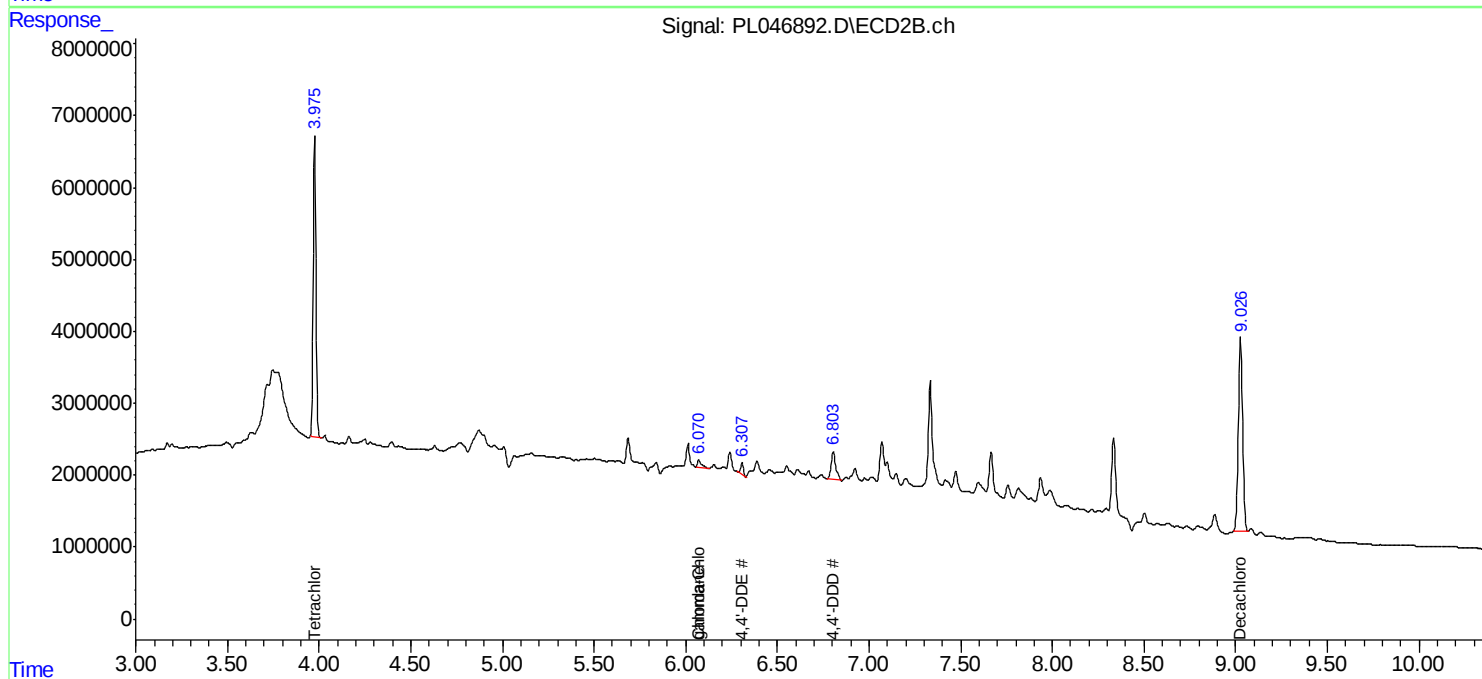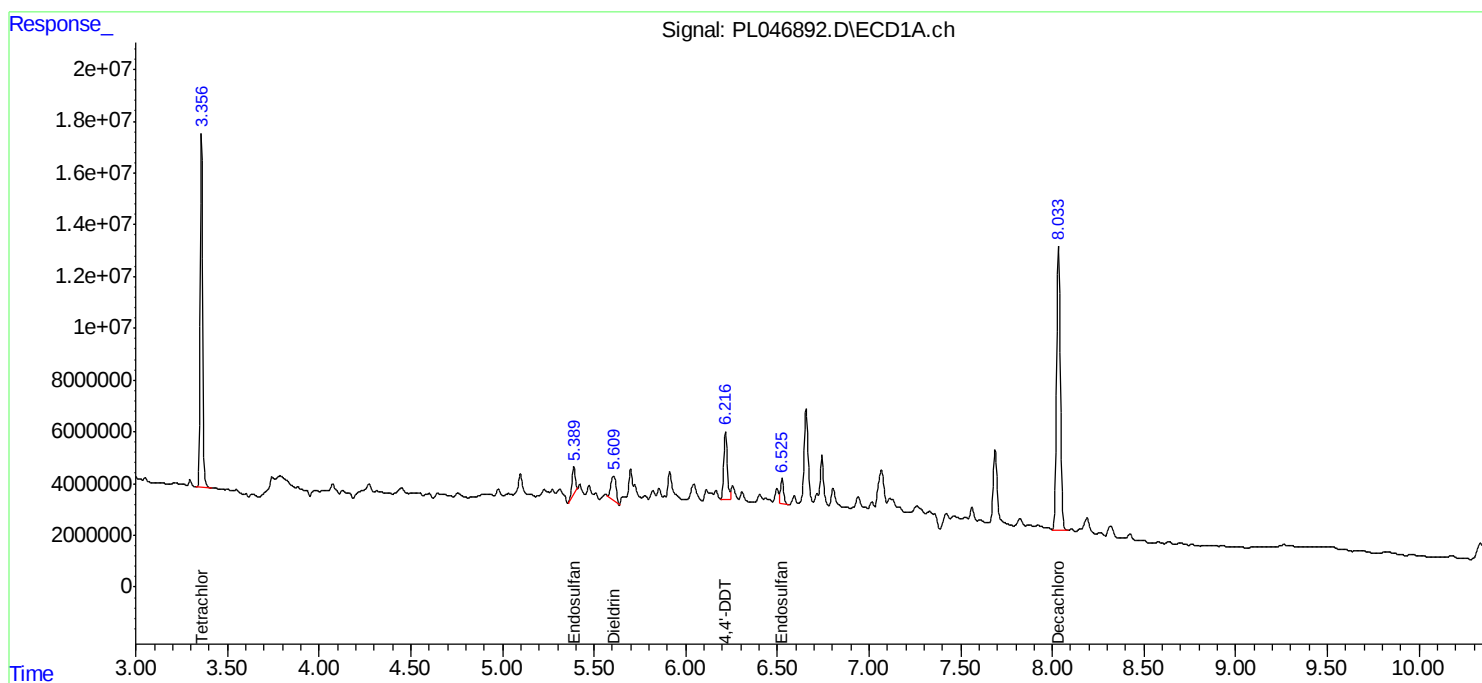


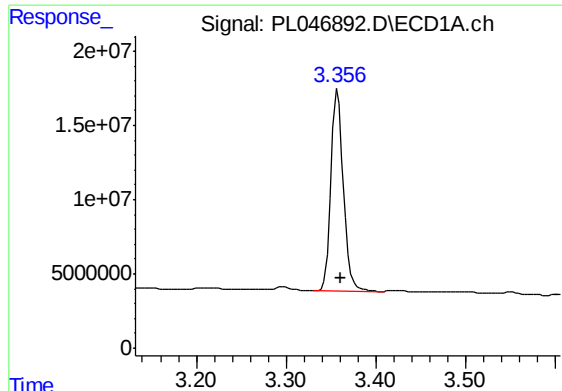

#1 Tetrachloro-m-xylene


R.T.: 3.358 min
Delta R.T.: -0.003 min
Response: 130493334
Conc: 17.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
S7C(2-10)COMP

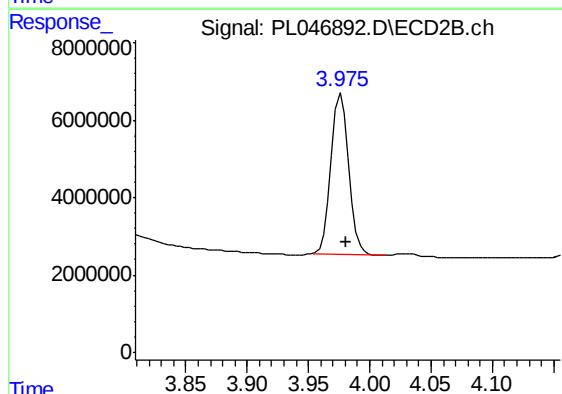


#1 Tetrachloro-m-xylene

R.T.: 3.977 min
Delta R.T.: -0.004 min
Response: 41891808
Conc: 18.30 ng/ml

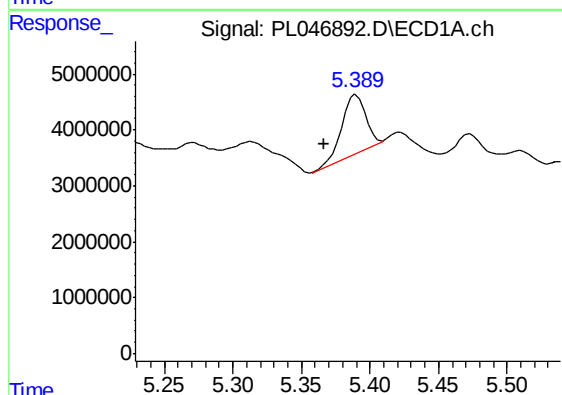


#9 Endosulfan I

R.T.: 5.390 min
Delta R.T.: 0.024 min
Response: 12223057
Conc: 1.30 ng/ml

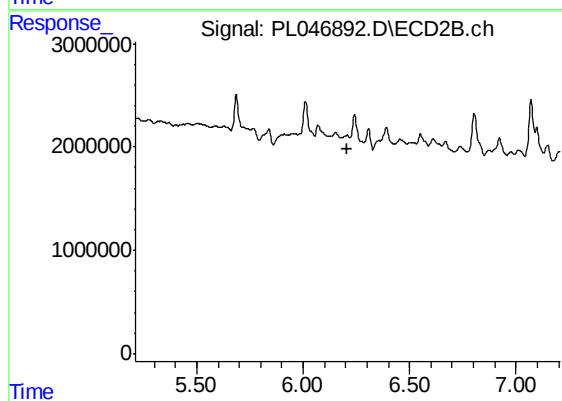

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.210 min
Response: 0
Conc: N.D.

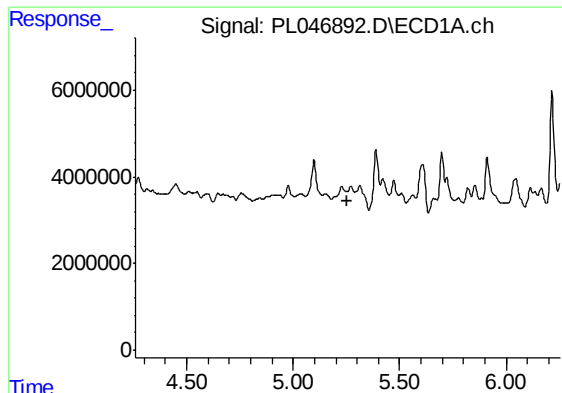

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.257 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
S7C(2-10)COMP

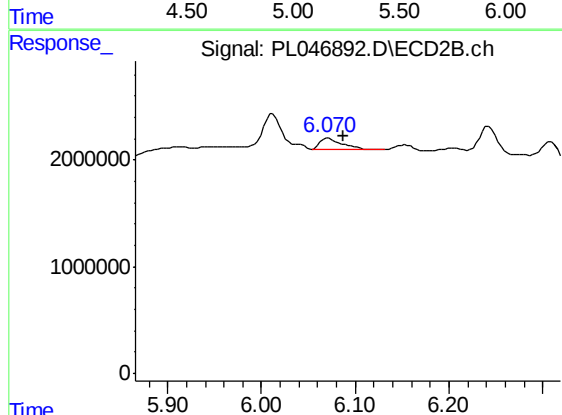


#10 gamma-Chlordane

R.T.: 6.071 min
Delta R.T.: -0.016 min
Response: 1668870
Conc: 0.59 ng/ml

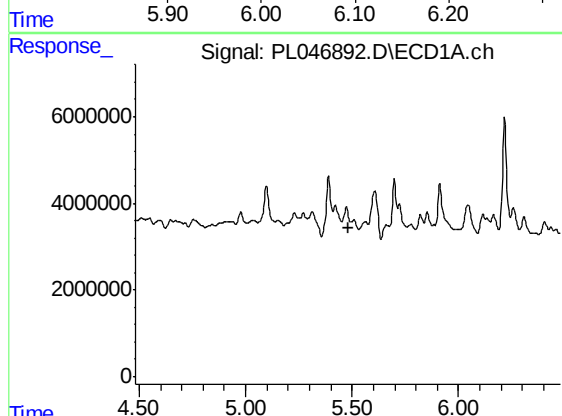


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 5.481 min
Response: 0
Conc: N.D.

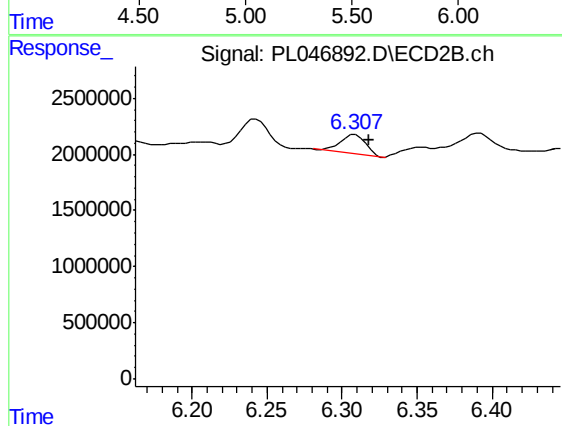

#12 4,4'-DDE


R.T.: 6.309 min
Delta R.T.: -0.009 min
Response: 2023223
Conc: 0.82 ng/ml

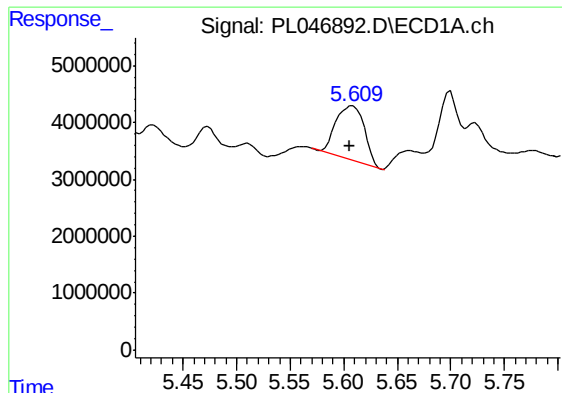

#13 Dieldrin


R.T.: 5.609 min
Delta R.T.: 0.002 min
Response: 17764326
Conc: 1.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
S7C(2-10)COMP

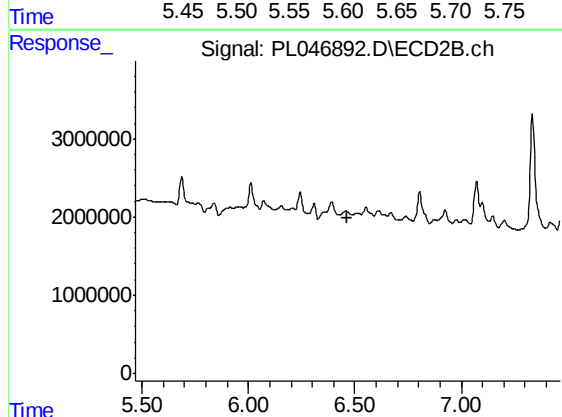


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.467 min
Response: 0
Conc: N.D.

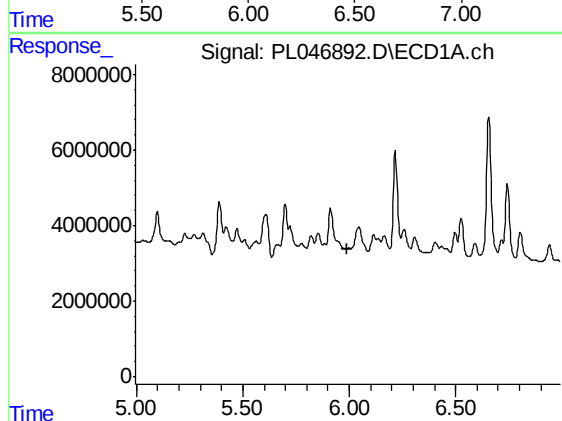


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.993 min
Response: 0
Conc: N.D.

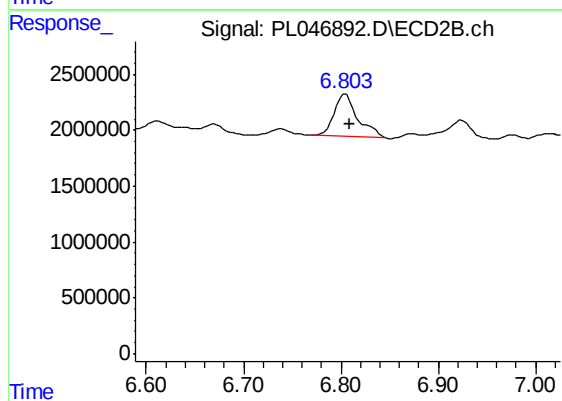

#16 4,4'-DDD


R.T.: 6.805 min
Delta R.T.: -0.004 min
Response: 6303969
Conc: 3.13 ng/ml

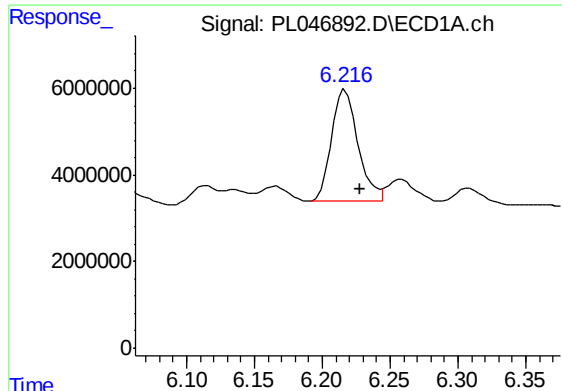

#17 4,4'-DDT


R.T.: 6.217 min
Delta R.T.: -0.011 min
Response: 34588242
Conc: 4.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
S7C(2-10)COMP

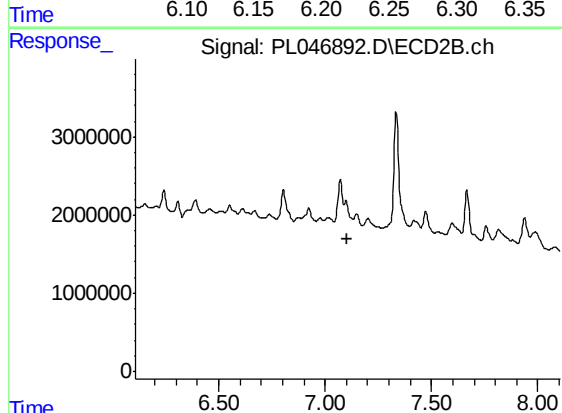


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.107 min
Response: 0
Conc: N.D.

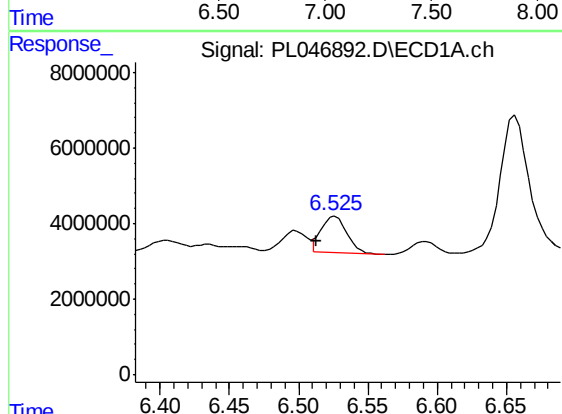


#19 Endosulfan Sulfate

R.T.: 6.527 min
Delta R.T.: 0.014 min
Response: 12701266
Conc: 1.55 ng/ml

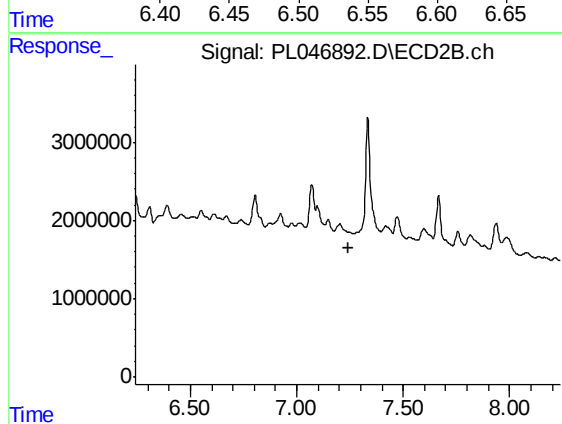

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 7.242 min
Response: 0
Conc: N.D.

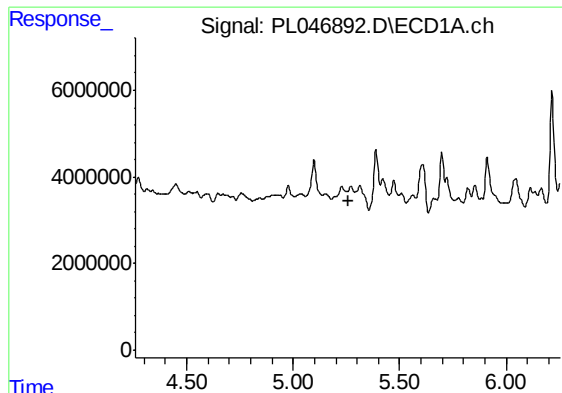

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.258 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
S7C(2-10)COMP

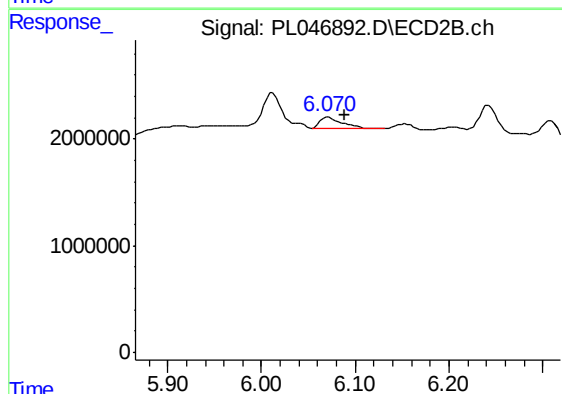


#25 Chlordane-3

R.T.: 6.071 min
Delta R.T.: -0.018 min
Response: 1668870
Conc: 4.38 ng/ml

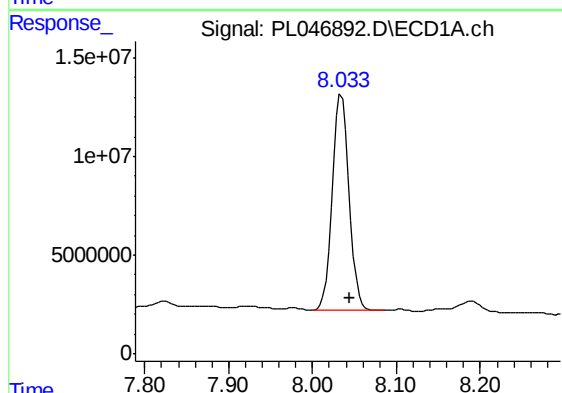

#28 Decachlorobiphenyl

R.T.: 8.035 min
Delta R.T.: -0.009 min
Response: 152288954
Conc: 18.11 ng/ml

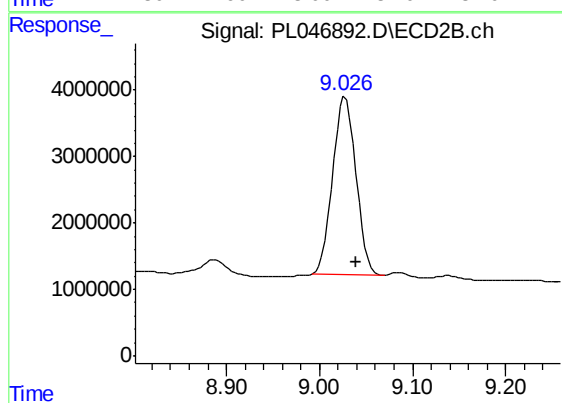

#28 Decachlorobiphenyl

R.T.: 9.028 min
Delta R.T.: -0.012 min
Response: 46762714
Conc: 20.17 ng/ml