

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040219\
 Data File : PL046902.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Apr 2019 16:26
 Operator : AJ\SJ
 Sample : K1695-08
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 DPC-91723-SO-TP5-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 01:16:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.358	3.977	121.0E6	38702784	16.634	16.904
28)	SA Decachlor...	8.035	9.030	116.5E6	40159607	13.846	17.322 #
Target Compounds							
9)	A Endosulfan I	5.391f	0.000	6571190	0	0.699	N.D. #
10)	B gamma-Chl...	5.251	0.000	13334100	0	1.298	N.D. #
11)	B alpha-Chl...	0.000	6.152	0	2425994	N.D.	0.855 #
12)	B 4,4'-DDE	5.474	6.311	18002762	5235867	1.955	2.109
16)	A 4,4'-DDD	5.986	6.801	26666053	9429670	3.528	4.687 #
19)	B Endosulfa...	6.532f	0.000	40416205	0	4.922	N.D. #
25)	Chlordane-3	5.251	0.000	13334100	0	11.973	N.D. #
26)	Chlordane-4	0.000	6.152	0	2425994	N.D.	5.258 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040219\
Data File : PL046902.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Apr 2019 16:26
Operator : AJ\SJ
Sample : K1695-08
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
DPC-91723-SO-TP5-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 01:16:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

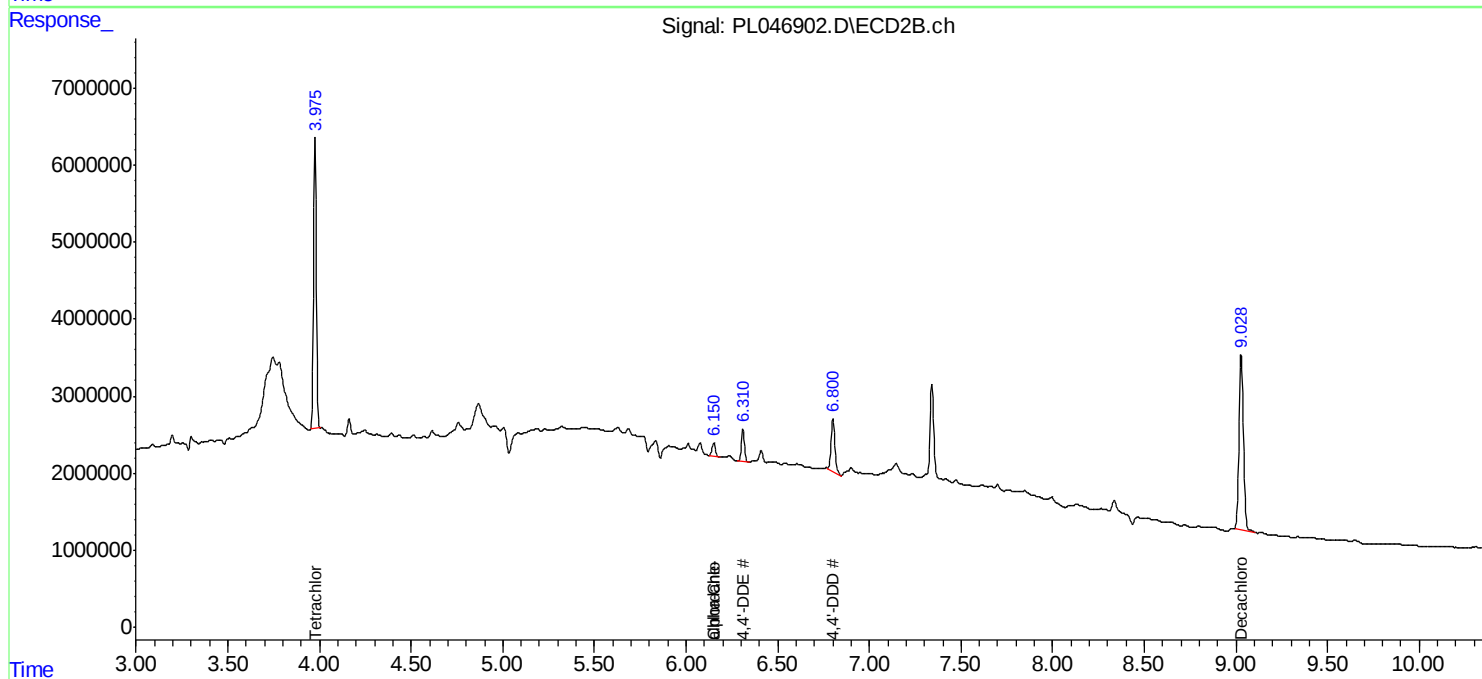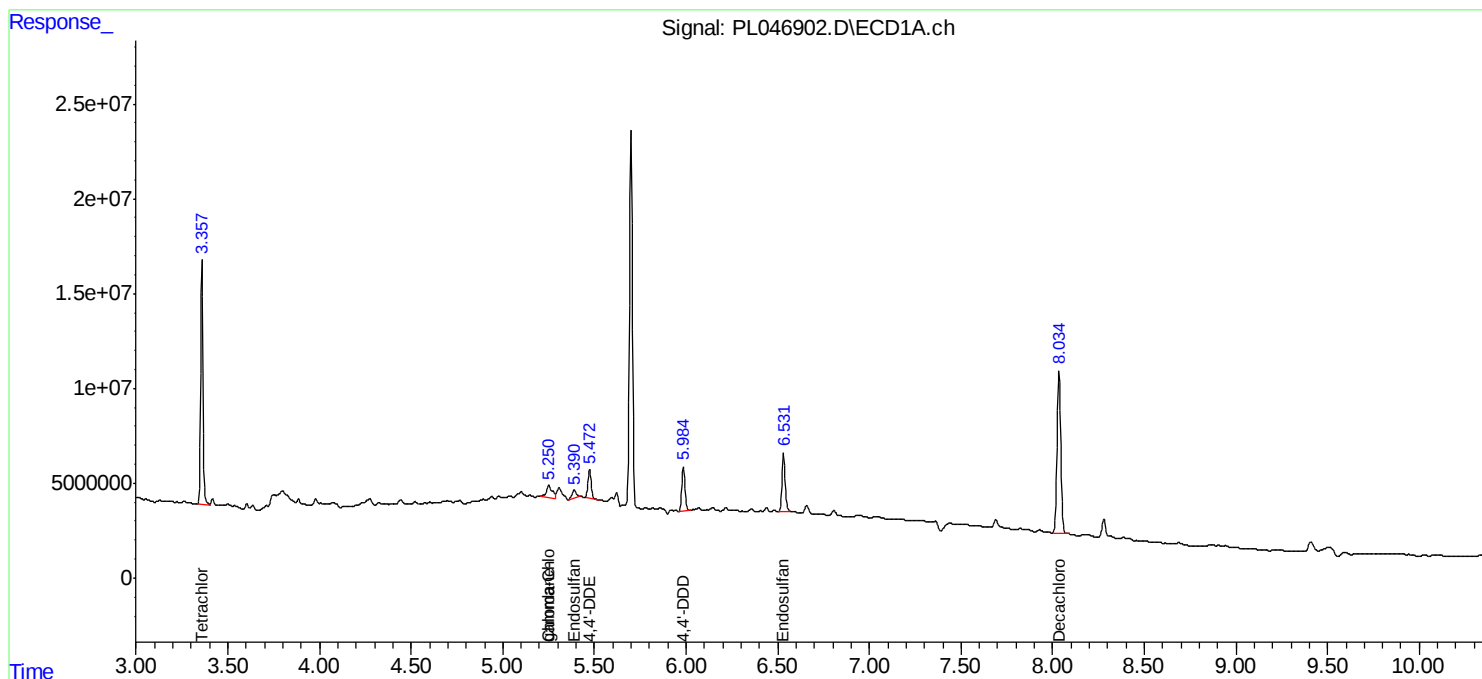


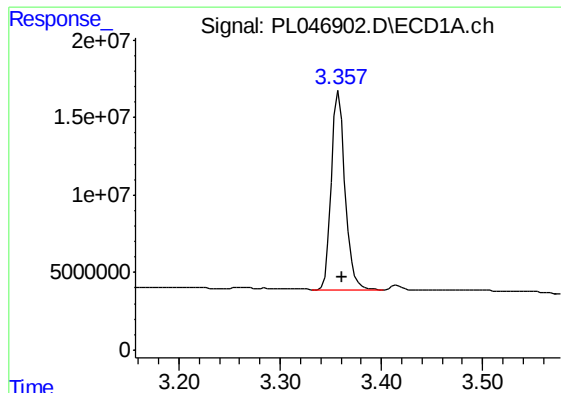

#1 Tetrachloro-m-xylene


R.T.: 3.358 min
Delta R.T.: -0.003 min
Response: 121010170
Conc: 16.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
DPC-91723-SO-TP5-B

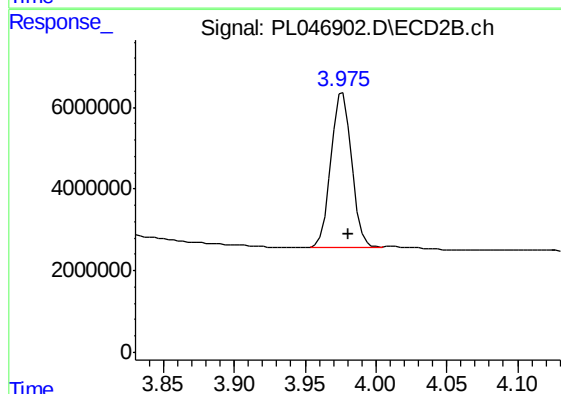


#1 Tetrachloro-m-xylene

R.T.: 3.977 min
Delta R.T.: -0.004 min
Response: 38702784
Conc: 16.90 ng/ml

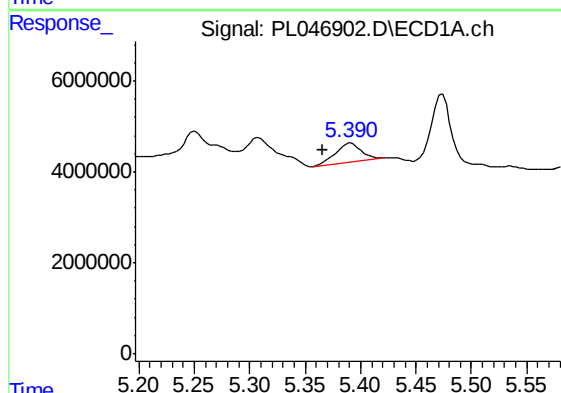


#9 Endosulfan I

R.T.: 5.391 min
Delta R.T.: 0.025 min
Response: 6571190
Conc: 0.70 ng/ml

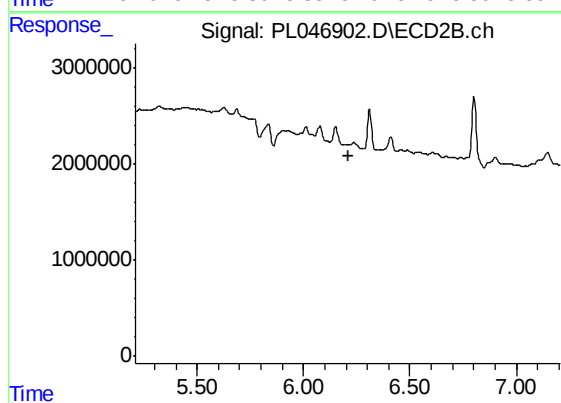

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.210 min
Response: 0
Conc: N.D.

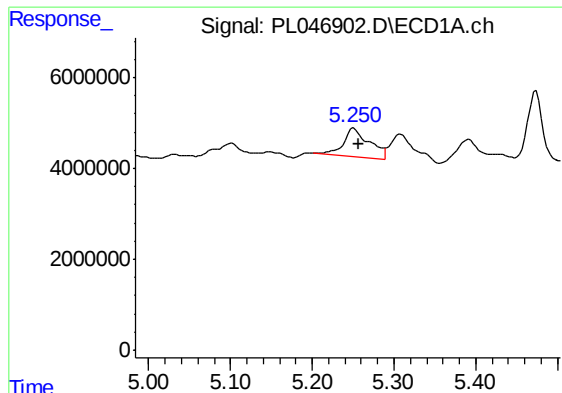

#10 gamma-Chlordane


R.T.: 5.251 min
Delta R.T.: -0.006 min
Response: 13334100
Conc: 1.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
DPC-91723-SO-TP5-B

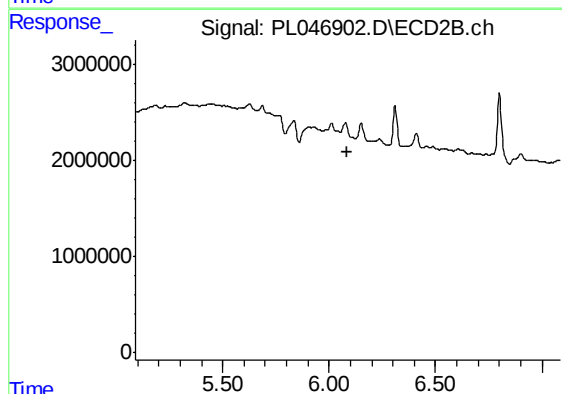


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.088 min
Response: 0
Conc: N.D.

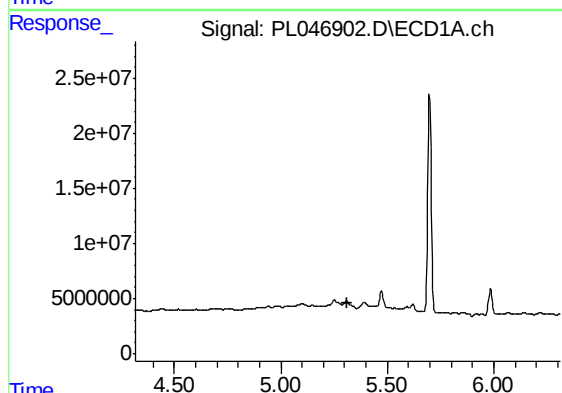


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.314 min
Response: 0
Conc: N.D.

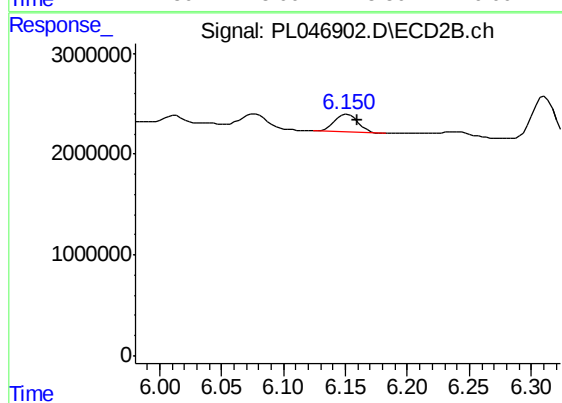

#11 alpha-Chlordane


R.T.: 6.152 min
Delta R.T.: -0.009 min
Response: 2425994
Conc: 0.86 ng/ml

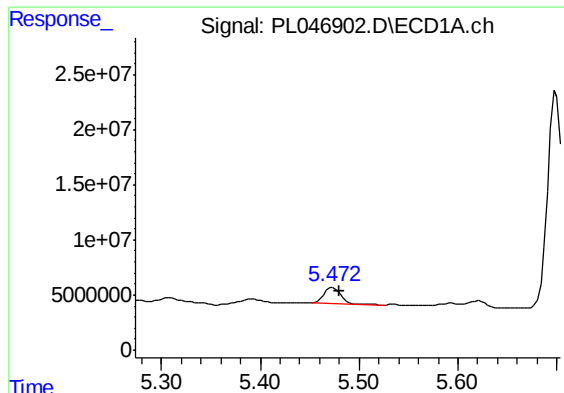

#12 4,4'-DDE


R.T.: 5.474 min
Delta R.T.: -0.007 min
Response: 18002762
Conc: 1.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
DPC-91723-SO-TP5-B

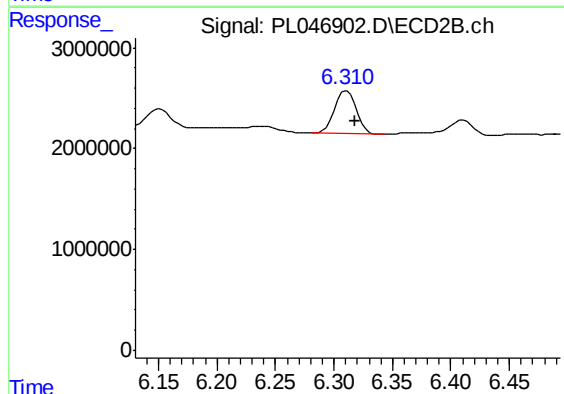


#12 4,4'-DDE

R.T.: 6.311 min
Delta R.T.: -0.007 min
Response: 5235867
Conc: 2.11 ng/ml

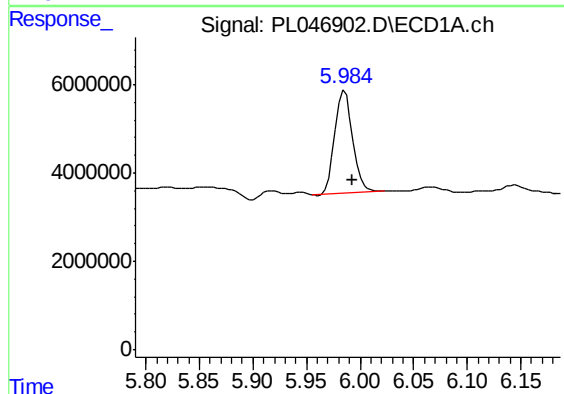


#16 4,4'-DDD

R.T.: 5.986 min
Delta R.T.: -0.007 min
Response: 26666053
Conc: 3.53 ng/ml

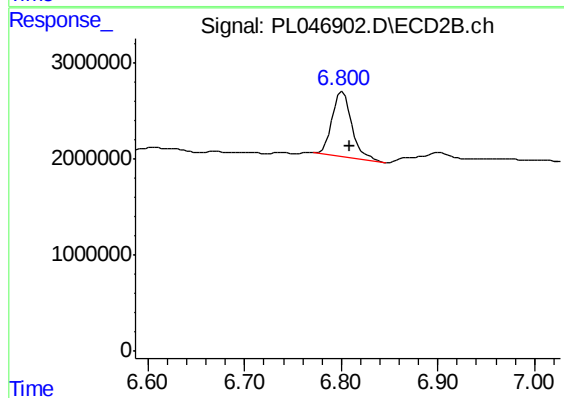

#16 4,4'-DDD


R.T.: 6.801 min
Delta R.T.: -0.007 min
Response: 9429670
Conc: 4.69 ng/ml

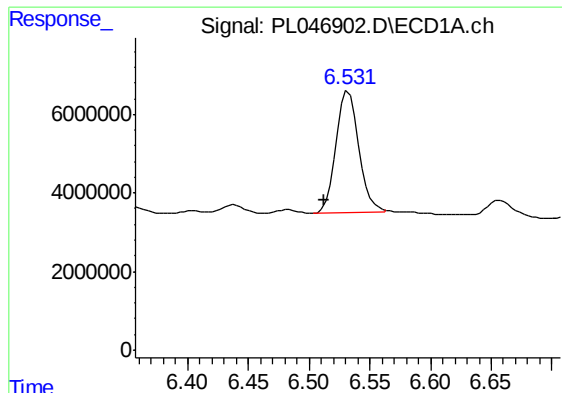

#19 Endosulfan Sulfate


R.T.: 6.532 min
Delta R.T.: 0.020 min
Response: 40416205
Conc: 4.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
DPC-91723-SO-TP5-B

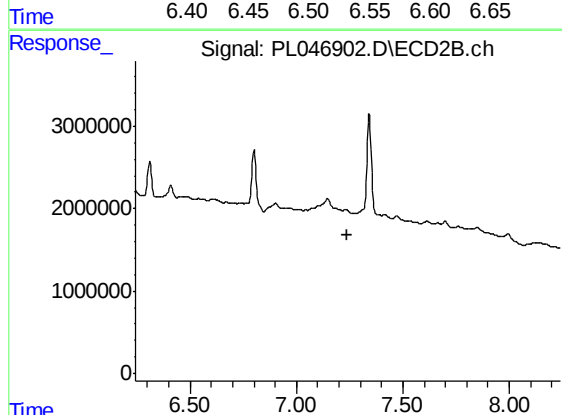


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.242 min
Response: 0
Conc: N.D.

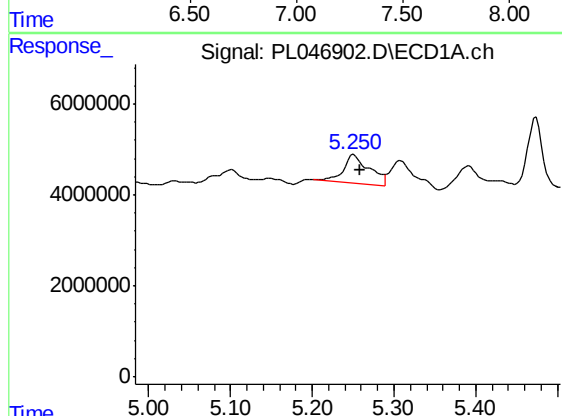


#25 Chlordane-3

R.T.: 5.251 min
Delta R.T.: -0.007 min
Response: 13334100
Conc: 11.97 ng/ml

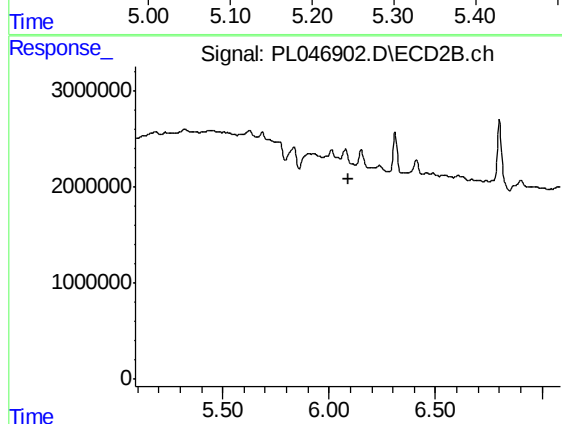

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.089 min
Response: 0
Conc: N.D.

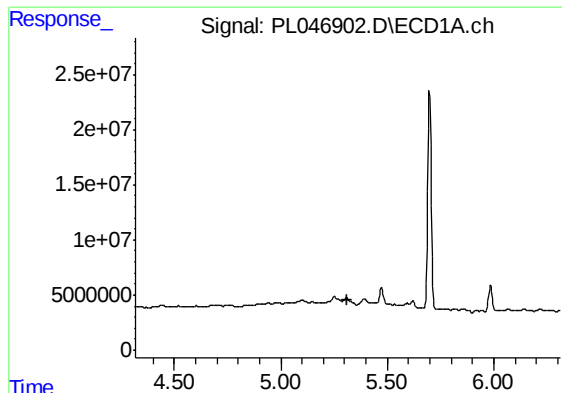

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.314 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
DPC-91723-SO-TP5-B

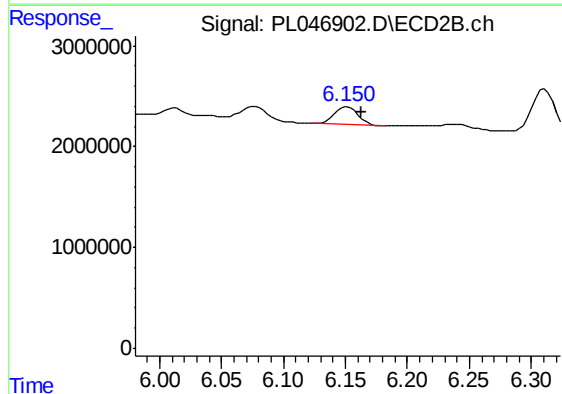


#26 Chlordane-4

R.T.: 6.152 min
Delta R.T.: -0.012 min
Response: 2425994
Conc: 5.26 ng/ml

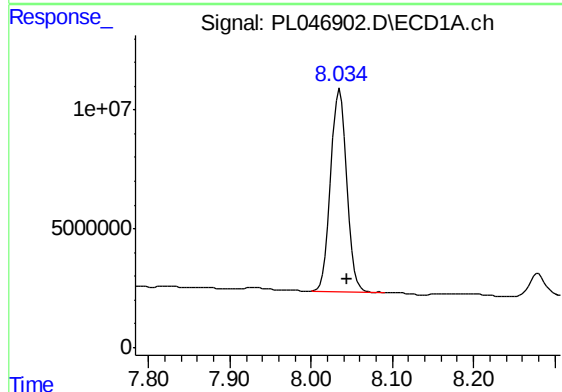

#28 Decachlorobiphenyl

R.T.: 8.035 min
Delta R.T.: -0.009 min
Response: 116458967
Conc: 13.85 ng/ml

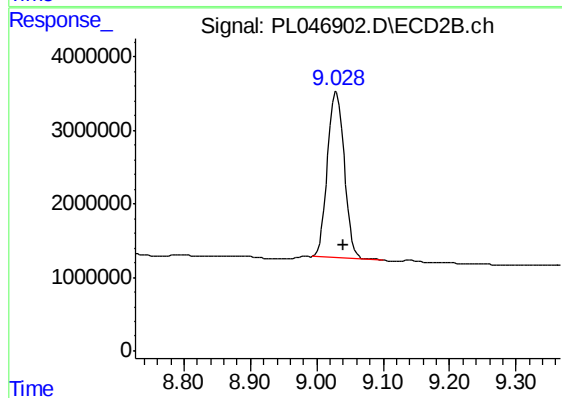

#28 Decachlorobiphenyl

R.T.: 9.030 min
Delta R.T.: -0.010 min
Response: 40159607
Conc: 17.32 ng/ml