

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040220\
 Data File : PL057728.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Apr 2020 11:19
 Operator : AJ\MA
 Sample : PB127936BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB127936BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 00:55:20 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031420.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 16 09:40:37 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.461	3.957	231.5E6	48232840	24.974	22.232
28)	SA Decachlor...	8.209	8.982	211.9E6	45838221	20.025	20.672
Target Compounds							
2)	A alpha-BHC	3.896	0.000	11758939	0	0.738	N.D. #
4)	MA Heptachlor	0.000	5.139	0	3314360	N.D.	1.053 #
8)	B Heptachlo...	5.179	5.814	2340243	19998466	0.183	7.329 #
9)	A Endosulfan I	5.517	0.000	823798	0	0.069	N.D. #
14)	MA Endrin	6.014	0.000	2980425	0	0.261	N.D. #
15)	B Endosulfa...	6.254f	0.000	4679922	0	0.431	N.D. #
17)	MA 4,4'-DDT	6.360f	0.000	1198089	0	0.120	N.D. #
18)	B Endrin al...	6.450	0.000	127960	0	0.014	N.D. #
20)	A Methoxychlor	6.907	0.000	416188	0	0.078	N.D. #
24)	Chlordane-2	4.838	0.000	1154200	0	3.176	N.D. #
27)	Chlordane-5	6.315f	0.000	638759	0	1.756	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040220\
Data File : PL057728.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Apr 2020 11:19
Operator : AJ\MA
Sample : PB127936BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB127936BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 00:55:20 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031420.M
Quant Title : GC Extractables
QLast Update : Mon Mar 16 09:40:37 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

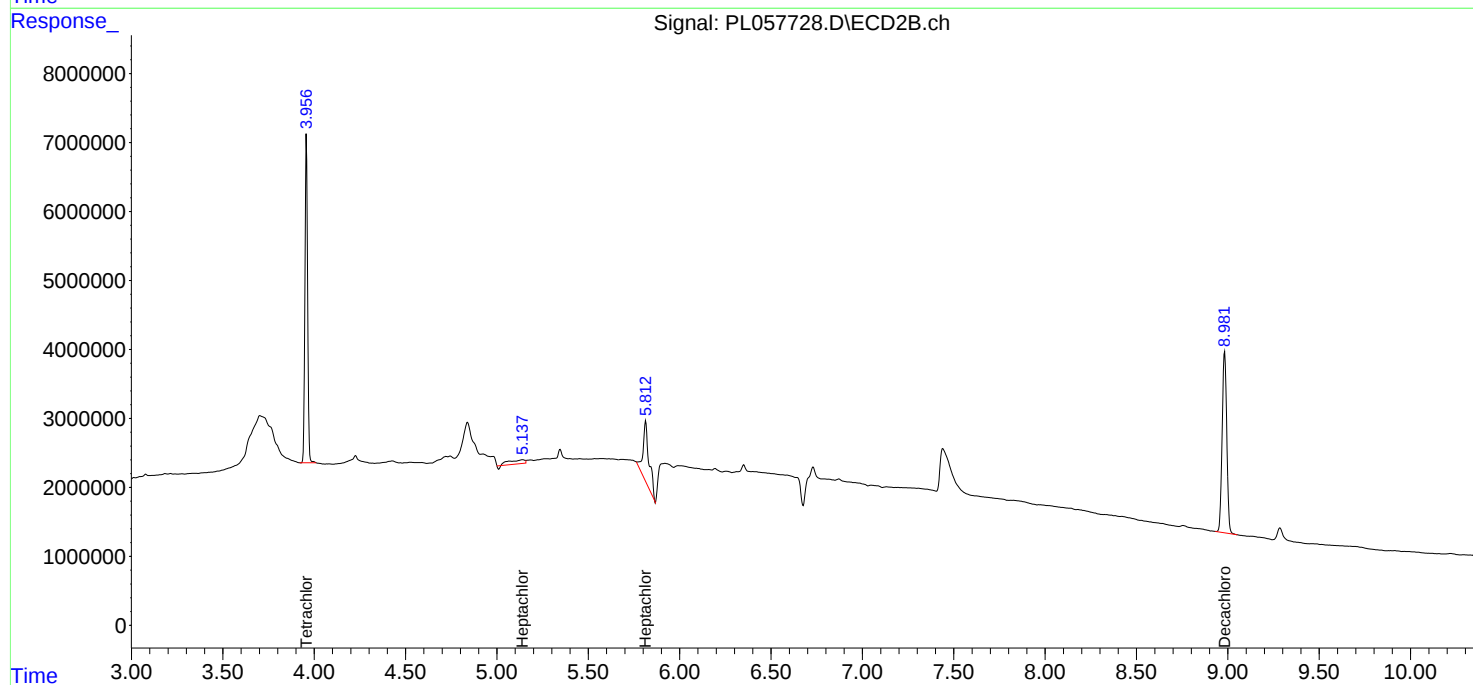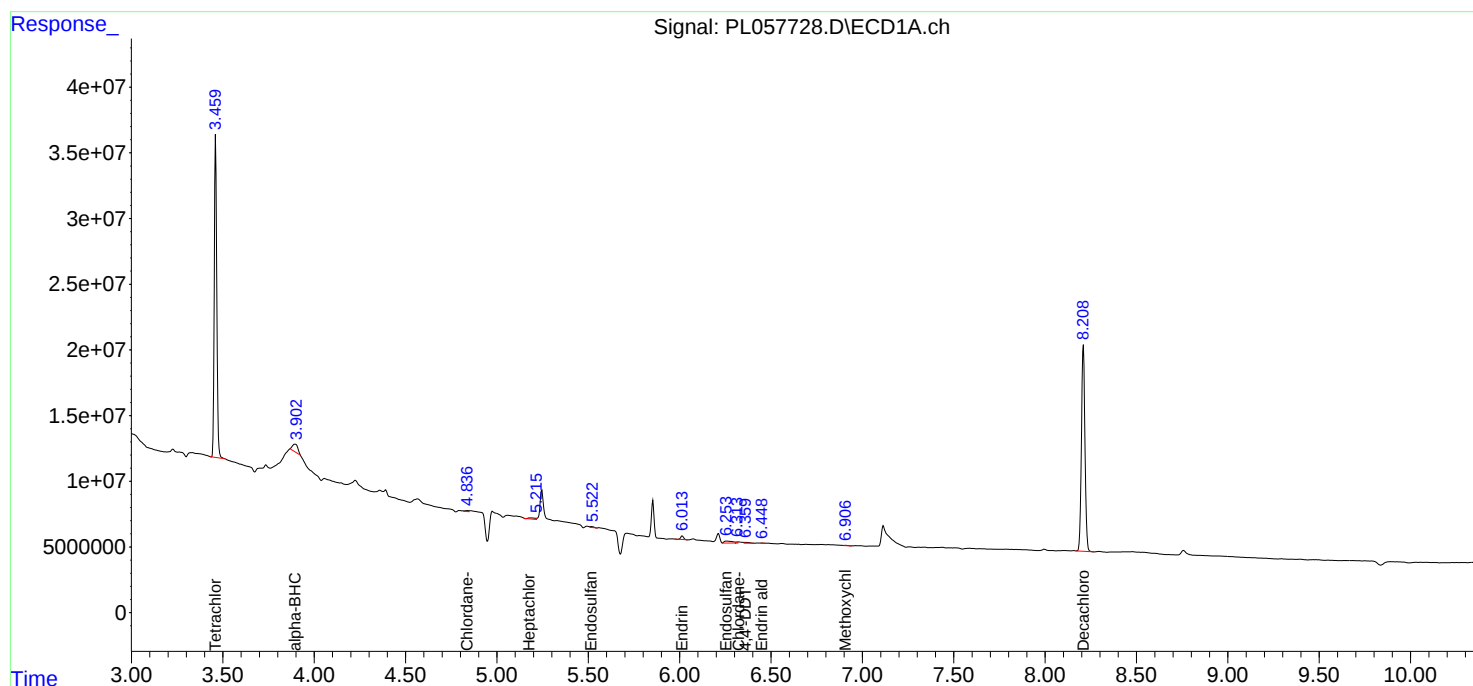


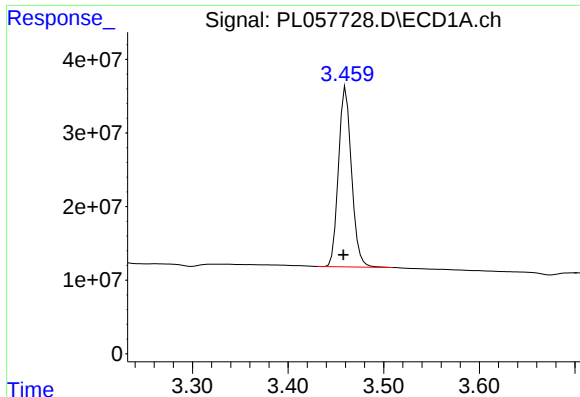

#1 Tetrachloro-m-xylene


R.T.: 3.461 min
Delta R.T.: 0.003 min
Response: 231491803
Conc: 24.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB127936BL

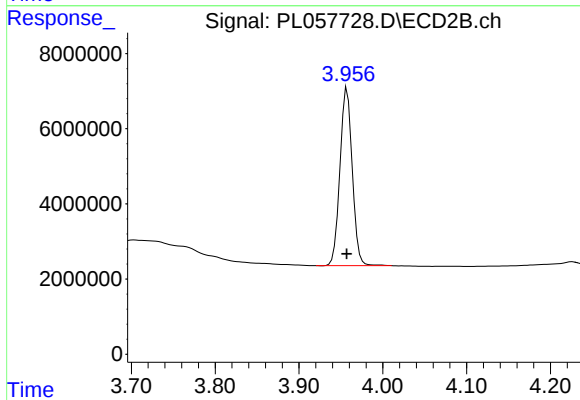


#1 Tetrachloro-m-xylene

R.T.: 3.957 min
Delta R.T.: 0.000 min
Response: 48232840
Conc: 22.23 ng/ml

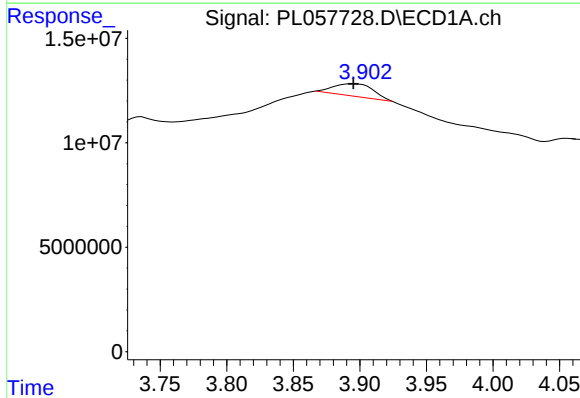


#2 alpha-BHC

R.T.: 3.896 min
Delta R.T.: 0.000 min
Response: 11758939
Conc: 0.74 ng/ml

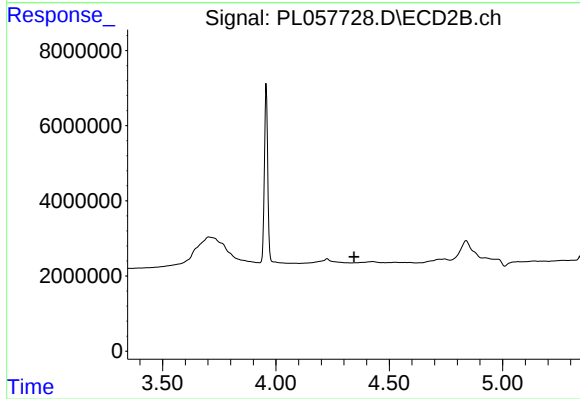

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.345 min
Response: 0
Conc: N.D.

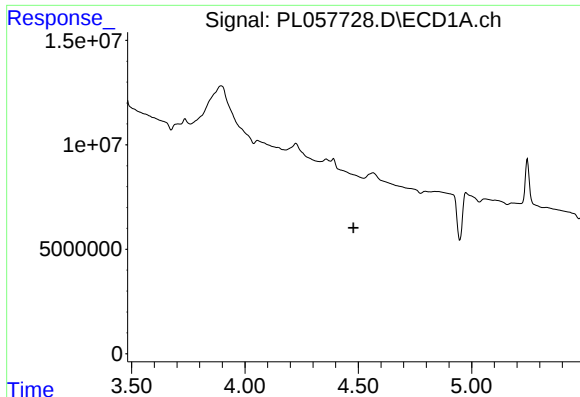

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.479 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB127936BL

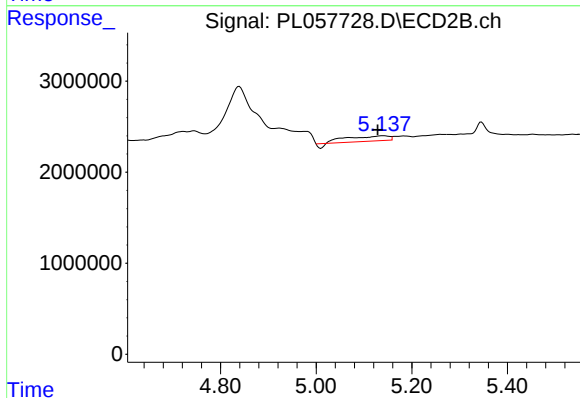


#4 Heptachlor

R.T.: 5.139 min
Delta R.T.: 0.010 min
Response: 3314360
Conc: 1.05 ng/ml

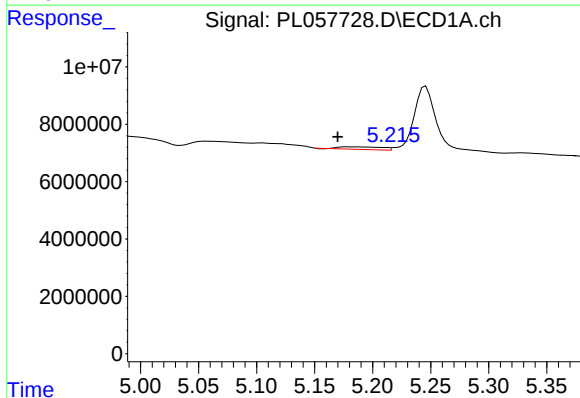


#8 Heptachlor epoxide

R.T.: 5.179 min
Delta R.T.: 0.009 min
Response: 2340243
Conc: 0.18 ng/ml

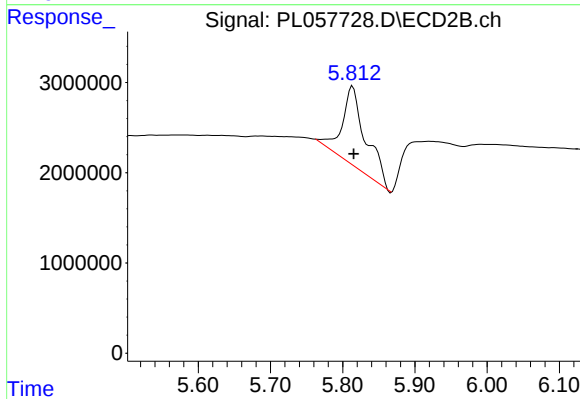

#8 Heptachlor epoxide


R.T.: 5.814 min
Delta R.T.: -0.002 min
Response: 19998466
Conc: 7.33 ng/ml

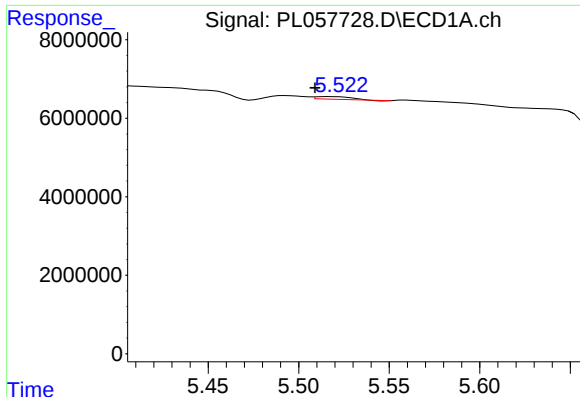

#9 Endosulfan I


R.T.: 5.517 min
Delta R.T.: 0.008 min
Response: 823798
Conc: 0.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB127936BL

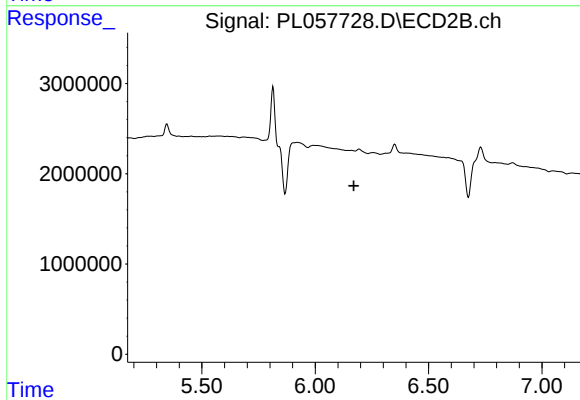


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.170 min
Response: 0
Conc: N.D.

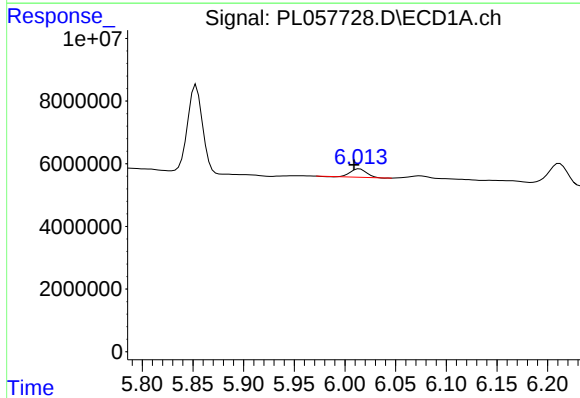


#14 Endrin

R.T.: 6.014 min
Delta R.T.: 0.005 min
Response: 2980425
Conc: 0.26 ng/ml

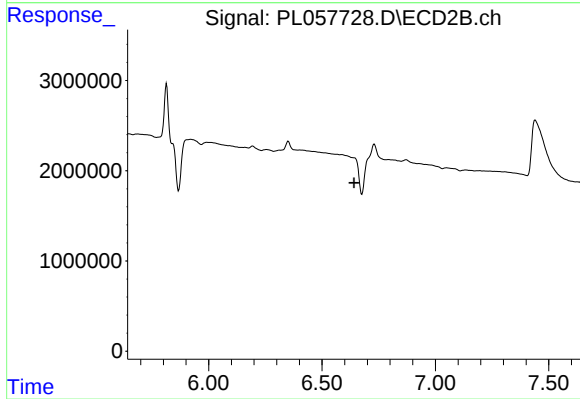

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.642 min
Response: 0
Conc: N.D.

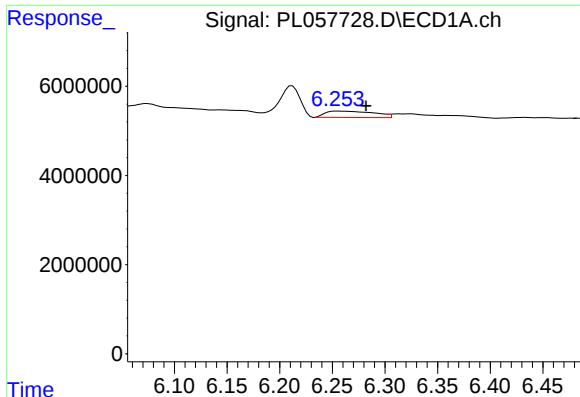

#15 Endosulfan II


R.T.: 6.254 min
Delta R.T.: -0.028 min
Response: 4679922
Conc: 0.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB127936BL

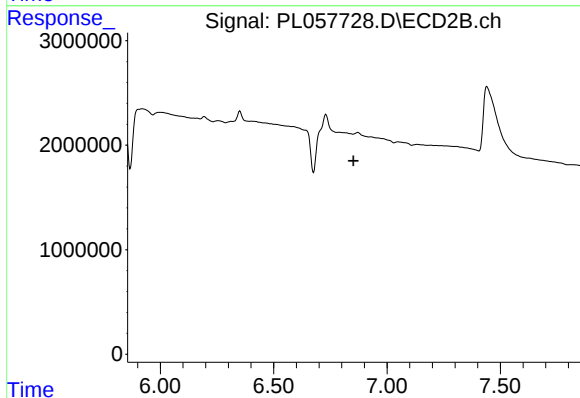


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.852 min
Response: 0
Conc: N.D.

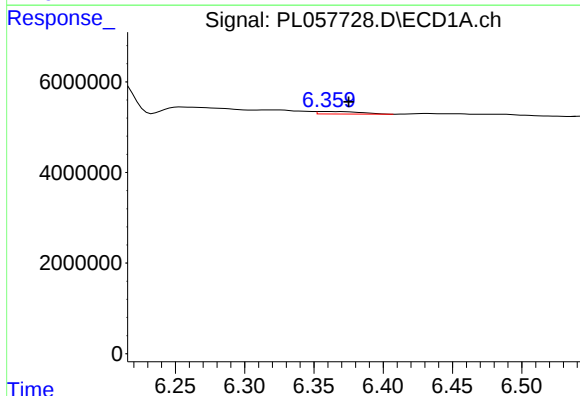


#17 4,4'-DDT

R.T.: 6.360 min
Delta R.T.: -0.015 min
Response: 1198089
Conc: 0.12 ng/ml

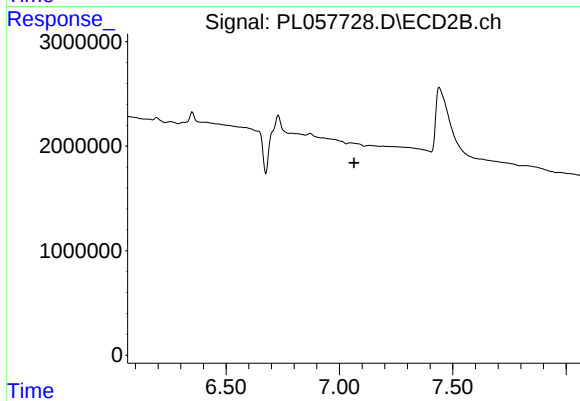

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 7.065 min
Response: 0
Conc: N.D.

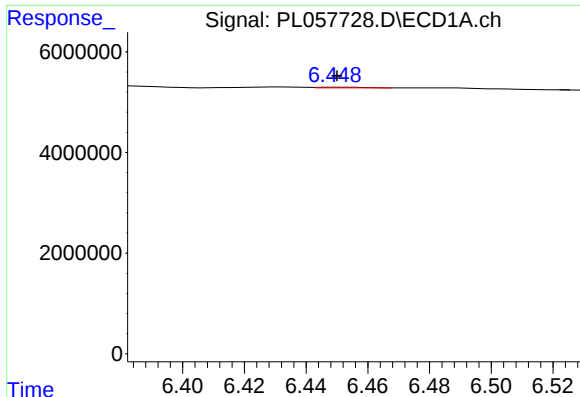

#18 Endrin aldehyde


R.T.: 6.450 min
Delta R.T.: 0.000 min
Response: 127960
Conc: 0.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB127936BL

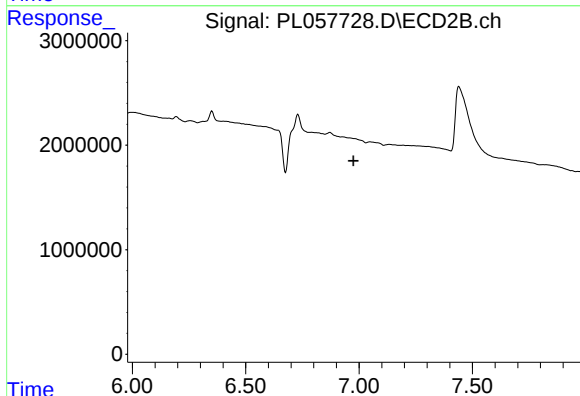


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.976 min
Response: 0
Conc: N.D.

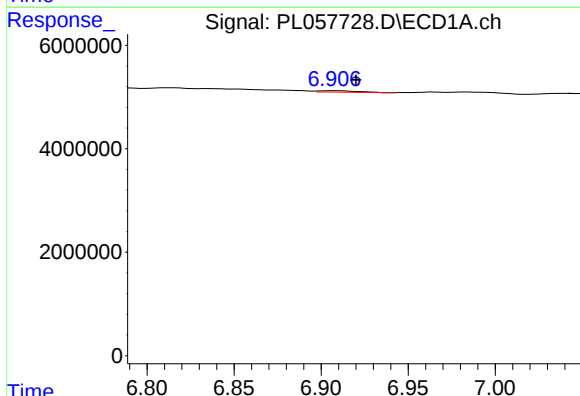


#20 Methoxychlor

R.T.: 6.907 min
Delta R.T.: -0.013 min
Response: 416188
Conc: 0.08 ng/ml

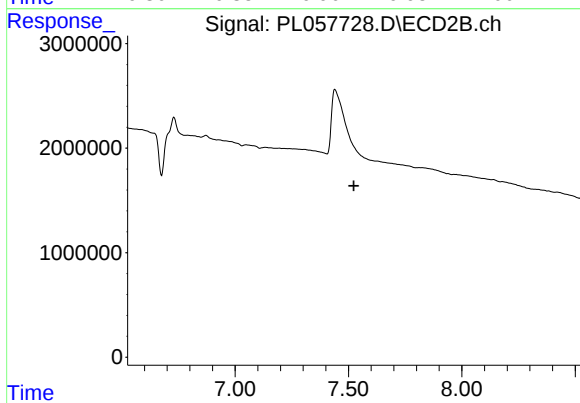

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.524 min
Response: 0
Conc: N.D.

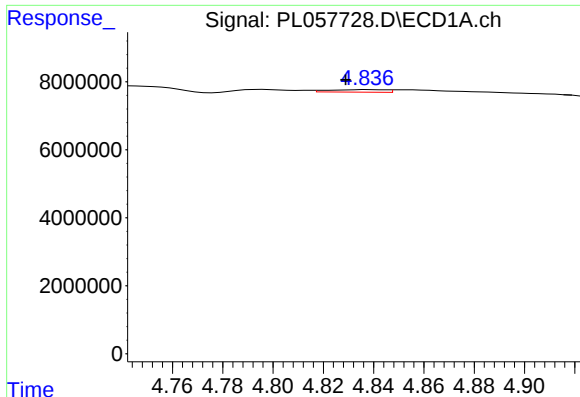

#24 Chlordane-2


R.T.: 4.838 min
Delta R.T.: 0.009 min
Response: 1154200
Conc: 3.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB127936BL

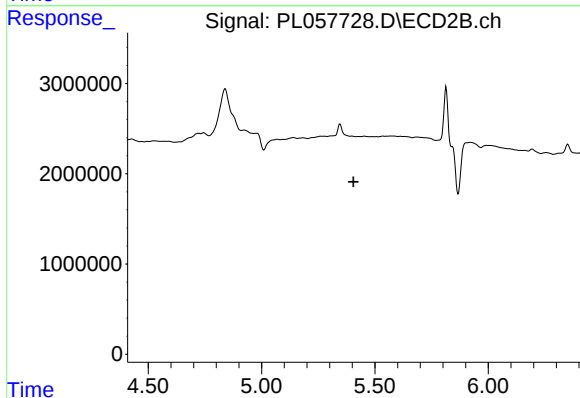


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.406 min
Response: 0
Conc: N.D.

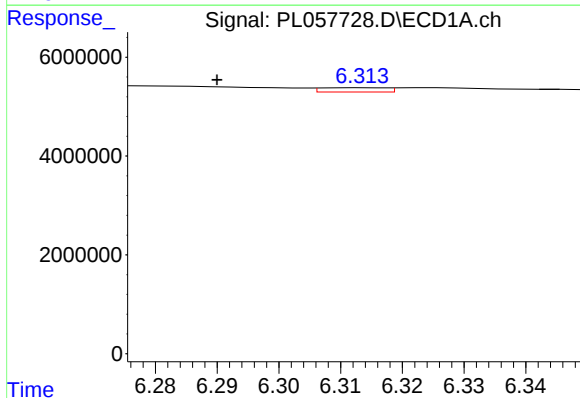


#27 Chlordane-5

R.T.: 6.315 min
Delta R.T.: 0.025 min
Response: 638759
Conc: 1.76 ng/ml

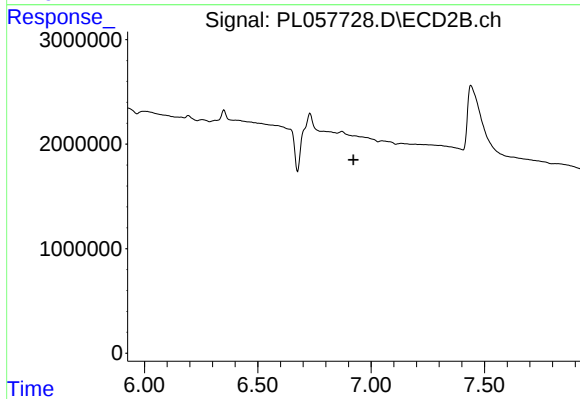

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 6.922 min
Response: 0
Conc: N.D.

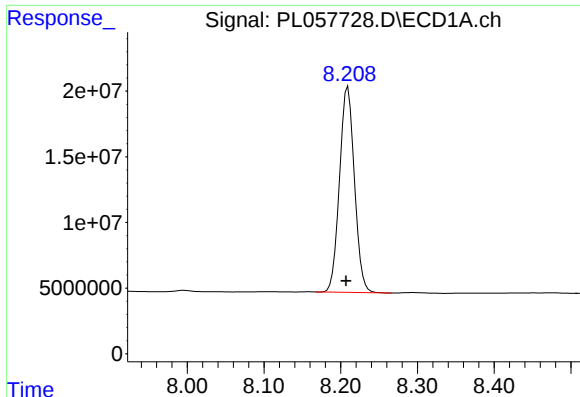

#28 Decachlorobiphenyl

R.T.: 8.209 min
Delta R.T.: 0.002 min
Response: 211894650
Conc: 20.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB127936BL

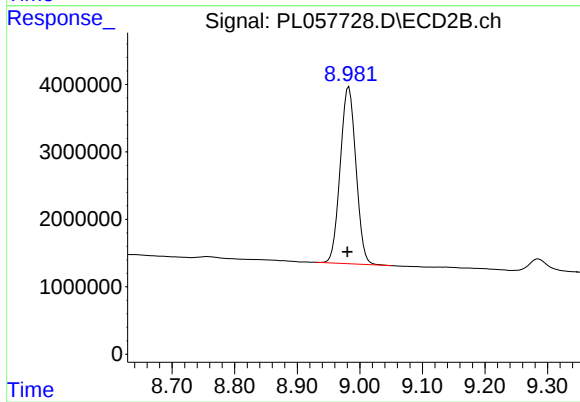

#28 Decachlorobiphenyl

R.T.: 8.982 min
Delta R.T.: 0.002 min
Response: 45838221
Conc: 20.67 ng/ml