

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040220\
 Data File : PL057743.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Apr 2020 18:09
 Operator : AJ\MA
 Sample : L2104-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BUS-WASH

Manual Integrations
 APPROVED

mohammad
 4/6/2020 1:29:45 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 01:00:00 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031420.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 16 09:40:37 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.457	3.955	88229105	22876416	9.518m	10.544m
28) SA Decachlor...	8.208	8.981	87651096	23019332	8.284	10.381m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040220\
Data File : PL057743.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Apr 2020 18:09
Operator : AJ\MA
Sample : L2104-02
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
BUS-WASH


Manual Integrations
APPROVED

mohammad
4/6/2020 1:29:45 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 01:00:00 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031420.M
Quant Title : GC Extractables
QLast Update : Mon Mar 16 09:40:37 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

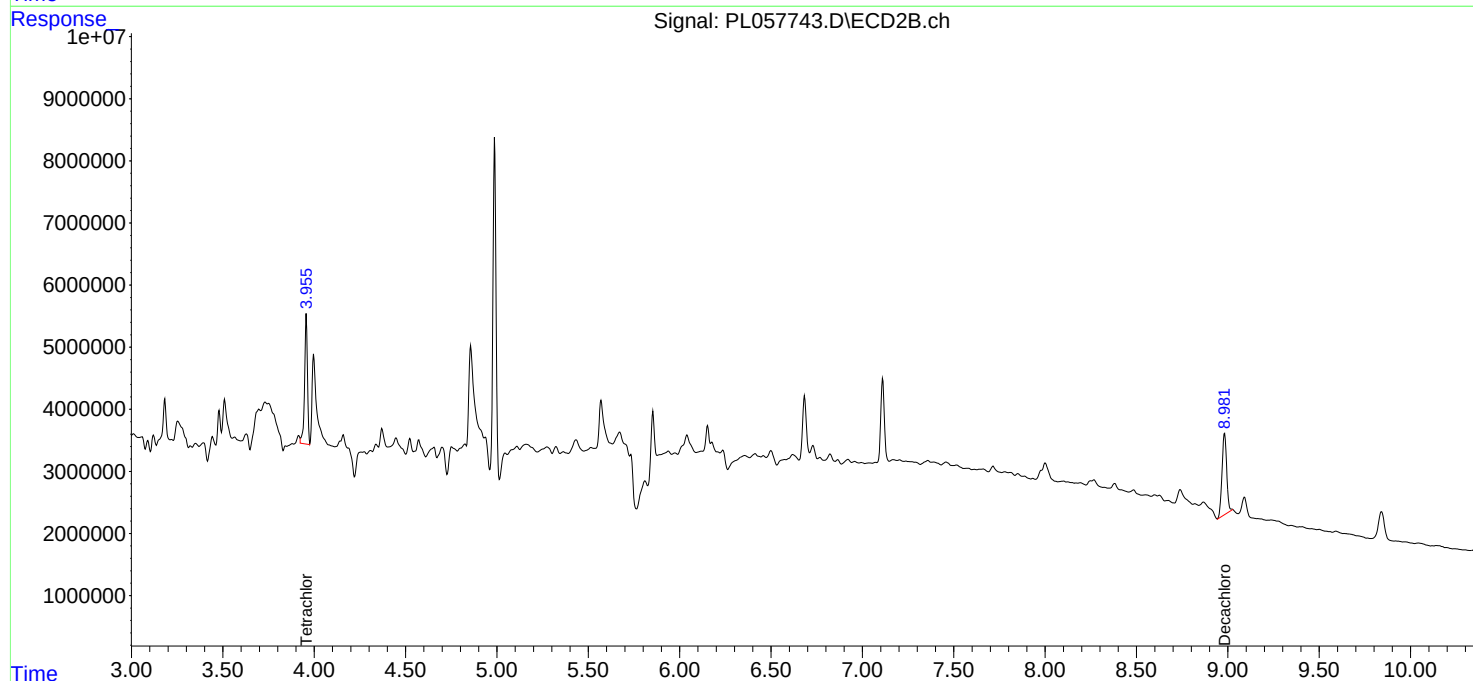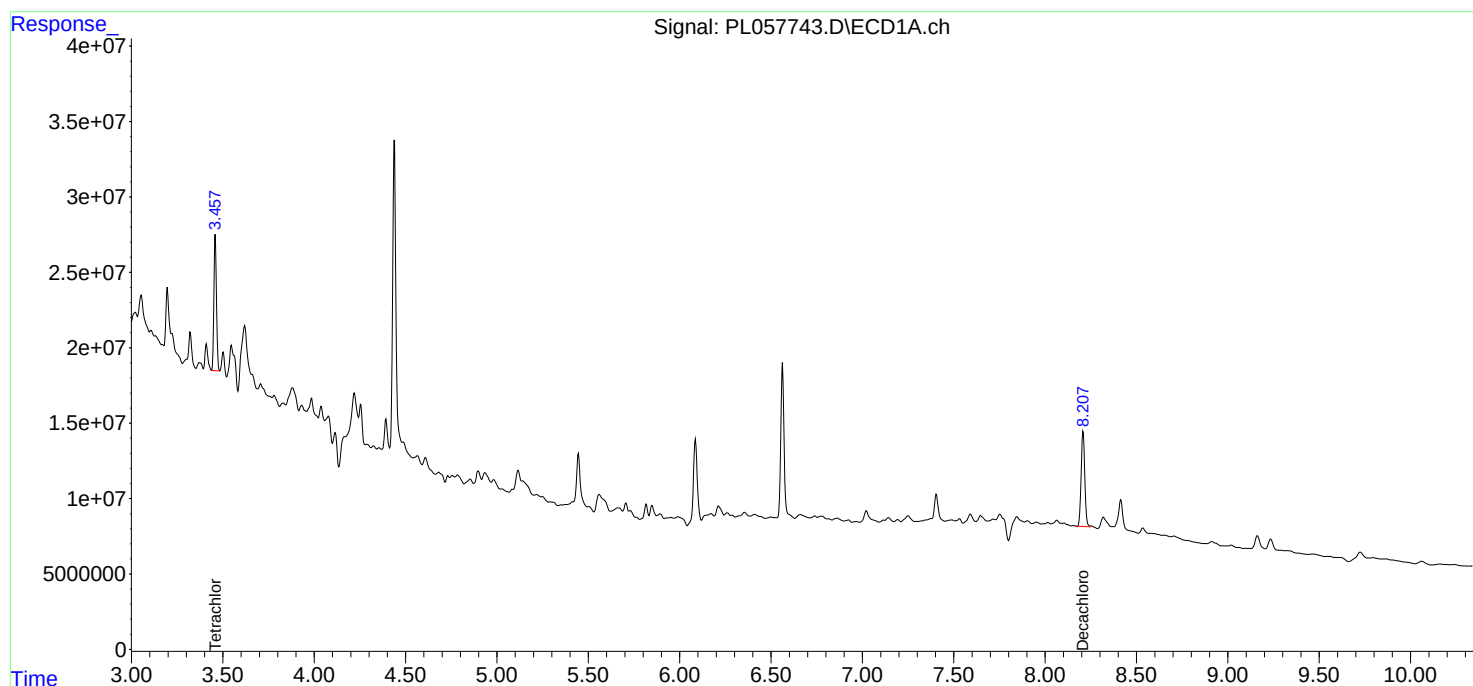

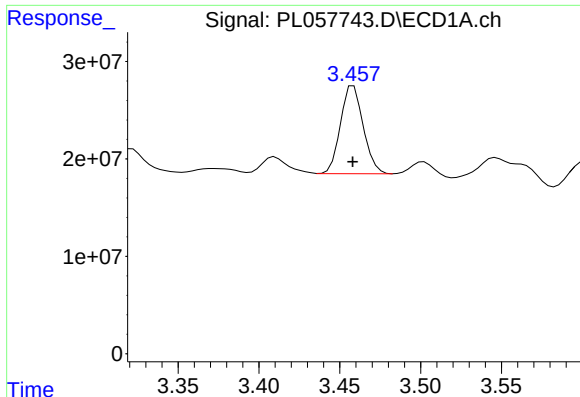


#1 Tetrachloro-m-xylene

R.T.: 3.457 min
Delta R.T.: 0.000 min
Response: 88229105
Conc: 9.52 ng/ml m

Instrument :
ECD_L
ClientSampleId :
BUS-WASH


Manual Integrations
APPROVED

mohammad
4/6/2020 1:29:45 PM

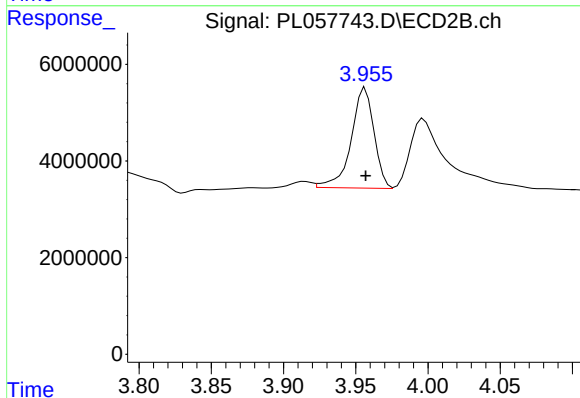


#1 Tetrachloro-m-xylene

R.T.: 3.955 min
Delta R.T.: -0.002 min
Response: 22876416
Conc: 10.54 ng/ml m

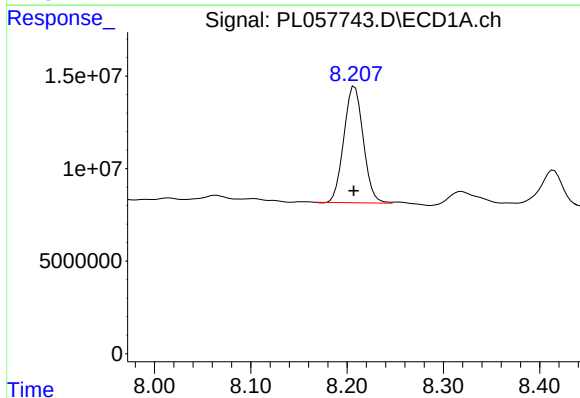

#28 Decachlorobiphenyl

R.T.: 8.208 min
Delta R.T.: 0.000 min
Response: 87651096
Conc: 8.28 ng/ml

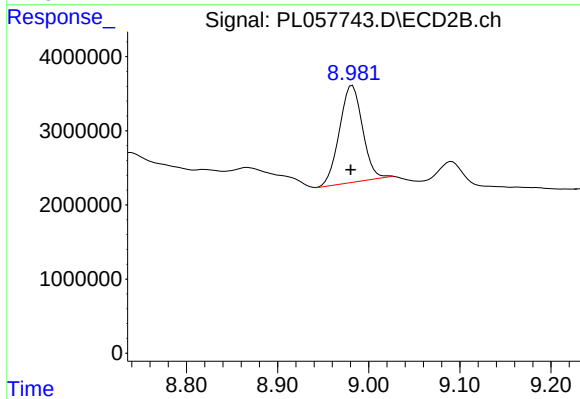

#28 Decachlorobiphenyl

R.T.: 8.981 min
Delta R.T.: 0.000 min
Response: 23019332
Conc: 10.38 ng/ml m