

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040221\
 Data File : PL065817.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Apr 2021 10:19
 Operator : AR\AJ
 Sample : PB135375BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB135375BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 04:52:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 31 15:57:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.278	3.780	52981026	55792443	20.338	20.325
28)	SA Decachlor...	7.911	8.727	50896723	47205140	21.976	20.938
Target Compounds							
5)	MB Aldrin	0.000	5.225	0	152723	N.D.	0.046 #
6)	B beta-BHC	0.000	4.628	0	3181762	N.D.	1.827 #
8)	B Heptachlo...	0.000	5.614	0	7418019	N.D.	2.389 #
9)	A Endosulfan I	0.000	5.993f	0	660011	N.D.	0.240 #
14)	MA Endrin	5.754	0.000	1636317	0	0.606	N.D. #
15)	B Endosulfa...	0.000	6.676f	0	273072	N.D.	0.116 #
18)	B Endrin al...	6.190	6.801f	152568	127549	0.081	0.067
23)	Chlordane-1	4.126	0.000	1189214	0	13.180	N.D. #
24)	Chlordane-2	0.000	5.225f	0	152723	N.D.	1.335 #
27)	Chlordane-5	0.000	6.736f	0	94100	N.D.	1.129 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040221\
Data File : PL065817.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Apr 2021 10:19
Operator : AR\AJ
Sample : PB135375BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB135375BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 04:52:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
Quant Title : GC Extractables
QLast Update : Wed Mar 31 15:57:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

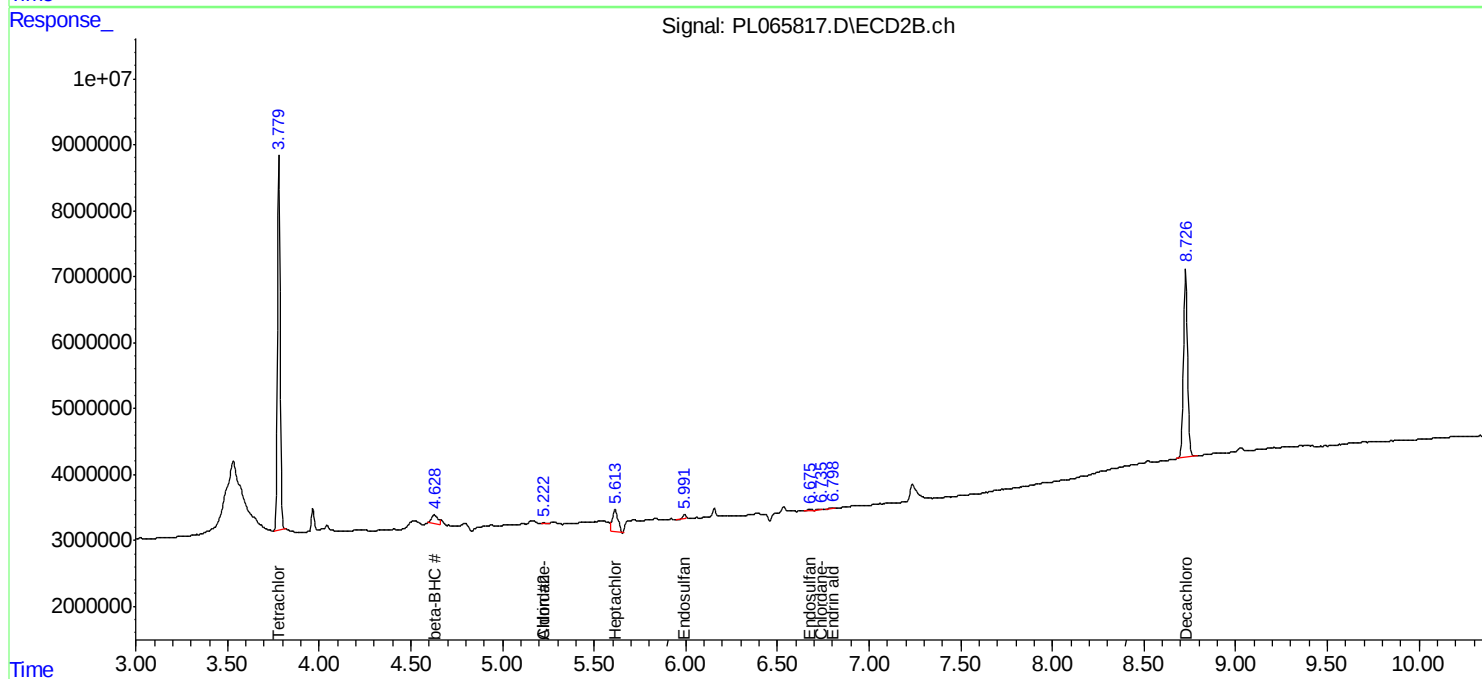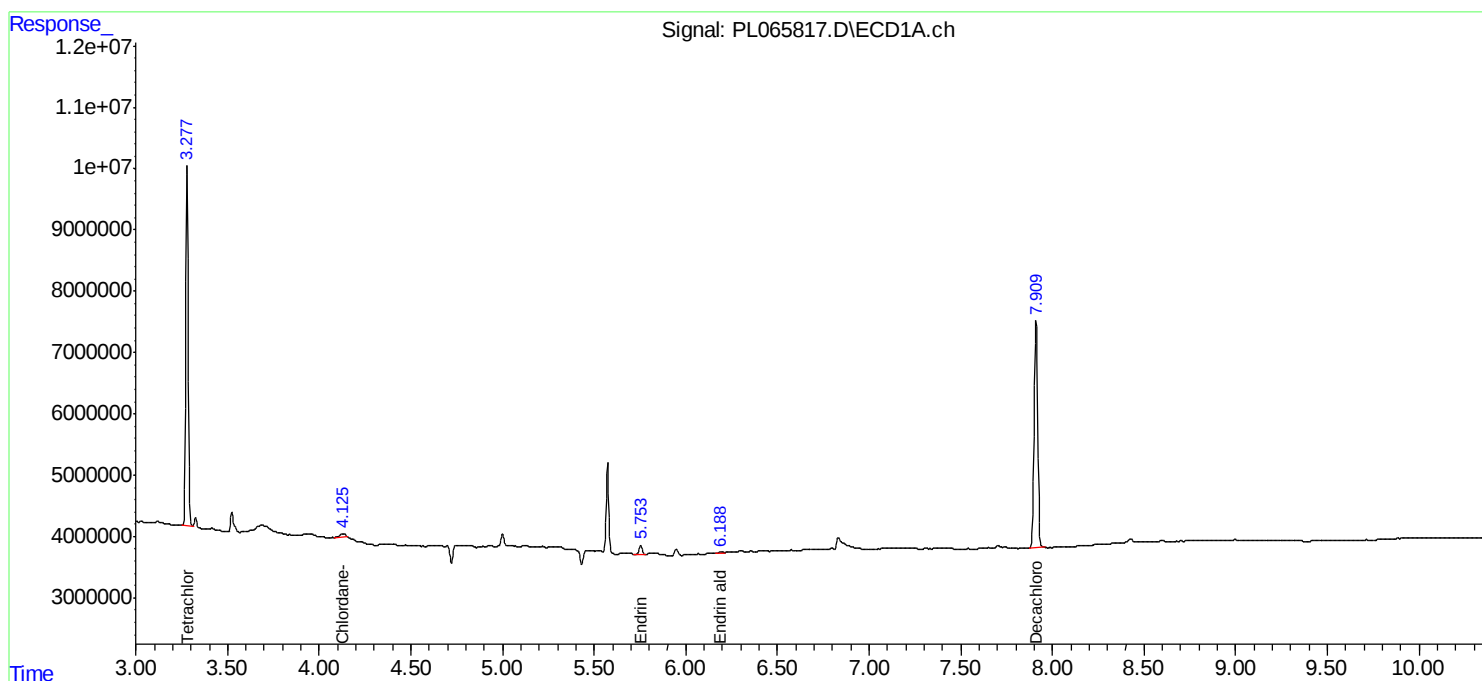


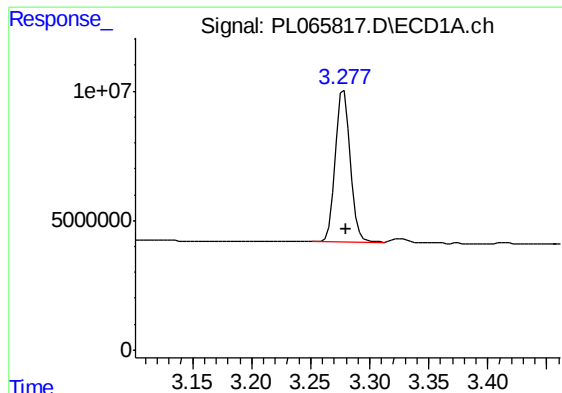

#1 Tetrachloro-m-xylene


R.T.: 3.278 min
Delta R.T.: -0.002 min
Response: 52981026
Conc: 20.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB135375BL

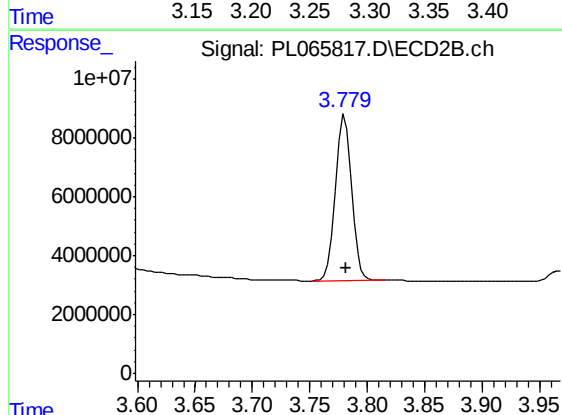


#1 Tetrachloro-m-xylene

R.T.: 3.780 min
Delta R.T.: -0.001 min
Response: 55792443
Conc: 20.33 ng/ml

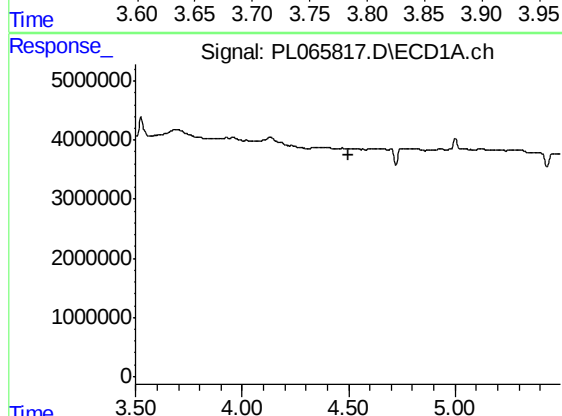


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.497 min
Response: 0
Conc: N.D.

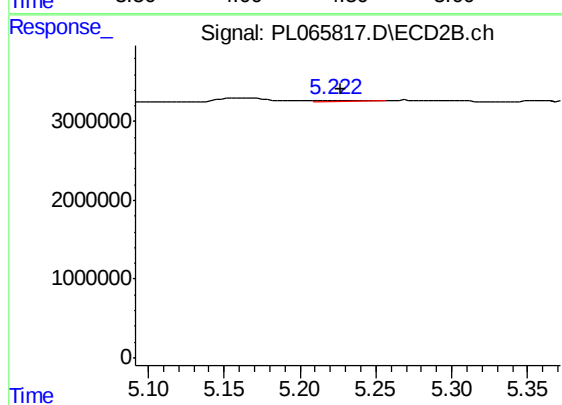

#5 Aldrin


R.T.: 5.225 min
Delta R.T.: -0.002 min
Response: 152723
Conc: 0.05 ng/ml

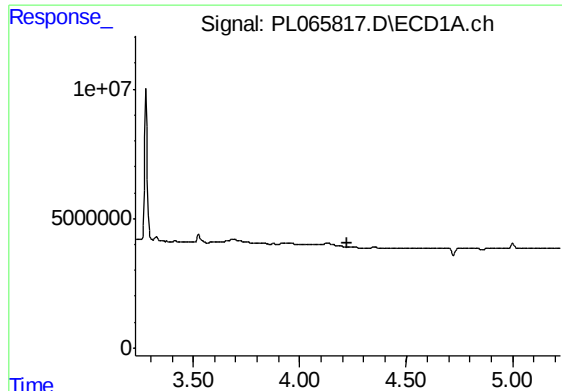

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.226 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB135375BL

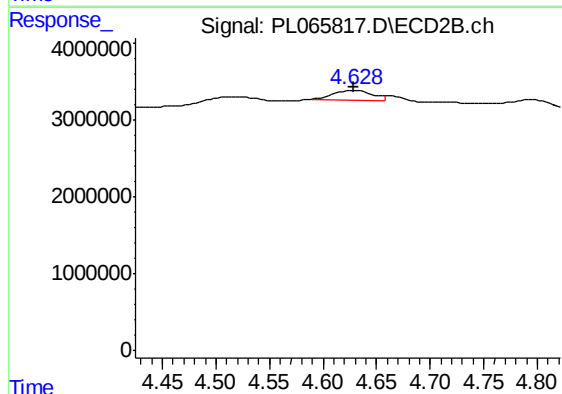


#6 beta-BHC

R.T.: 4.628 min
Delta R.T.: 0.000 min
Response: 3181762
Conc: 1.83 ng/ml

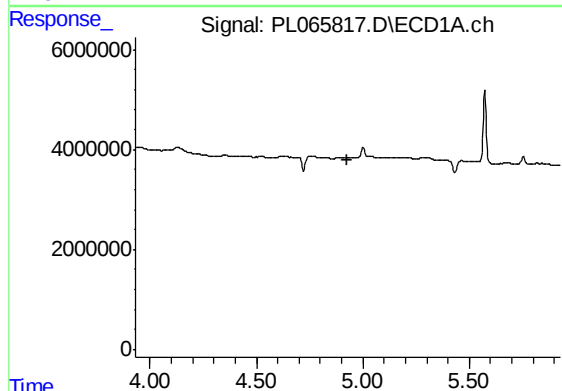


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.929 min
Response: 0
Conc: N.D.

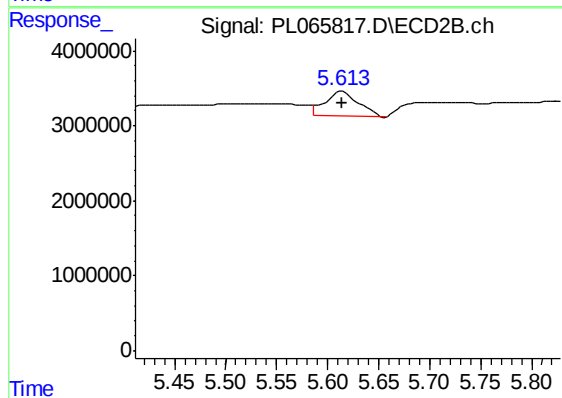

#8 Heptachlor epoxide


R.T.: 5.614 min
Delta R.T.: 0.000 min
Response: 7418019
Conc: 2.39 ng/ml

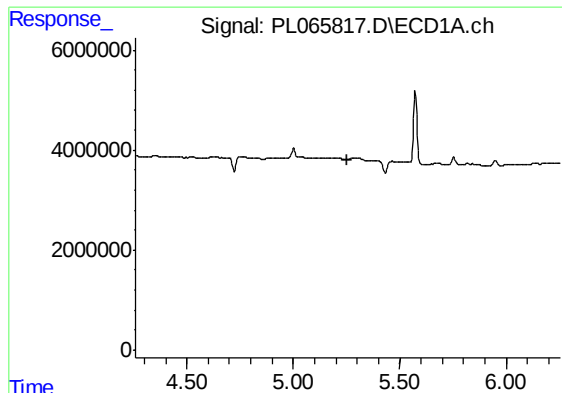

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 5.255 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB135375BL

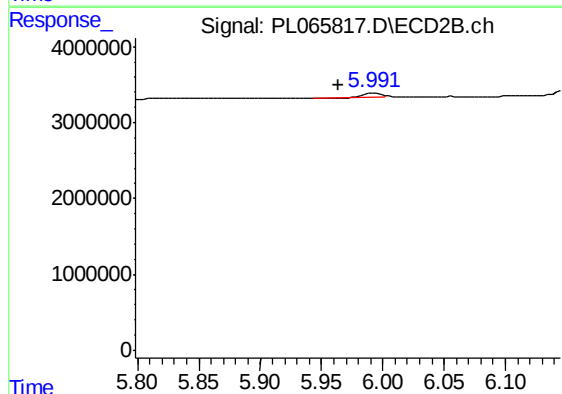


#9 Endosulfan I

R.T.: 5.993 min
Delta R.T.: 0.029 min
Response: 660011
Conc: 0.24 ng/ml

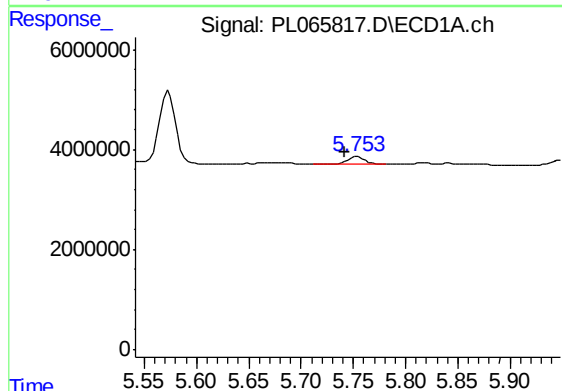


#14 Endrin

R.T.: 5.754 min
Delta R.T.: 0.012 min
Response: 1636317
Conc: 0.61 ng/ml

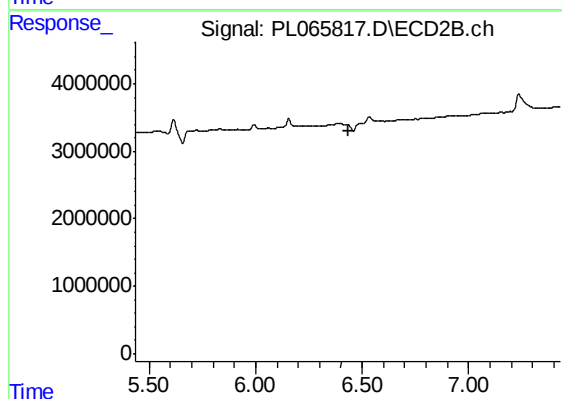

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.434 min
Response: 0
Conc: N.D.

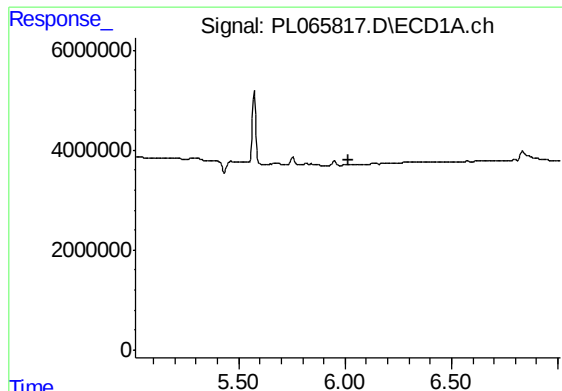

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.015 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB135375BL

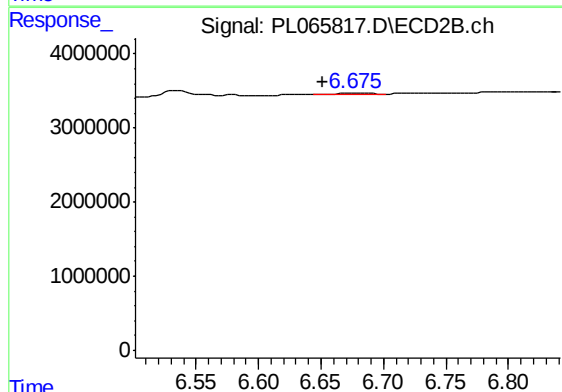


#15 Endosulfan II

R.T.: 6.676 min
Delta R.T.: 0.025 min
Response: 273072
Conc: 0.12 ng/ml

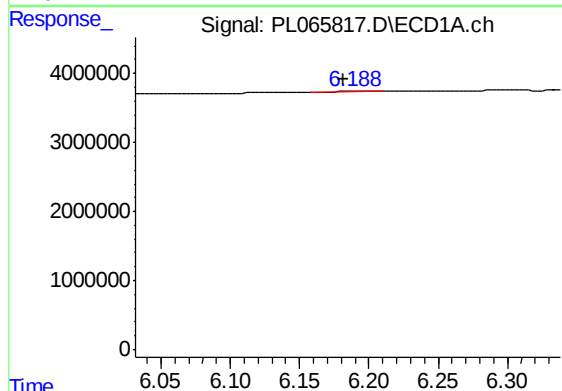


#18 Endrin aldehyde

R.T.: 6.190 min
Delta R.T.: 0.009 min
Response: 152568
Conc: 0.08 ng/ml

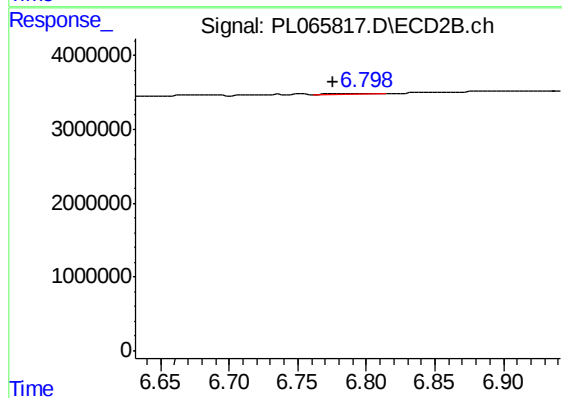

#18 Endrin aldehyde


R.T.: 6.801 min
Delta R.T.: 0.025 min
Response: 127549
Conc: 0.07 ng/ml

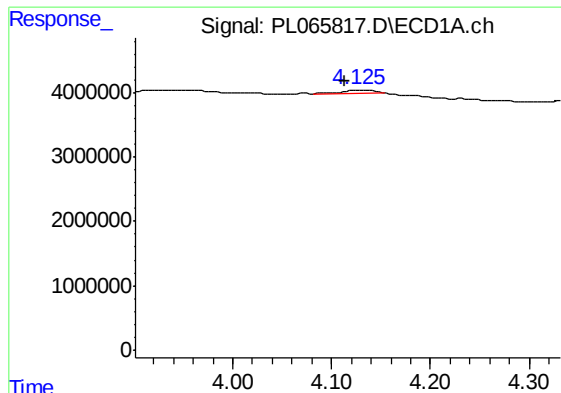

#23 Chlordane-1


R.T.: 4.126 min
Delta R.T.: 0.012 min
Response: 1189214
Conc: 13.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB135375BL

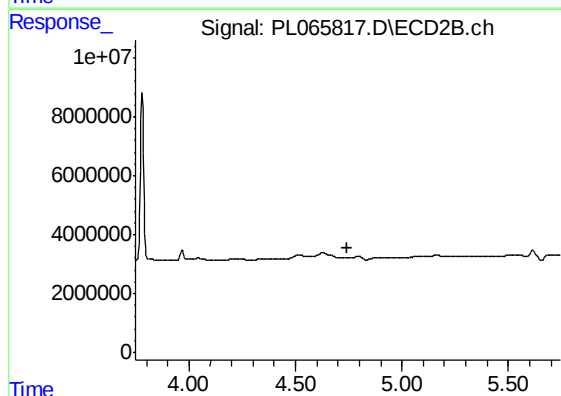


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.745 min
Response: 0
Conc: N.D.

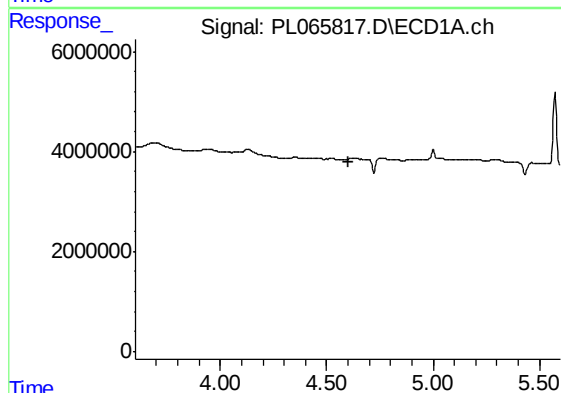


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.600 min
Response: 0
Conc: N.D.

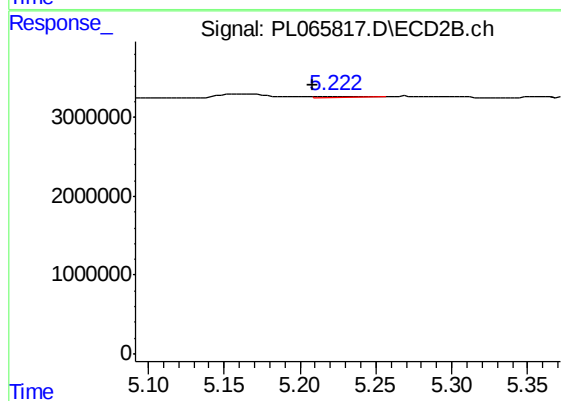

#24 Chlordane-2


R.T.: 5.225 min
Delta R.T.: 0.017 min
Response: 152723
Conc: 1.33 ng/ml

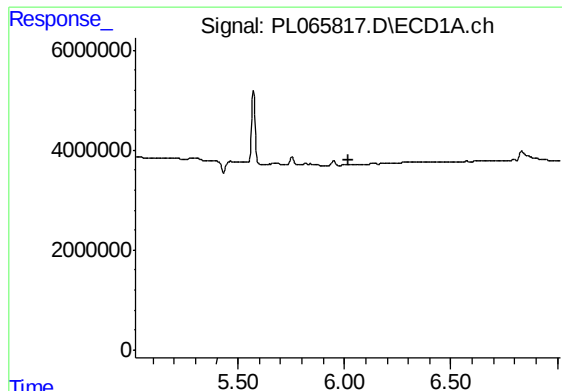

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.017 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB135375BL

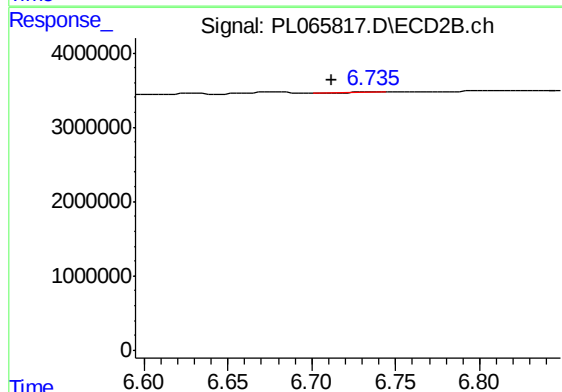


#27 Chlordane-5

R.T.: 6.736 min
Delta R.T.: 0.024 min
Response: 94100
Conc: 1.13 ng/ml

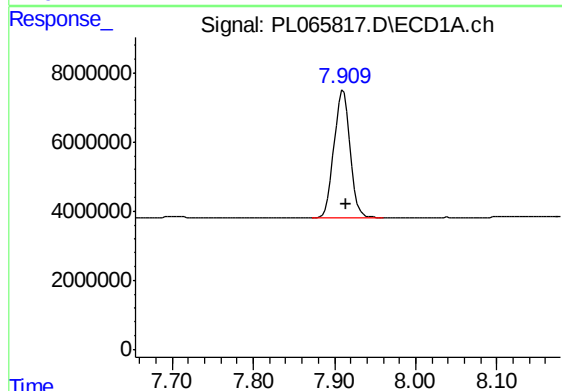

#28 Decachlorobiphenyl

R.T.: 7.911 min
Delta R.T.: -0.003 min
Response: 50896723
Conc: 21.98 ng/ml

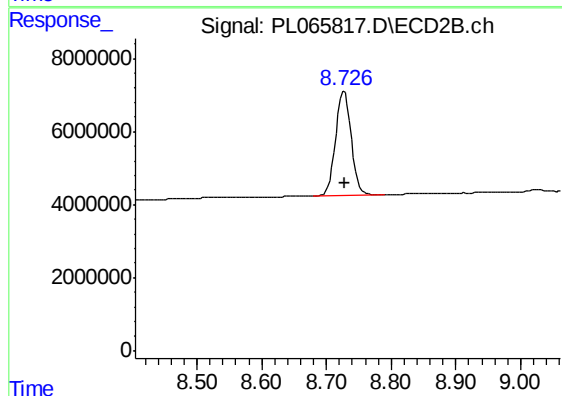

#28 Decachlorobiphenyl

R.T.: 8.727 min
Delta R.T.: 0.000 min
Response: 47205140
Conc: 20.94 ng/ml