

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040221\
 Data File : PL065851.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Apr 2021 19:35
 Operator : AR\AJ
 Sample : PB135509TB
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB135509TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 05:07:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 31 15:57:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.277	3.780	47700215	49881968	18.311	18.172
28)	SA Decachlor...	7.908	8.725	47777886	44056989	20.629	19.542
Target Compounds							
4)	MA Heptachlor	0.000	4.943	0	802257	N.D.	0.227 #
6)	B beta-BHC	0.000	4.627	0	7412419	N.D.	4.256 #
8)	B Heptachlo...	0.000	5.613	0	1467283	N.D.	0.472 #
13)	MA Dieldrin	0.000	6.236f	0	210766	N.D.	0.075 #
14)	MA Endrin	5.752	0.000	264980	0	0.098	N.D. #
15)	B Endosulfa...	0.000	6.679f	0	80134	N.D.	0.034 #
17)	MA 4,4'-DDT	0.000	6.873	0	99887	N.D.	0.045 #
23)	Chlordane-1	4.141f	0.000	1400060	0	15.517	N.D. #
24)	Chlordane-2	4.622f	0.000	1140154	0	9.920	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040221\
Data File : PL065851.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Apr 2021 19:35
Operator : AR\AJ
Sample : PB135509TB
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB135509TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 05:07:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
Quant Title : GC Extractables
QLast Update : Wed Mar 31 15:57:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

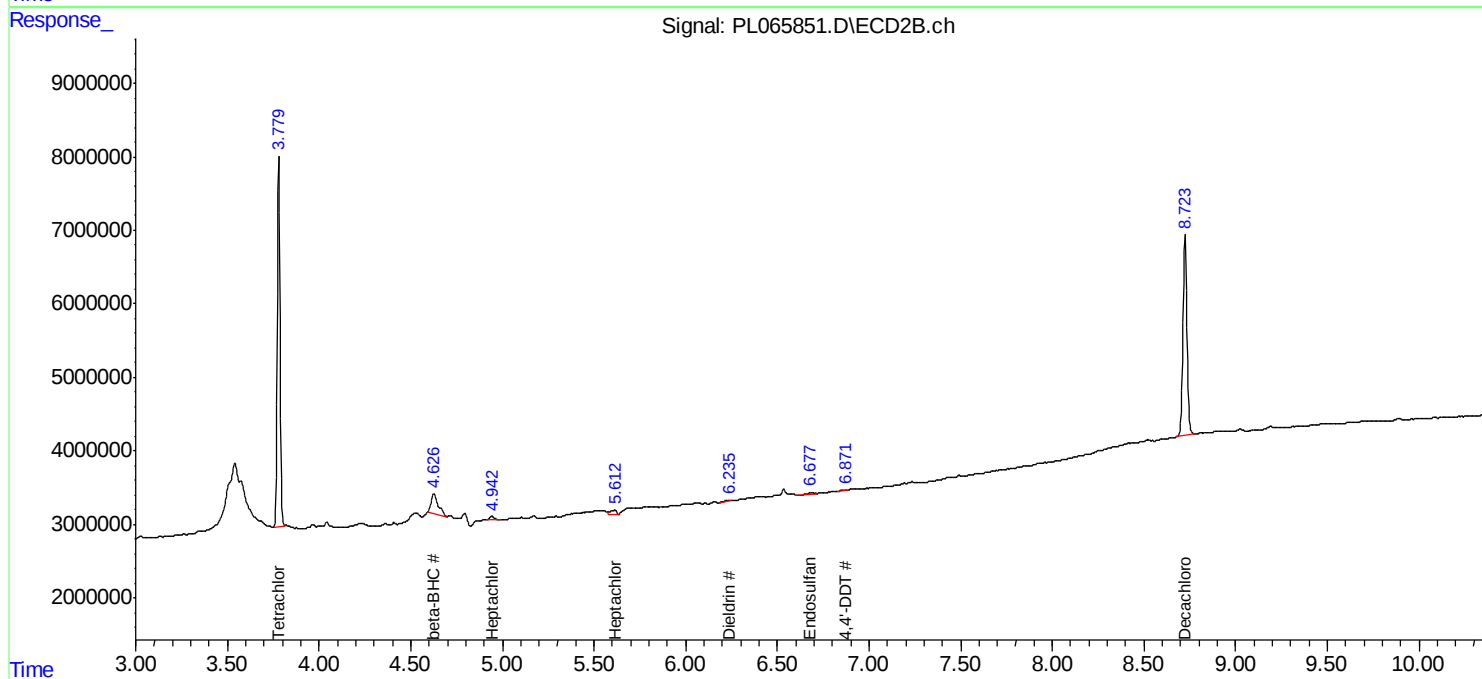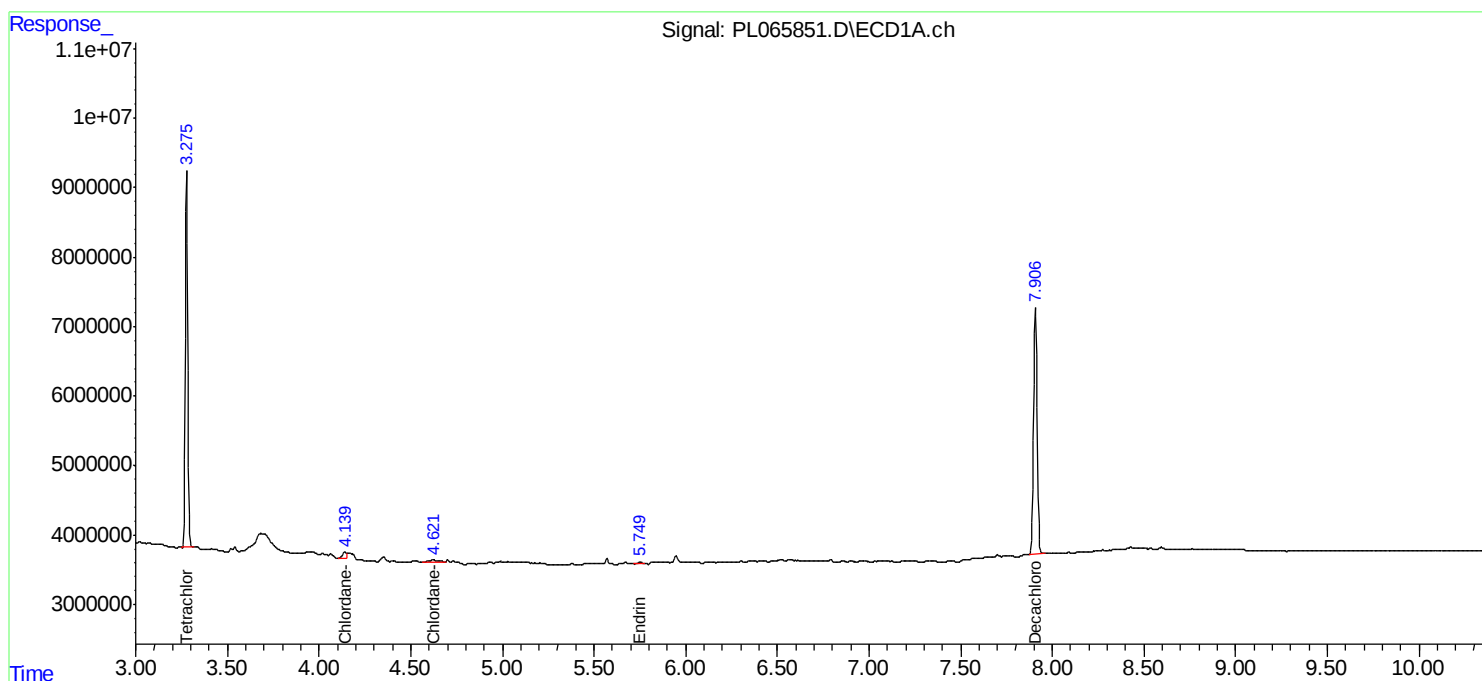


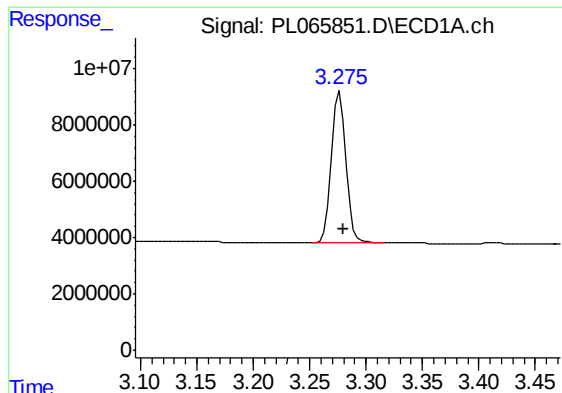

#1 Tetrachloro-m-xylene


R.T.: 3.277 min
Delta R.T.: -0.003 min
Response: 47700215
Conc: 18.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB135509TB

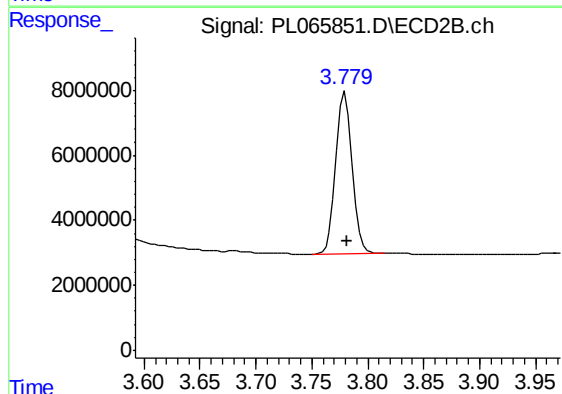


#1 Tetrachloro-m-xylene

R.T.: 3.780 min
Delta R.T.: -0.002 min
Response: 49881968
Conc: 18.17 ng/ml

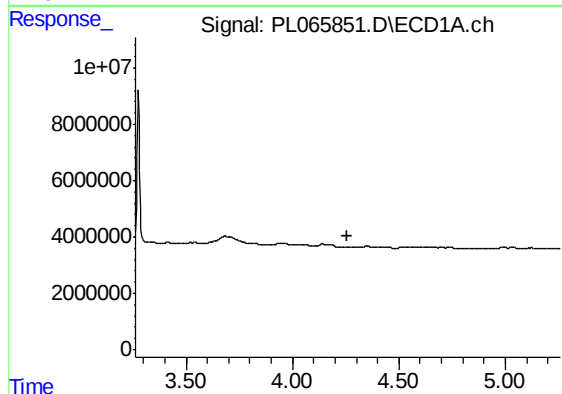


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.260 min
Response: 0
Conc: N.D.

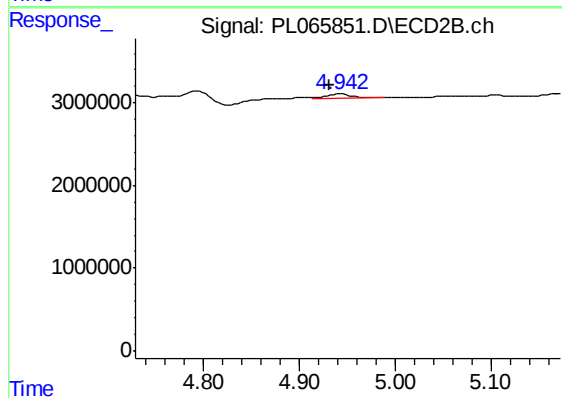

#4 Heptachlor


R.T.: 4.943 min
Delta R.T.: 0.012 min
Response: 802257
Conc: 0.23 ng/ml

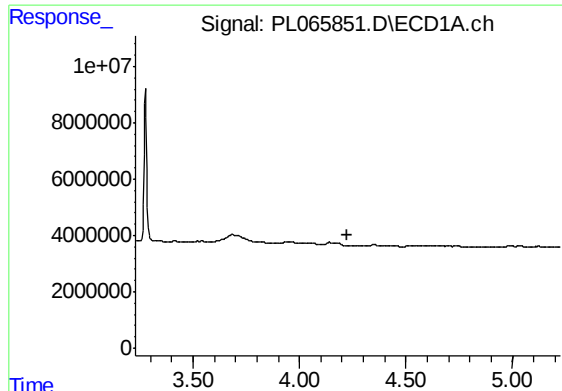

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.226 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB135509TB

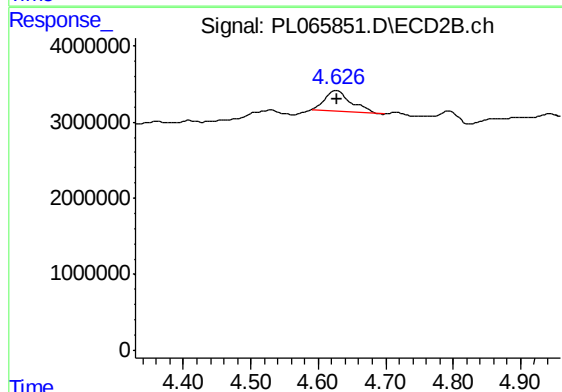


#6 beta-BHC

R.T.: 4.627 min
Delta R.T.: -0.002 min
Response: 7412419
Conc: 4.26 ng/ml

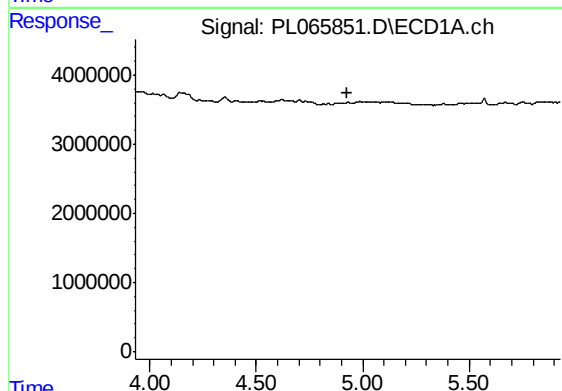


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.929 min
Response: 0
Conc: N.D.

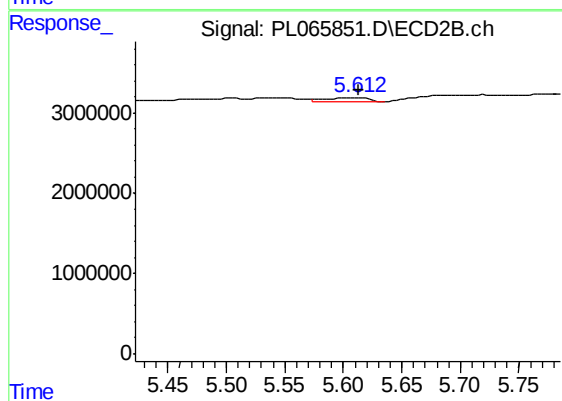

#8 Heptachlor epoxide


R.T.: 5.613 min
Delta R.T.: 0.000 min
Response: 1467283
Conc: 0.47 ng/ml

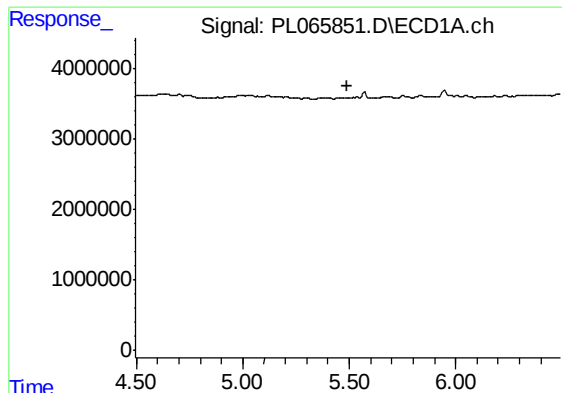

#13 Dielldrin


R.T.: 0.000 min
Exp R.T. : 5.493 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB135509TB

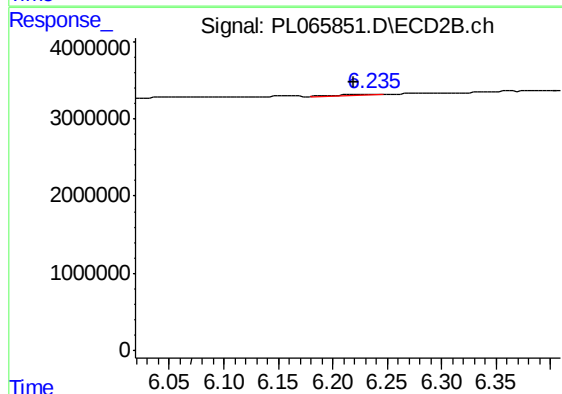


#13 Dielldrin

R.T.: 6.236 min
Delta R.T.: 0.017 min
Response: 210766
Conc: 0.07 ng/ml

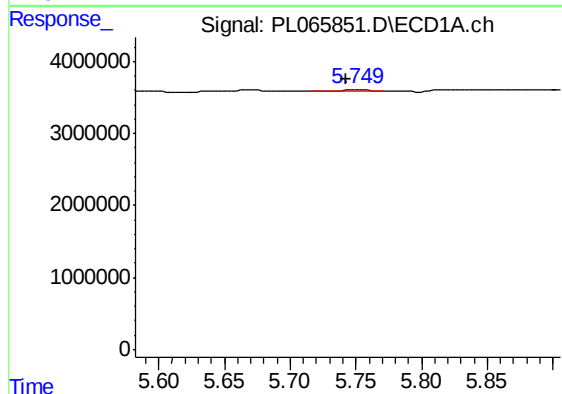


#14 Endrin

R.T.: 5.752 min
Delta R.T.: 0.010 min
Response: 264980
Conc: 0.10 ng/ml

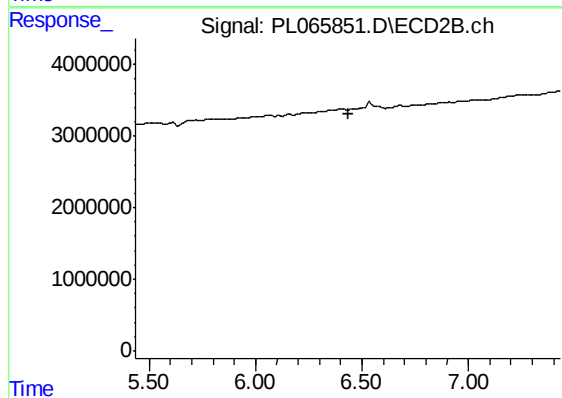

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.434 min
Response: 0
Conc: N.D.

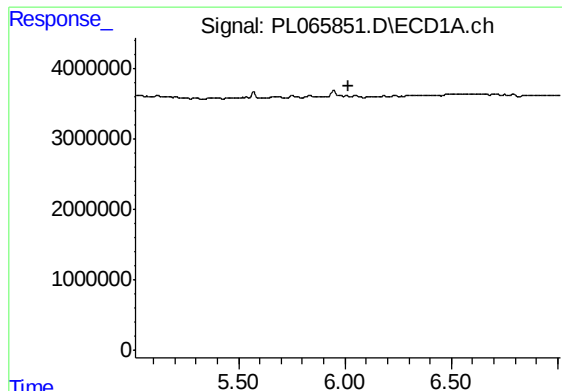

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.015 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB135509TB

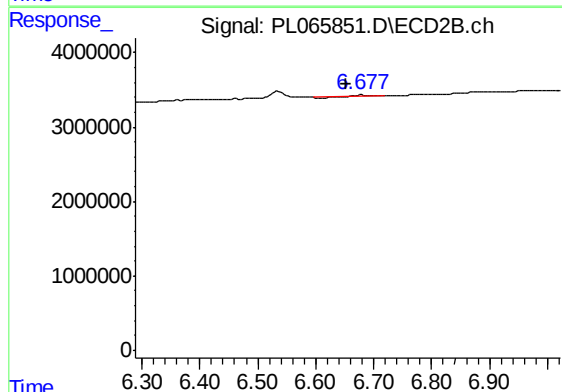


#15 Endosulfan II

R.T.: 6.679 min
Delta R.T.: 0.027 min
Response: 80134
Conc: 0.03 ng/ml

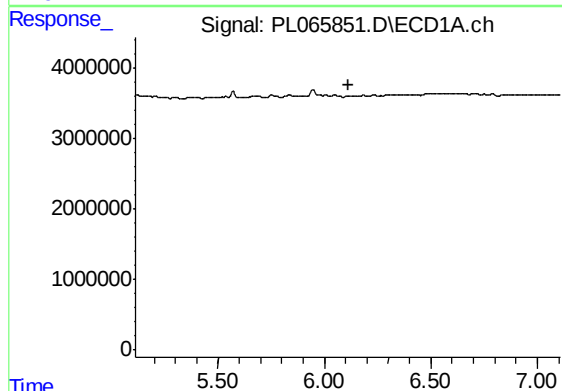


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.111 min
Response: 0
Conc: N.D.

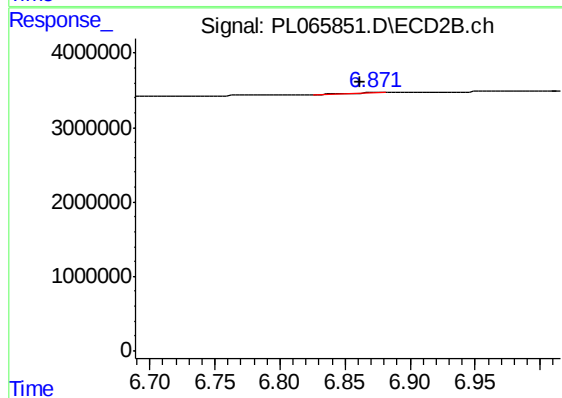

#17 4,4'-DDT


R.T.: 6.873 min
Delta R.T.: 0.011 min
Response: 99887
Conc: 0.04 ng/ml

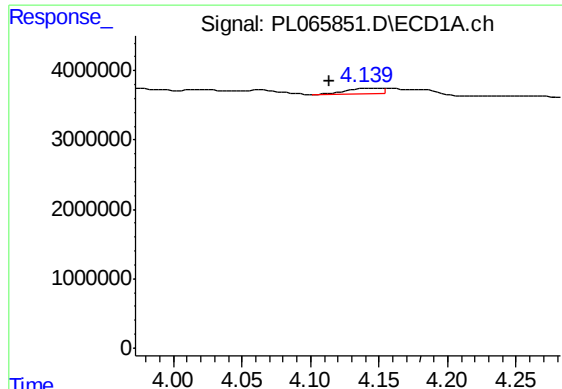

#23 Chlordane-1


R.T.: 4.141 min
Delta R.T.: 0.027 min
Response: 1400060
Conc: 15.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB135509TB

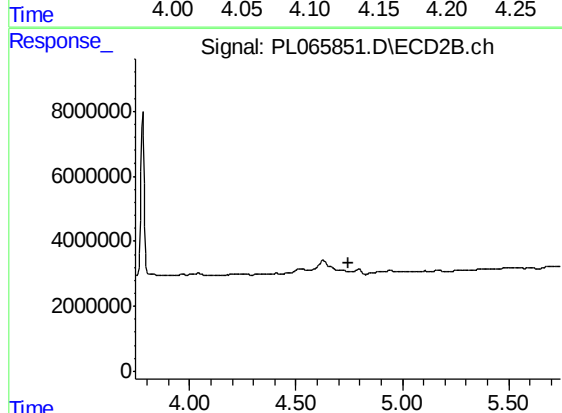


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.745 min
Response: 0
Conc: N.D.

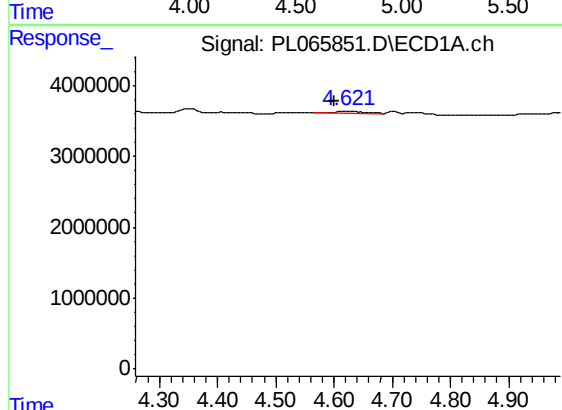


#24 Chlordane-2

R.T.: 4.622 min
Delta R.T.: 0.022 min
Response: 1140154
Conc: 9.92 ng/ml

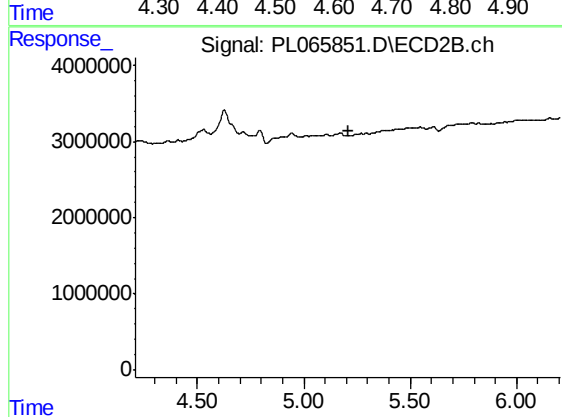

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.208 min
Response: 0
Conc: N.D.

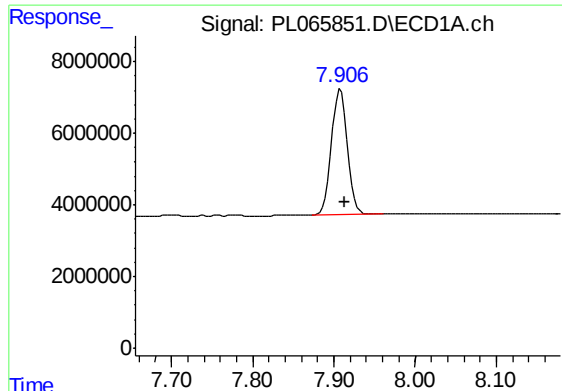

#28 Decachlorobiphenyl

R.T.: 7.908 min
Delta R.T.: -0.006 min
Response: 47777886
Conc: 20.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB135509TB

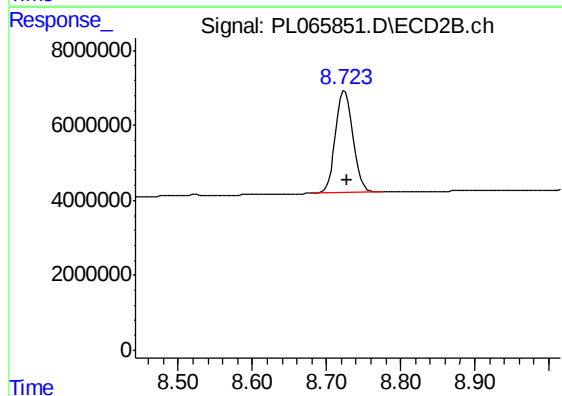

#28 Decachlorobiphenyl

R.T.: 8.725 min
Delta R.T.: -0.003 min
Response: 44056989
Conc: 19.54 ng/ml