

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040221\
 Data File : PL065857.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Apr 2021 21:01
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 05:10:26 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 31 15:57:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.276	3.780	55784441	57472512	21.414	20.937
28)	SA Decachlor...	7.907	8.726	52348396	49211659	22.603	21.828
Target Compounds							
4)	MA Heptachlor	4.232f	4.944	635931	559963	0.177	0.159
5)	MB Aldrin	0.000	5.248f	0	91884	N.D.	0.028 #
6)	B beta-BHC	4.232	4.628	635931	5500696	0.399	3.158 #
8)	B Heptachlo...	0.000	5.613	0	1778267	N.D.	0.573 #
14)	MA Endrin	5.752	0.000	651832	0	0.241	N.D. #
17)	MA 4,4'-DDT	6.104	0.000	512177	0	0.243	N.D. #
18)	B Endrin al...	6.188	6.775	357201	192556	0.189	0.101 #
20)	A Methoxychlor	0.000	7.354f	0	960453	N.D.	0.758 #
23)	Chlordane-1	4.139f	0.000	577106	0	6.396	N.D. #
24)	Chlordane-2	4.629f	0.000	2638690	0	22.958	N.D. #
27)	Chlordane-5	0.000	6.704	0	847488	N.D.	10.165 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040221\
Data File : PL065857.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Apr 2021 21:01
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 05:10:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
Quant Title : GC Extractables
QLast Update : Wed Mar 31 15:57:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

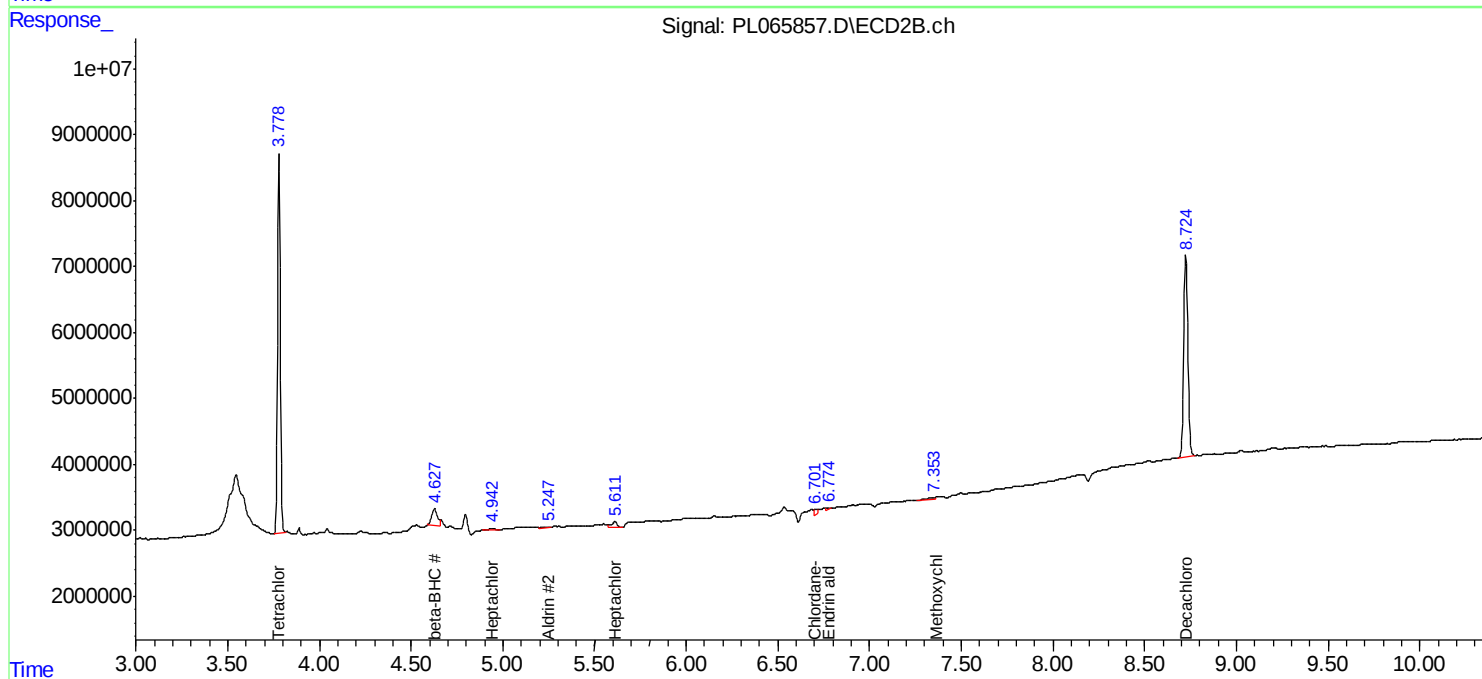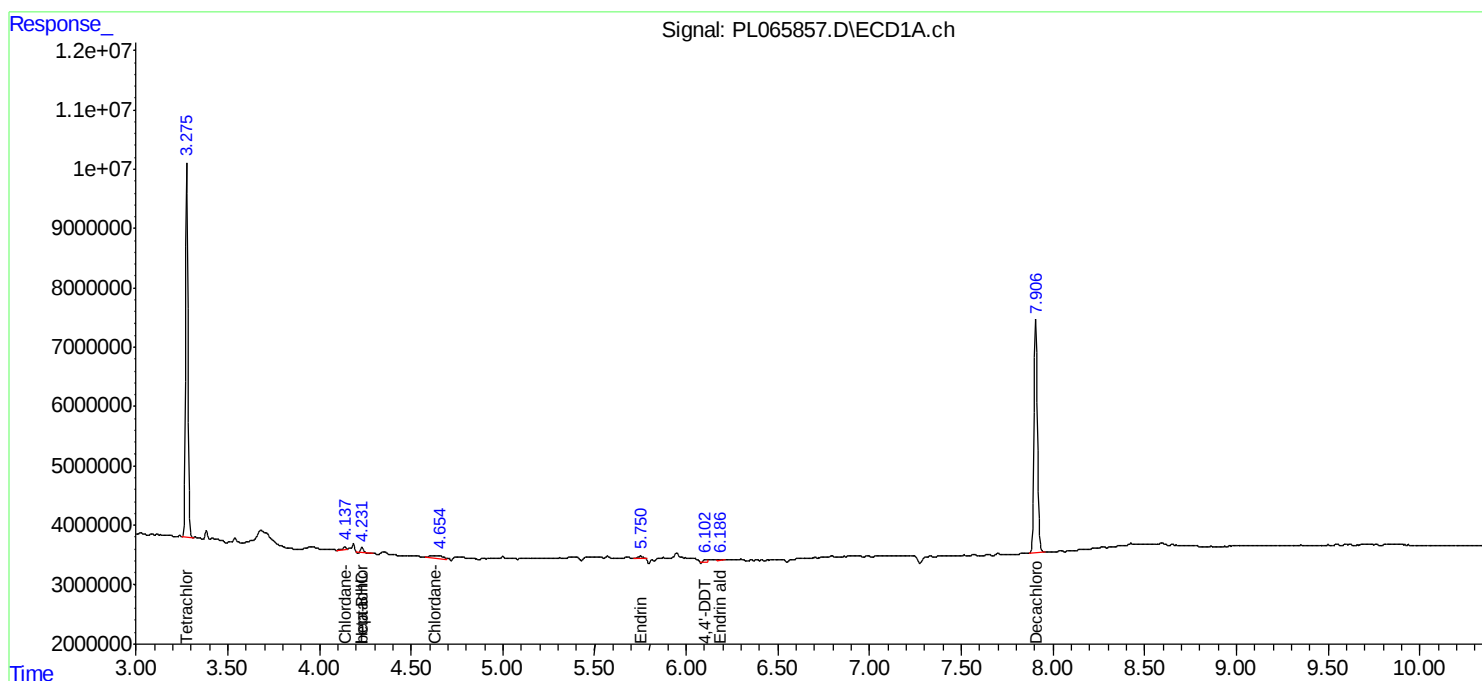


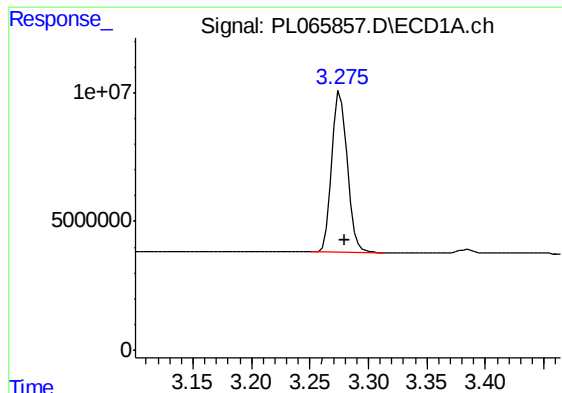

#1 Tetrachloro-m-xylene


R.T.: 3.276 min
Delta R.T.: -0.004 min
Response: 55784441
Conc: 21.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

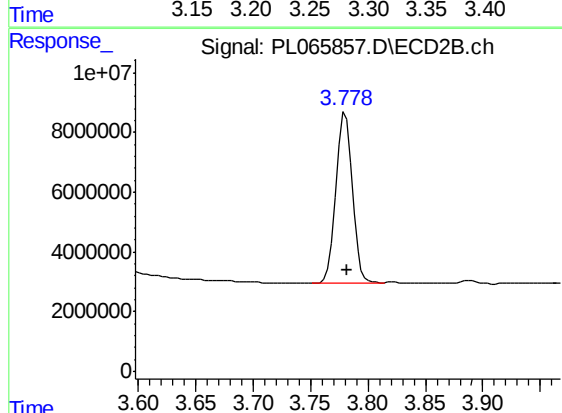


#1 Tetrachloro-m-xylene

R.T.: 3.780 min
Delta R.T.: -0.002 min
Response: 57472512
Conc: 20.94 ng/ml

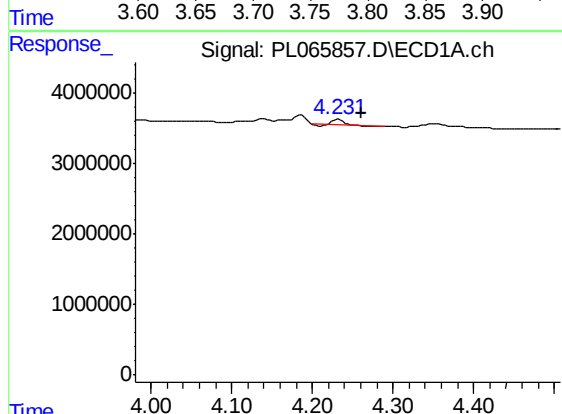


#4 Heptachlor

R.T.: 4.232 min
Delta R.T.: -0.028 min
Response: 635931
Conc: 0.18 ng/ml

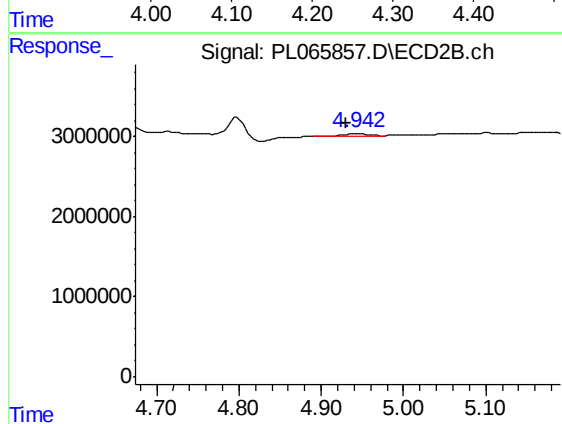

#4 Heptachlor


R.T.: 4.944 min
Delta R.T.: 0.013 min
Response: 559963
Conc: 0.16 ng/ml

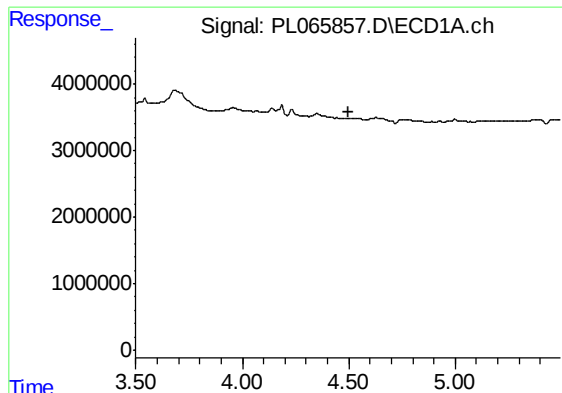

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 4.497 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

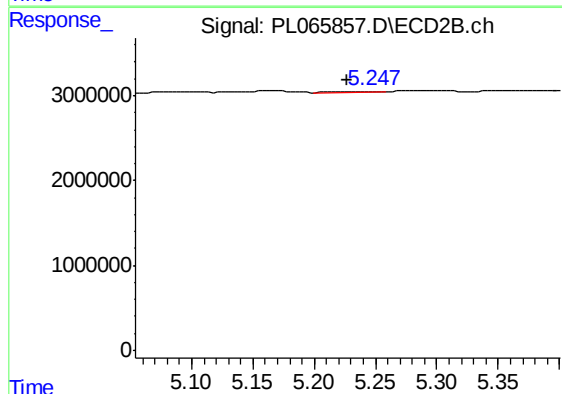


#5 Aldrin

R.T.: 5.248 min
Delta R.T.: 0.021 min
Response: 91884
Conc: 0.03 ng/ml

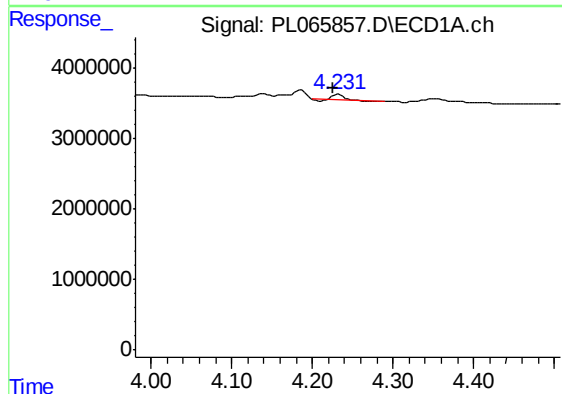


#6 beta-BHC

R.T.: 4.232 min
Delta R.T.: 0.006 min
Response: 635931
Conc: 0.40 ng/ml

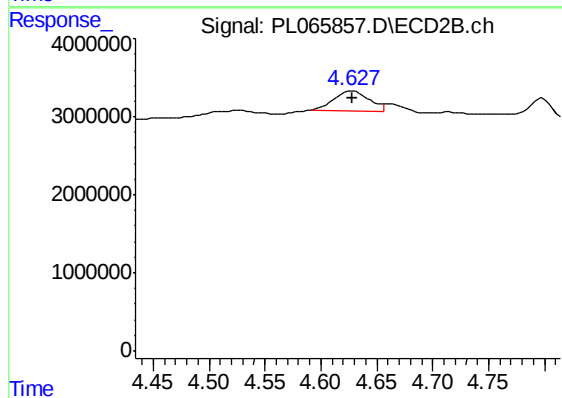

#6 beta-BHC


R.T.: 4.628 min
Delta R.T.: 0.000 min
Response: 5500696
Conc: 3.16 ng/ml

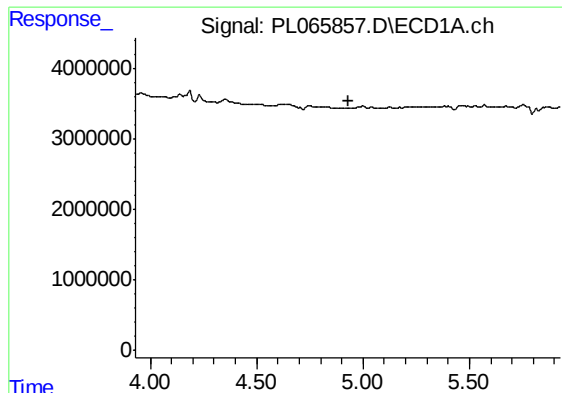

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.929 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

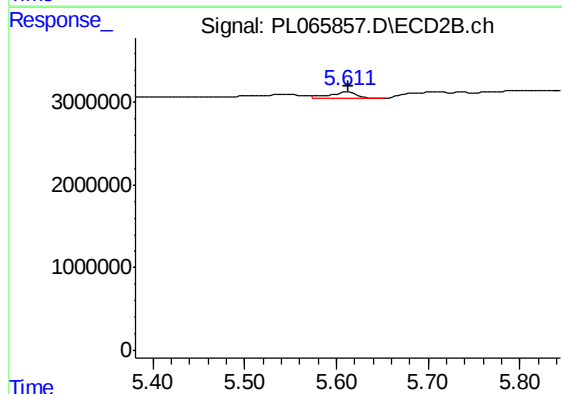


#8 Heptachlor epoxide

R.T.: 5.613 min
Delta R.T.: 0.000 min
Response: 1778267
Conc: 0.57 ng/ml

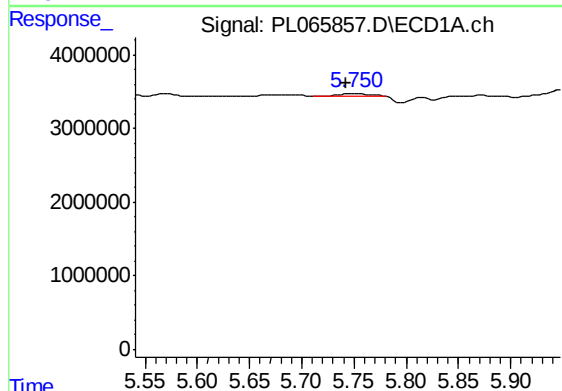


#14 Endrin

R.T.: 5.752 min
Delta R.T.: 0.009 min
Response: 651832
Conc: 0.24 ng/ml

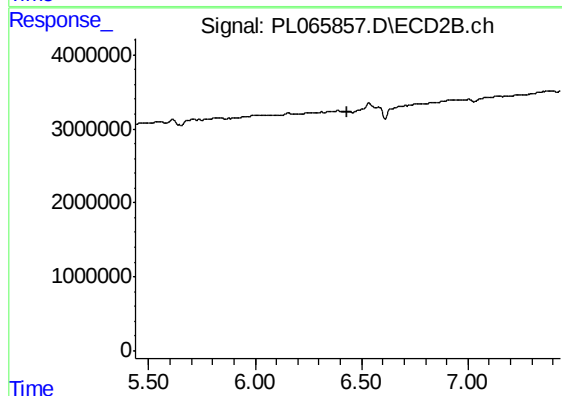

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.434 min
Response: 0
Conc: N.D.

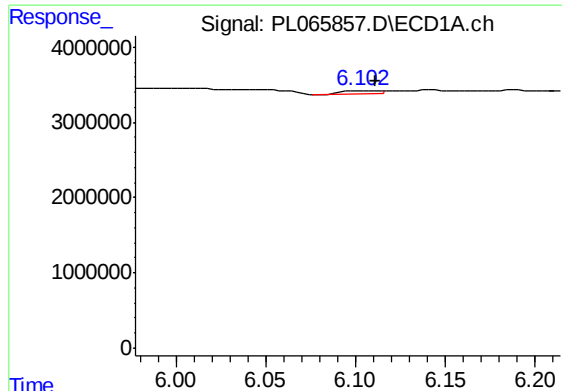

#17 4,4'-DDT


R.T.: 6.104 min
Delta R.T.: -0.007 min
Response: 512177
Conc: 0.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

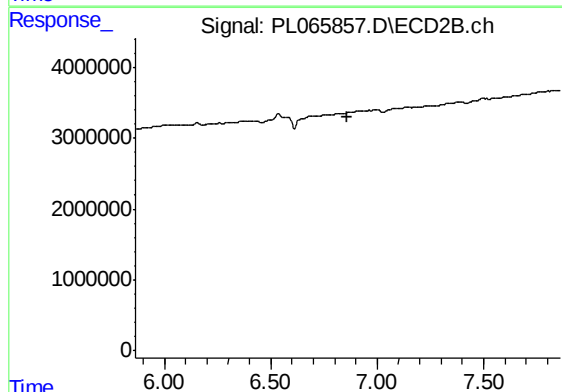


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.861 min
Response: 0
Conc: N.D.

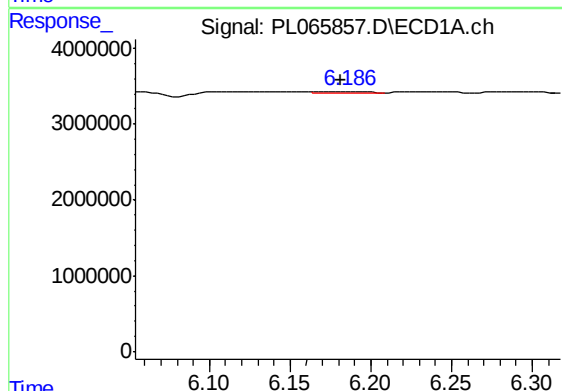


#18 Endrin aldehyde

R.T.: 6.188 min
Delta R.T.: 0.007 min
Response: 357201
Conc: 0.19 ng/ml

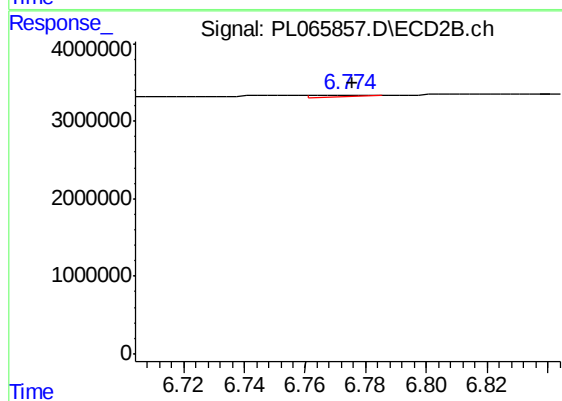

#18 Endrin aldehyde


R.T.: 6.775 min
Delta R.T.: 0.000 min
Response: 192556
Conc: 0.10 ng/ml

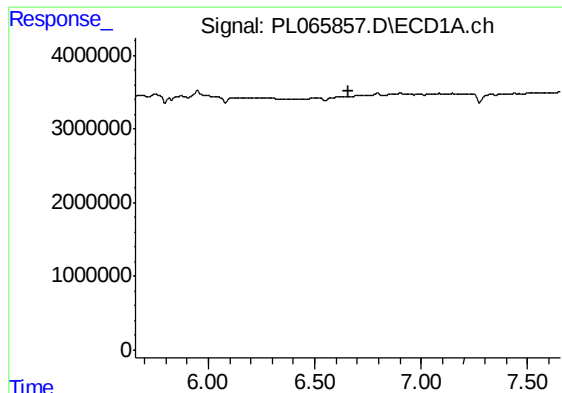

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 6.656 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

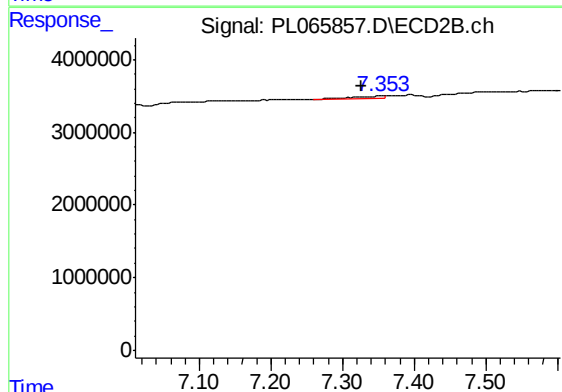


#20 Methoxychlor

R.T.: 7.354 min
Delta R.T.: 0.028 min
Response: 960453
Conc: 0.76 ng/ml

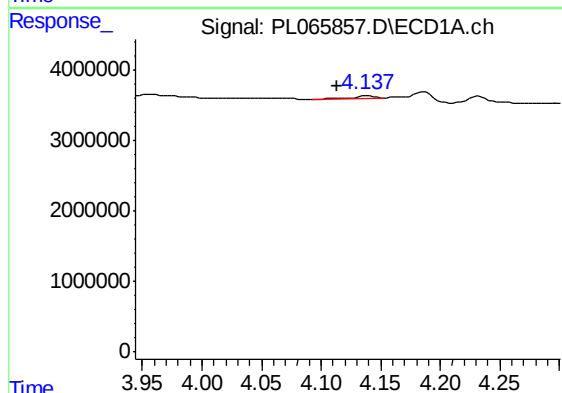


#23 Chlordane-1

R.T.: 4.139 min
Delta R.T.: 0.025 min
Response: 577106
Conc: 6.40 ng/ml

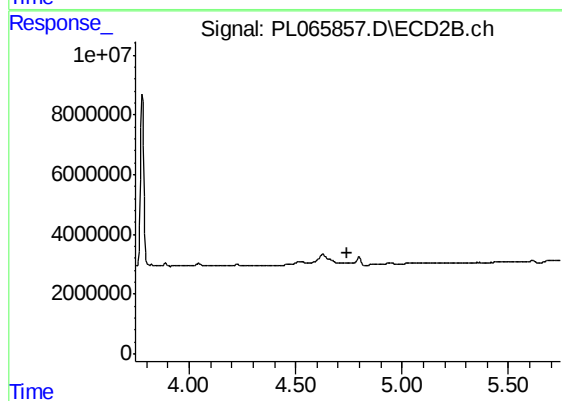

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.745 min
Response: 0
Conc: N.D.

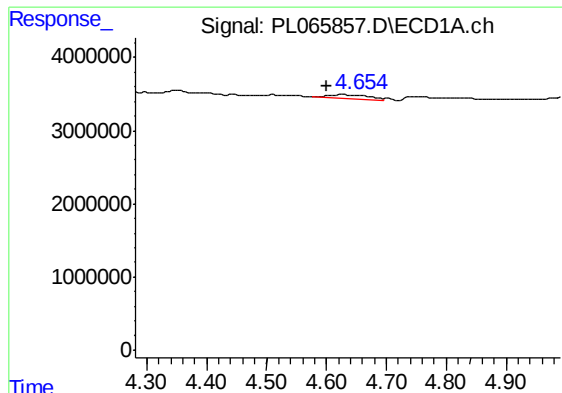

#24 Chlordane-2


R.T.: 4.629 min
Delta R.T.: 0.028 min
Response: 2638690
Conc: 22.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

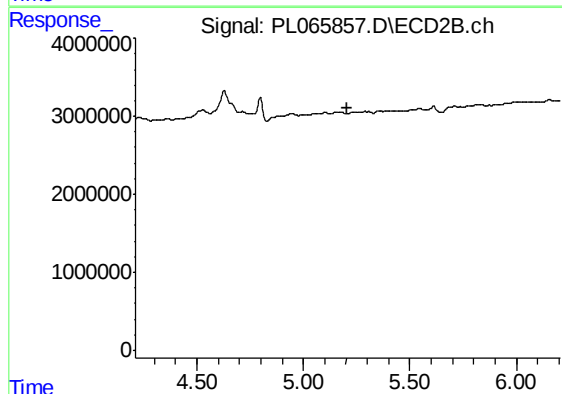


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.208 min
Response: 0
Conc: N.D.

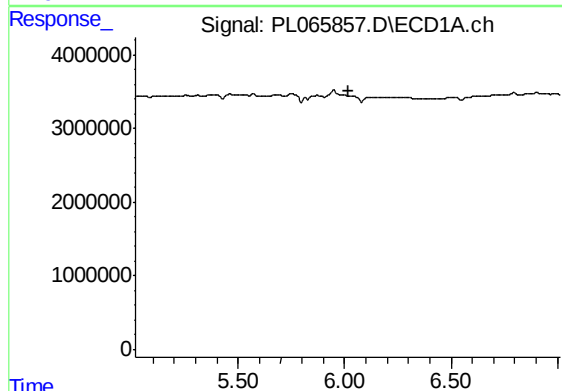


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.017 min
Response: 0
Conc: N.D.

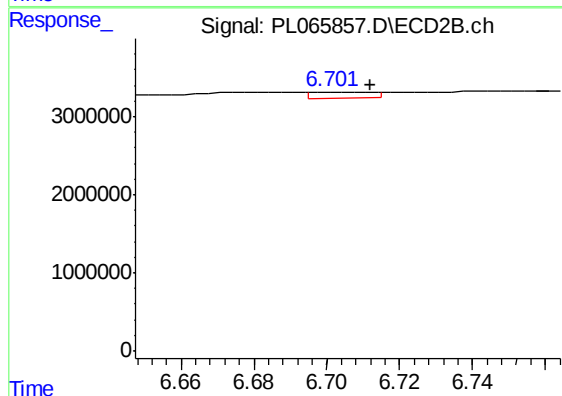

#27 Chlordane-5


R.T.: 6.704 min
Delta R.T.: -0.008 min
Response: 847488
Conc: 10.16 ng/ml

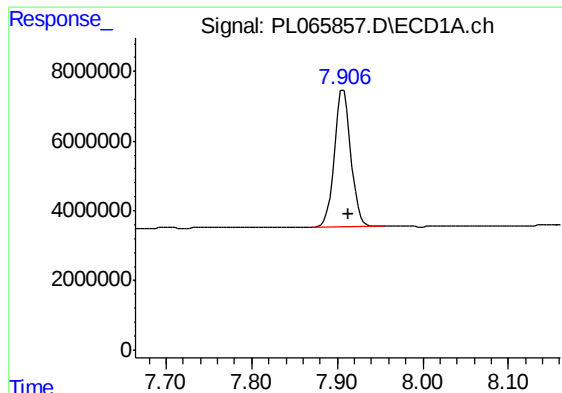

#28 Decachlorobiphenyl

R.T.: 7.907 min
Delta R.T.: -0.006 min
Response: 52348396
Conc: 22.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

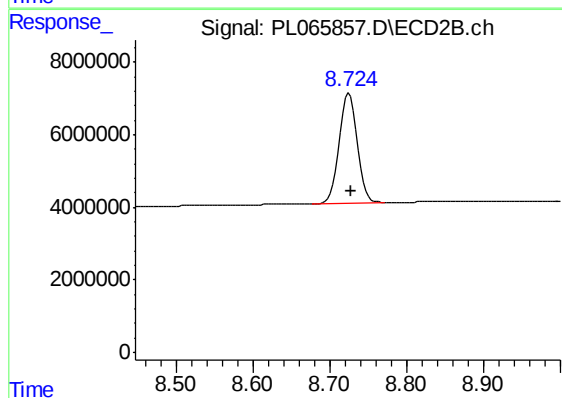

#28 Decachlorobiphenyl

R.T.: 8.726 min
Delta R.T.: -0.002 min
Response: 49211659
Conc: 21.83 ng/ml