

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040221\
 Data File : PL065819.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Apr 2021 10:51
 Operator : AR\AJ
 Sample : PB135375BS
 Misc : CHLOR BS
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB135375BS

Manual Integrations
 APPROVED

Ankita
 4/5/2021 3:34:54 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 04:53:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 31 15:57:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.281	3.781	49114991	47690781	18.854	17.374
28)	SA Decachlor...	7.913	8.729	43165294	39516644	18.638	17.528
Target Compounds							
23)	Chlordane-1	4.114	4.745	18232315	19280766	202.071	174.567
24)	Chlordane-2	4.600	5.207	20714689	20252462	180.232m	176.973
25)	Chlordane-3	5.151	5.842	54422563	71422325	175.099	168.036m
26)	Chlordane-4	5.205	5.913	50911365	85624036	178.315	169.257
27)	Chlordane-5	6.018	6.711	16924437	14646344	165.467	175.665

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040221\
Data File : PL065819.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Apr 2021 10:51
Operator : AR\AJ
Sample : PB135375BS
Misc : CHLOR BS
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
PB135375BS


Manual Integrations
APPROVED

Ankita
4/5/2021 3:34:54 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 04:53:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
Quant Title : GC Extractables
QLast Update : Wed Mar 31 15:57:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

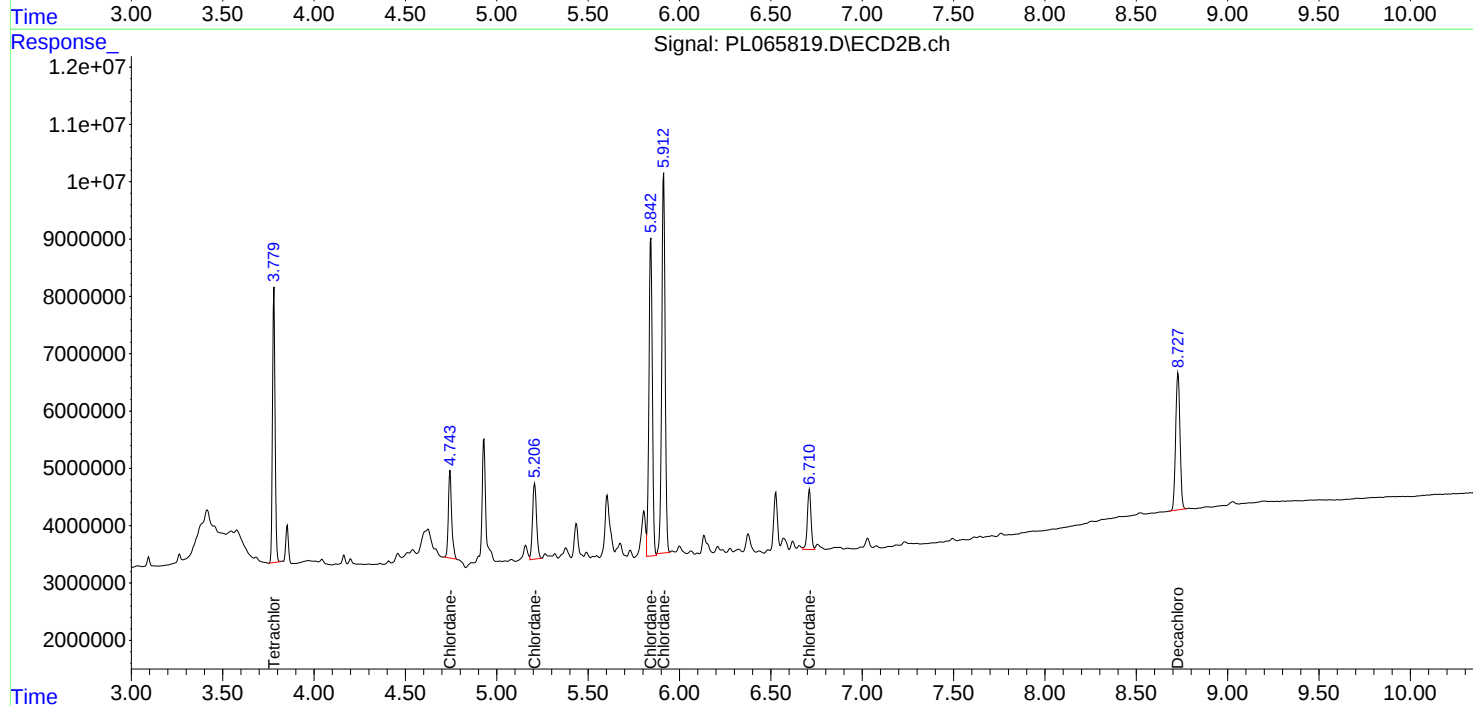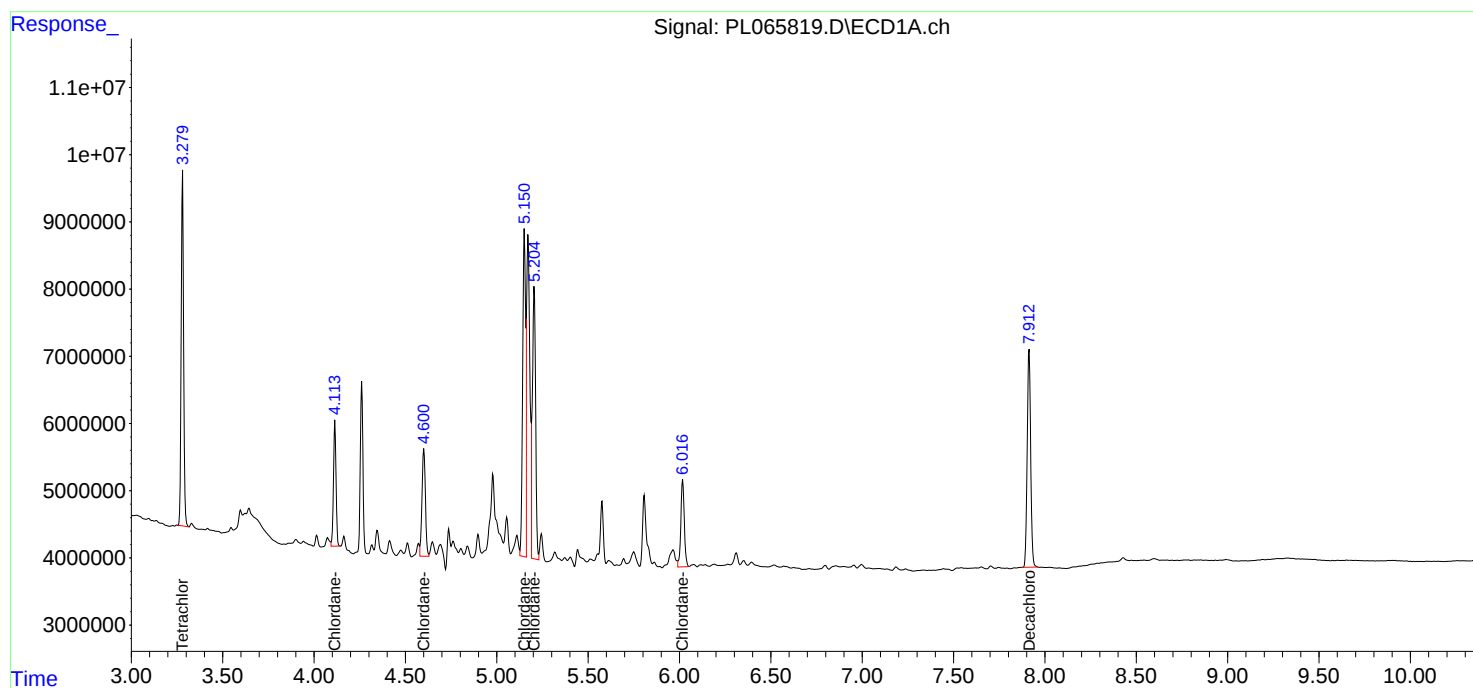

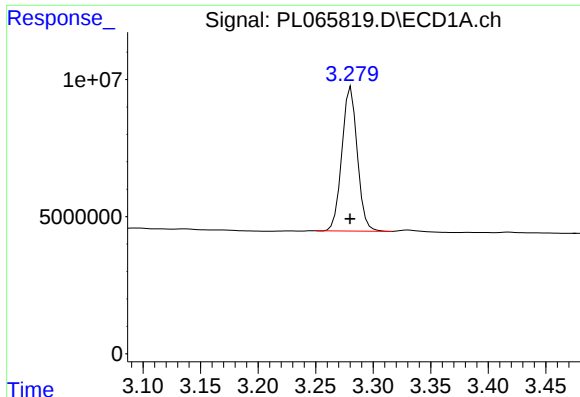


#1 Tetrachloro-m-xylene

R.T.: 3.281 min
Delta R.T.: 0.000 min
Response: 49114991
Conc: 18.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB135375BS


Manual Integrations
APPROVED

Ankita
4/5/2021 3:34:54 PM

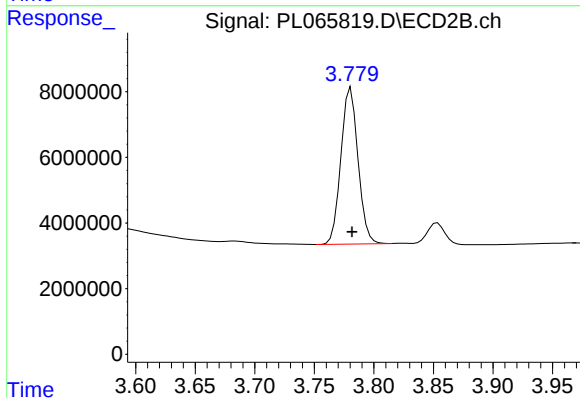


#1 Tetrachloro-m-xylene

R.T.: 3.781 min
Delta R.T.: 0.000 min
Response: 47690781
Conc: 17.37 ng/ml

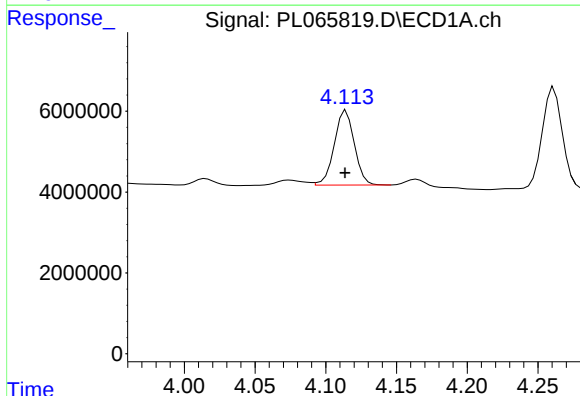


#23 Chlordane-1

R.T.: 4.114 min
Delta R.T.: 0.000 min
Response: 18232315
Conc: 202.07 ng/ml

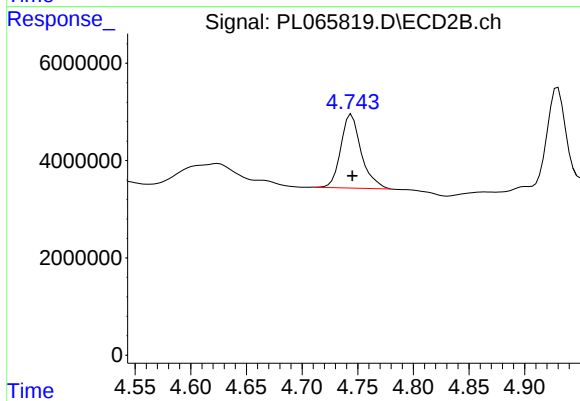

#23 Chlordane-1

R.T.: 4.745 min
Delta R.T.: 0.000 min
Response: 19280766
Conc: 174.57 ng/ml

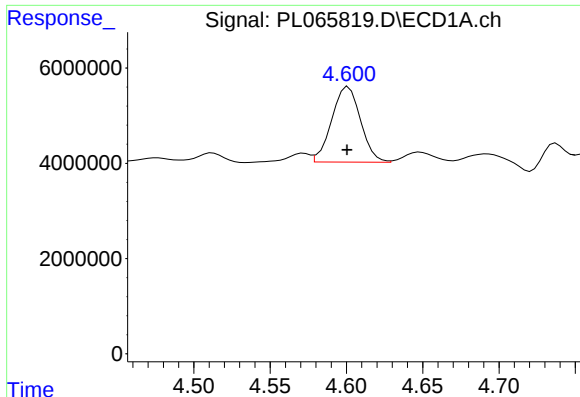


#24 Chlordane-2

R.T.: 4.600 min
Delta R.T.: 0.000 min
Response: 20714689
Conc: 180.23 ng/ml m

Instrument :
ECD_L
ClientSampleId :
PB135375BS


Manual Integrations
APPROVED

Ankita
4/5/2021 3:34:54 PM

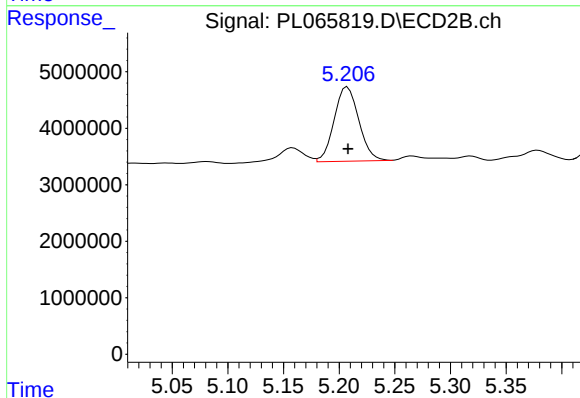


#24 Chlordane-2

R.T.: 5.207 min
Delta R.T.: 0.000 min
Response: 20252462
Conc: 176.97 ng/ml

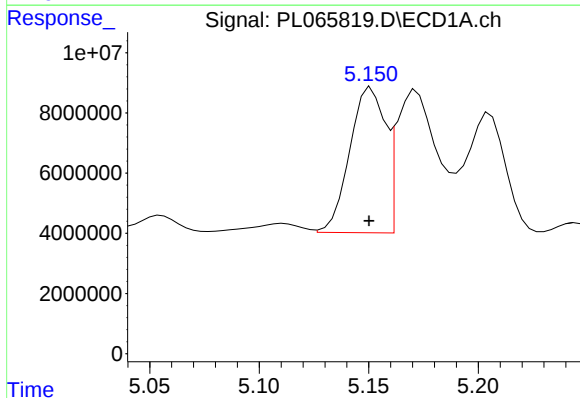


#25 Chlordane-3

R.T.: 5.151 min
Delta R.T.: 0.001 min
Response: 54422563
Conc: 175.10 ng/ml

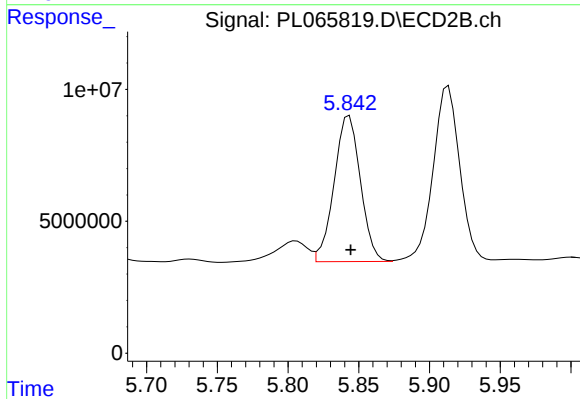

#25 Chlordane-3

R.T.: 5.842 min
Delta R.T.: -0.002 min
Response: 71422325
Conc: 168.04 ng/ml m

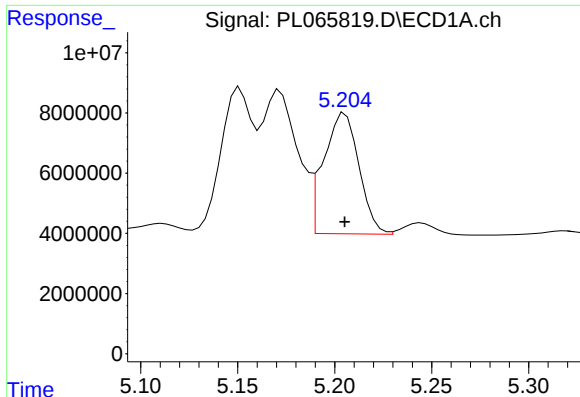


#26 Chlordane-4

R.T.: 5.205 min
Delta R.T.: 0.000 min
Response: 50911365
Conc: 178.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB135375BS


Manual Integrations
APPROVED

Ankita
4/5/2021 3:34:54 PM

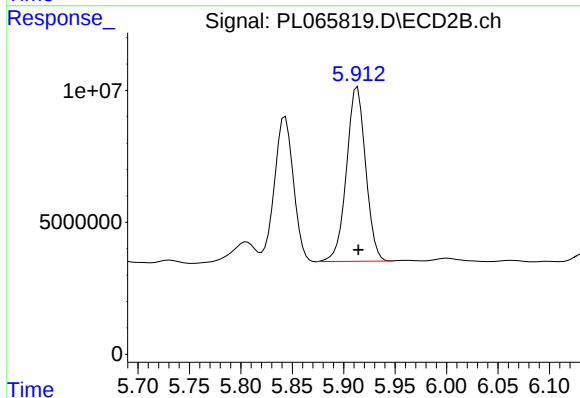


#26 Chlordane-4

R.T.: 5.913 min
Delta R.T.: 0.000 min
Response: 85624036
Conc: 169.26 ng/ml

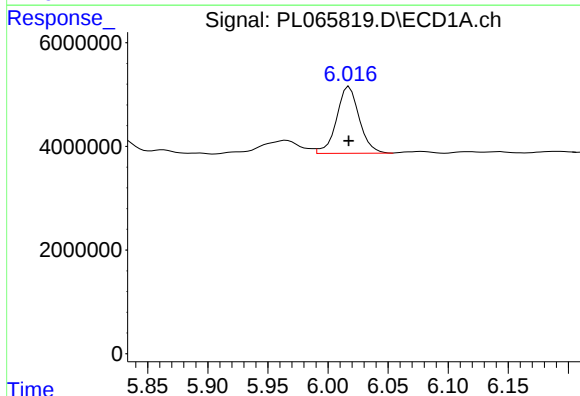


#27 Chlordane-5

R.T.: 6.018 min
Delta R.T.: 0.000 min
Response: 16924437
Conc: 165.47 ng/ml

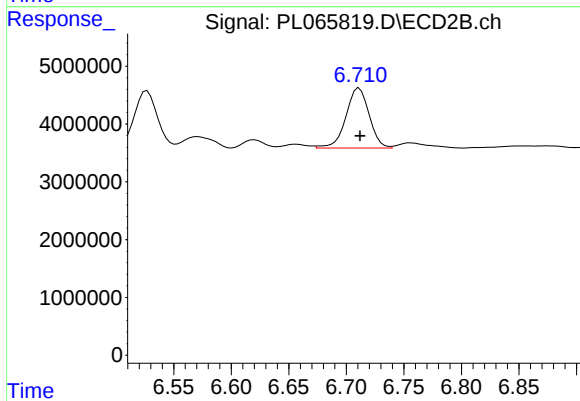

#27 Chlordane-5

R.T.: 6.711 min
Delta R.T.: 0.000 min
Response: 14646344
Conc: 175.66 ng/ml

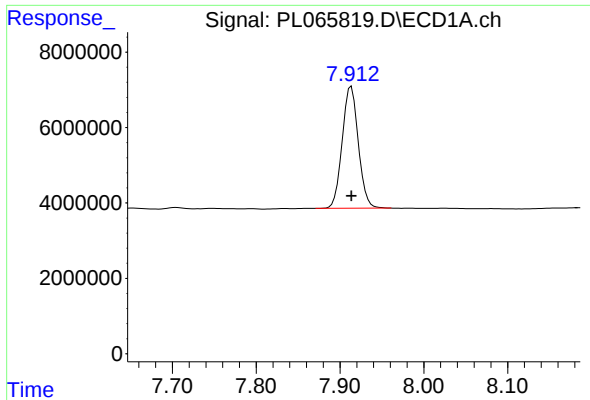


#28 Decachlorobiphenyl

R.T.: 7.913 min
Delta R.T.: 0.000 min
Response: 43165294
Conc: 18.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB135375BS

Manual Integrations
APPROVED

Ankita
4/5/2021 3:34:54 PM

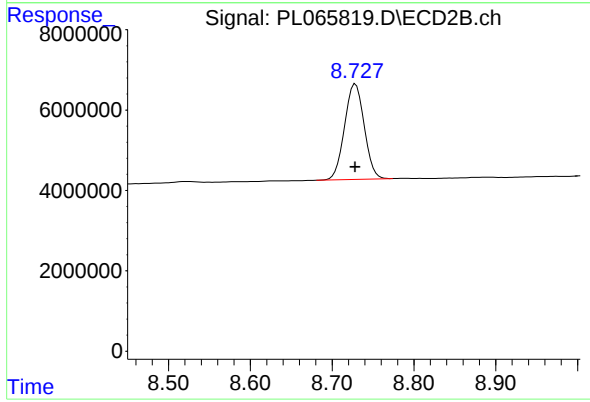

#28 Decachlorobiphenyl

R.T.: 8.729 min
Delta R.T.: 0.000 min
Response: 39516644
Conc: 17.53 ng/ml