

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040221\
 Data File : PL065827.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Apr 2021 13:48
 Operator : AR\AJ
 Sample : M1888-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-3S-(0-4)

Manual Integrations
 APPROVED

Ankita
 4/5/2021 3:34:58 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 04:57:10 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 31 15:57:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.283	3.781	29337475	31785701	11.262	11.580
28)	SA Decachlor...	7.917	8.730	27324484	25248969	11.798	11.199
Target Compounds							
12)	B 4,4'-DDE	5.377	6.077	2416596	1823328	0.876	0.698
17)	MA 4,4'-DDT	6.113	6.861	1860192	1309049	0.883m	0.585m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040221\
Data File : PL065827.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Apr 2021 13:48
Operator : AR\AJ
Sample : M1888-01
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
TP-3S-(0-4)


Manual Integrations
APPROVED

Ankita
4/5/2021 3:34:58 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 04:57:10 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
Quant Title : GC Extractables
QLast Update : Wed Mar 31 15:57:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

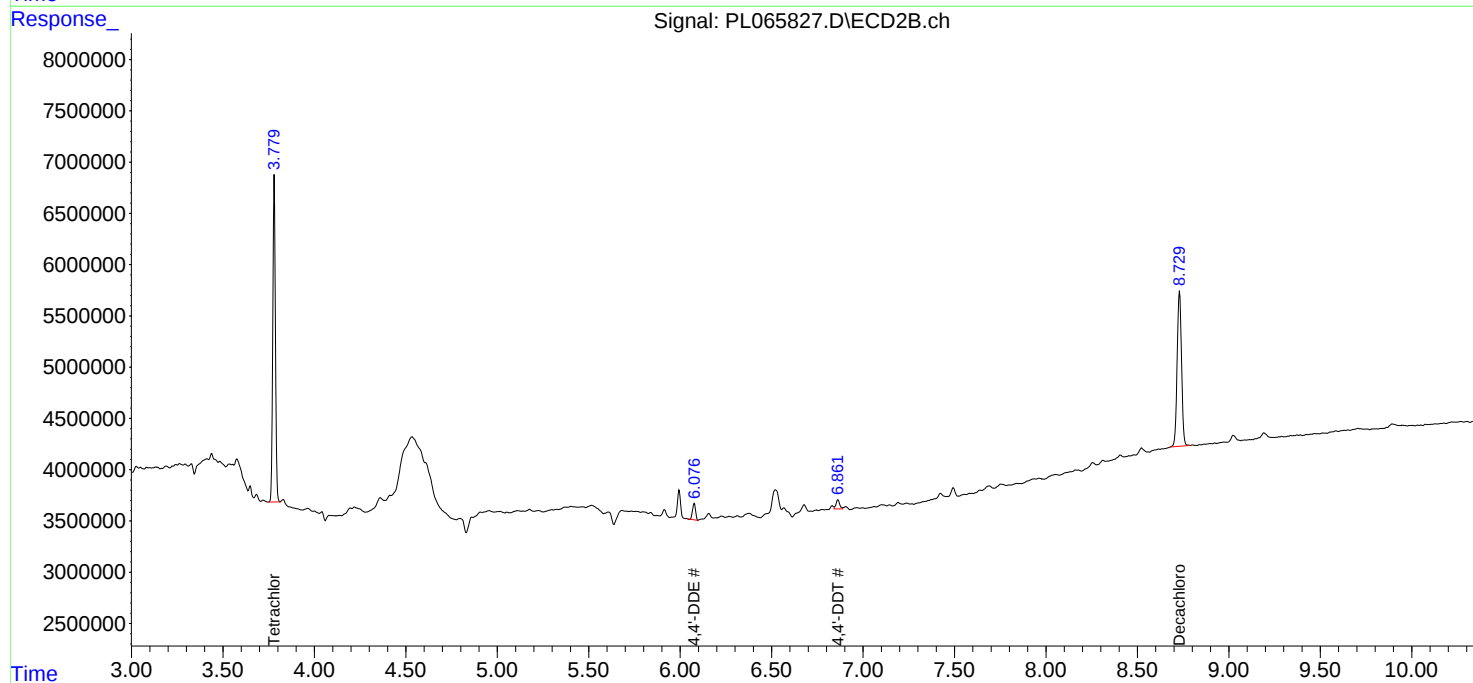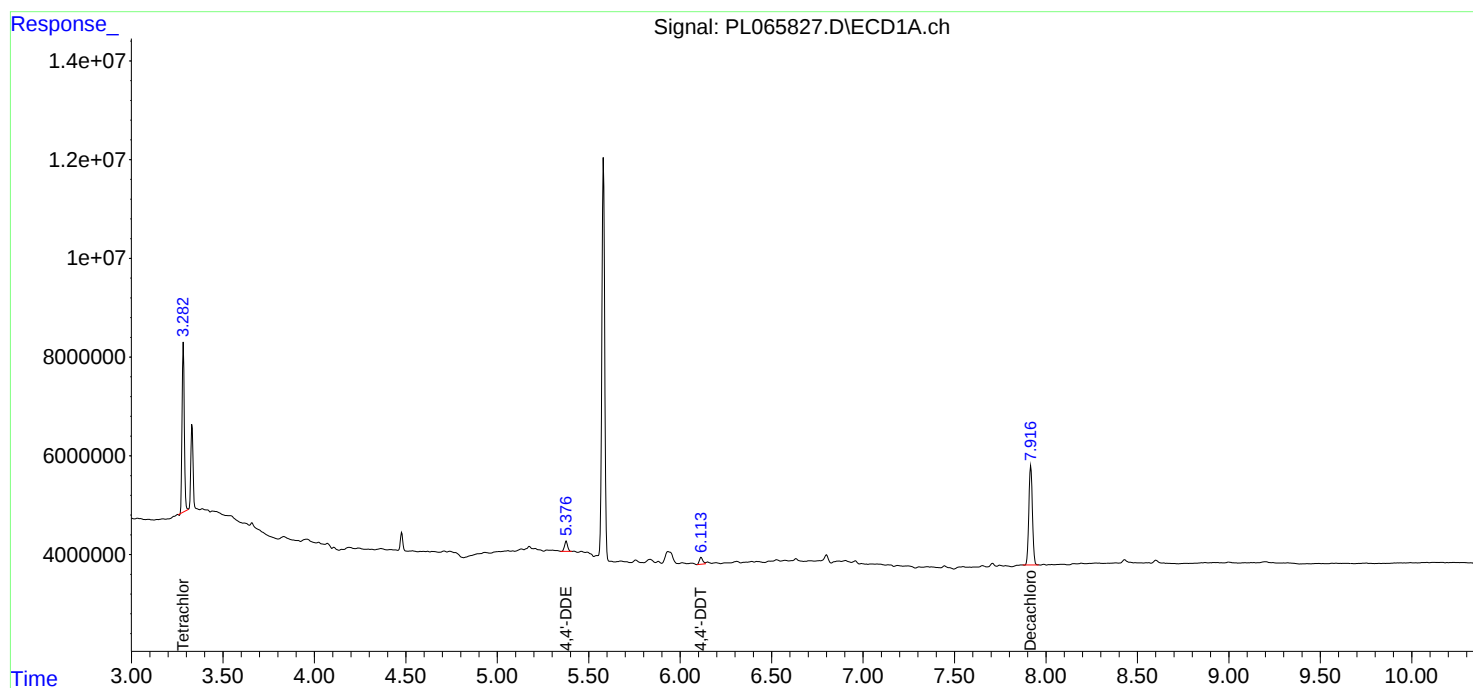

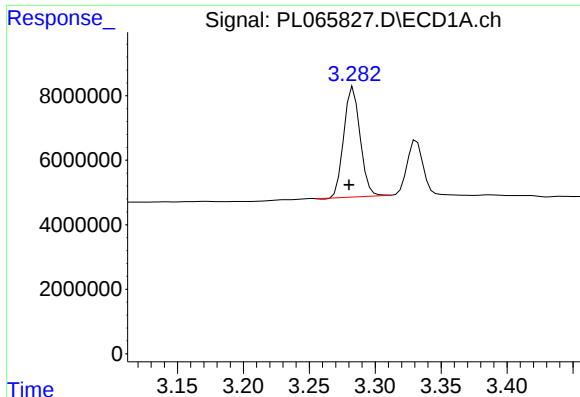


#1 Tetrachloro-m-xylene

R.T.: 3.283 min
Delta R.T.: 0.003 min
Response: 29337475
Conc: 11.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3S-(0-4)


Manual Integrations
APPROVED

Ankita
4/5/2021 3:34:58 PM

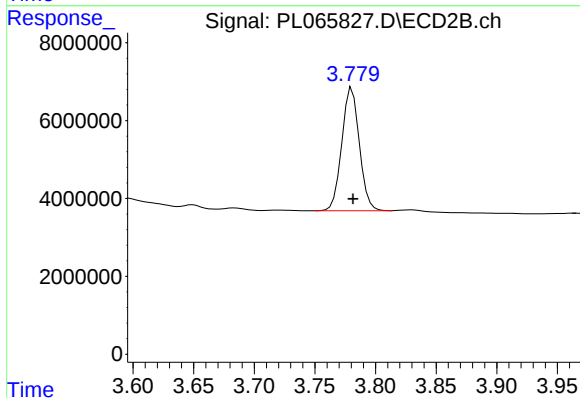


#1 Tetrachloro-m-xylene

R.T.: 3.781 min
Delta R.T.: 0.000 min
Response: 31785701
Conc: 11.58 ng/ml

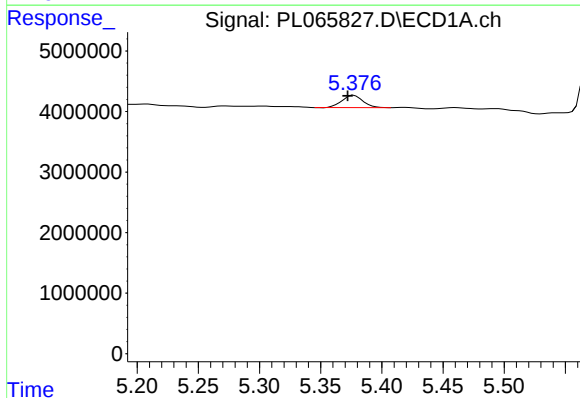


#12 4,4'-DDE

R.T.: 5.377 min
Delta R.T.: 0.005 min
Response: 2416596
Conc: 0.88 ng/ml

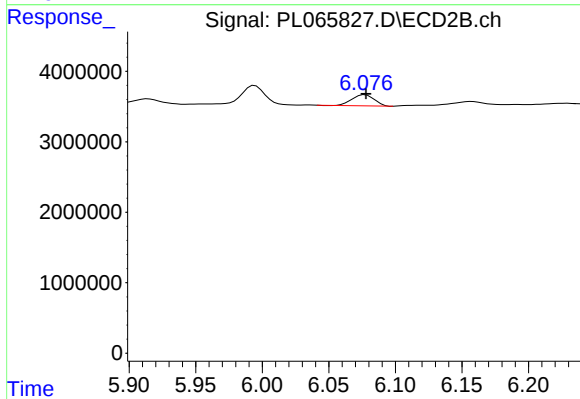

#12 4,4'-DDE

R.T.: 6.077 min
Delta R.T.: 0.000 min
Response: 1823328
Conc: 0.70 ng/ml

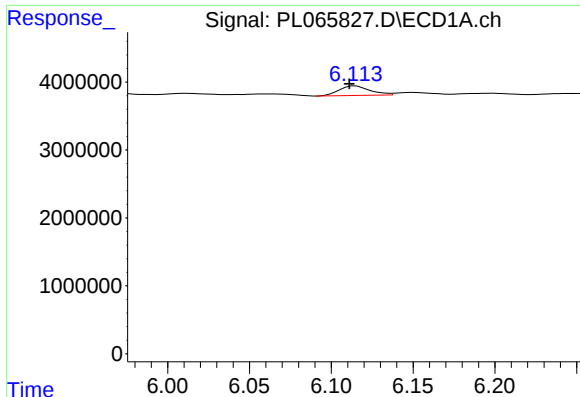


#17 4,4'-DDT

R.T.: 6.113 min
Delta R.T.: 0.002 min
Response: 1860192
Conc: 0.88 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TP-3S-(0-4)


Manual Integrations
APPROVED

Ankita
4/5/2021 3:34:58 PM

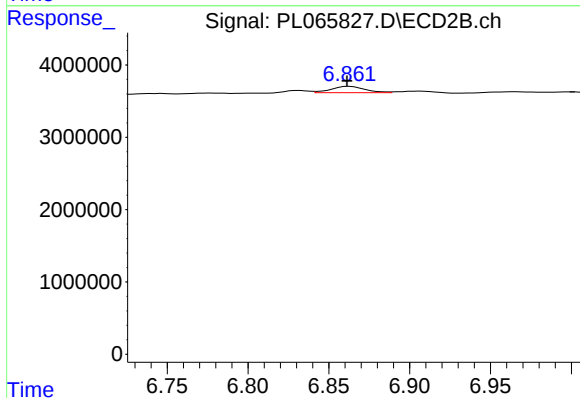


#17 4,4'-DDT

R.T.: 6.861 min
Delta R.T.: 0.000 min
Response: 1309049
Conc: 0.58 ng/ml m

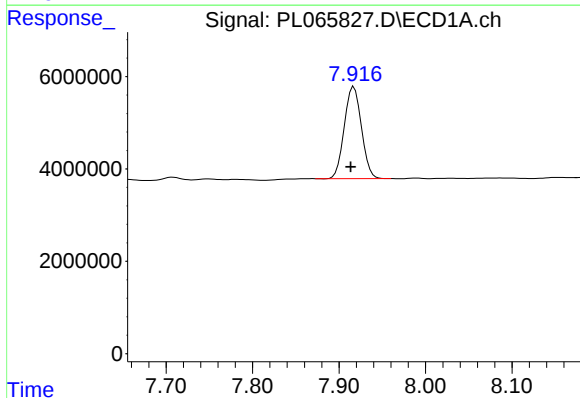

#28 Decachlorobiphenyl

R.T.: 7.917 min
Delta R.T.: 0.004 min
Response: 27324484
Conc: 11.80 ng/ml

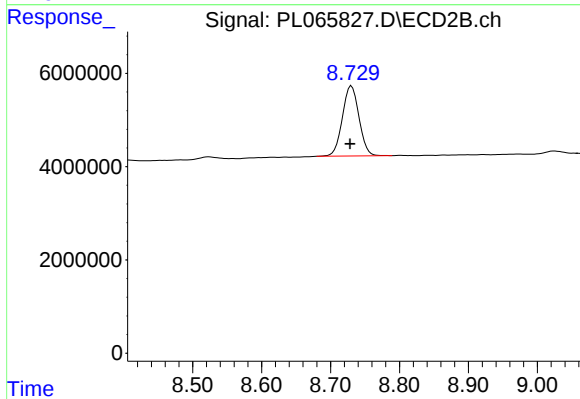

#28 Decachlorobiphenyl

R.T.: 8.730 min
Delta R.T.: 0.002 min
Response: 25248969
Conc: 11.20 ng/ml