

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040221\
 Data File : PL065835.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Apr 2021 15:46
 Operator : AR\AJ
 Sample : M1897-02
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-1

Manual Integrations
 APPROVED

Ankita
 4/5/2021 3:35:06 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 05:00:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 31 15:57:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.275	3.780	45773922	46864154	17.571m	17.073
28)	SA Decachlor...	7.909	8.726	43911810	43949799	18.960	19.494

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040221\
Data File : PL065835.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Apr 2021 15:46
Operator : AR\AJ
Sample : M1897-02
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-1


Manual Integrations
APPROVED

Ankita
4/5/2021 3:35:06 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 05:00:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
Quant Title : GC Extractables
QLast Update : Wed Mar 31 15:57:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

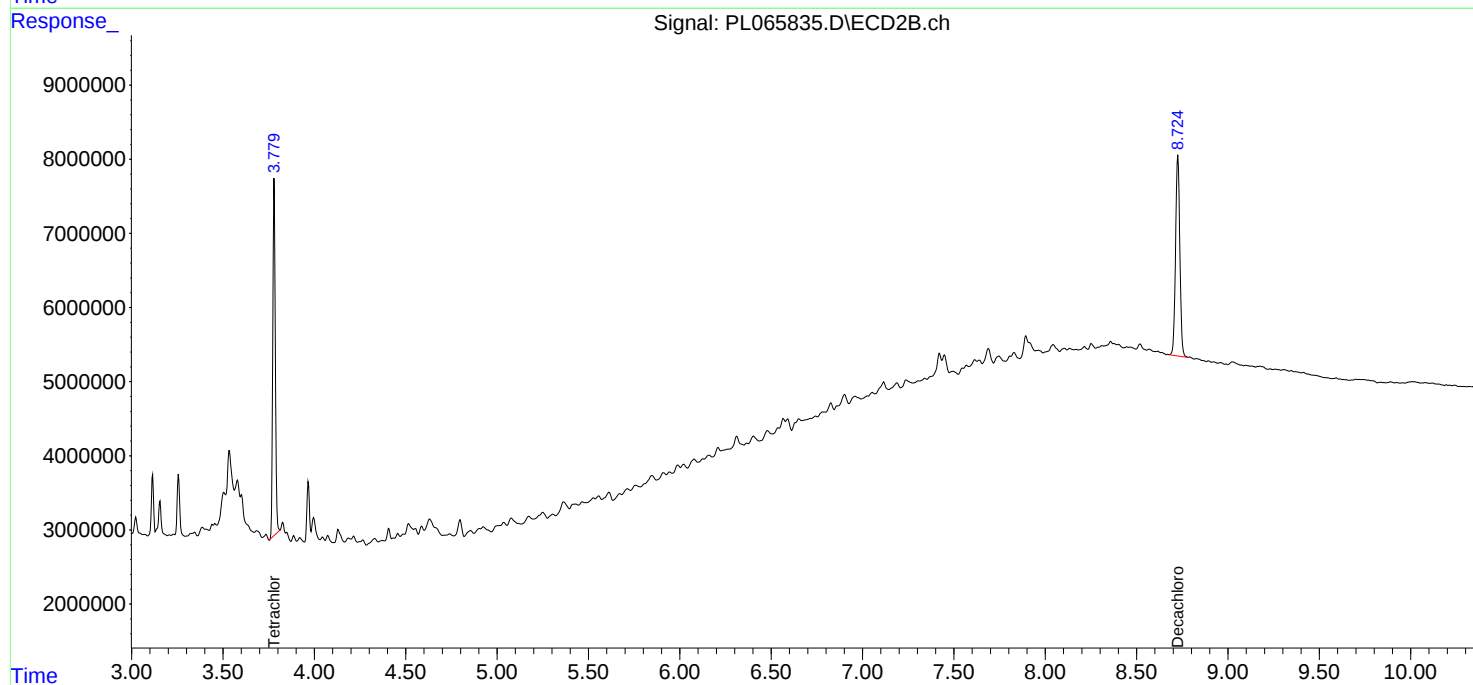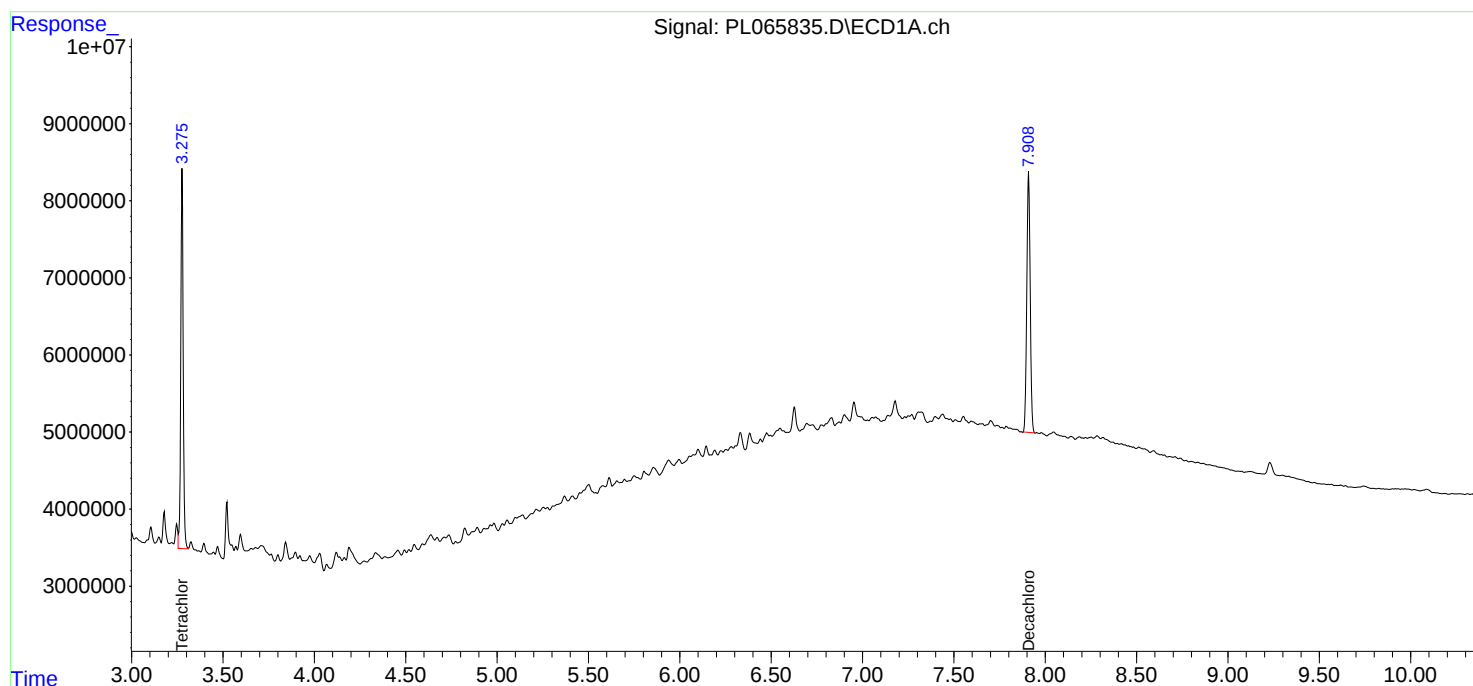

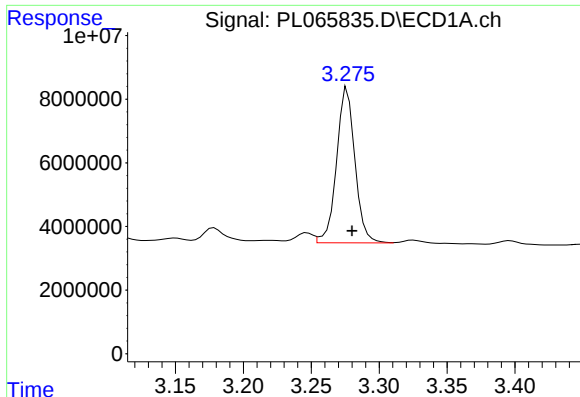

#1 Tetrachloro-m-xylene

R.T.: 3.275 min

Delta R.T.: -0.005 min


Response: 45773922

Conc: 17.57 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TP-1

Manual Integrations
APPROVED

Ankita
4/5/2021 3:35:06 PM

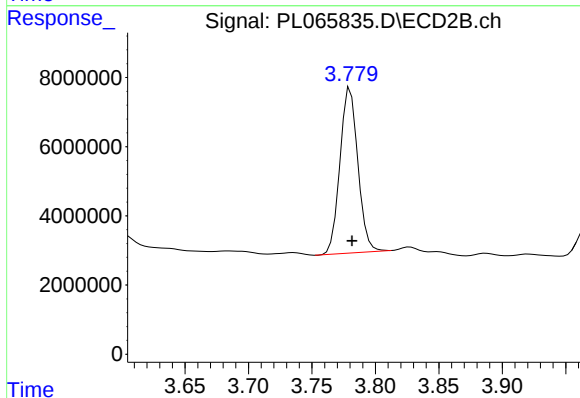


#1 Tetrachloro-m-xylene

R.T.: 3.780 min

Delta R.T.: -0.001 min

Response: 46864154

Conc: 17.07 ng/ml

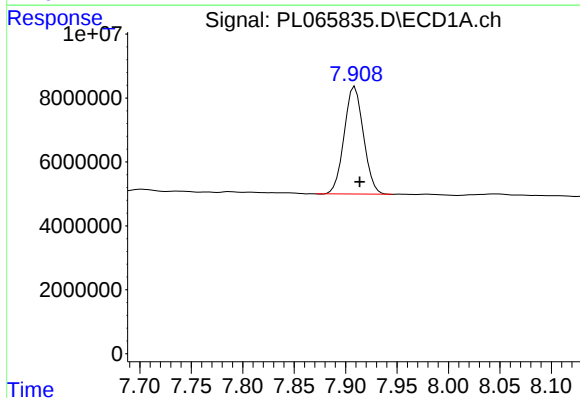


#28 Decachlorobiphenyl

R.T.: 7.909 min

Delta R.T.: -0.005 min

Response: 43911810

Conc: 18.96 ng/ml

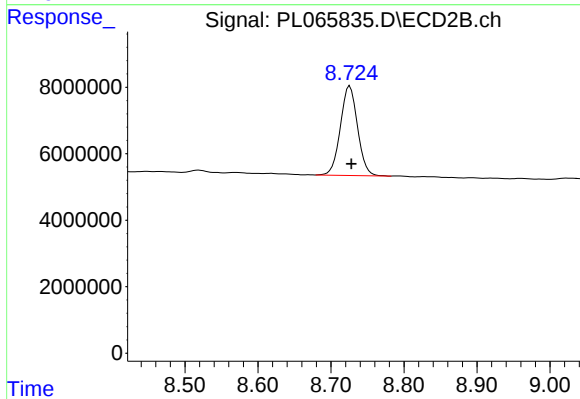

#28 Decachlorobiphenyl

R.T.: 8.726 min

Delta R.T.: -0.002 min

Response: 43949799

Conc: 19.49 ng/ml