

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040221\
 Data File : PL065837.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Apr 2021 16:14
 Operator : AR\AJ
 Sample : M1900-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CHRT-26586

Manual Integrations
 APPROVED

Ankita
 4/5/2021 3:35:07 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 05:01:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 31 15:57:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.277	3.780	26736179	29333809	10.263	10.686
28)	SA Decachlor...	7.908	8.727	32657770	29848032	14.101	13.239
Target Compounds							
11)	B alpha-Chl...	5.201	5.913	2523268	6478121	0.811	2.189 #
12)	B 4,4'-DDE	5.369	6.076	4296953	5507242	1.557	2.108 #
17)	MA 4,4'-DDT	6.104	6.858	5480150	2831865	2.601	1.265m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040221\
Data File : PL065837.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Apr 2021 16:14
Operator : AR\AJ
Sample : M1900-01
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
CHRT-26586


Manual Integrations
APPROVED

Ankita
4/5/2021 3:35:07 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 05:01:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
Quant Title : GC Extractables
QLast Update : Wed Mar 31 15:57:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

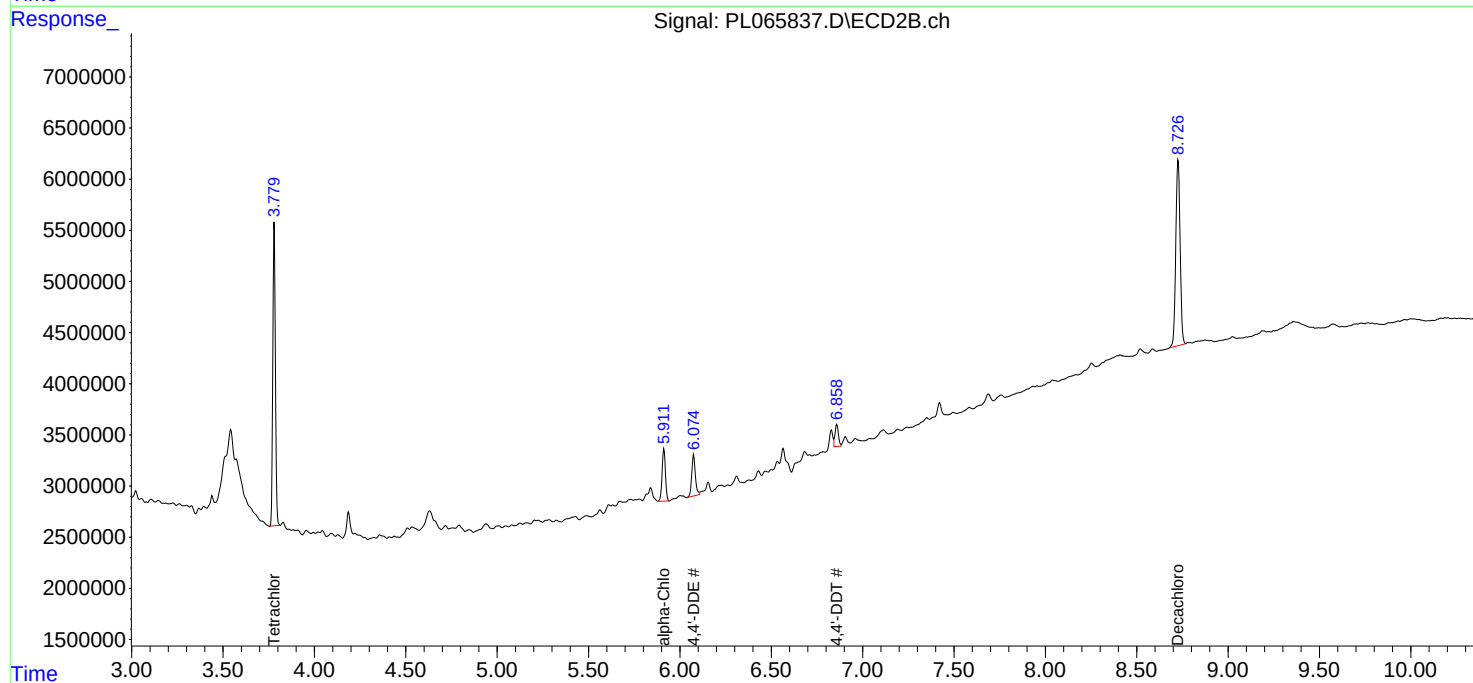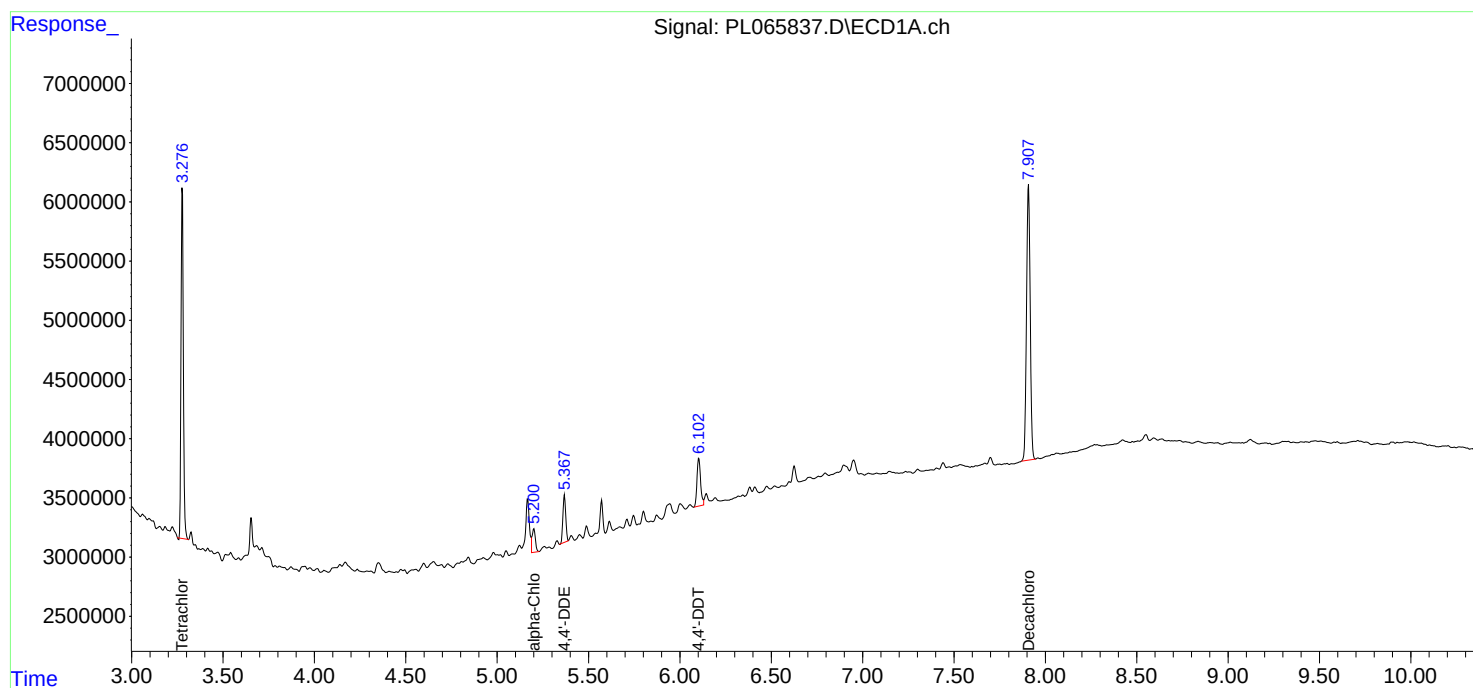

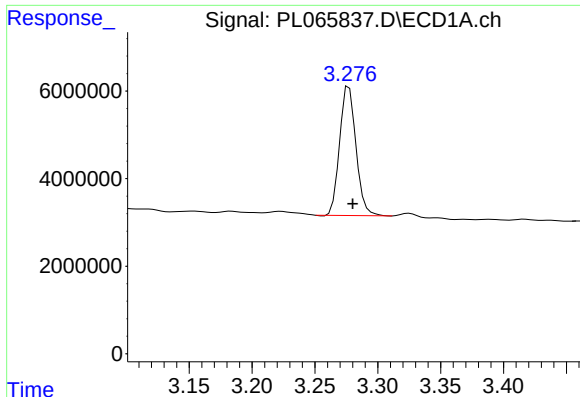


#1 Tetrachloro-m-xylene

R.T.: 3.277 min
Delta R.T.: -0.003 min
Response: 26736179
Conc: 10.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
CHRT-26586


Manual Integrations
APPROVED

Ankita
4/5/2021 3:35:07 PM

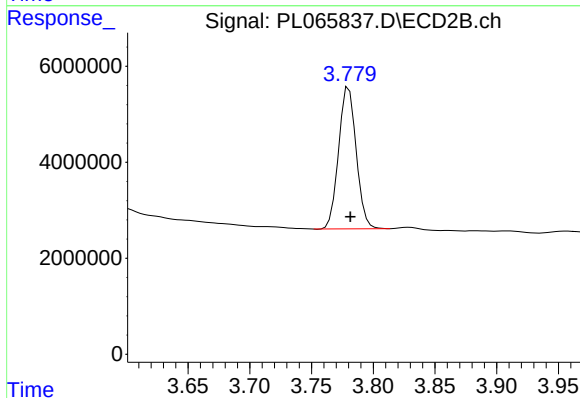


#1 Tetrachloro-m-xylene

R.T.: 3.780 min
Delta R.T.: -0.001 min
Response: 29333809
Conc: 10.69 ng/ml

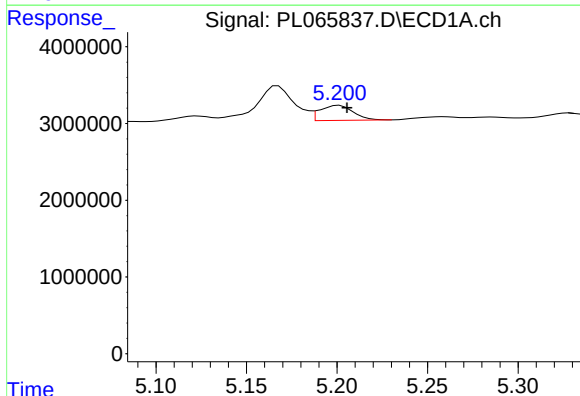


#11 alpha-Chlordane

R.T.: 5.201 min
Delta R.T.: -0.004 min
Response: 2523268
Conc: 0.81 ng/ml

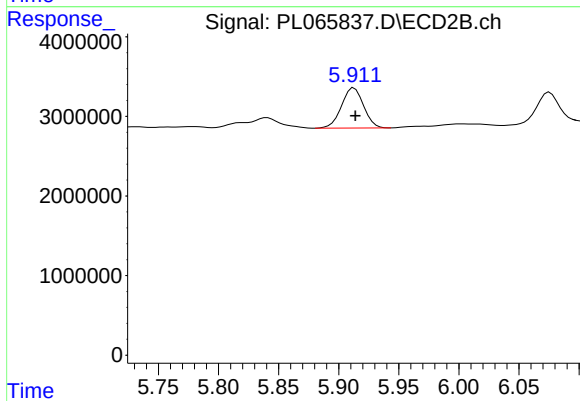

#11 alpha-Chlordane

R.T.: 5.913 min
Delta R.T.: -0.001 min
Response: 6478121
Conc: 2.19 ng/ml

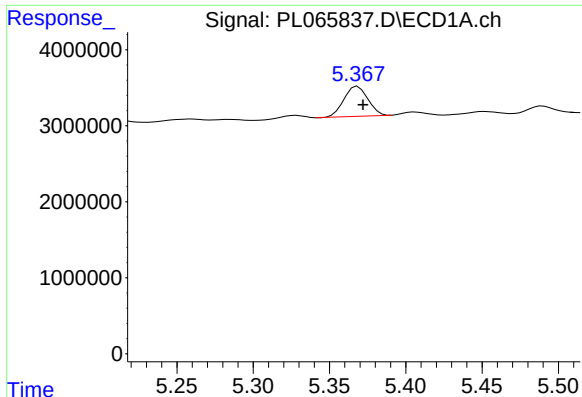


#12 4,4'-DDE

R.T.: 5.369 min
Delta R.T.: -0.004 min
Response: 4296953
Conc: 1.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
CHRT-26586


Manual Integrations
APPROVED

Ankita
4/5/2021 3:35:07 PM

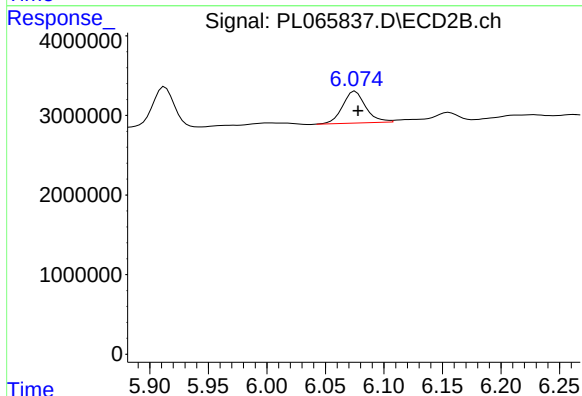


#12 4,4'-DDE

R.T.: 6.076 min
Delta R.T.: -0.003 min
Response: 5507242
Conc: 2.11 ng/ml

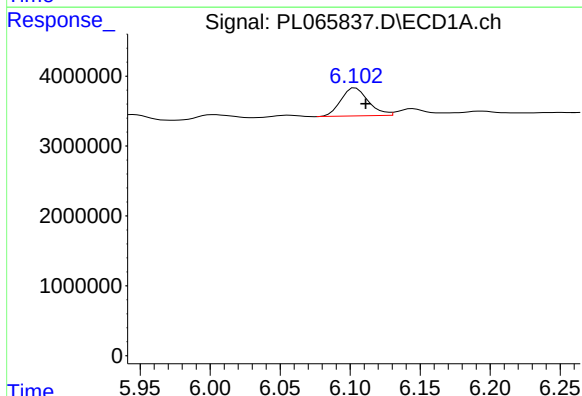


#17 4,4'-DDT

R.T.: 6.104 min
Delta R.T.: -0.007 min
Response: 5480150
Conc: 2.60 ng/ml

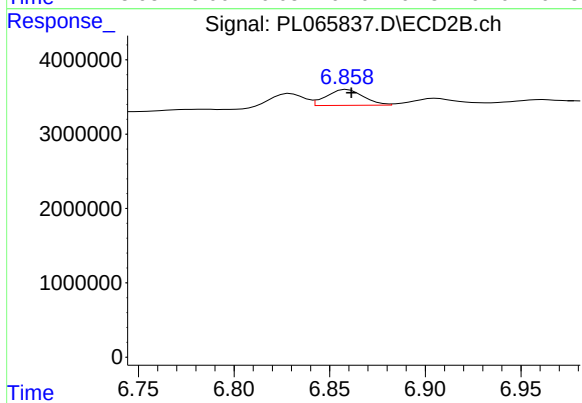

#17 4,4'-DDT

R.T.: 6.858 min
Delta R.T.: -0.004 min
Response: 2831865
Conc: 1.26 ng/ml m

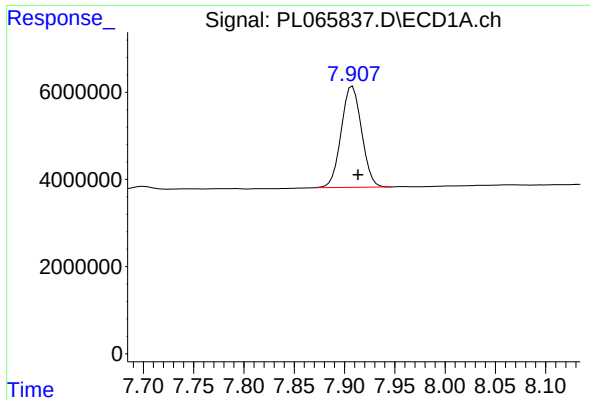


#28 Decachlorobiphenyl

R.T.: 7.908 min
Delta R.T.: -0.006 min
Response: 32657770
Conc: 14.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
CHRT-26586

Manual Integrations
APPROVED

Ankita
4/5/2021 3:35:07 PM

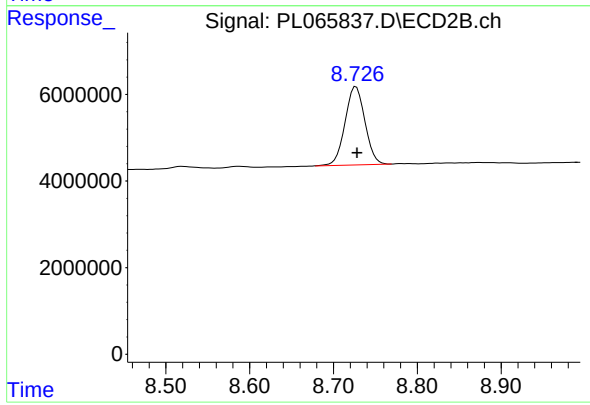

#28 Decachlorobiphenyl

R.T.: 8.727 min
Delta R.T.: -0.001 min
Response: 29848032
Conc: 13.24 ng/ml