

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040221\
 Data File : PL065842.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Apr 2021 17:26
 Operator : AR\AJ
 Sample : M1909-02
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FS-SB-10-26-27

Manual Integrations
 APPROVED

Ankita
 4/5/2021 3:35:15 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 05:04:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 31 15:57:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.283	3.780	65973228	16915175	25.325m	6.162 #
28)	SA Decachlor...	7.909	8.726	27909384	15259997	12.051	6.769 #
Target Compounds							
12)	B 4,4'-DDE	5.382	6.071	4400.0E6	1348.2E6	1594.768	516.042 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040221\
Data File : PL065842.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Apr 2021 17:26
Operator : AR\AJ
Sample : M1909-02
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
FS-SB-10-26-27


Manual Integrations
APPROVED

Ankita
4/5/2021 3:35:15 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 05:04:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
Quant Title : GC Extractables
QLast Update : Wed Mar 31 15:57:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

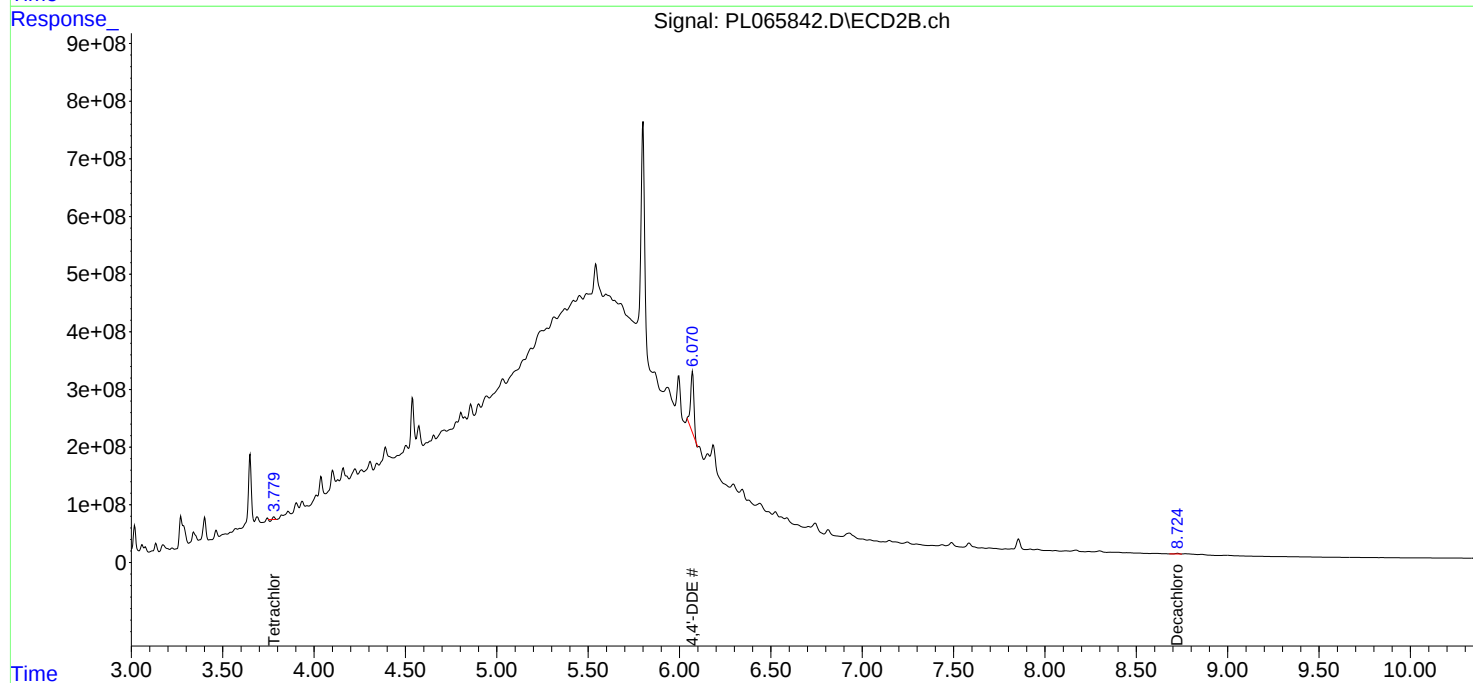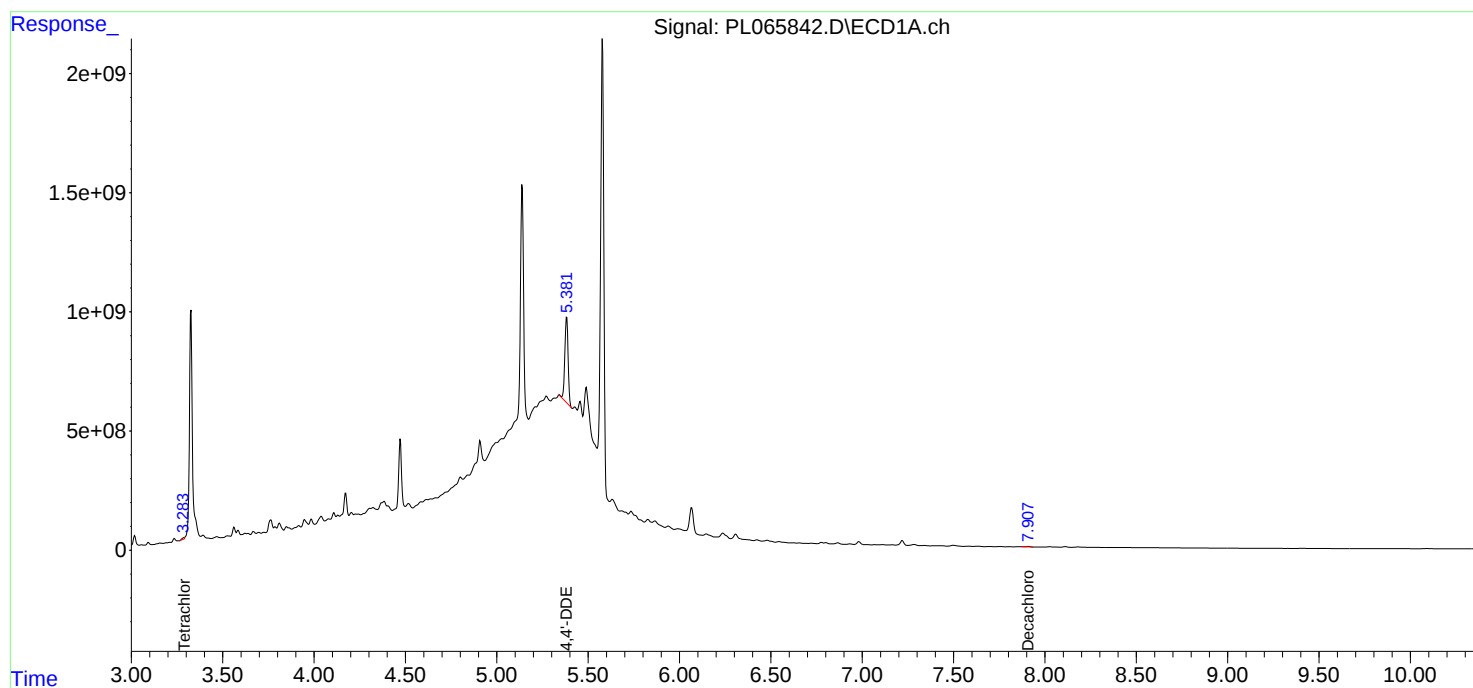

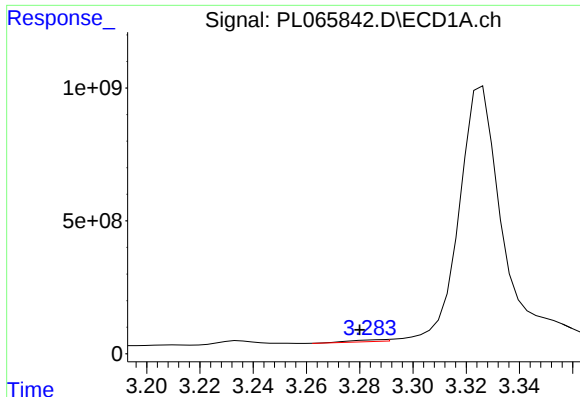


#1 Tetrachloro-m-xylene

R.T.: 3.283 min
Delta R.T.: 0.003 min
Response: 65973228
Conc: 25.33 ng/ml m

Instrument :
ECD_L
ClientSampleId :
FS-SB-10-26-27


Manual Integrations
APPROVED

Ankita
4/5/2021 3:35:15 PM

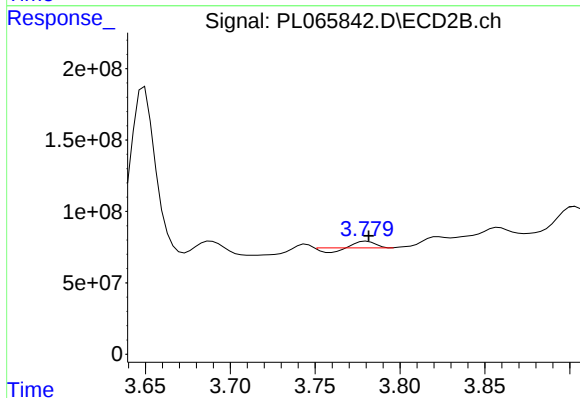


#1 Tetrachloro-m-xylene

R.T.: 3.780 min
Delta R.T.: -0.001 min
Response: 16915175
Conc: 6.16 ng/ml

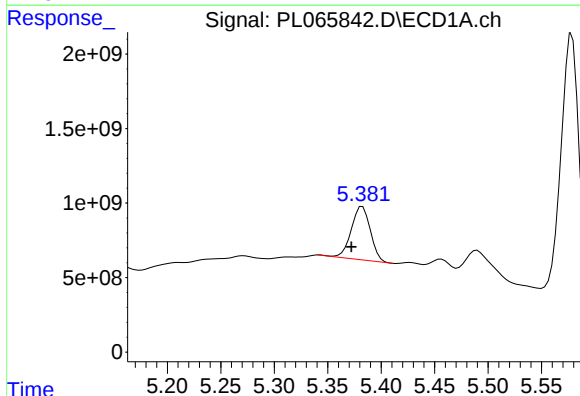


#12 4,4'-DDE

R.T.: 5.382 min
Delta R.T.: 0.010 min
Response: 4400008491
Conc: 1594.77 ng/ml

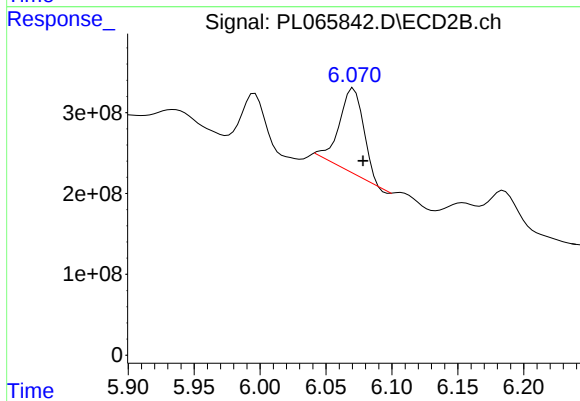

#12 4,4'-DDE

R.T.: 6.071 min
Delta R.T.: -0.007 min
Response: 1348178522
Conc: 516.04 ng/ml

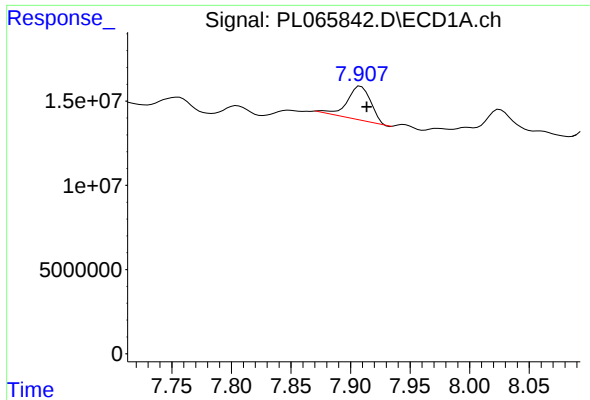


#28 Decachlorobiphenyl

R.T.: 7.909 min
Delta R.T.: -0.005 min
Response: 27909384
Conc: 12.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
FS-SB-10-26-27

Manual Integrations
APPROVED

Ankita
4/5/2021 3:35:15 PM

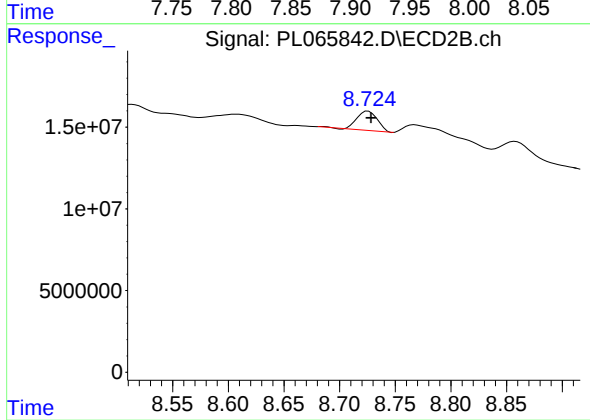

#28 Decachlorobiphenyl

R.T.: 8.726 min
Delta R.T.: -0.002 min
Response: 15259997
Conc: 6.77 ng/ml