

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040224\
 Data File : PL088870.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Apr 2024 10:50
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 01:13:37 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031324.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 13 15:45:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.638	2.851	116.0E6	77842828	43.778	58.408 #
28)	SA Decachlor...	9.305	8.079	101.6E6	68017149	41.093	50.163
Target Compounds							
23)	Chlordane-1	4.822	3.873	50659806	23037815	435.658	474.465
24)	Chlordane-2	5.358	4.460	56648476	29164667	430.890	480.351
25)	Chlordane-3	6.079	5.101	213.0E6	84007926	428.332	492.222
26)	Chlordane-4	6.162	5.165	257.0E6	78405974	428.483	491.451
27)	Chlordane-5	7.022	5.841	45668587	25153608	432.042	495.976



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040224\
Data File : PL088870.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Apr 2024 10:50
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 01:13:37 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031324.M
Quant Title : GC Extractables
QLast Update : Wed Mar 13 15:45:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

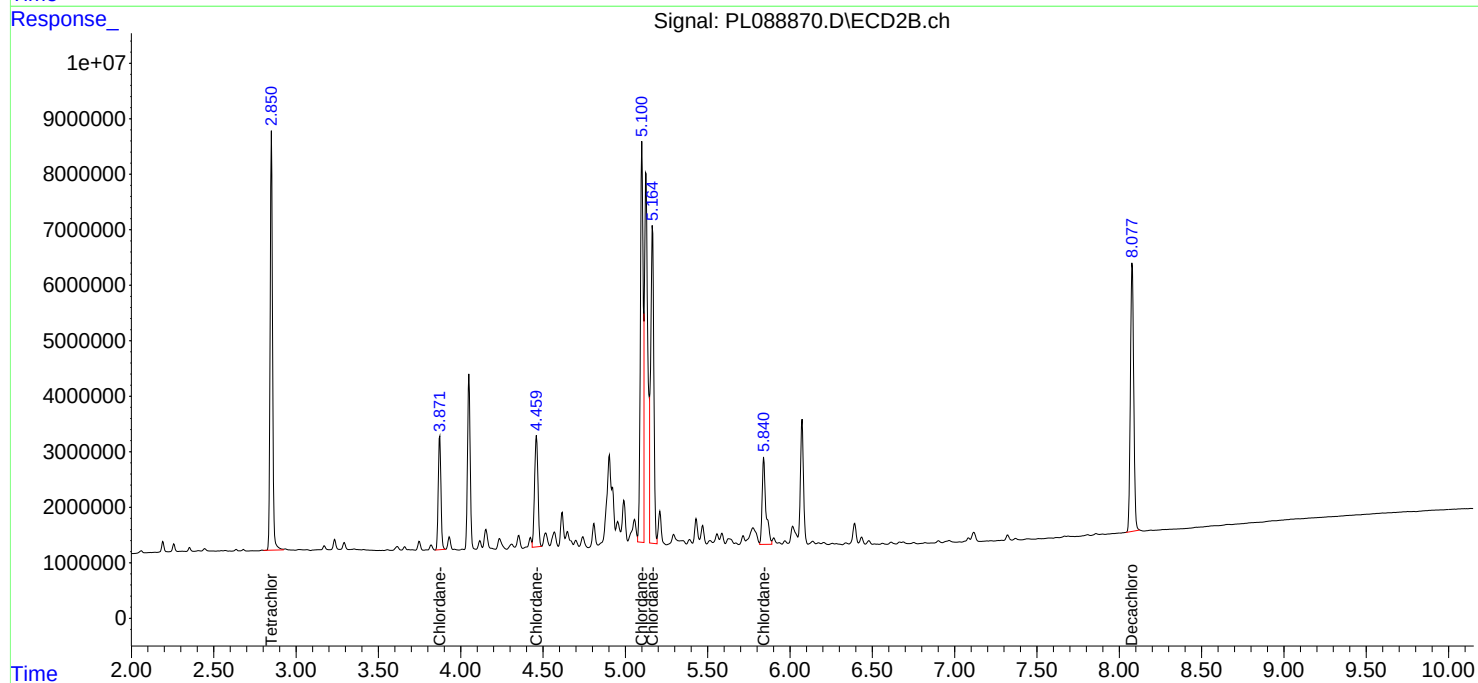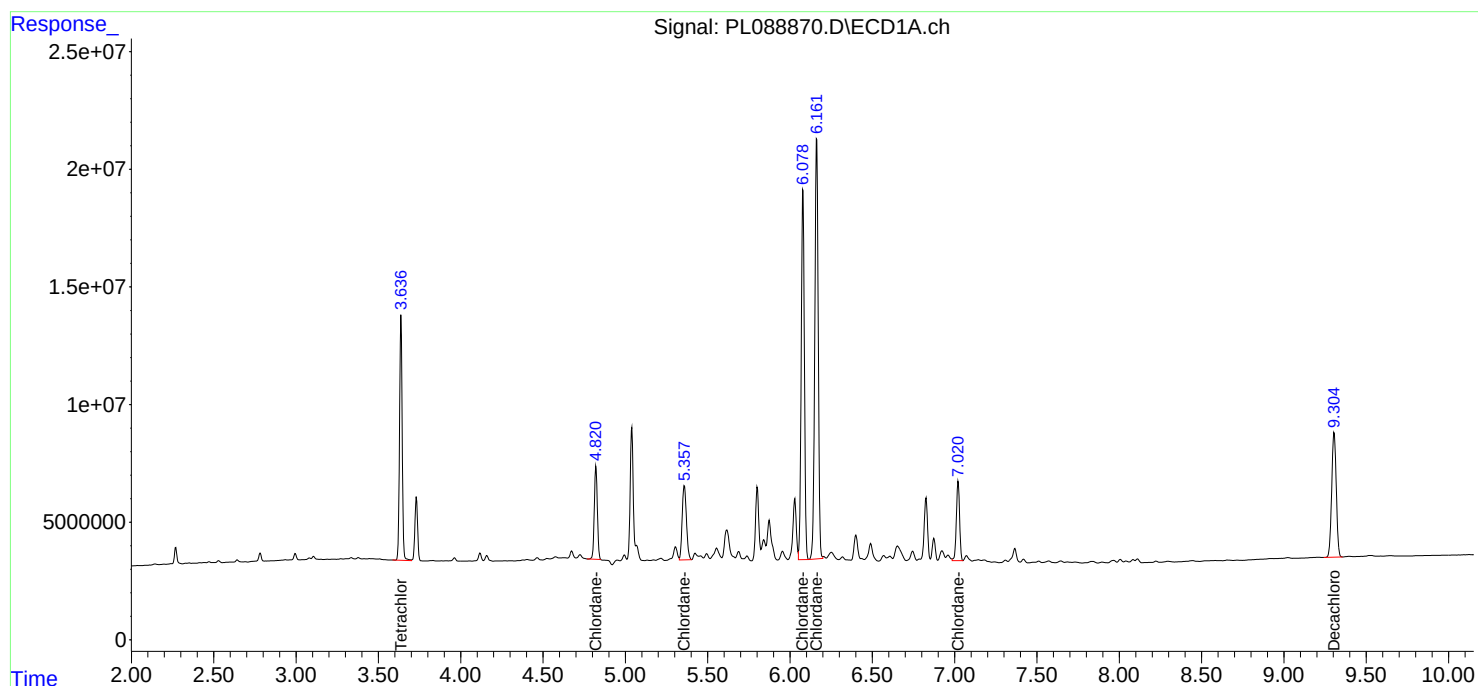


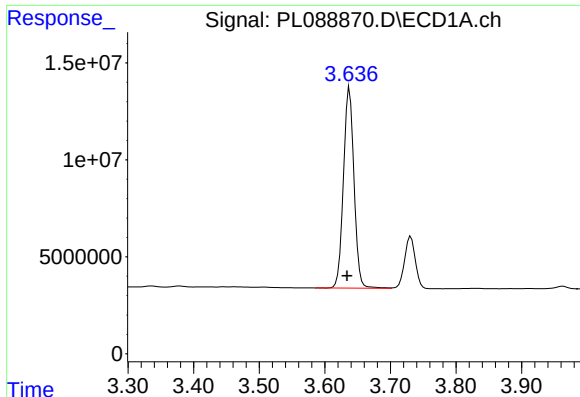

#1 Tetrachloro-m-xylene


R.T.: 3.638 min
Delta R.T.: 0.004 min
Response: 116009639
Conc: 43.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

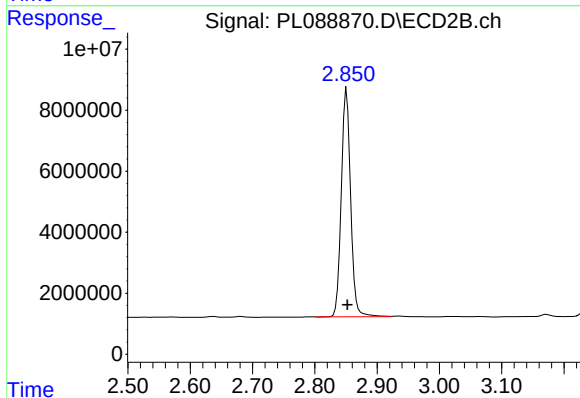


#1 Tetrachloro-m-xylene

R.T.: 2.851 min
Delta R.T.: -0.001 min
Response: 77842828
Conc: 58.41 ng/ml

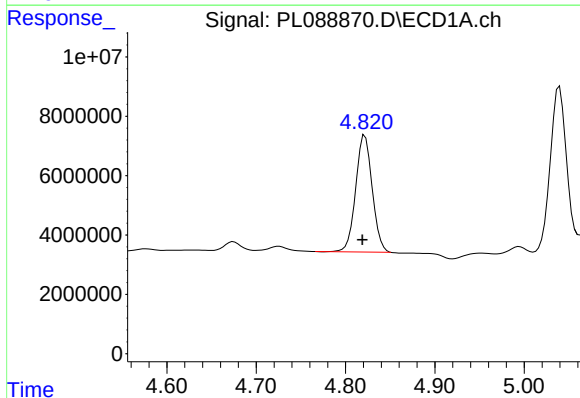


#23 Chlordane-1

R.T.: 4.822 min
Delta R.T.: 0.003 min
Response: 50659806
Conc: 435.66 ng/ml

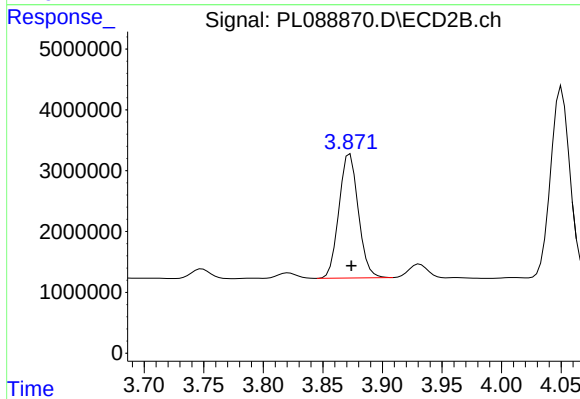

#23 Chlordane-1


R.T.: 3.873 min
Delta R.T.: -0.001 min
Response: 23037815
Conc: 474.47 ng/ml

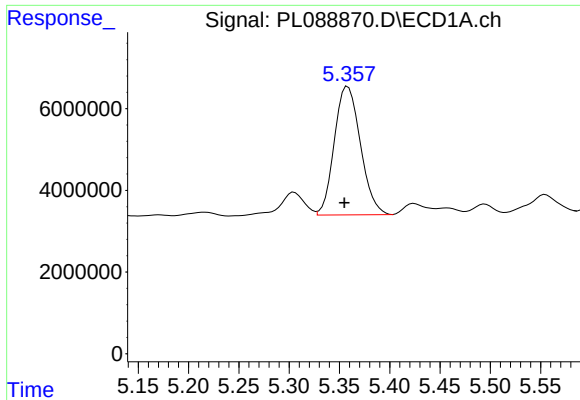

#24 Chlordane-2


R.T.: 5.358 min
Delta R.T.: 0.003 min
Response: 56648476
Conc: 430.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

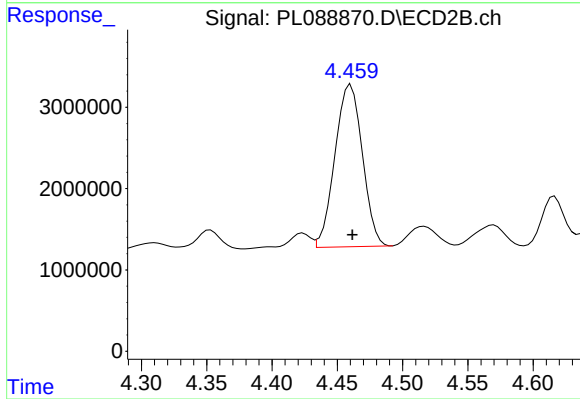


#24 Chlordane-2

R.T.: 4.460 min
Delta R.T.: -0.001 min
Response: 29164667
Conc: 480.35 ng/ml

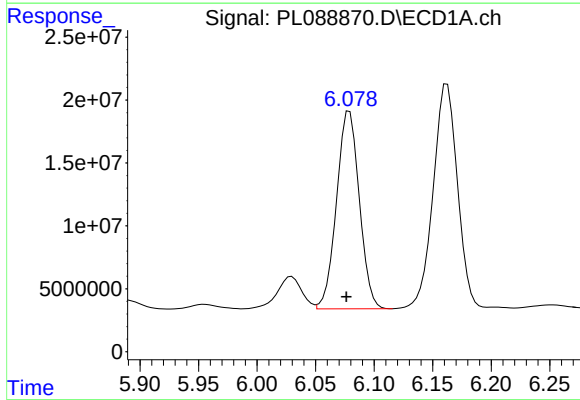


#25 Chlordane-3

R.T.: 6.079 min
Delta R.T.: 0.003 min
Response: 212981911
Conc: 428.33 ng/ml

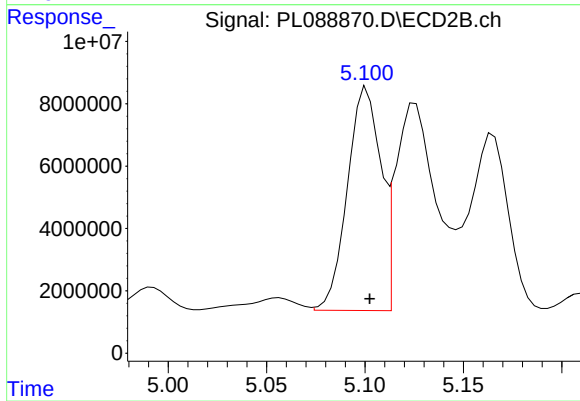

#25 Chlordane-3


R.T.: 5.101 min
Delta R.T.: -0.001 min
Response: 84007926
Conc: 492.22 ng/ml

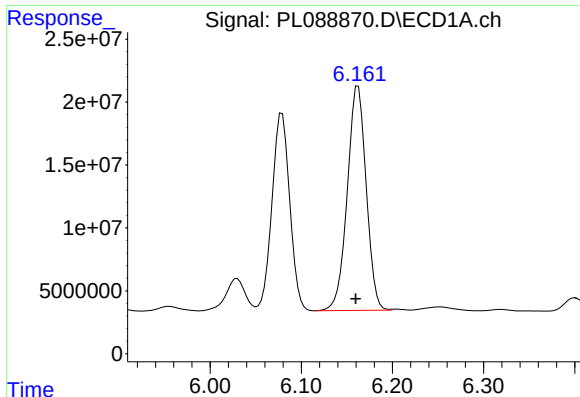

#26 Chlordane-4


R.T.: 6.162 min
Delta R.T.: 0.003 min
Response: 257032567
Conc: 428.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

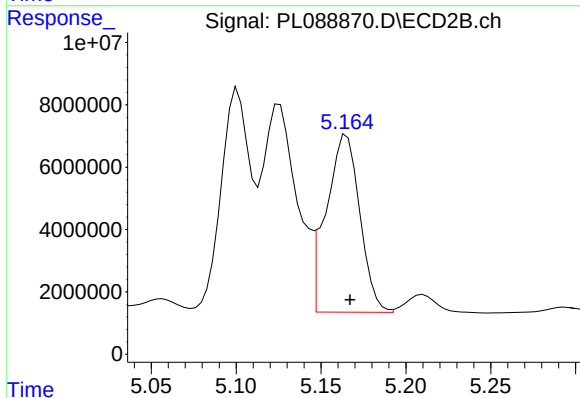


#26 Chlordane-4

R.T.: 5.165 min
Delta R.T.: -0.002 min
Response: 78405974
Conc: 491.45 ng/ml

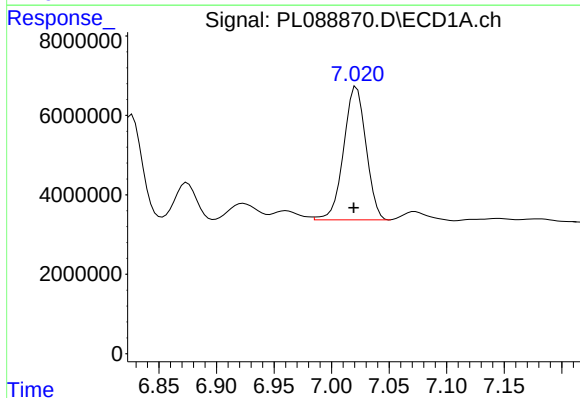


#27 Chlordane-5

R.T.: 7.022 min
Delta R.T.: 0.002 min
Response: 45668587
Conc: 432.04 ng/ml

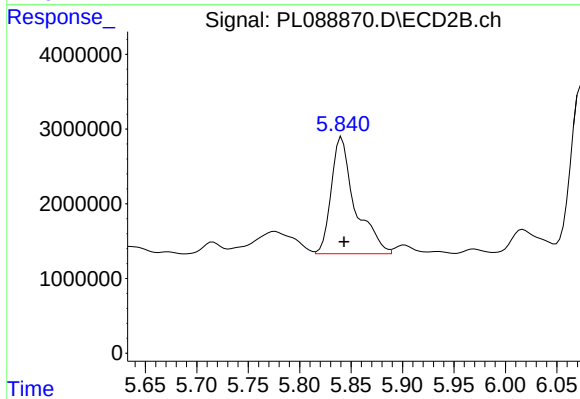

#27 Chlordane-5


R.T.: 5.841 min
Delta R.T.: -0.002 min
Response: 25153608
Conc: 495.98 ng/ml

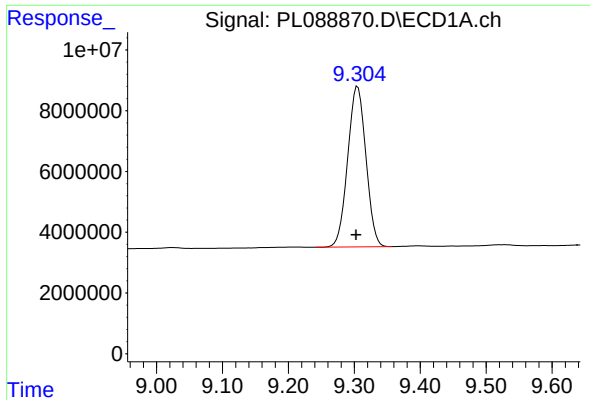

#28 Decachlorobiphenyl

R.T.: 9.305 min
Delta R.T.: 0.002 min
Response: 101578340
Conc: 41.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

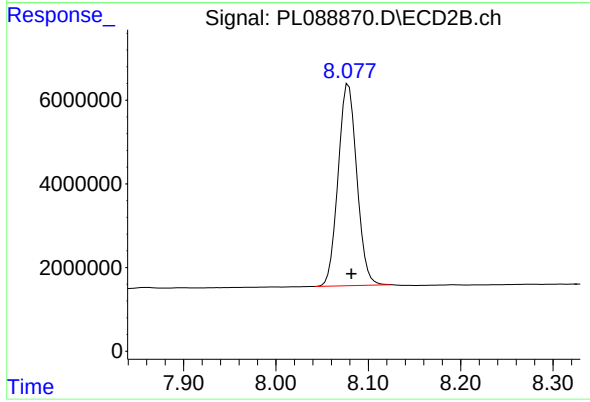

#28 Decachlorobiphenyl

R.T.: 8.079 min
Delta R.T.: -0.003 min
Response: 68017149
Conc: 50.16 ng/ml