

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040224\
 Data File : PL088877.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Apr 2024 12:54
 Operator : AR\AJ
 Sample : PB159873BS
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB159873BS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 01:15:14 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031324.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 13 15:45:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.641	2.852	52334085	34502621	19.749	25.888 #
28)	SA Decachlor...	9.309	8.082	46007297	30912872	18.612	22.798
Target Compounds							
23)	Chlordane-1	4.825	3.874	25982184	12071451	223.438	248.612
24)	Chlordane-2	5.361	4.461	30755532	15186303	233.939	250.123
25)	Chlordane-3	6.081	5.102	110.9E6	40859323	223.034	239.404
26)	Chlordane-4	6.164	5.166	136.0E6	38000184	226.700	238.186
27)	Chlordane-5	7.024	5.843	24472206	12980136	231.516	255.941



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040224\
Data File : PL088877.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Apr 2024 12:54
Operator : AR\AJ
Sample : PB159873BS
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB159873BS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 01:15:14 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031324.M
Quant Title : GC Extractables
QLast Update : Wed Mar 13 15:45:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

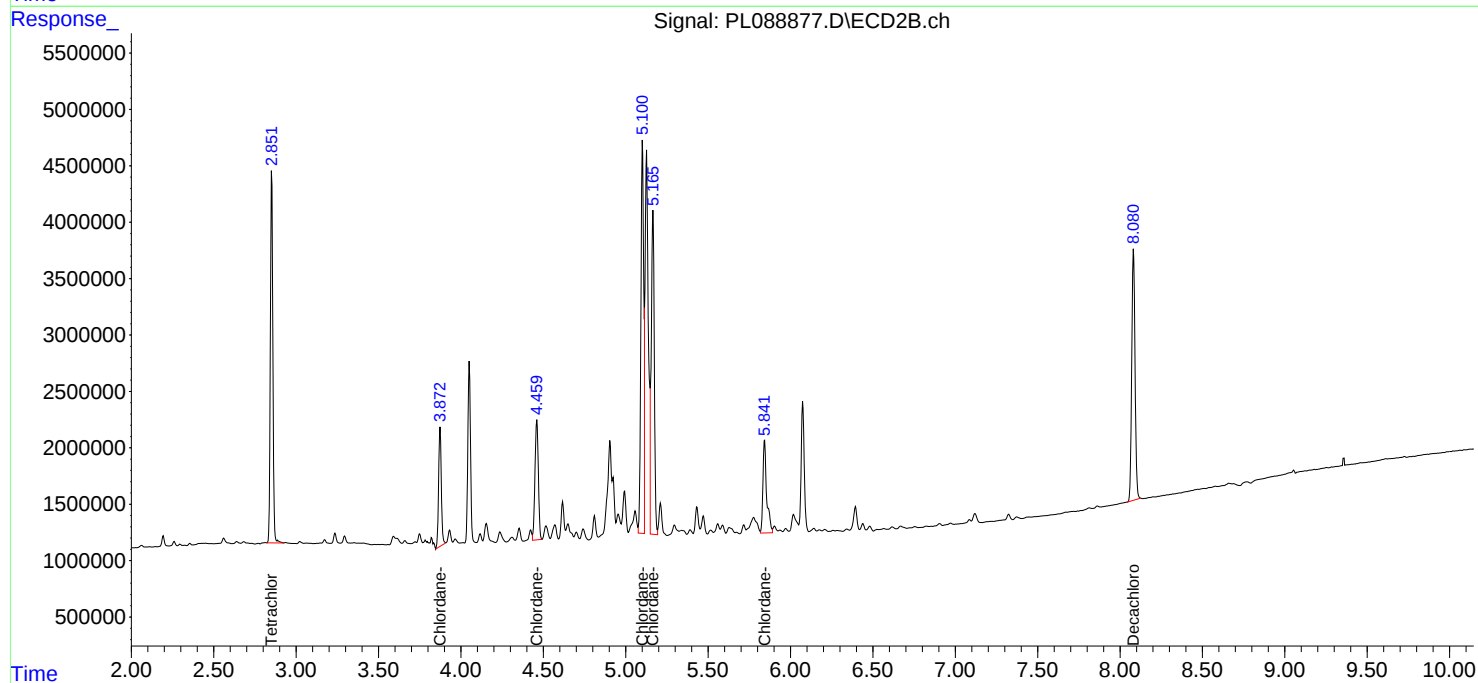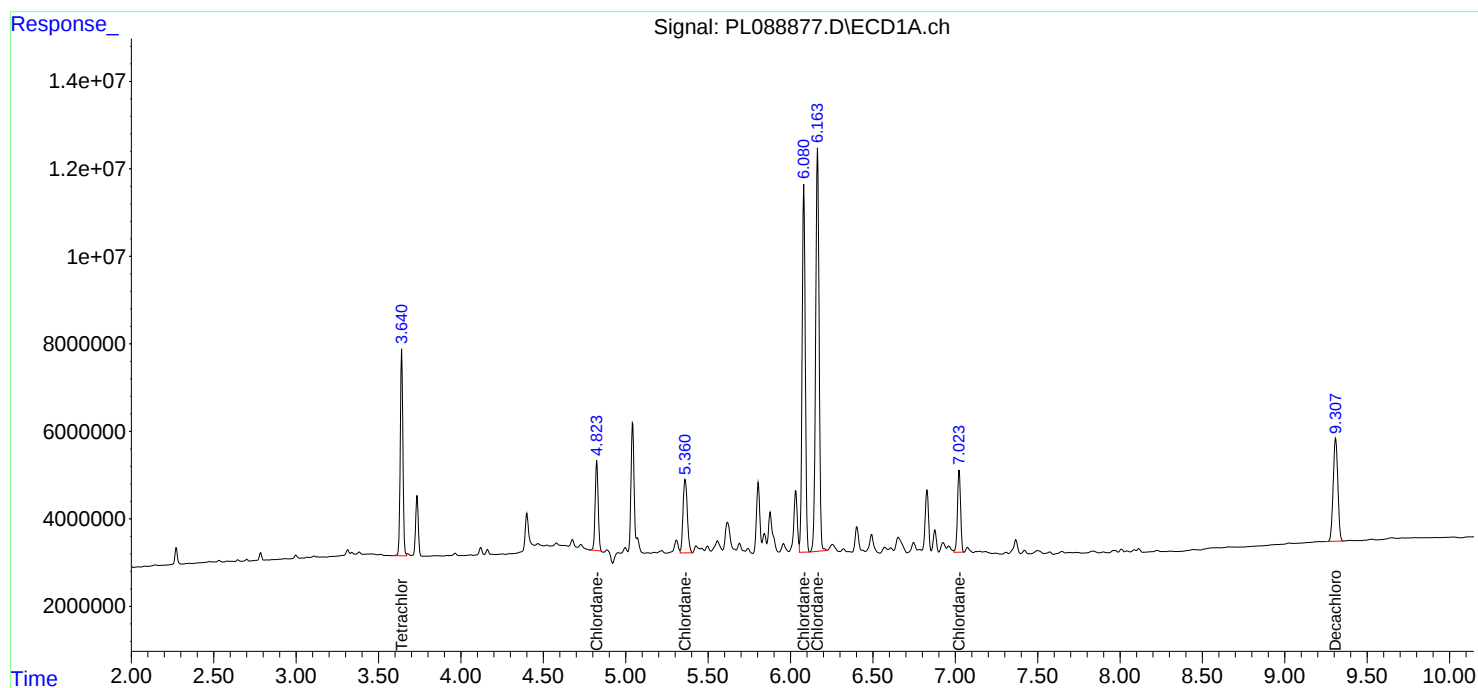


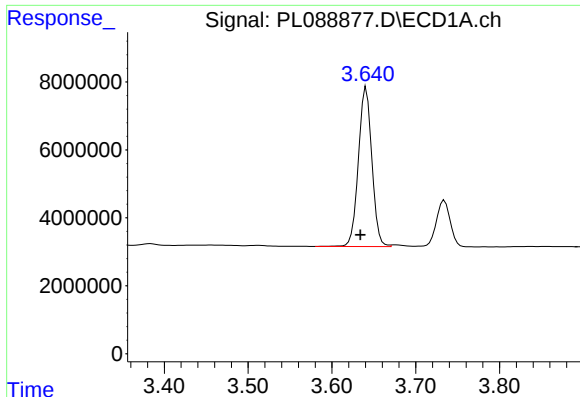

#1 Tetrachloro-m-xylene


R.T.: 3.641 min
Delta R.T.: 0.007 min
Response: 52334085
Conc: 19.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB159873BS

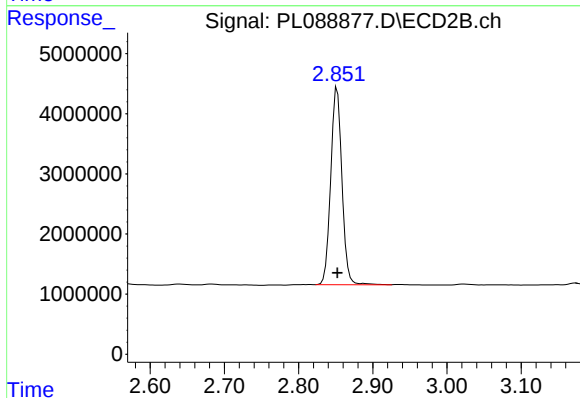


#1 Tetrachloro-m-xylene

R.T.: 2.852 min
Delta R.T.: 0.000 min
Response: 34502621
Conc: 25.89 ng/ml

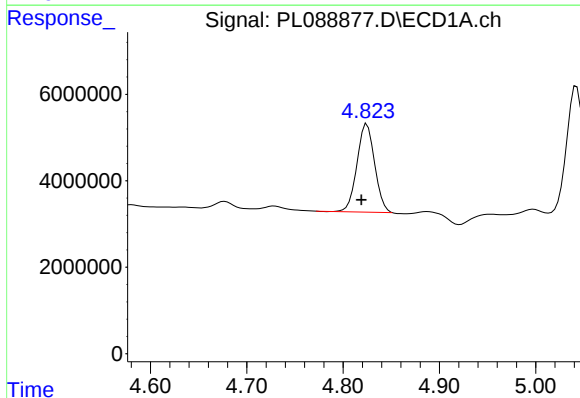


#23 Chlordane-1

R.T.: 4.825 min
Delta R.T.: 0.006 min
Response: 25982184
Conc: 223.44 ng/ml

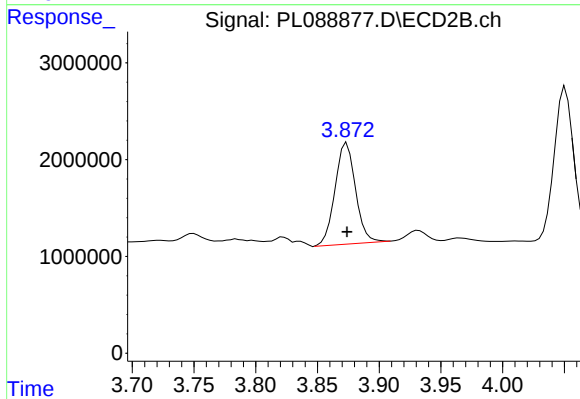

#23 Chlordane-1


R.T.: 3.874 min
Delta R.T.: 0.000 min
Response: 12071451
Conc: 248.61 ng/ml

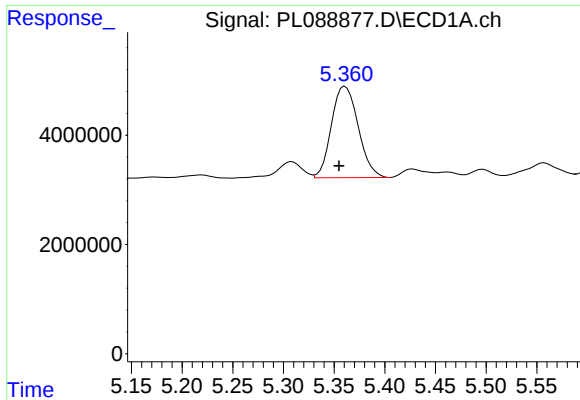

#24 Chlordane-2


R.T.: 5.361 min
Delta R.T.: 0.006 min
Response: 30755532
Conc: 233.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB159873BS

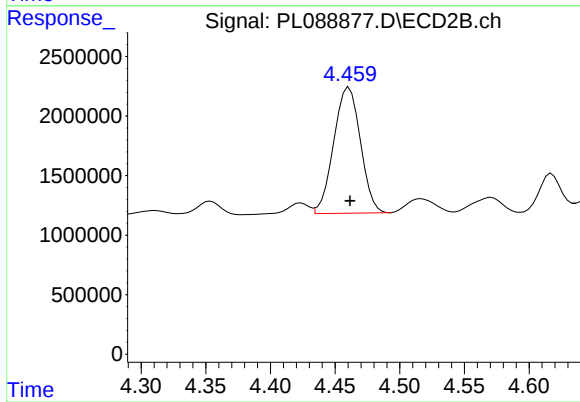


#24 Chlordane-2

R.T.: 4.461 min
Delta R.T.: 0.000 min
Response: 15186303
Conc: 250.12 ng/ml

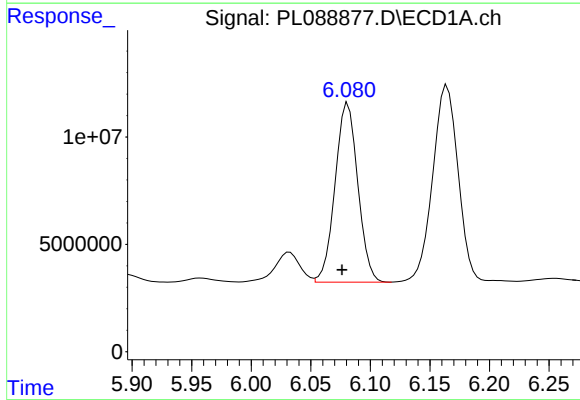


#25 Chlordane-3

R.T.: 6.081 min
Delta R.T.: 0.005 min
Response: 110900266
Conc: 223.03 ng/ml

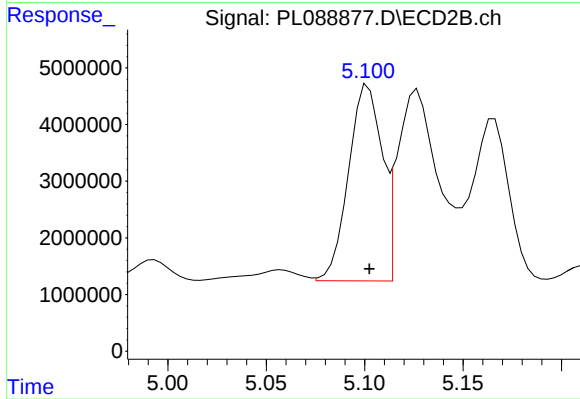

#25 Chlordane-3


R.T.: 5.102 min
Delta R.T.: 0.000 min
Response: 40859323
Conc: 239.40 ng/ml

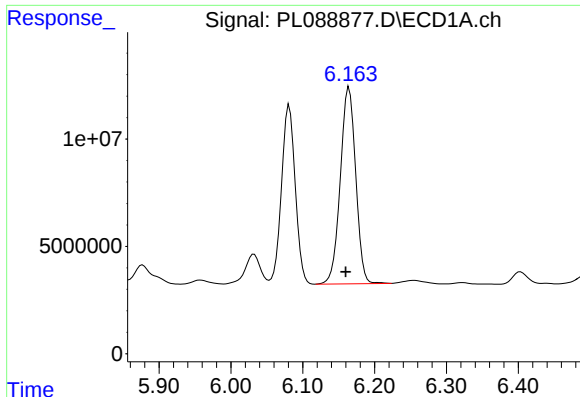

#26 Chlordane-4


R.T.: 6.164 min
Delta R.T.: 0.005 min
Response: 135989864
Conc: 226.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB159873BS

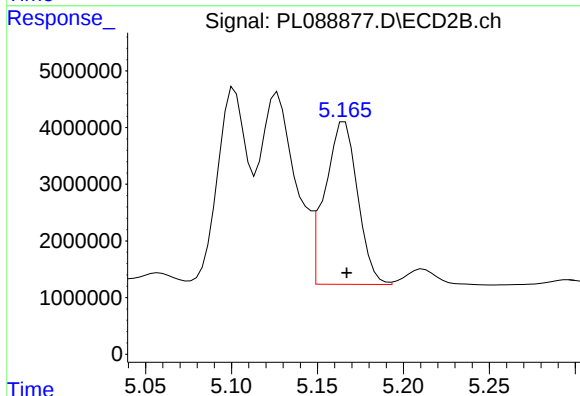


#26 Chlordane-4

R.T.: 5.166 min
Delta R.T.: -0.001 min
Response: 38000184
Conc: 238.19 ng/ml

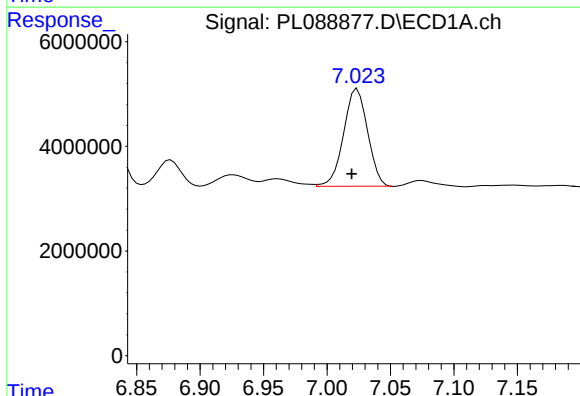


#27 Chlordane-5

R.T.: 7.024 min
Delta R.T.: 0.004 min
Response: 24472206
Conc: 231.52 ng/ml

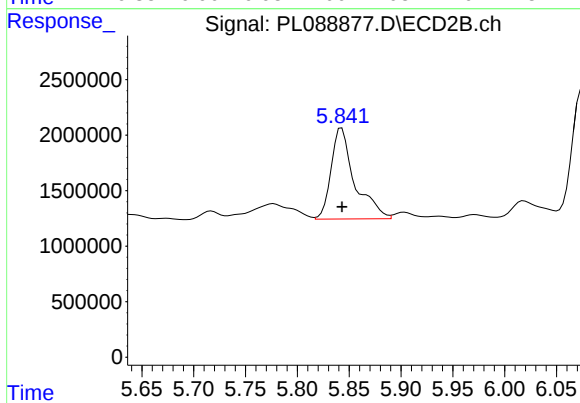

#27 Chlordane-5


R.T.: 5.843 min
Delta R.T.: 0.000 min
Response: 12980136
Conc: 255.94 ng/ml

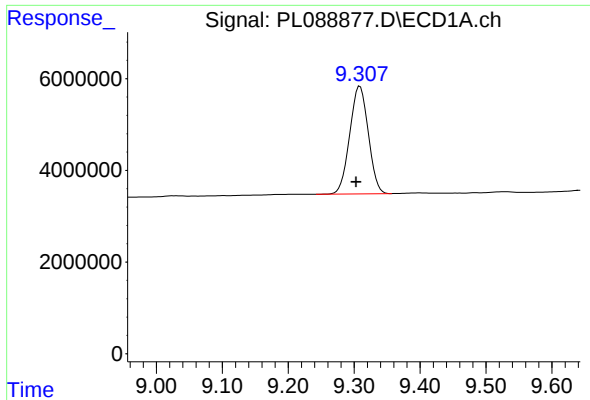

#28 Decachlorobiphenyl

R.T.: 9.309 min
Delta R.T.: 0.006 min
Response: 46007297
Conc: 18.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB159873BS

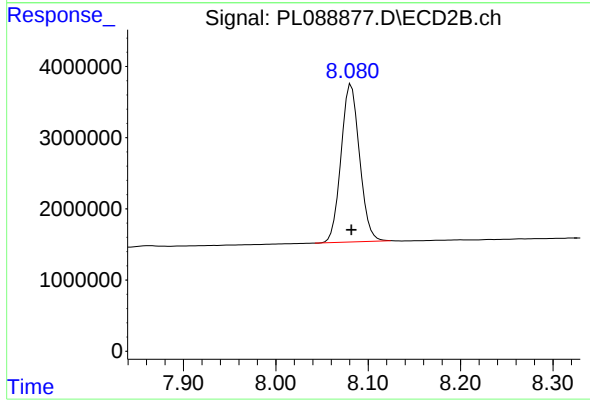

#28 Decachlorobiphenyl

R.T.: 8.082 min
Delta R.T.: 0.000 min
Response: 30912872
Conc: 22.80 ng/ml