

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040224\
 Data File : PL088878.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Apr 2024 13:08
 Operator : AR\AJ
 Sample : P1908-11
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PT-CHLR-WP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 01:15:27 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031324.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 13 15:45:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.634	2.850	59601027	53035775	22.491	39.795 #
28)	SA Decachlor...	9.300	8.078	47547764	33815814	19.235	24.939 #
Target Compounds							
23)	Chlordane-1	4.818	3.872	238.8E6	115.4E6	2053.256	2375.898
24)	Chlordane-2	5.355	4.458	236.0E6	122.5E6	1795.080	2017.646
25)	Chlordane-3	6.075	5.099	872.8E6	392.8E6	1755.223	2301.671 #
26)	Chlordane-4	6.158	5.164	1010.6E6	376.2E6	1684.679	2357.815 #
27)	Chlordane-5	7.018	5.840	197.7E6	68865690	1870.544	1357.886 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040224\
Data File : PL088878.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Apr 2024 13:08
Operator : AR\AJ
Sample : P1908-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PT-CHLR-WP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 01:15:27 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031324.M
Quant Title : GC Extractables
QLast Update : Wed Mar 13 15:45:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

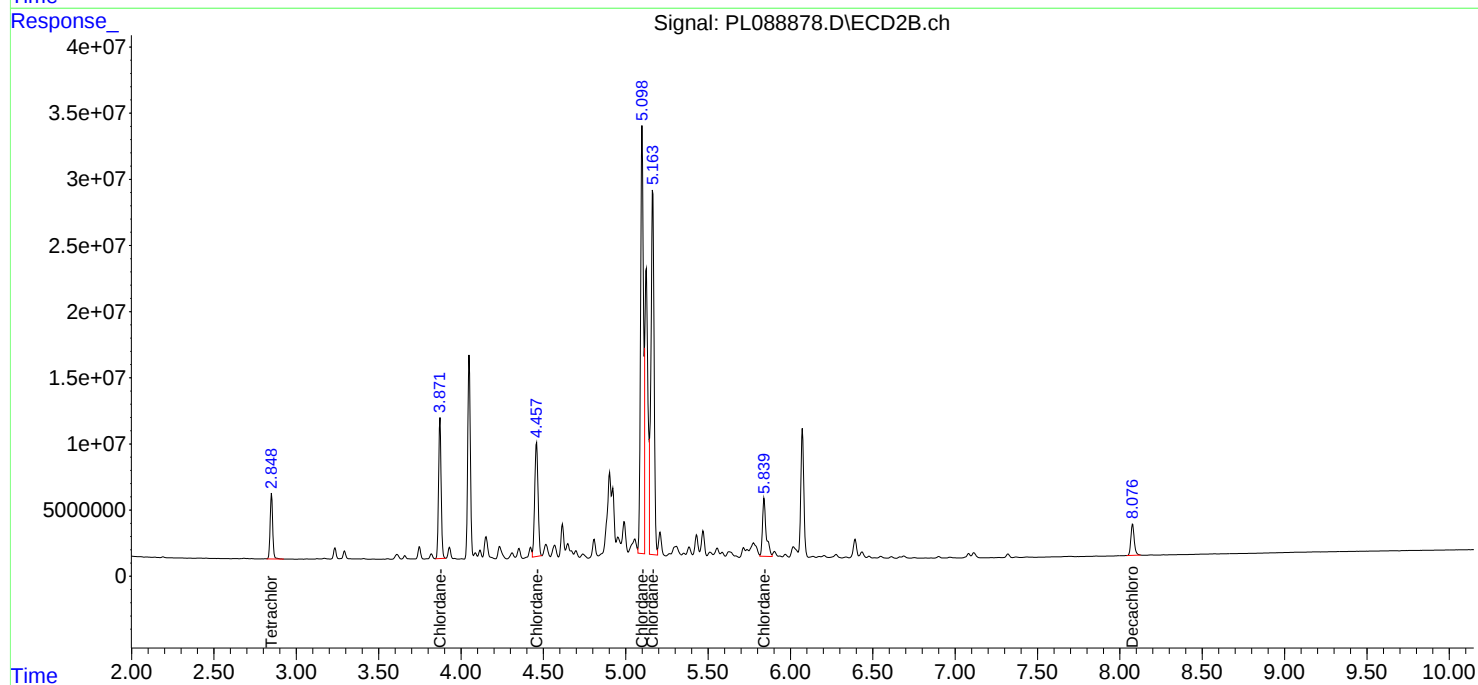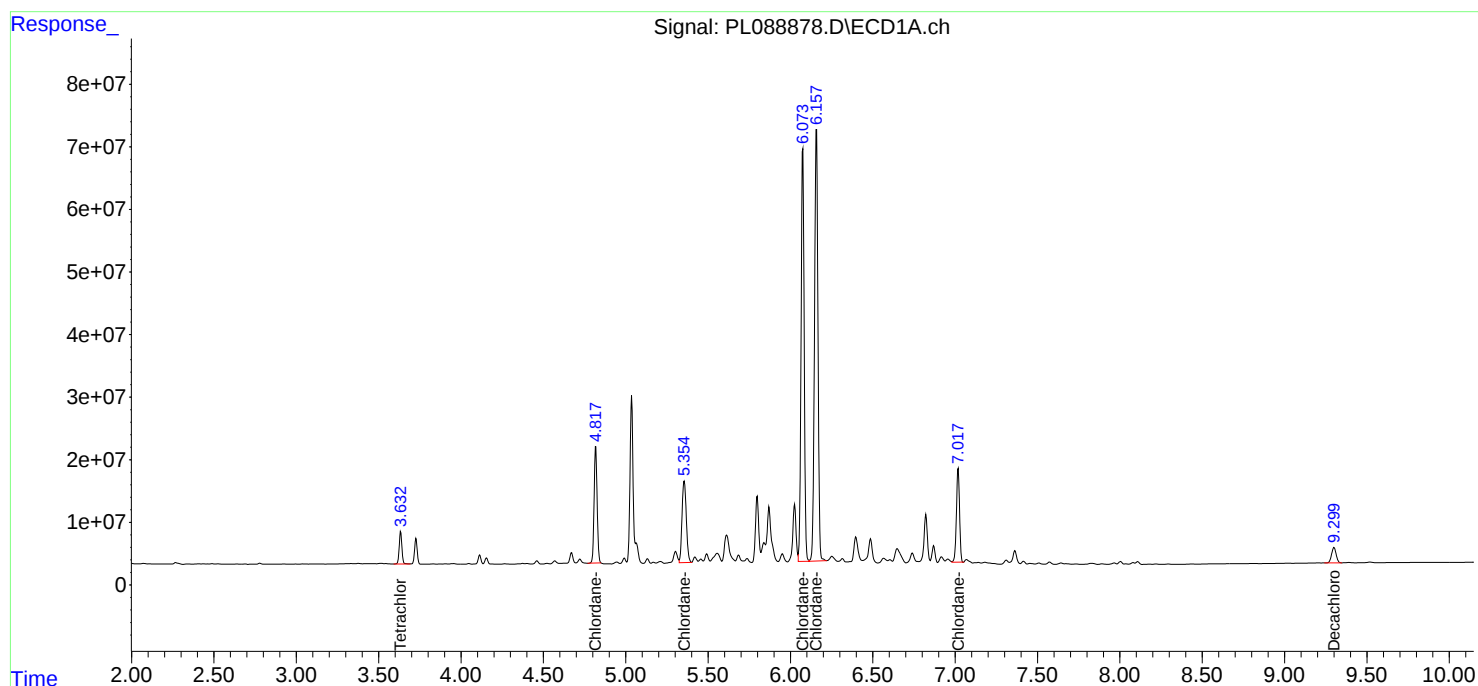


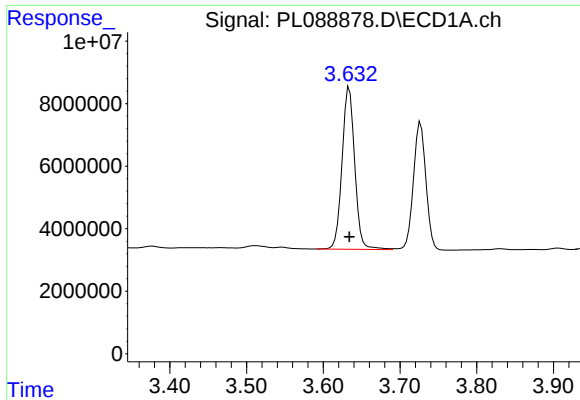

#1 Tetrachloro-m-xylene


R.T.: 3.634 min
Delta R.T.: 0.000 min
Response: 59601027
Conc: 22.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
PT-CHLR-WP

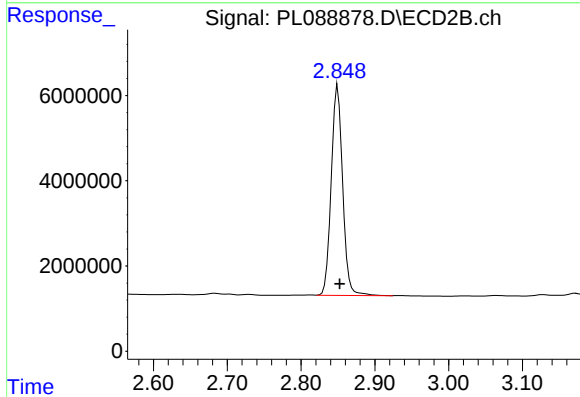


#1 Tetrachloro-m-xylene

R.T.: 2.850 min
Delta R.T.: -0.003 min
Response: 53035775
Conc: 39.79 ng/ml

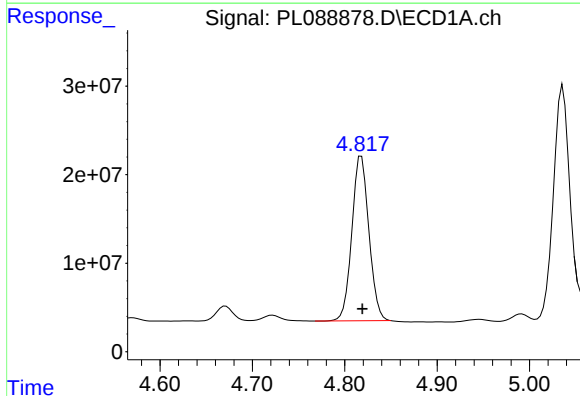


#23 Chlordane-1

R.T.: 4.818 min
Delta R.T.: -0.001 min
Response: 238759677
Conc: 2053.26 ng/ml

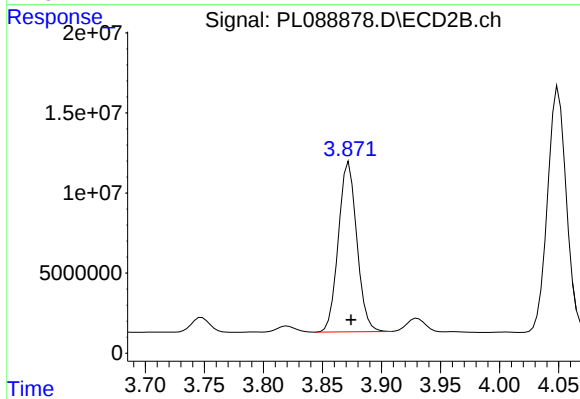

#23 Chlordane-1


R.T.: 3.872 min
Delta R.T.: -0.002 min
Response: 115362561
Conc: 2375.90 ng/ml

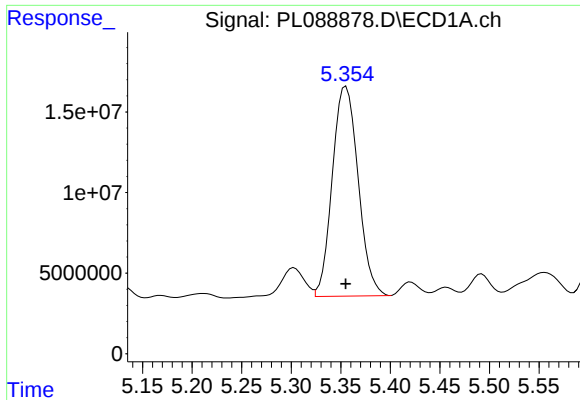

#24 Chlordane-2


R.T.: 5.355 min
Delta R.T.: 0.000 min
Response: 235996320
Conc: 1795.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
PT-CHLR-WP

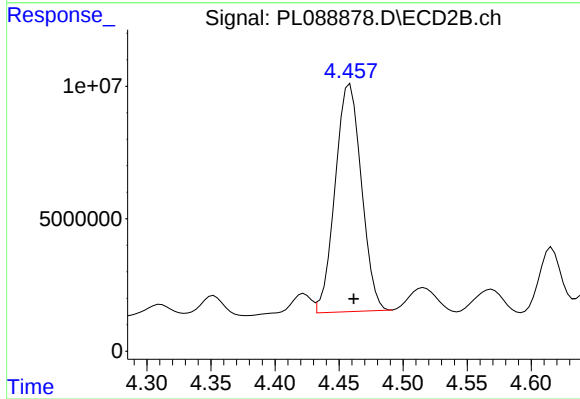


#24 Chlordane-2

R.T.: 4.458 min
Delta R.T.: -0.003 min
Response: 122502092
Conc: 2017.65 ng/ml

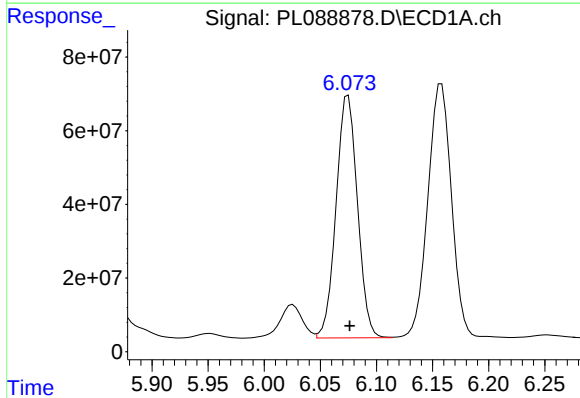


#25 Chlordane-3

R.T.: 6.075 min
Delta R.T.: -0.001 min
Response: 872759875
Conc: 1755.22 ng/ml

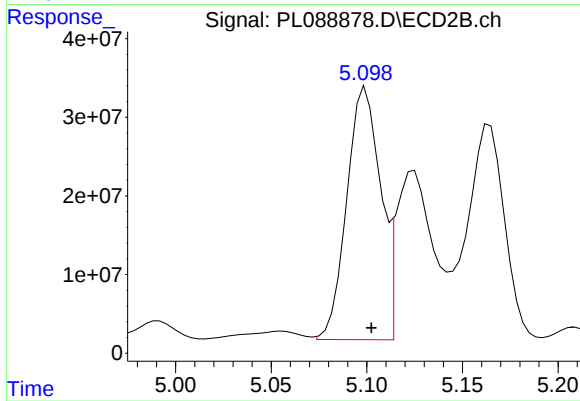

#25 Chlordane-3


R.T.: 5.099 min
Delta R.T.: -0.003 min
Response: 392827799
Conc: 2301.67 ng/ml

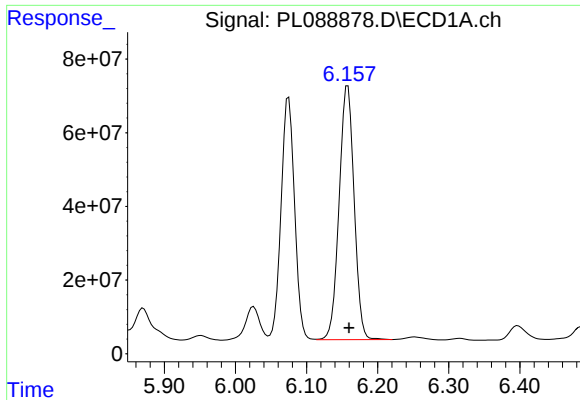

#26 Chlordane-4


R.T.: 6.158 min
Delta R.T.: -0.002 min
Response: 1010583215
Conc: 1684.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
PT-CHLR-WP

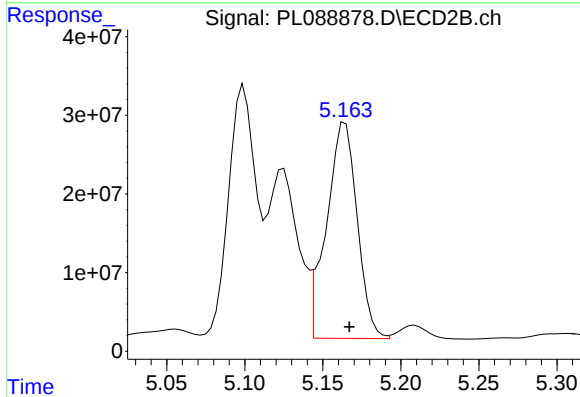


#26 Chlordane-4

R.T.: 5.164 min
Delta R.T.: -0.003 min
Response: 376165394
Conc: 2357.81 ng/ml

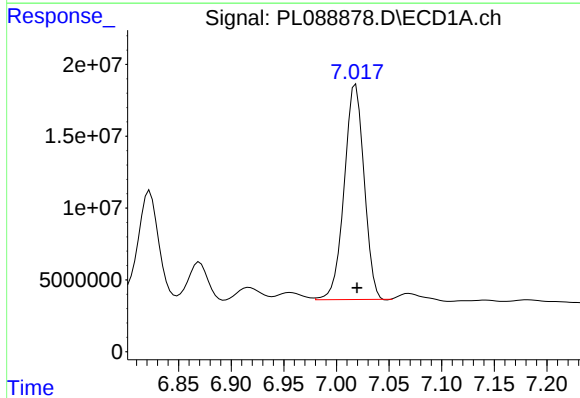


#27 Chlordane-5

R.T.: 7.018 min
Delta R.T.: -0.001 min
Response: 197724115
Conc: 1870.54 ng/ml

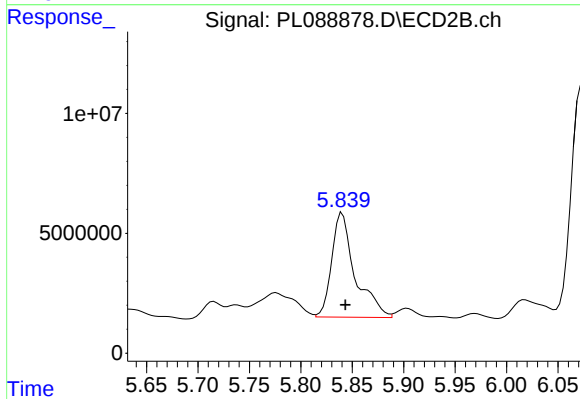

#27 Chlordane-5


R.T.: 5.840 min
Delta R.T.: -0.003 min
Response: 68865690
Conc: 1357.89 ng/ml

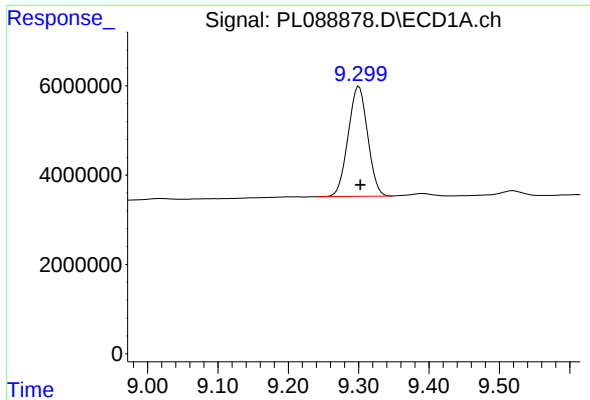

#28 Decachlorobiphenyl

R.T.: 9.300 min
Delta R.T.: -0.002 min
Response: 47547764
Conc: 19.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
PT-CHLR-WP

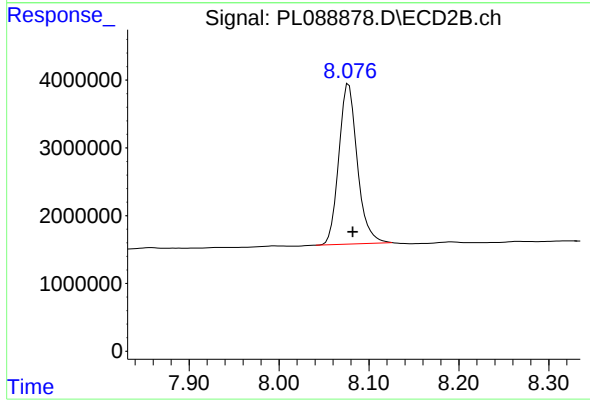

#28 Decachlorobiphenyl

R.T.: 8.078 min
Delta R.T.: -0.004 min
Response: 33815814
Conc: 24.94 ng/ml