

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040224\
 Data File : PL088882.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Apr 2024 14:03
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 01:16:20 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031324.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 13 15:45:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.634	2.851	112.0E6	74819098	42.271	56.139 #
28)	SA Decachlor...	9.300	8.078	99373337	67067397	40.201	49.463
Target Compounds							
23)	Chlordane-1	4.818	3.872	49363038	22315336	424.506	459.586
24)	Chlordane-2	5.354	4.459	55509979	28467736	422.231	468.872
25)	Chlordane-3	6.074	5.100	208.8E6	81676825	419.912	478.564
26)	Chlordane-4	6.158	5.164	252.3E6	75067772	420.608	470.527
27)	Chlordane-5	7.018	5.840	44739900	24601460	423.256	485.089

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040224\
Data File : PL088882.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Apr 2024 14:03
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e

Integration File signal 2: autoint2.e

Quant Time: Apr 03 01:16:20 2024

Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031324.M

Quant Title : GC Extractables

QLast Update : Wed Mar 13 15:45:55 2024

Response via : Initial Calibration



Integrator: ChemStation


Volume Inj. : 1 µl

Signal #1 Phase : ZB-MR2

Signal #2 Phase: ZB-MR1

Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

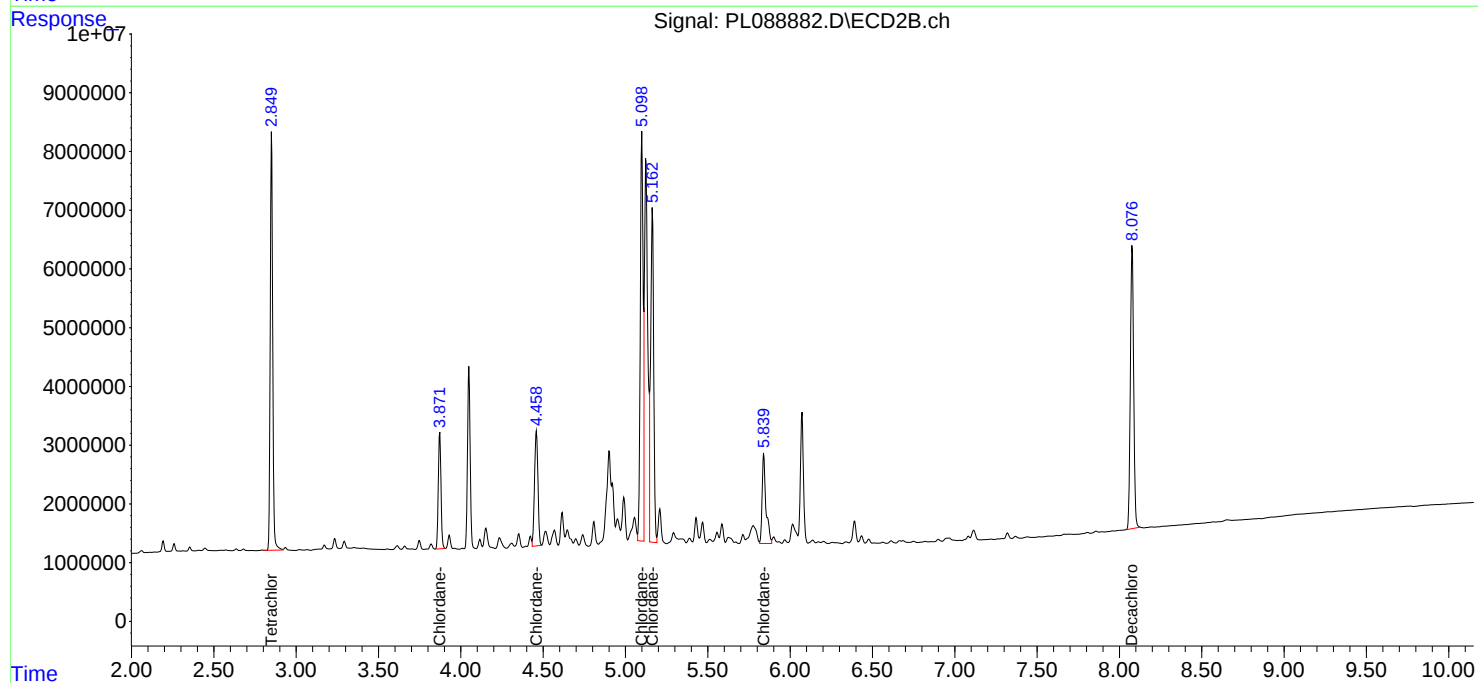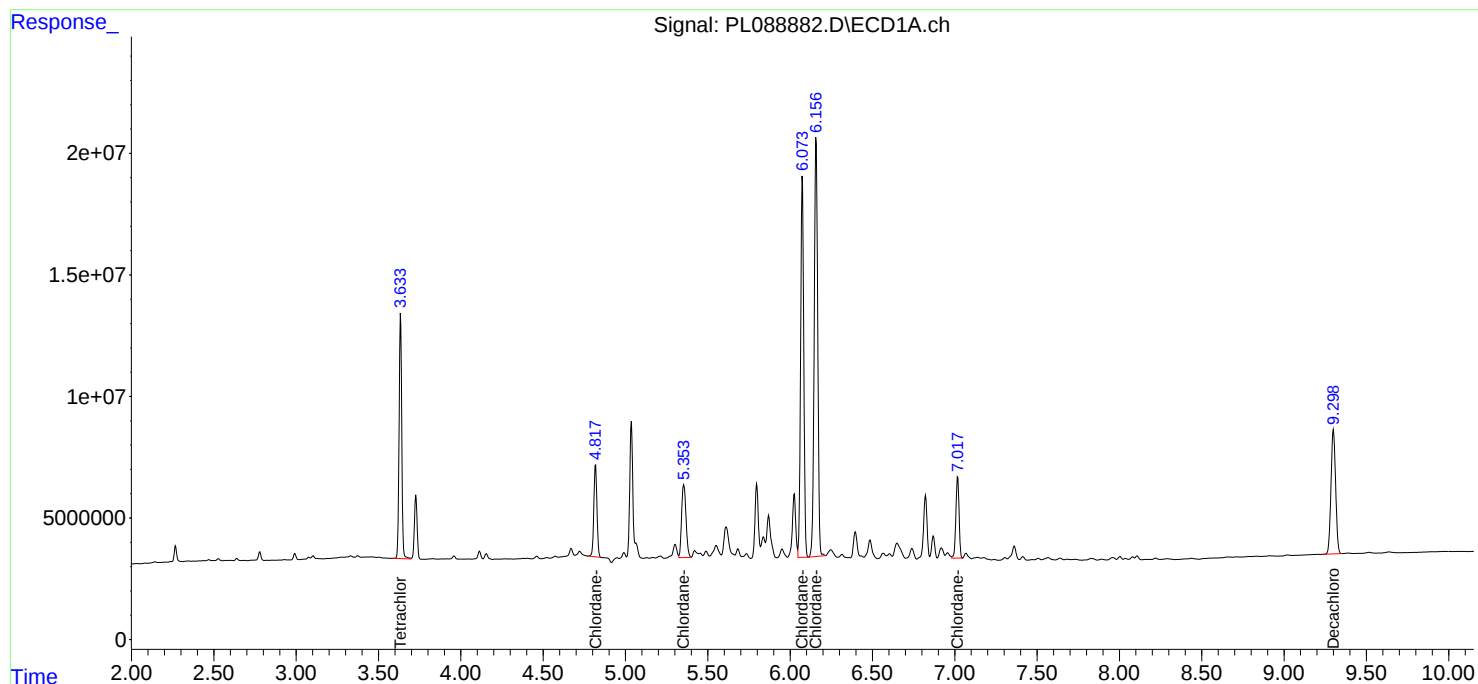


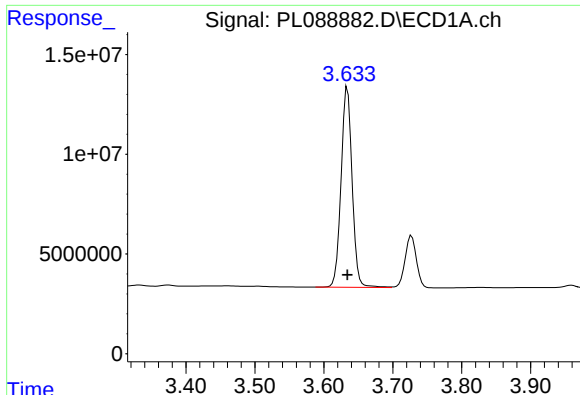

#1 Tetrachloro-m-xylene


R.T.: 3.634 min
Delta R.T.: 0.000 min
Response: 112016345
Conc: 42.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

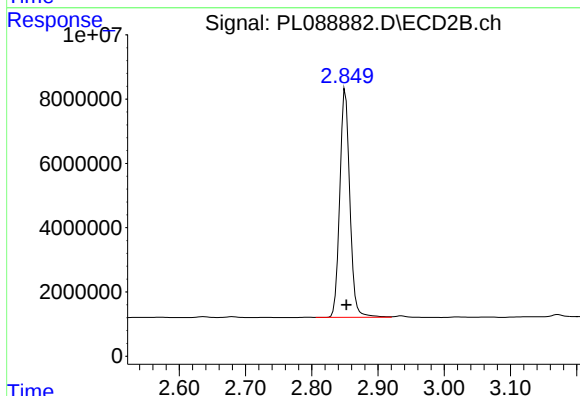


#1 Tetrachloro-m-xylene

R.T.: 2.851 min
Delta R.T.: -0.001 min
Response: 74819098
Conc: 56.14 ng/ml

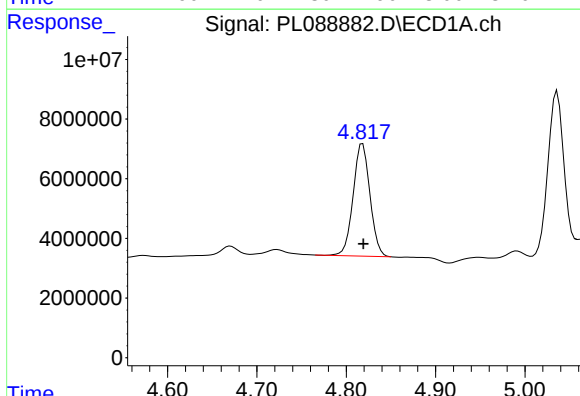


#23 Chlordane-1

R.T.: 4.818 min
Delta R.T.: 0.000 min
Response: 49363038
Conc: 424.51 ng/ml

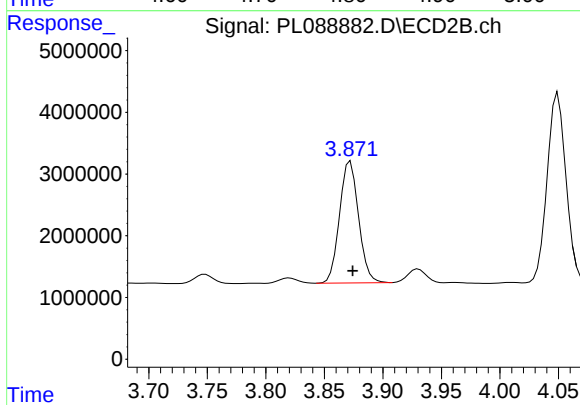

#23 Chlordane-1


R.T.: 3.872 min
Delta R.T.: -0.002 min
Response: 22315336
Conc: 459.59 ng/ml

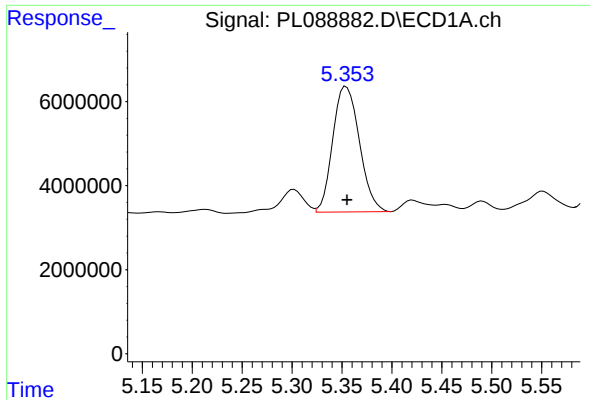

#24 Chlordane-2


R.T.: 5.354 min
Delta R.T.: 0.000 min
Response: 55509979
Conc: 422.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

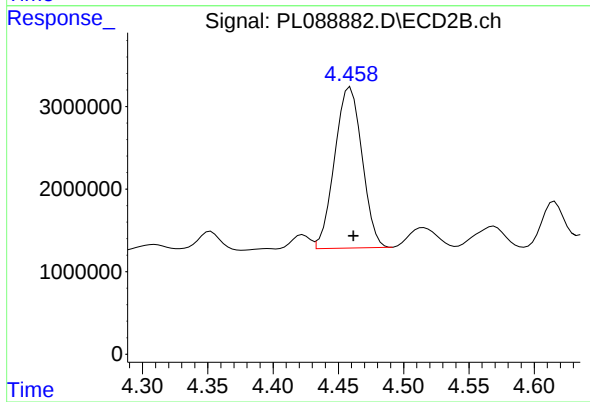


#24 Chlordane-2

R.T.: 4.459 min
Delta R.T.: -0.002 min
Response: 28467736
Conc: 468.87 ng/ml

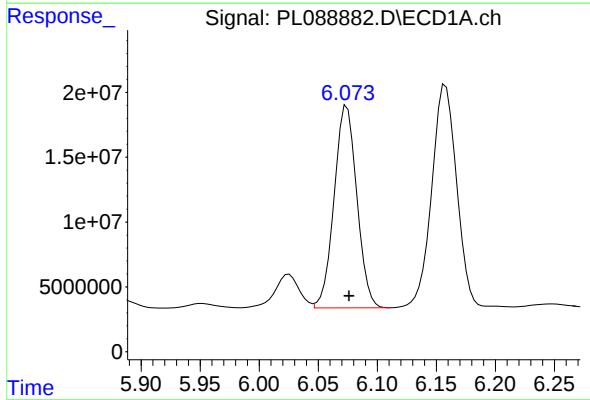


#25 Chlordane-3

R.T.: 6.074 min
Delta R.T.: -0.002 min
Response: 208795523
Conc: 419.91 ng/ml

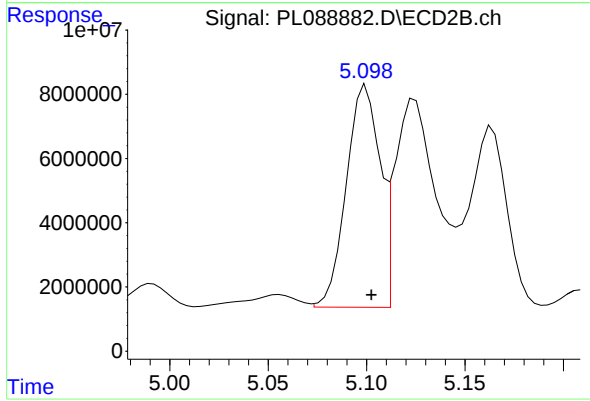

#25 Chlordane-3


R.T.: 5.100 min
Delta R.T.: -0.003 min
Response: 81676825
Conc: 478.56 ng/ml

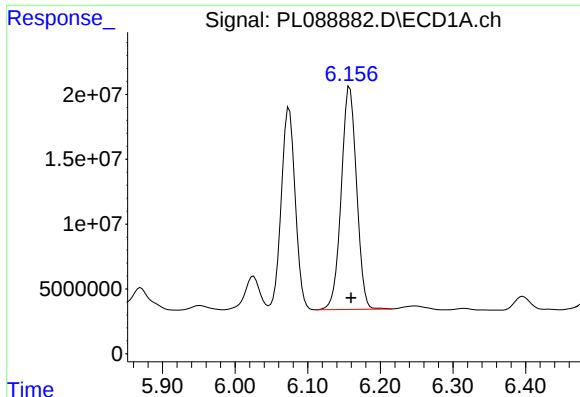

#26 Chlordane-4


R.T.: 6.158 min
Delta R.T.: -0.002 min
Response: 252309097
Conc: 420.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

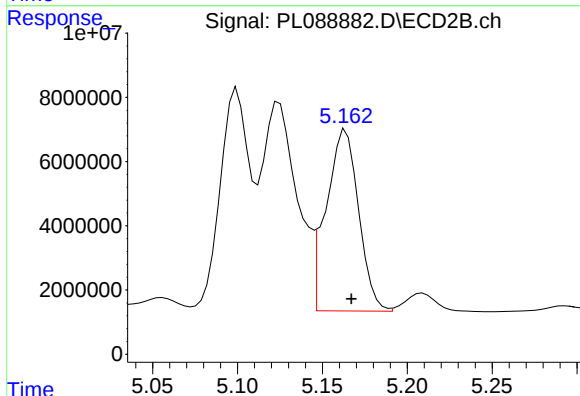


#26 Chlordane-4

R.T.: 5.164 min
Delta R.T.: -0.003 min
Response: 75067772
Conc: 470.53 ng/ml

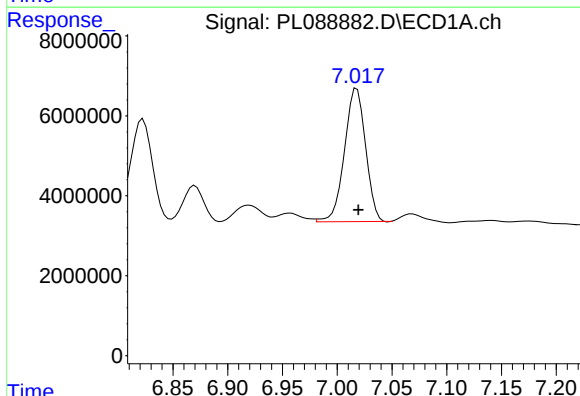


#27 Chlordane-5

R.T.: 7.018 min
Delta R.T.: -0.001 min
Response: 44739900
Conc: 423.26 ng/ml

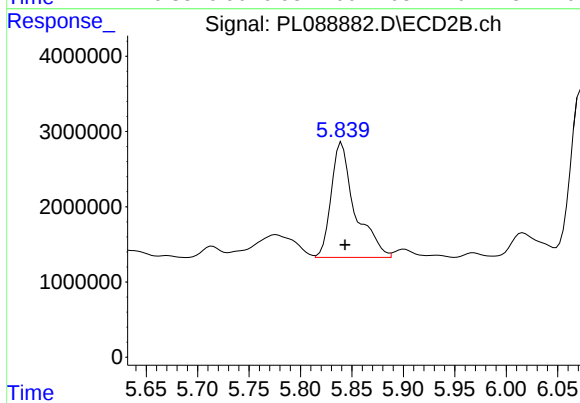

#27 Chlordane-5


R.T.: 5.840 min
Delta R.T.: -0.003 min
Response: 24601460
Conc: 485.09 ng/ml

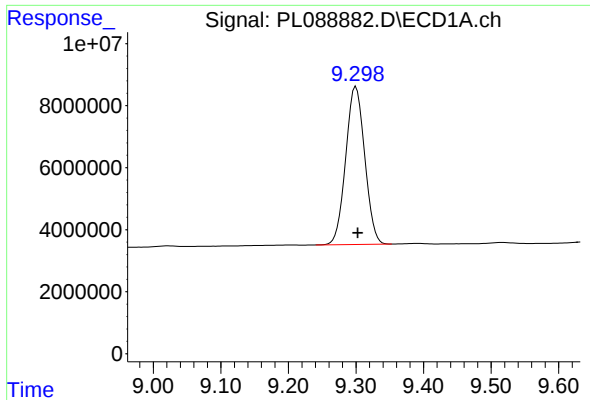

#28 Decachlorobiphenyl

R.T.: 9.300 min
Delta R.T.: -0.003 min
Response: 99373337
Conc: 40.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

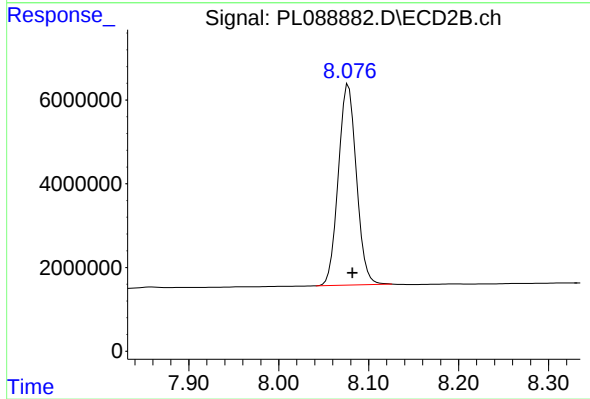

#28 Decachlorobiphenyl

R.T.: 8.078 min
Delta R.T.: -0.004 min
Response: 67067397
Conc: 49.46 ng/ml