

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040225\
 Data File : PL095007.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Apr 2025 11:27
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 01:22:23 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 11 17:42:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
14) MA	Endrin	0.000	5.648	0	6098764	N.D. 1.398 #
17) MA	4,4'-DDT	0.000	6.006f	0	8626631	N.D. 2.139 #
18) B	Endrin al...	0.000	6.097	0	1859758	N.D. 0.553 #
22)	Mirex	8.144f	7.044f	9208823	234.3E6	4.457 61.735 #
23)	Chlordane-1	0.000	3.752	0	8280060	N.D. 54.823 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040225\
Data File : PL095007.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Apr 2025 11:27
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 01:22:23 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
Quant Title : GC Extractables
QLast Update : Tue Mar 11 17:42:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

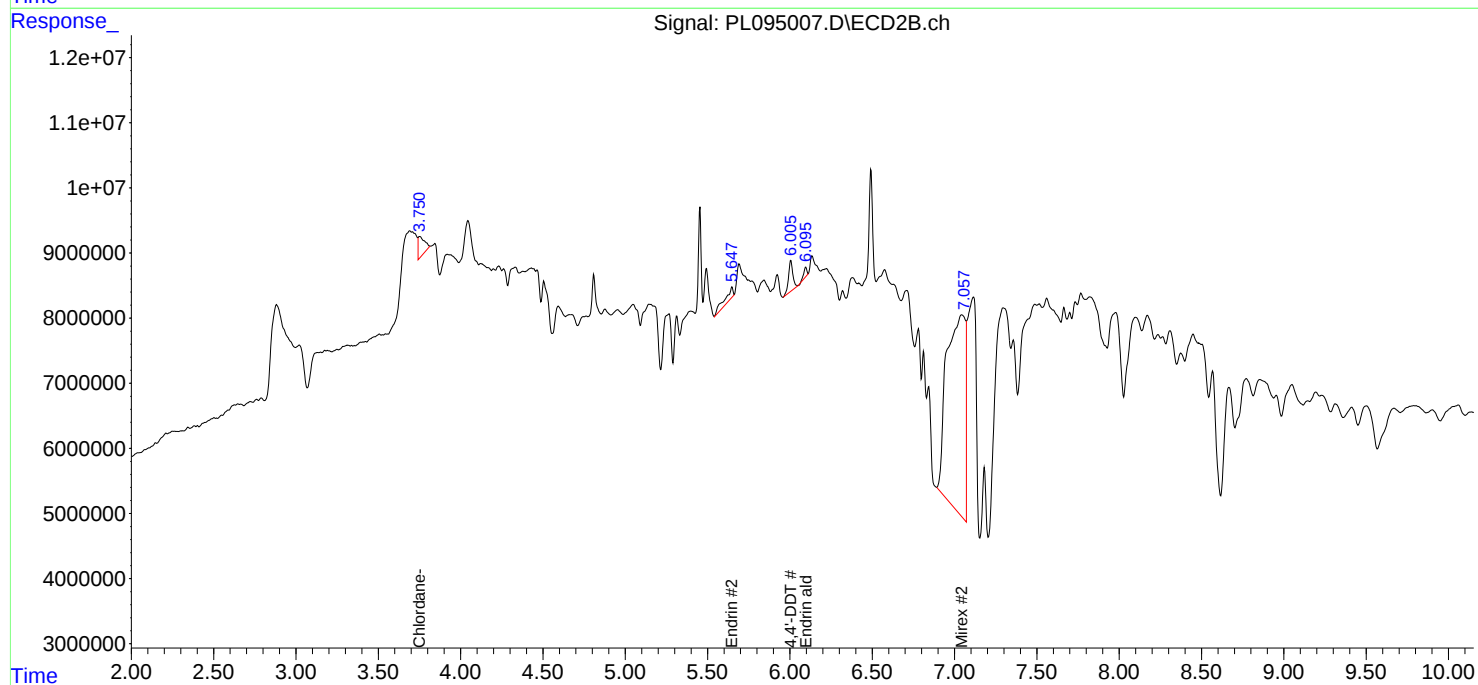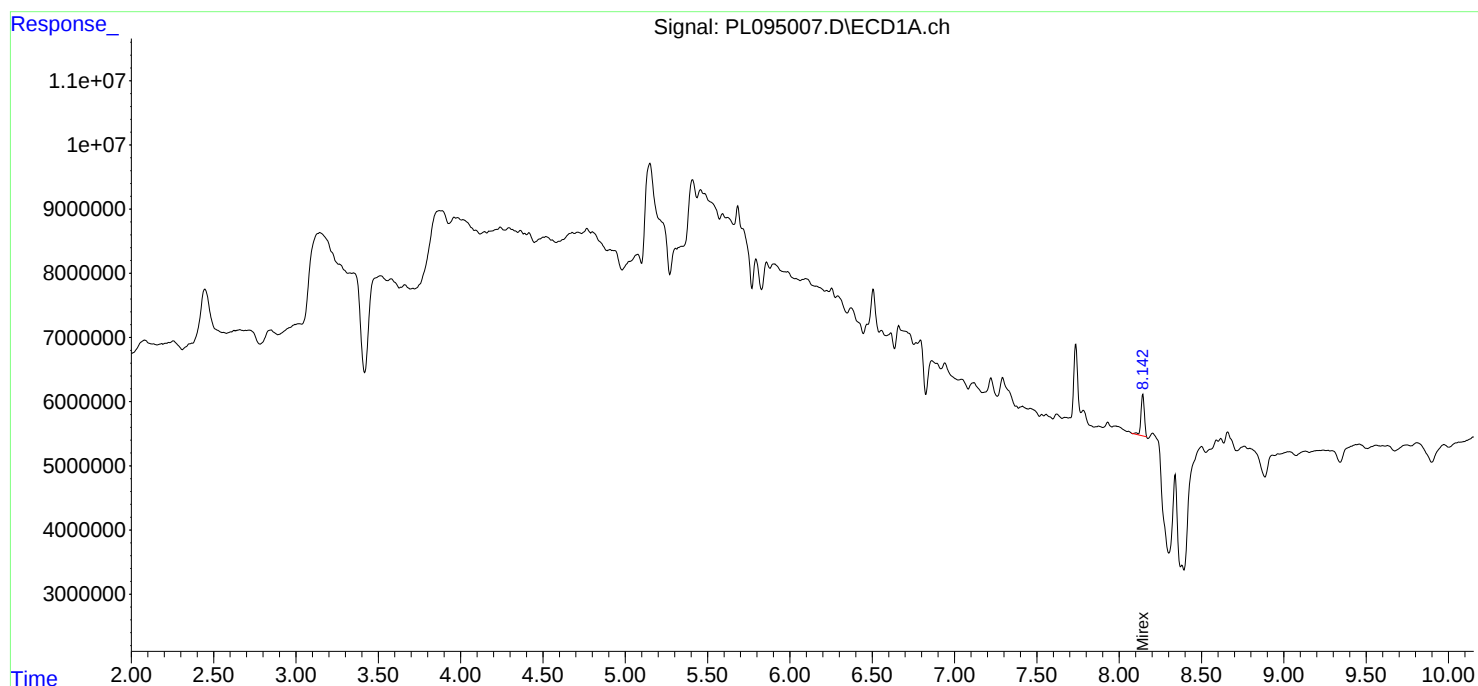


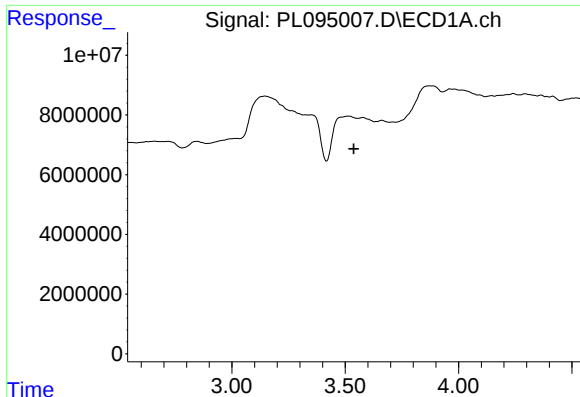

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.538 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

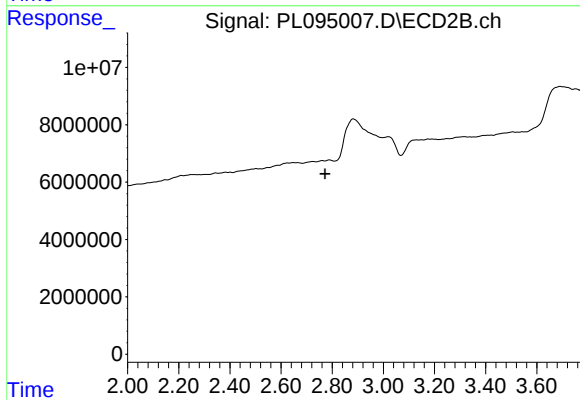


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 2.772 min
Response: 0
Conc: N.D.

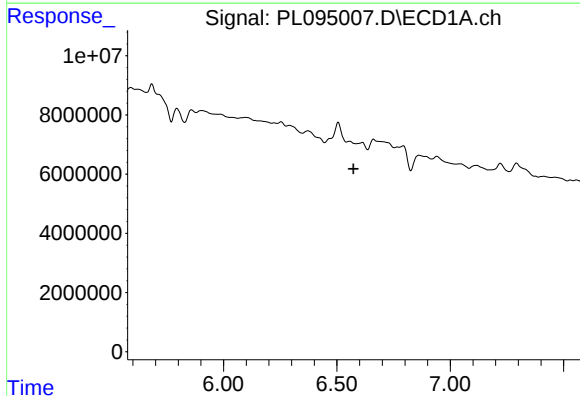


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.574 min
Response: 0
Conc: N.D.

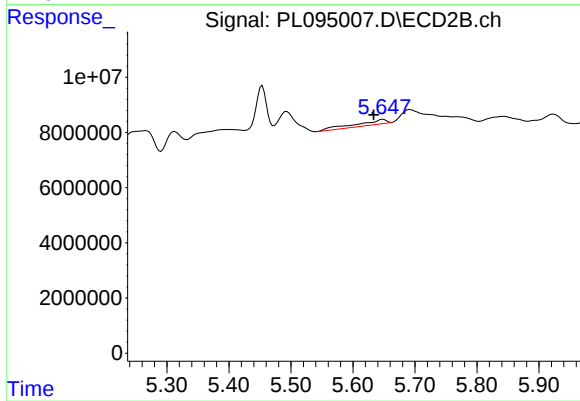

#14 Endrin


R.T.: 5.648 min
Delta R.T.: 0.015 min
Response: 6098764
Conc: 1.40 ng/ml

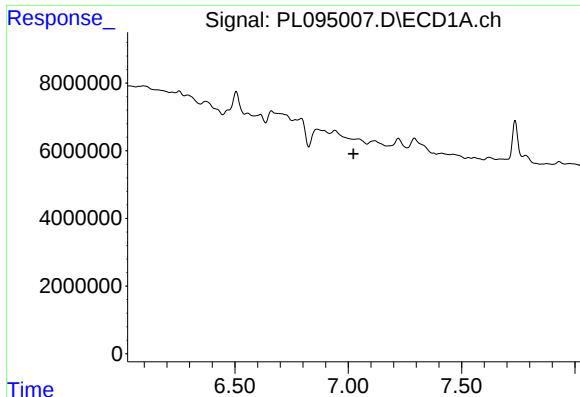

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 7.024 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

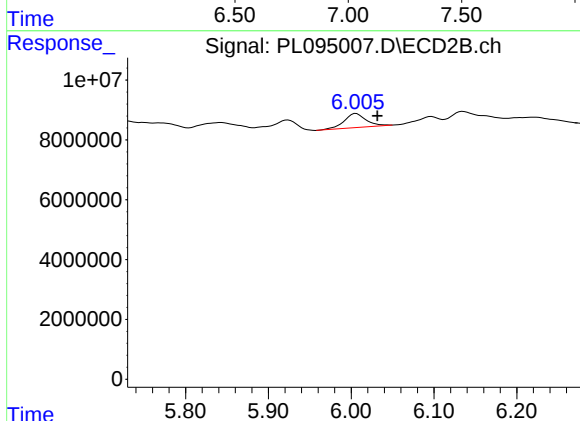


#17 4,4'-DDT

R.T.: 6.006 min
Delta R.T.: -0.026 min
Response: 8626631
Conc: 2.14 ng/ml

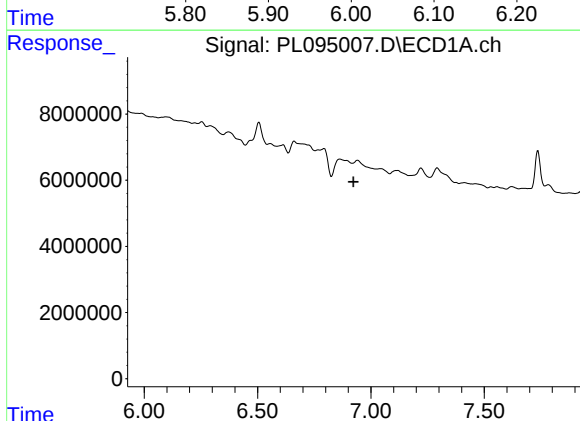


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.924 min
Response: 0
Conc: N.D.

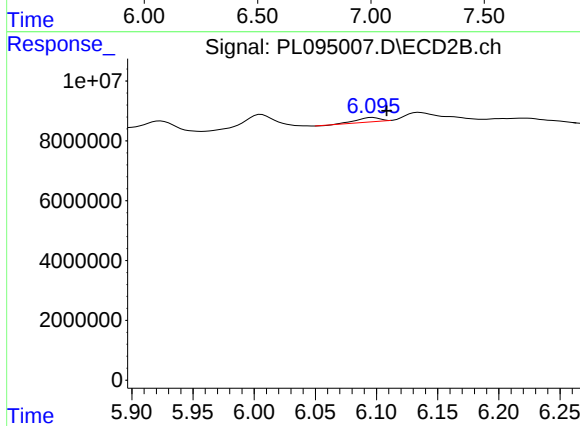

#18 Endrin aldehyde


R.T.: 6.097 min
Delta R.T.: -0.012 min
Response: 1859758
Conc: 0.55 ng/ml

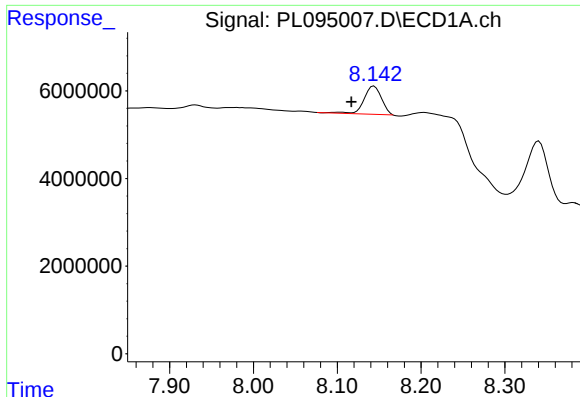

#22 Mirex


R.T.: 8.144 min
Delta R.T.: 0.027 min
Response: 9208823
Conc: 4.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

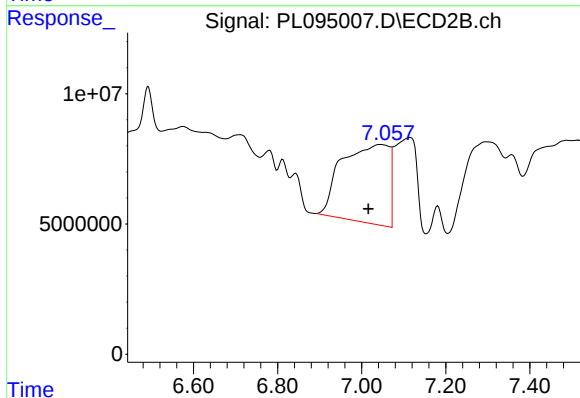


#22 Mirex

R.T.: 7.044 min
Delta R.T.: 0.029 min
Response: 234304134
Conc: 61.74 ng/ml

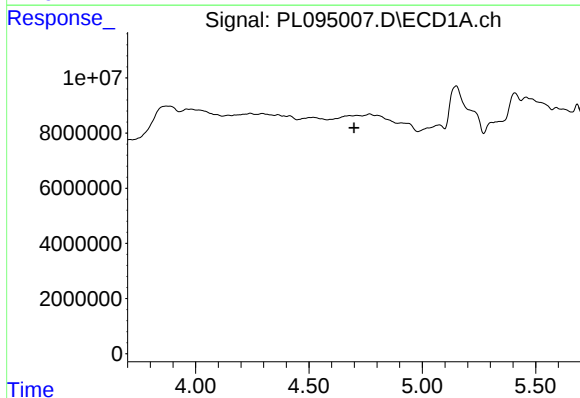


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.700 min
Response: 0
Conc: N.D.

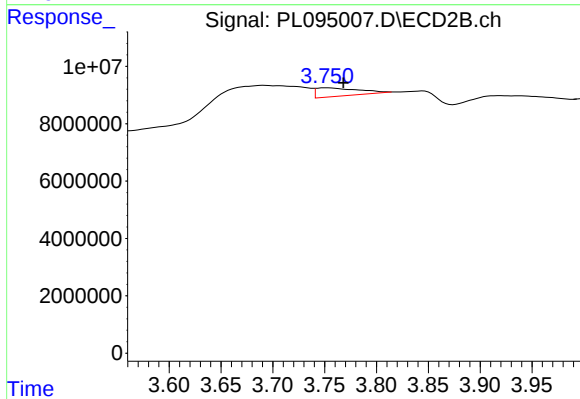

#23 Chlordane-1


R.T.: 3.752 min
Delta R.T.: -0.016 min
Response: 8280060
Conc: 54.82 ng/ml

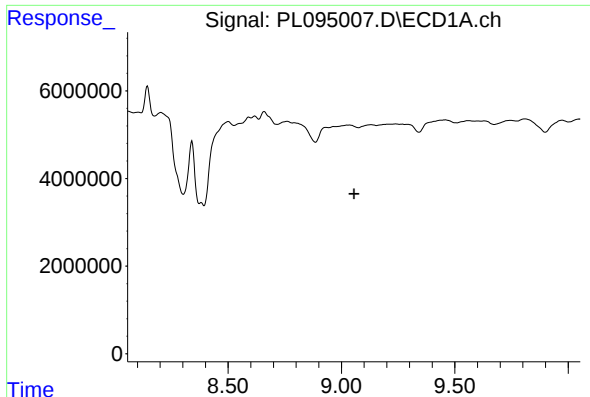

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.056 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

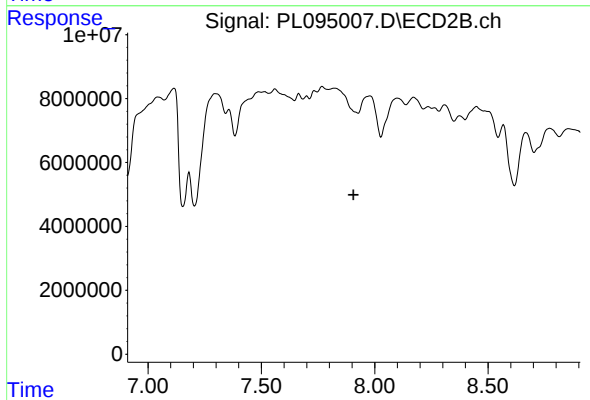

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.907 min
Response: 0
Conc: N.D.