

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040319\
 Data File : PL047002.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Apr 2019 01:49
 Operator : AJ\SJ
 Sample : K2203-03
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SU-03-040219-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 04 05:54:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.357	3.976	78321048	26100903	10.766	11.400
28)	SA Decachlor...	8.033	9.027	86230908	28031717	10.252	12.091
Target Compounds							
2)	A alpha-BHC	3.793	0.000	8574960	0	0.735	N.D. #
10)	B gamma-Chl...	5.270	6.080	15392739	4134897	1.498	1.457
11)	B alpha-Chl...	5.306	6.154	12006732	6064700	1.184	2.138 #
12)	B 4,4'-DDE	5.473	6.309	18257475	6237011	1.983	2.513 #
14)	MA Endrin	5.855	6.705f	6208323	2052068	0.659	0.859 #
17)	MA 4,4'-DDT	6.219	7.098	21860941	7519738	2.886	3.586
25)	Chlordane-3	5.270	6.080	15392739	4134897	13.822	10.845
26)	Chlordane-4	5.306	6.154	12006732	6064700	11.611	13.143



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040319\
Data File : PL047002.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Apr 2019 01:49
Operator : AJ\SJ
Sample : K2203-03
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SU-03-040219-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 04 05:54:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

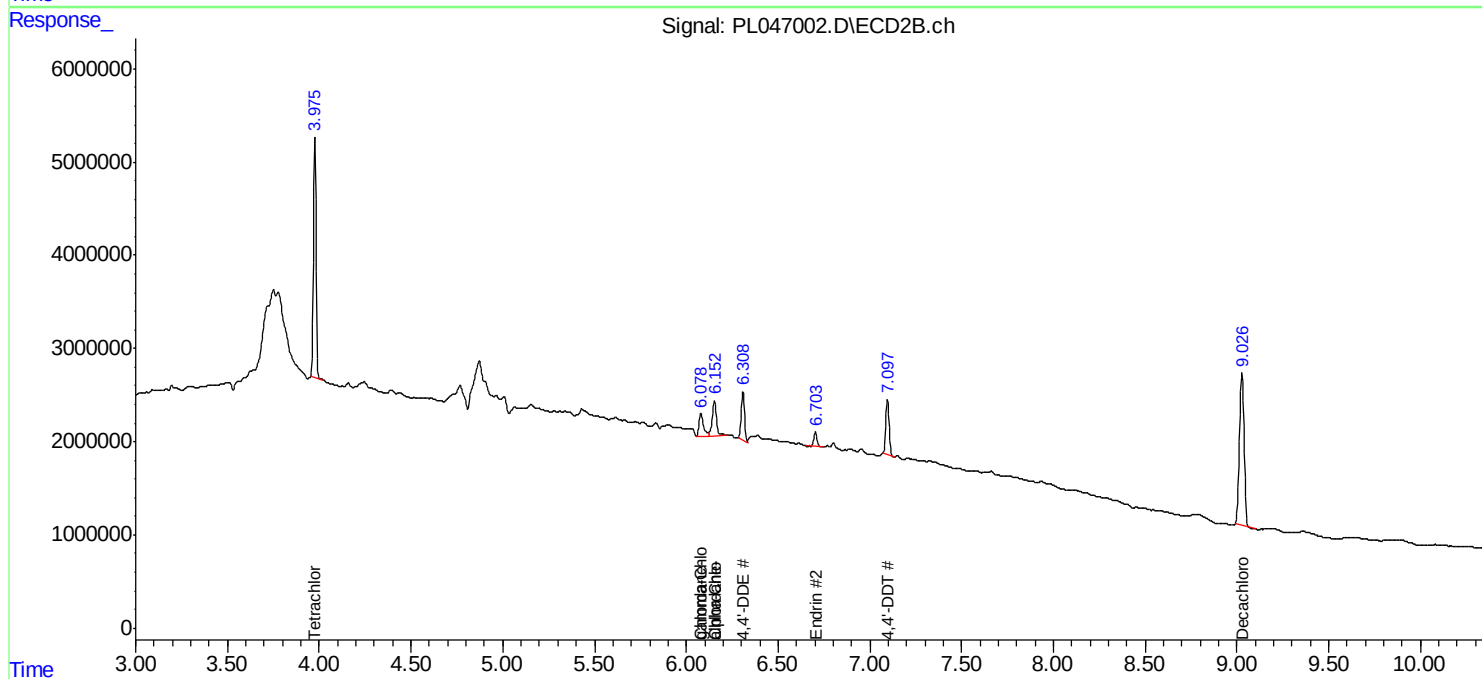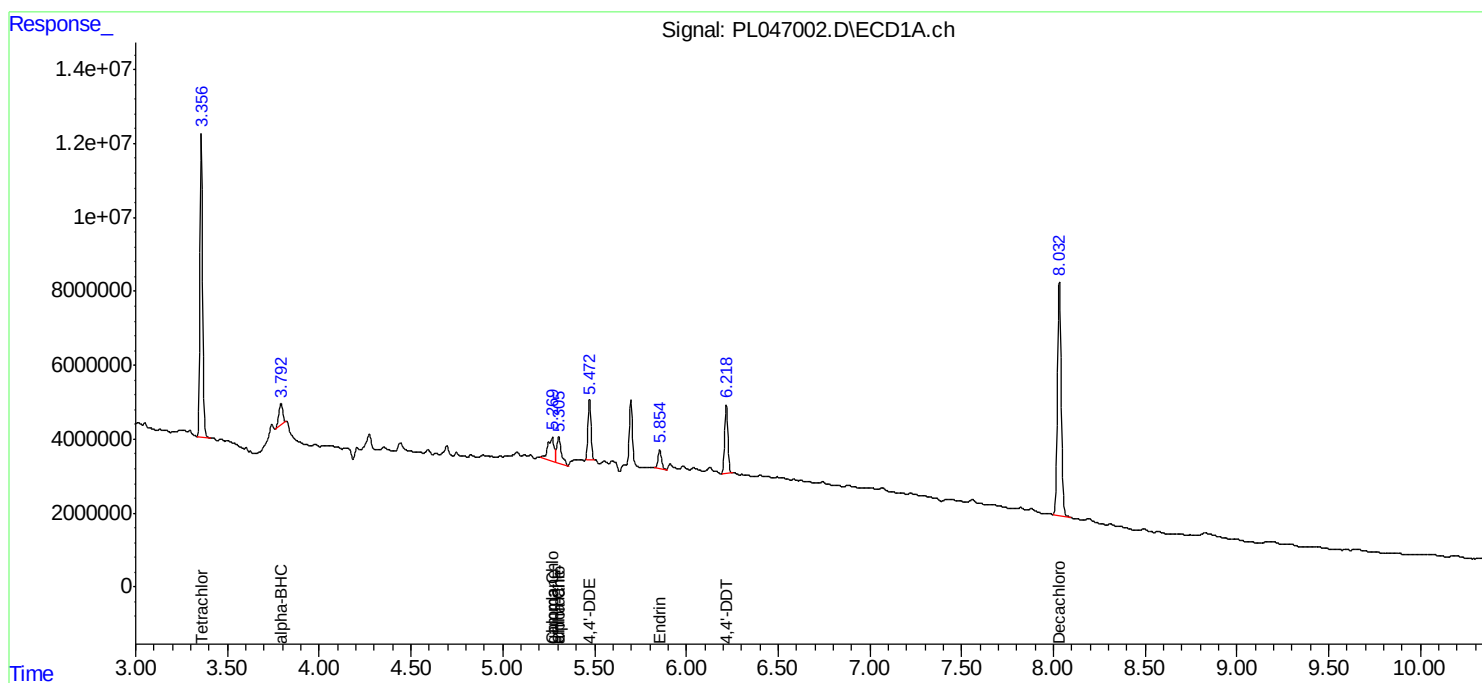


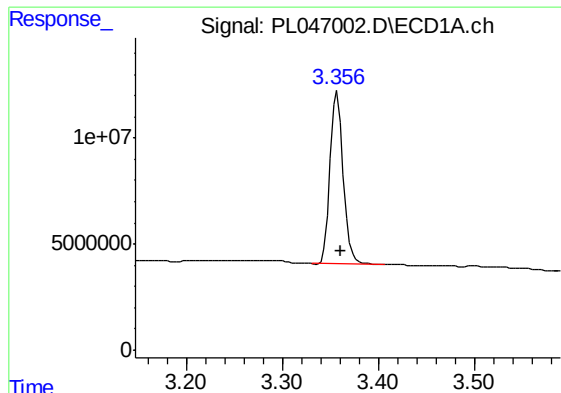

#1 Tetrachloro-m-xylene


R.T.: 3.357 min
Delta R.T.: -0.004 min
Response: 78321048
Conc: 10.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
SU-03-040219-B

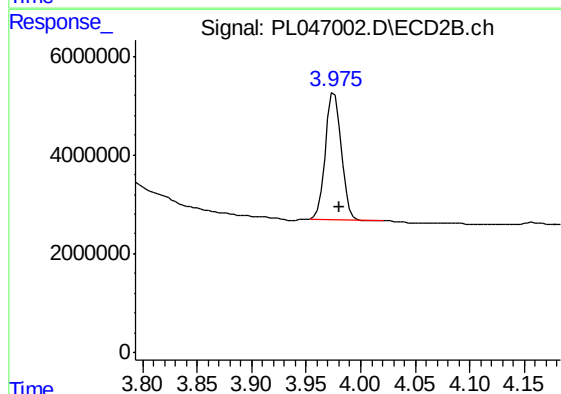


#1 Tetrachloro-m-xylene

R.T.: 3.976 min
Delta R.T.: -0.005 min
Response: 26100903
Conc: 11.40 ng/ml

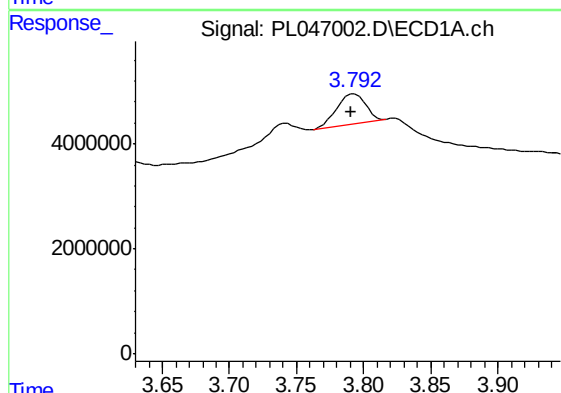


#2 alpha-BHC

R.T.: 3.793 min
Delta R.T.: 0.002 min
Response: 8574960
Conc: 0.74 ng/ml

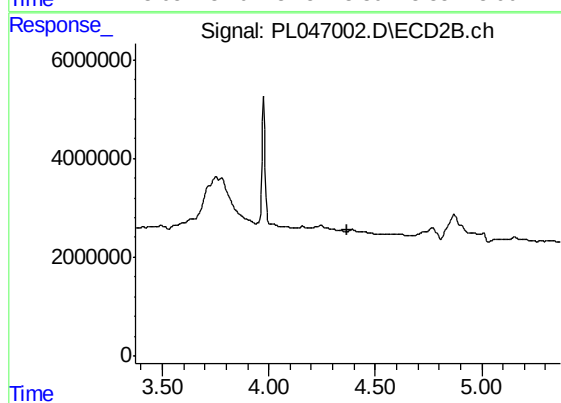

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.371 min
Response: 0
Conc: N.D.

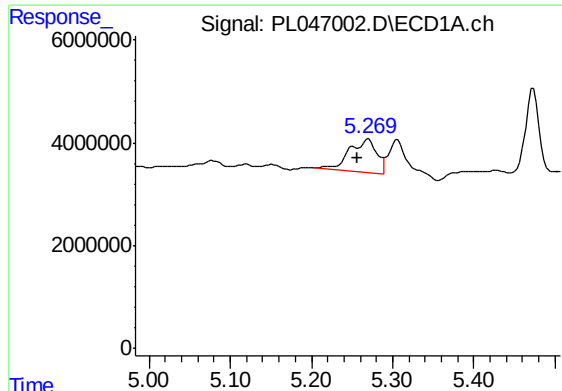

#10 gamma-Chlordane


R.T.: 5.270 min
Delta R.T.: 0.013 min
Response: 15392739
Conc: 1.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
SU-03-040219-B

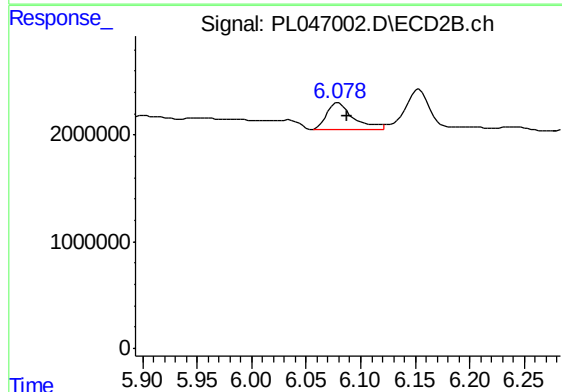


#10 gamma-Chlordane

R.T.: 6.080 min
Delta R.T.: -0.008 min
Response: 4134897
Conc: 1.46 ng/ml

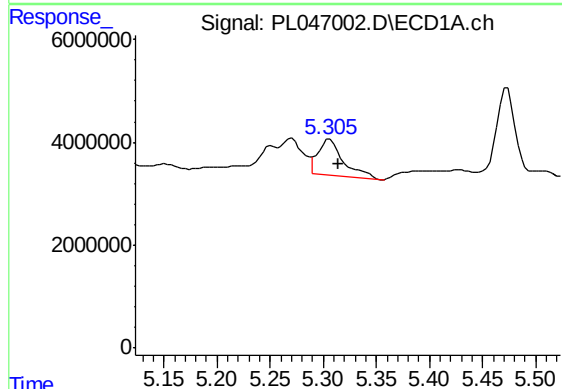


#11 alpha-Chlordane

R.T.: 5.306 min
Delta R.T.: -0.008 min
Response: 12006732
Conc: 1.18 ng/ml

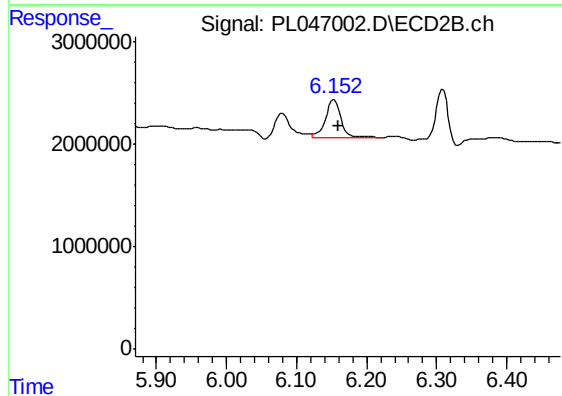

#11 alpha-Chlordane


R.T.: 6.154 min
Delta R.T.: -0.007 min
Response: 6064700
Conc: 2.14 ng/ml

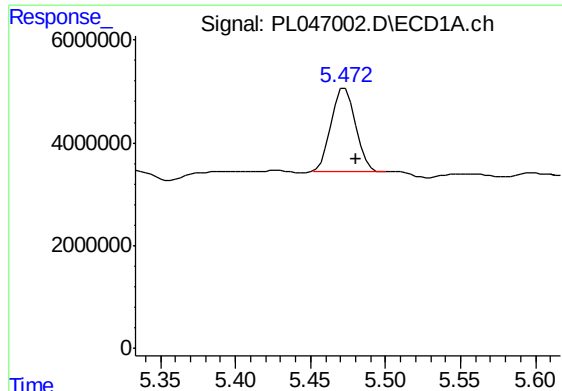

#12 4,4'-DDE


R.T.: 5.473 min
Delta R.T.: -0.008 min
Response: 18257475
Conc: 1.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
SU-03-040219-B

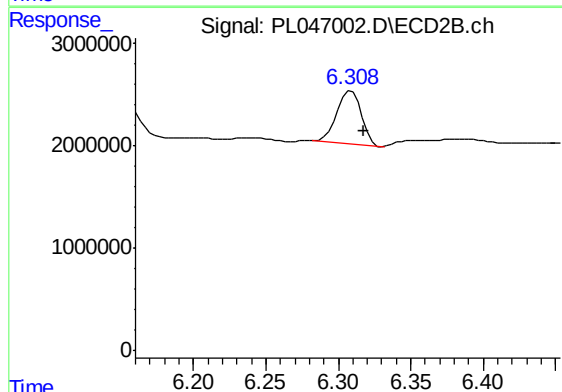


#12 4,4'-DDE

R.T.: 6.309 min
Delta R.T.: -0.009 min
Response: 6237011
Conc: 2.51 ng/ml

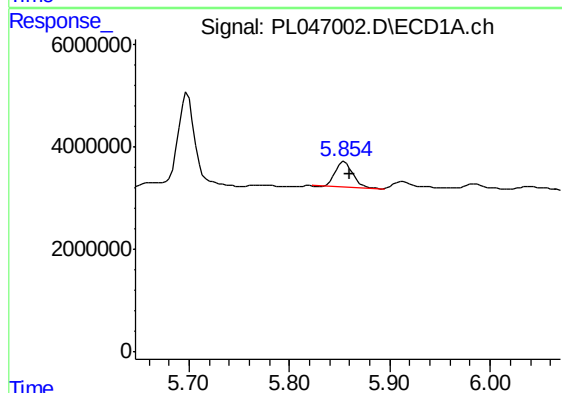


#14 Endrin

R.T.: 5.855 min
Delta R.T.: -0.004 min
Response: 6208323
Conc: 0.66 ng/ml

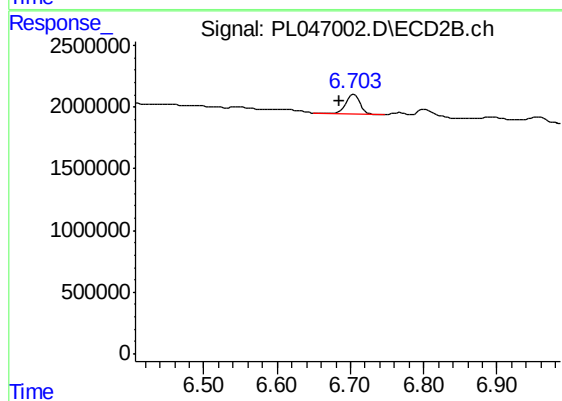

#14 Endrin


R.T.: 6.705 min
Delta R.T.: 0.020 min
Response: 2052068
Conc: 0.86 ng/ml

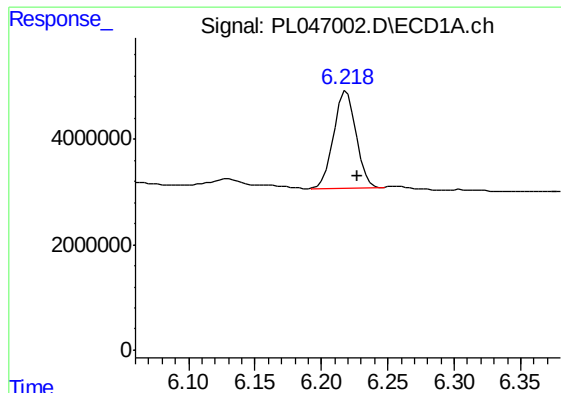

#17 4,4'-DDT


R.T.: 6.219 min
Delta R.T.: -0.009 min
Response: 21860941
Conc: 2.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
SU-03-040219-B

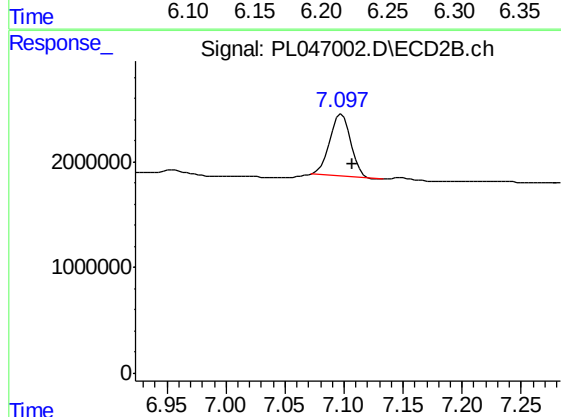


#17 4,4'-DDT

R.T.: 7.098 min
Delta R.T.: -0.009 min
Response: 7519738
Conc: 3.59 ng/ml

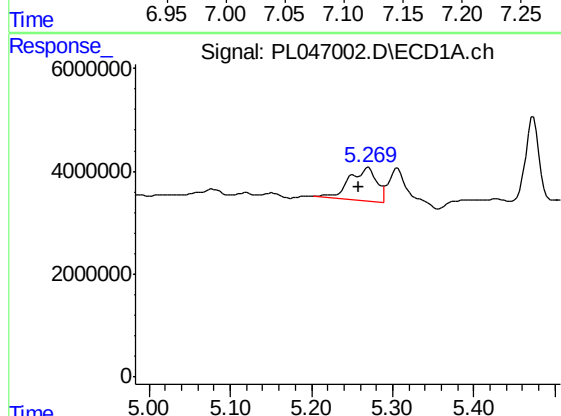


#25 Chlordane-3

R.T.: 5.270 min
Delta R.T.: 0.012 min
Response: 15392739
Conc: 13.82 ng/ml

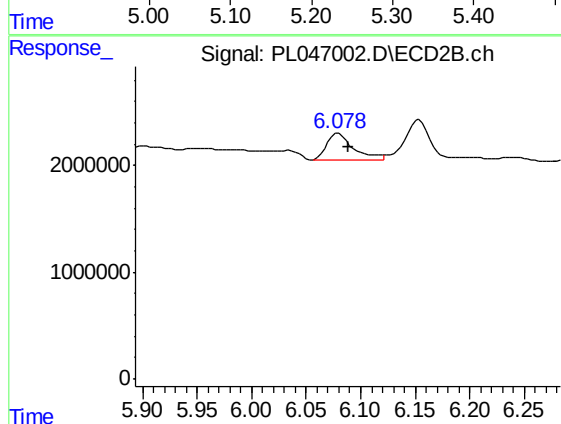

#25 Chlordane-3


R.T.: 6.080 min
Delta R.T.: -0.009 min
Response: 4134897
Conc: 10.85 ng/ml

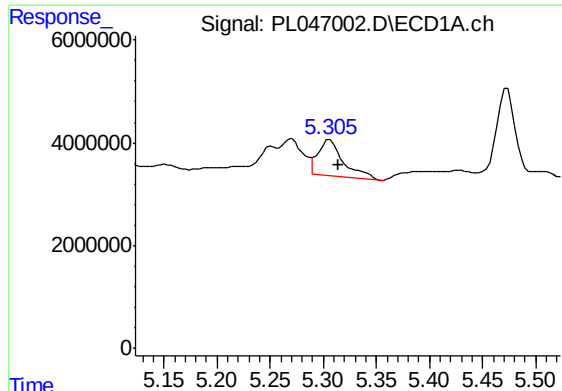

#26 Chlordane-4


R.T.: 5.306 min
Delta R.T.: -0.008 min
Response: 12006732
Conc: 11.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
SU-03-040219-B

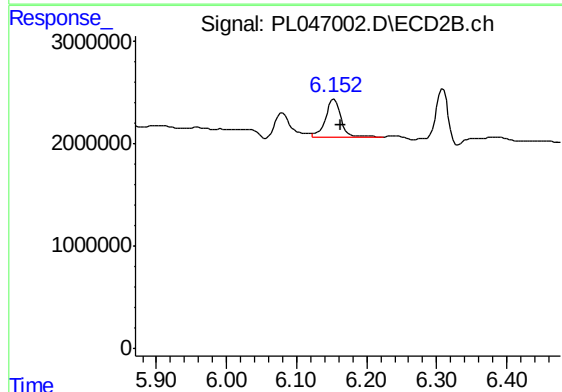


#26 Chlordane-4

R.T.: 6.154 min
Delta R.T.: -0.010 min
Response: 6064700
Conc: 13.14 ng/ml

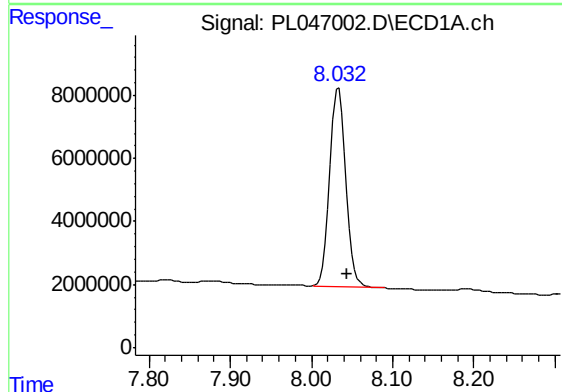

#28 Decachlorobiphenyl

R.T.: 8.033 min
Delta R.T.: -0.011 min
Response: 86230908
Conc: 10.25 ng/ml

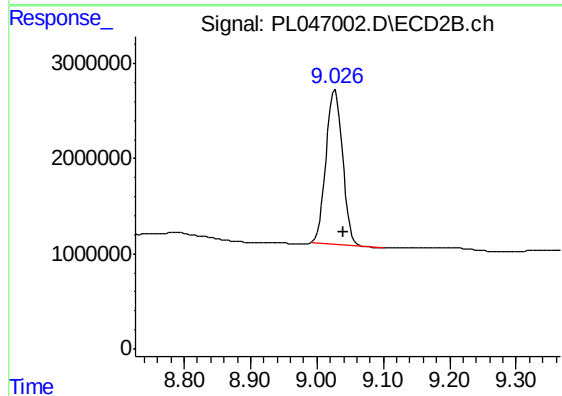

#28 Decachlorobiphenyl

R.T.: 9.027 min
Delta R.T.: -0.012 min
Response: 28031717
Conc: 12.09 ng/ml