

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040319\
 Data File : PL046961.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Apr 2019 15:59
 Operator : AJ\SJ
 Sample : K2234-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SSSI-0401-S-DH-3

Manual Integrations
 APPROVED

Sohil
 4/4/2019 5:19:57 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 04 01:28:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.358	3.978	54148768	17712755	7.443	7.736
28) SA Decachlor...	8.038	9.033	337.3E6	96603486	40.098	41.667
Target Compounds						
12) B 4,4'-DDE	5.476	6.314	898.5E6	244.5E6	97.587	98.506
17) MA 4,4'-DDT	6.223	7.102	753.3E6	181.9E6	99.459	86.767m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040319\
Data File : PL046961.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Apr 2019 15:59
Operator : AJ\SJ
Sample : K2234-02
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SSSI-0401-S-DH-3


Manual Integrations
APPROVED

Sohil
4/4/2019 5:19:57 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 04 01:28:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

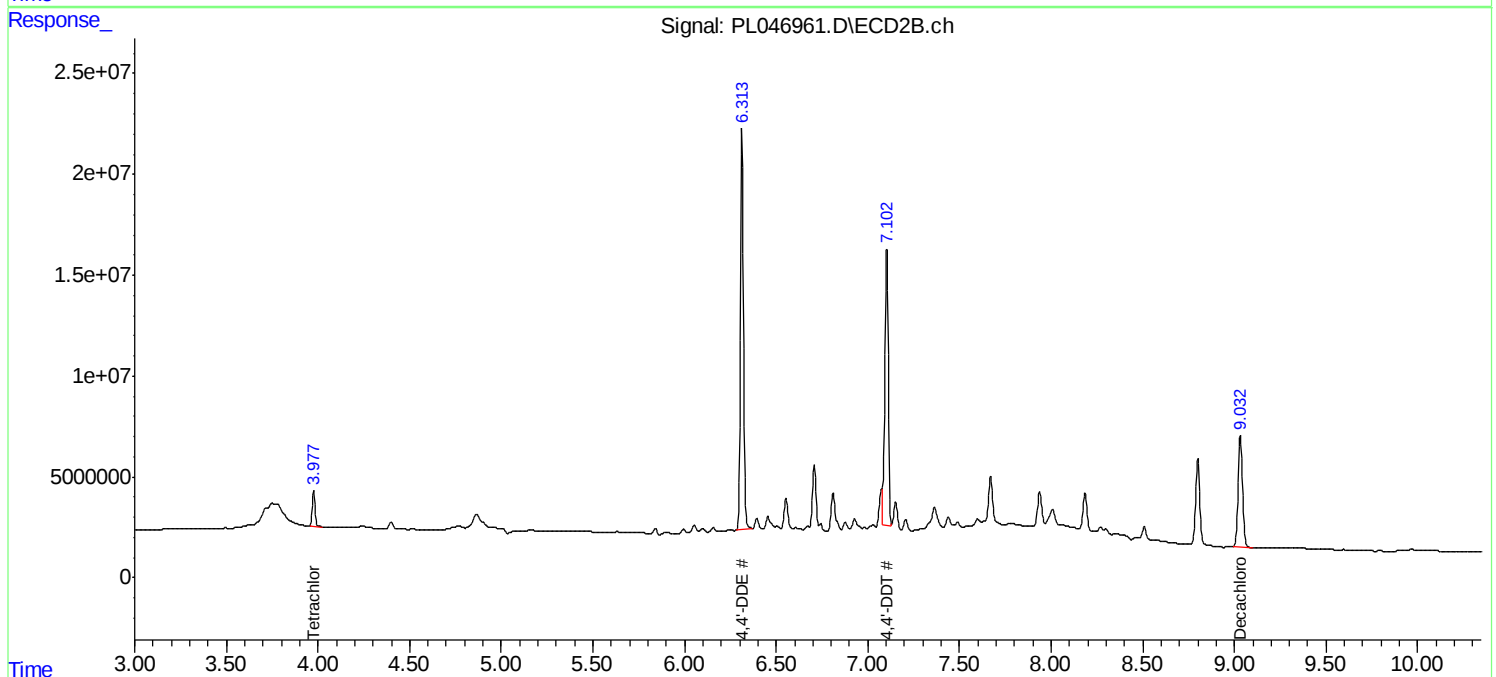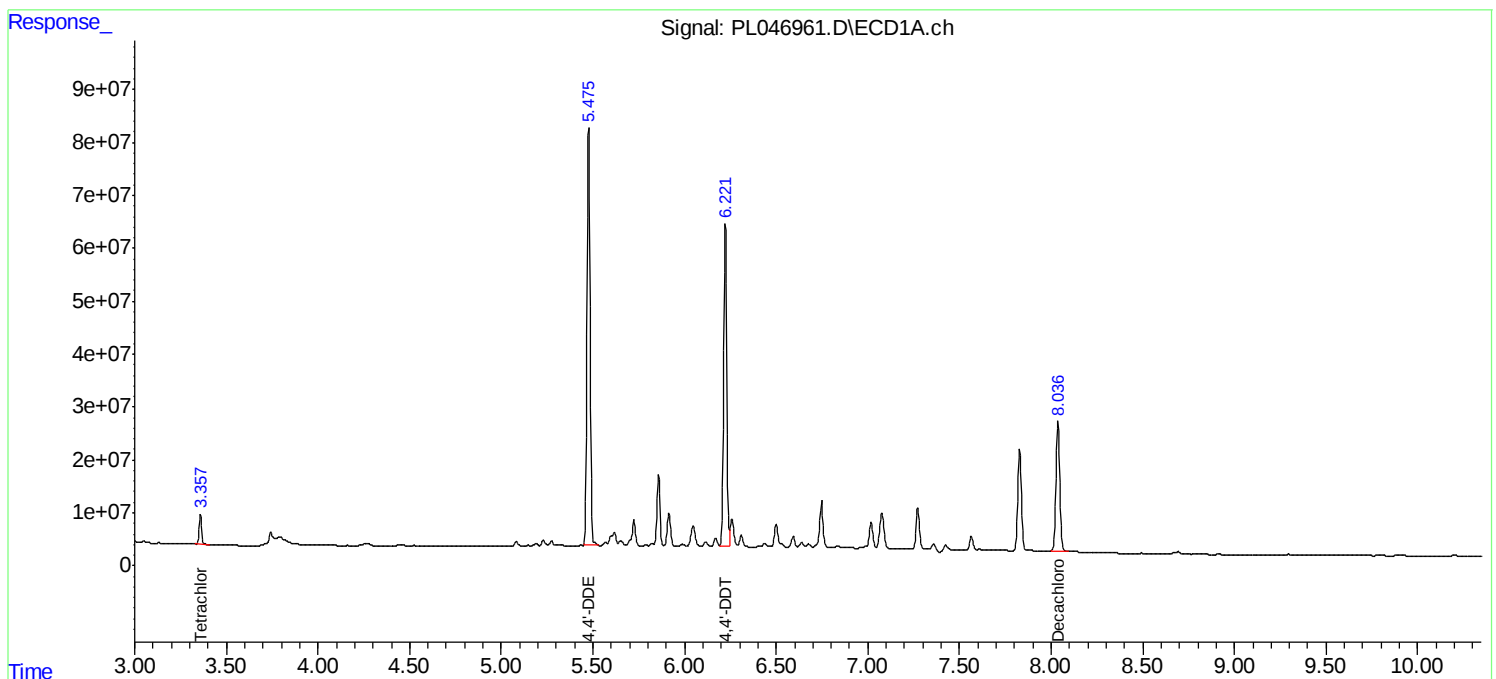

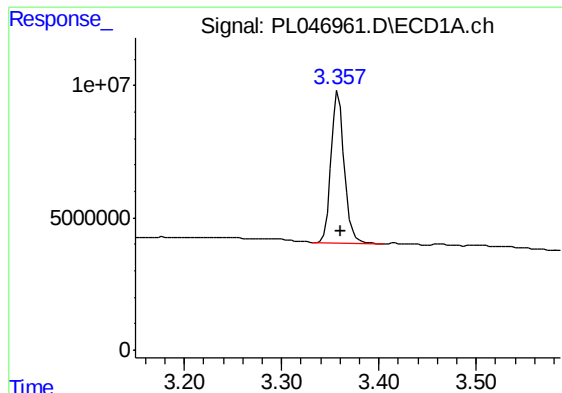


#1 Tetrachloro-m-xylene

R.T.: 3.358 min
Delta R.T.: -0.003 min
Response: 54148768
Conc: 7.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
SSSI-0401-S-DH-3


Manual Integrations
APPROVED

Sohil
4/4/2019 5:19:57 PM

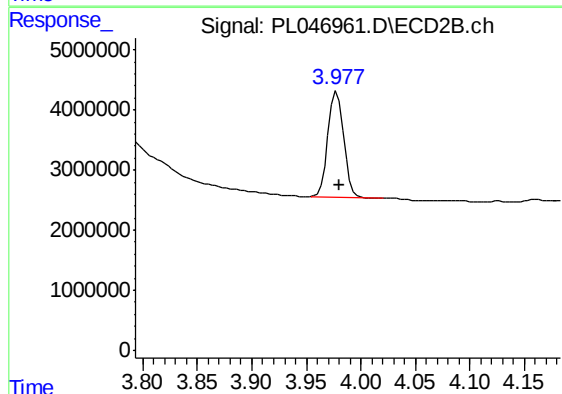


#1 Tetrachloro-m-xylene

R.T.: 3.978 min
Delta R.T.: -0.003 min
Response: 17712755
Conc: 7.74 ng/ml

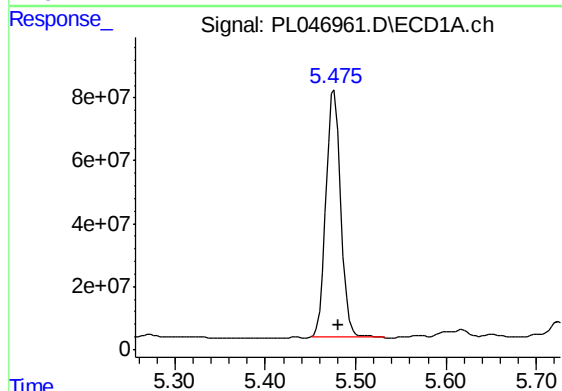


#12 4,4'-DDE

R.T.: 5.476 min
Delta R.T.: -0.004 min
Response: 898476412
Conc: 97.59 ng/ml

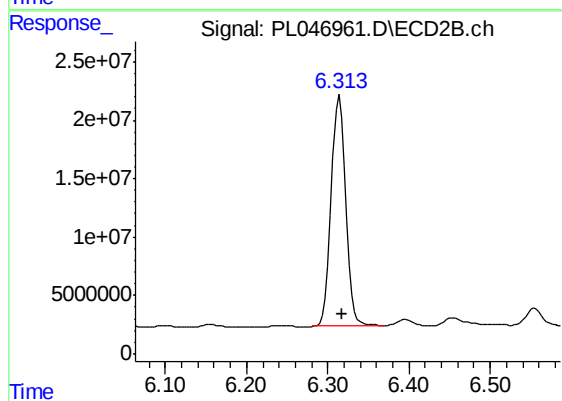

#12 4,4'-DDE

R.T.: 6.314 min
Delta R.T.: -0.004 min
Response: 244525801
Conc: 98.51 ng/ml

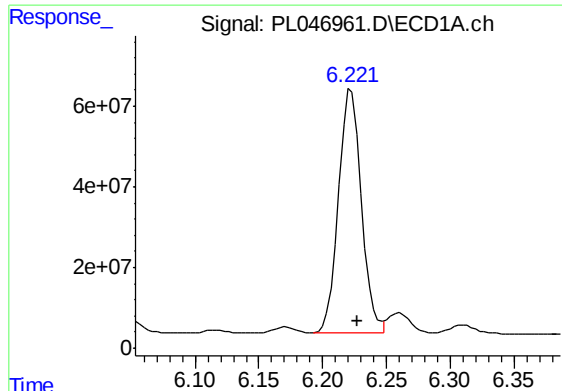


#17 4,4'-DDT

R.T.: 6.223 min
Delta R.T.: -0.005 min
Response: 753339359
Conc: 99.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
SSSI-0401-S-DH-3


Manual Integrations
APPROVED

Sohil
4/4/2019 5:19:57 PM

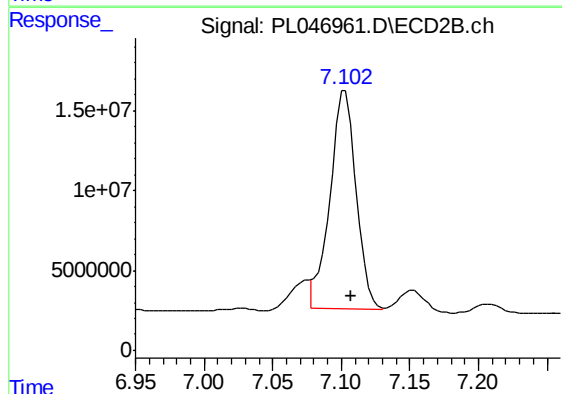


#17 4,4'-DDT

R.T.: 7.102 min
Delta R.T.: -0.005 min
Response: 181945538
Conc: 86.77 ng/ml m

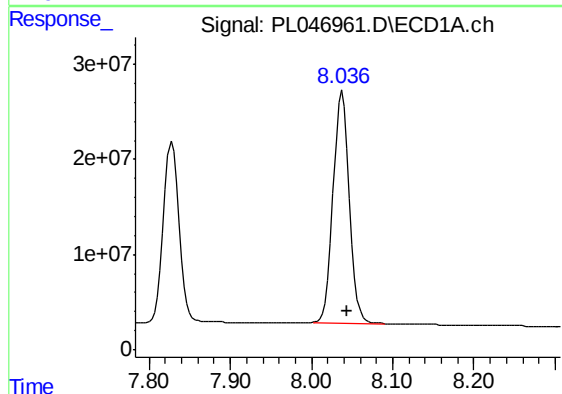

#28 Decachlorobiphenyl

R.T.: 8.038 min
Delta R.T.: -0.006 min
Response: 337270475
Conc: 40.10 ng/ml

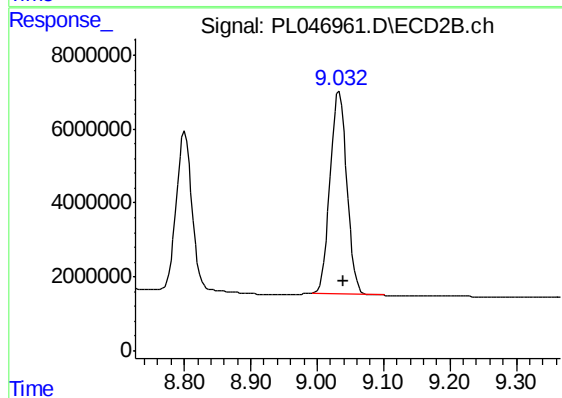

#28 Decachlorobiphenyl

R.T.: 9.033 min
Delta R.T.: -0.006 min
Response: 96603486
Conc: 41.67 ng/ml