

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040320\
 Data File : PL057762.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Apr 2020 11:57
 Operator : AJ\MA
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 04 06:38:43 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:38:27 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.457	3.957	601.6E6	110.3E6	50.000	50.000
28)	SA Decachlor...	8.207	8.981	521.5E6	112.6E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.327	4.942	184.9E6	44091914	500.000	500.000
24)	Chlordane-2	4.828	5.407	201.9E6	52179313	500.000	500.000
25)	Chlordane-3	5.398	6.049	611.3E6	216.3E6	500.000	500.000
26)	Chlordane-4	5.454	6.123	520.1E6	262.5E6	500.000	500.000
27)	Chlordane-5	6.290	6.922	189.1E6	42630887	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040320\
Data File : PL057762.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Apr 2020 11:57
Operator : AJ\MA
Sample : PCHLORICC500
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 04 06:38:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:38:27 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

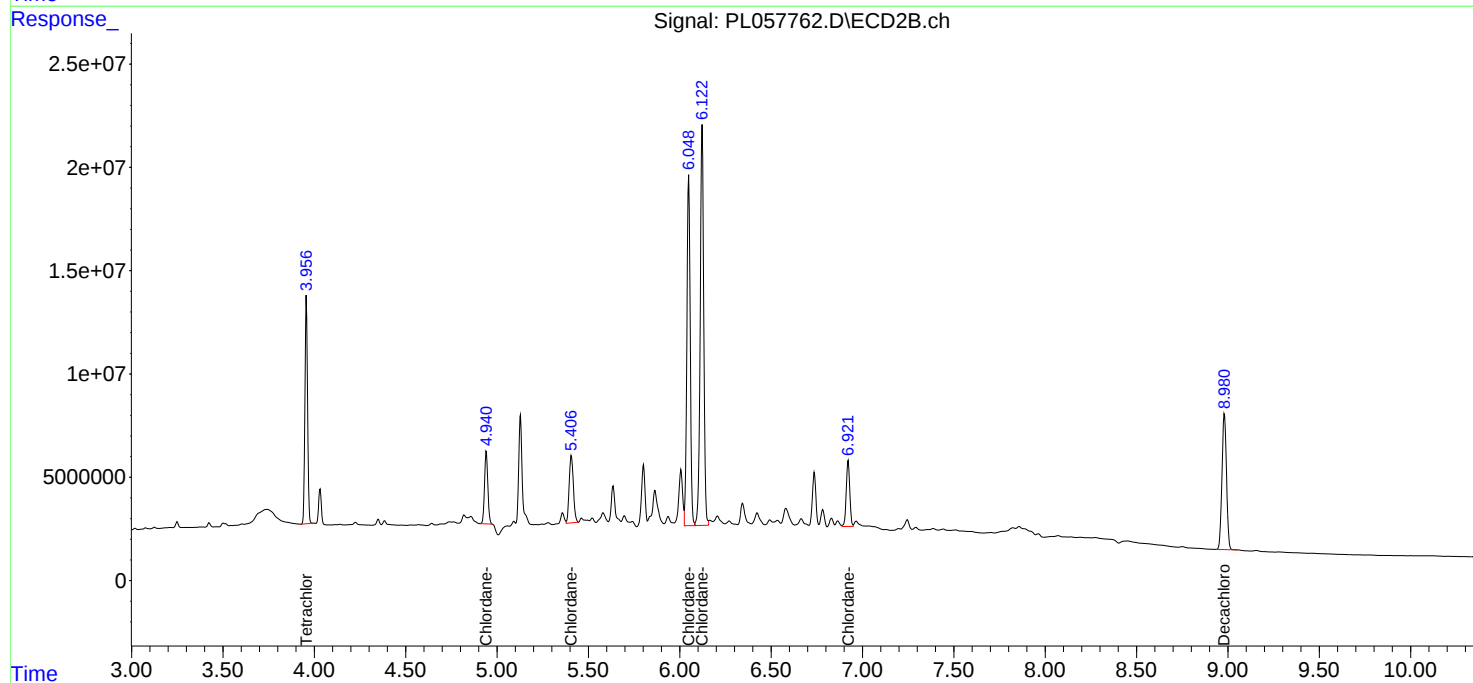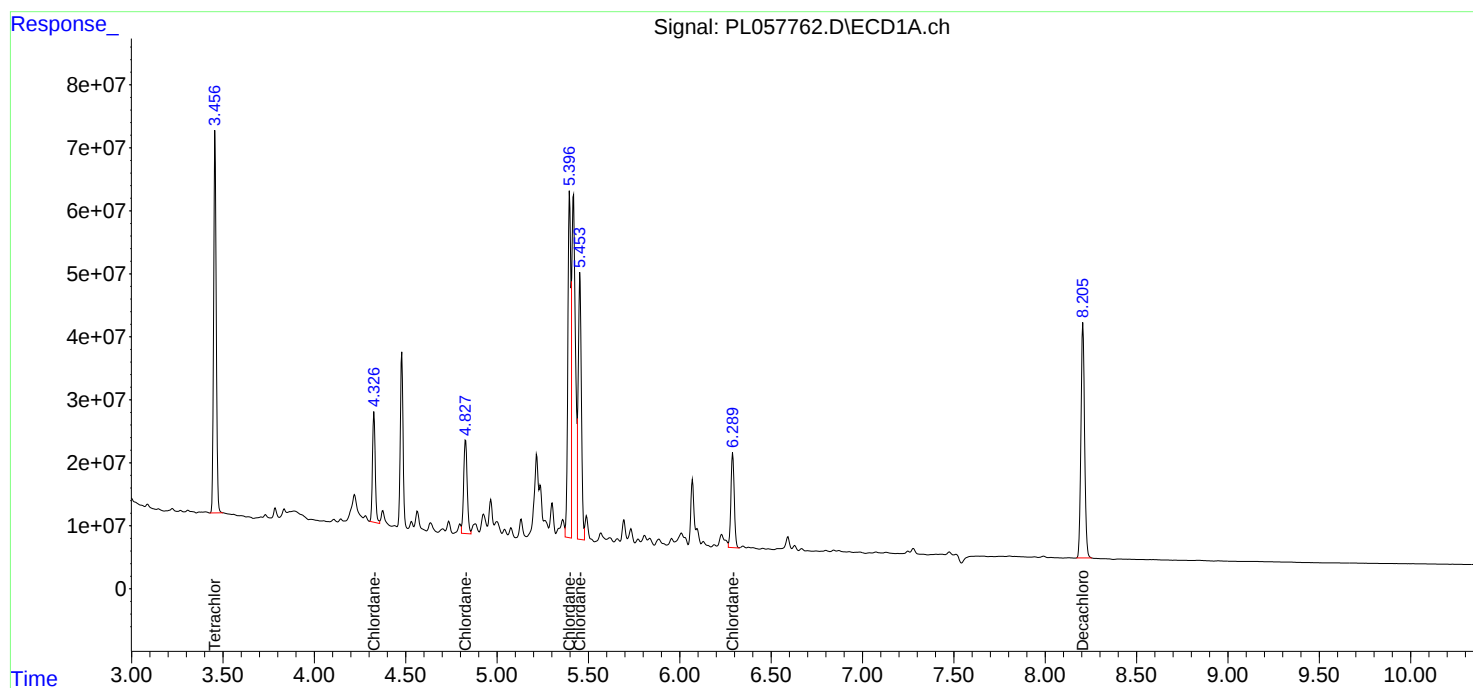


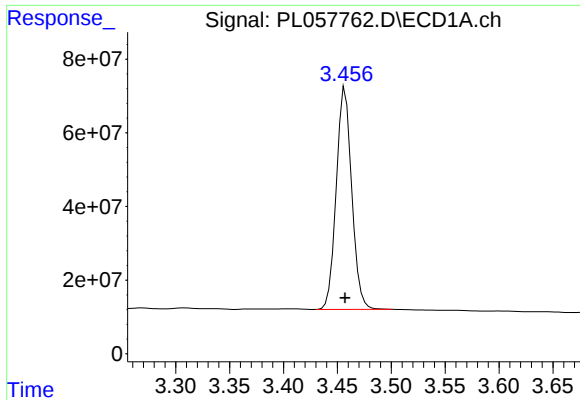

#1 Tetrachloro-m-xylene


R.T.: 3.457 min
Delta R.T.: 0.000 min
Response: 601587011
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

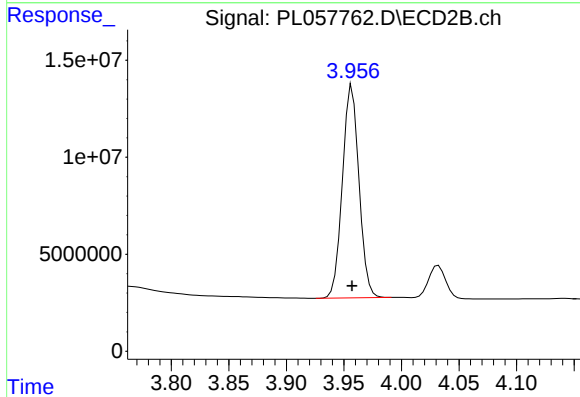


#1 Tetrachloro-m-xylene

R.T.: 3.957 min
Delta R.T.: 0.000 min
Response: 110253394
Conc: 50.00 ng/ml

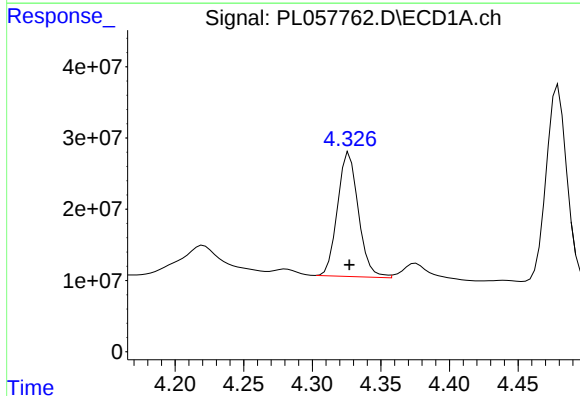


#23 Chlordane-1

R.T.: 4.327 min
Delta R.T.: 0.000 min
Response: 184925262
Conc: 500.00 ng/ml

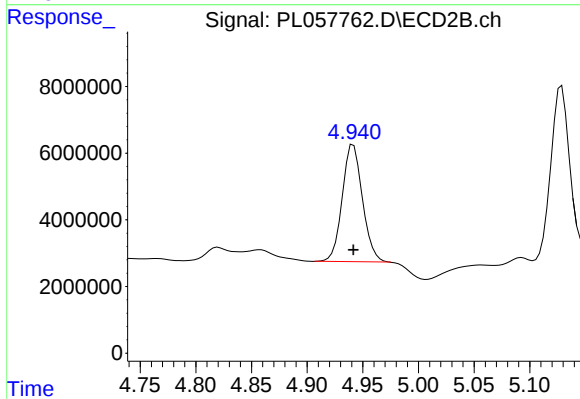

#23 Chlordane-1


R.T.: 4.942 min
Delta R.T.: 0.000 min
Response: 44091914
Conc: 500.00 ng/ml

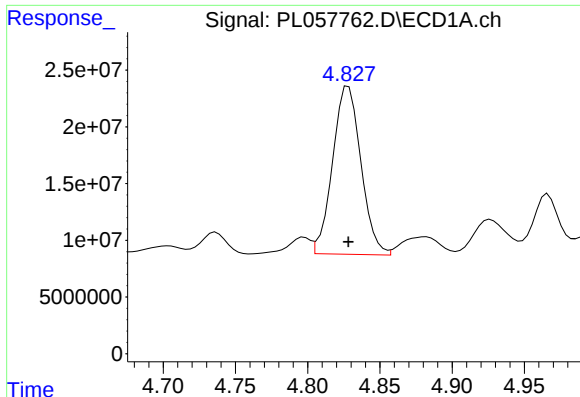

#24 Chlordane-2


R.T.: 4.828 min
Delta R.T.: 0.000 min
Response: 201857880
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

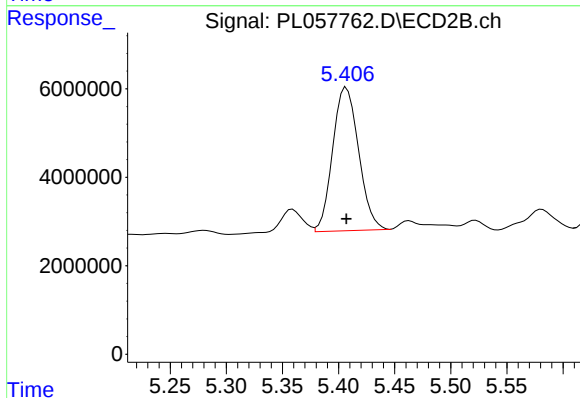


#24 Chlordane-2

R.T.: 5.407 min
Delta R.T.: 0.000 min
Response: 52179313
Conc: 500.00 ng/ml

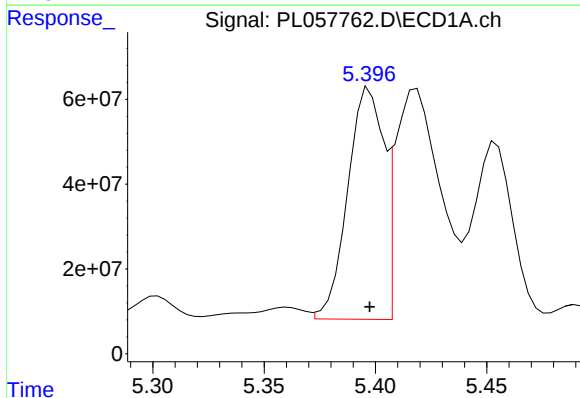


#25 Chlordane-3

R.T.: 5.398 min
Delta R.T.: 0.000 min
Response: 611307052
Conc: 500.00 ng/ml

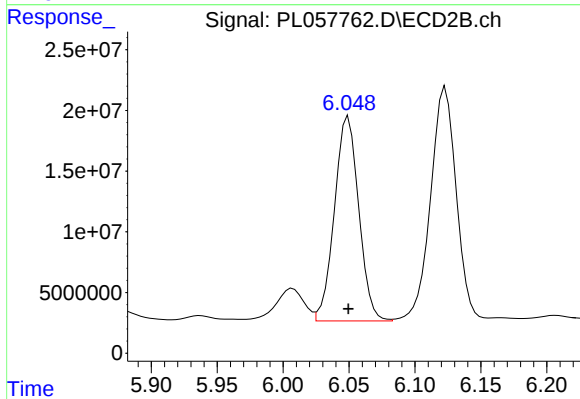

#25 Chlordane-3


R.T.: 6.049 min
Delta R.T.: 0.000 min
Response: 216336772
Conc: 500.00 ng/ml

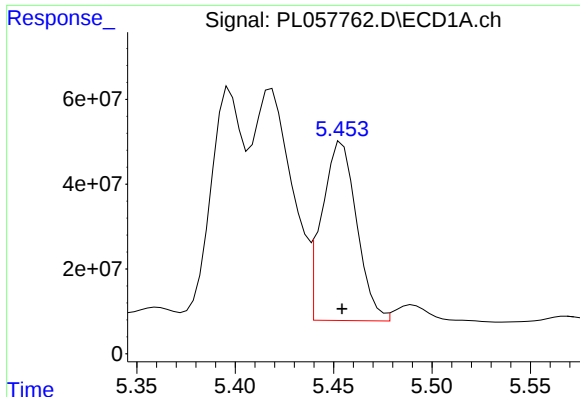

#26 Chlordane-4


R.T.: 5.454 min
Delta R.T.: 0.000 min
Response: 520104872
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

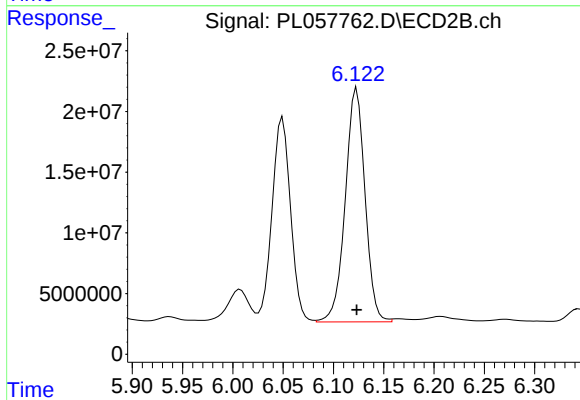


#26 Chlordane-4

R.T.: 6.123 min
Delta R.T.: 0.000 min
Response: 262468714
Conc: 500.00 ng/ml

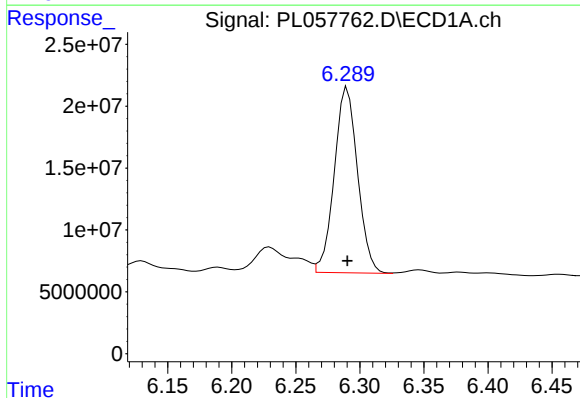


#27 Chlordane-5

R.T.: 6.290 min
Delta R.T.: 0.000 min
Response: 189137594
Conc: 500.00 ng/ml

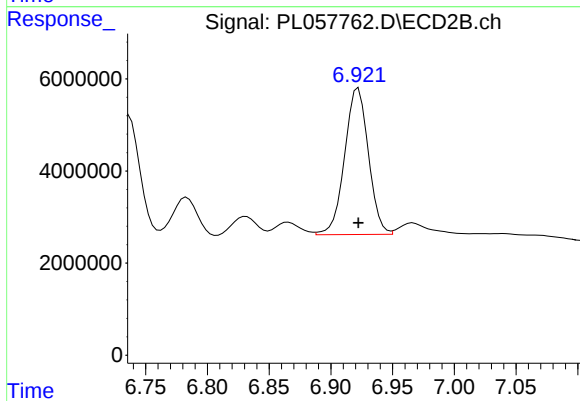

#27 Chlordane-5


R.T.: 6.922 min
Delta R.T.: 0.000 min
Response: 42630887
Conc: 500.00 ng/ml

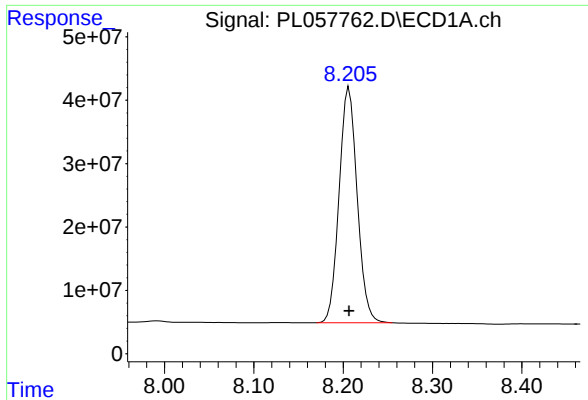

#28 Decachlorobiphenyl

R.T.: 8.207 min
Delta R.T.: 0.000 min
Response: 521542184
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

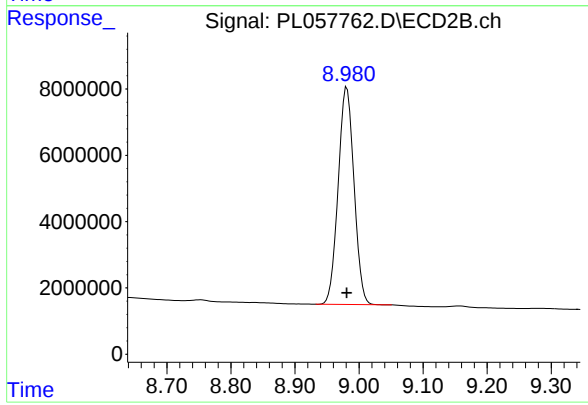

#28 Decachlorobiphenyl

R.T.: 8.981 min
Delta R.T.: 0.000 min
Response: 112586376
Conc: 50.00 ng/ml