

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040320\
 Data File : PL057792.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Apr 2020 21:17
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 04 07:04:47 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:41:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.458	3.957	223.0E6	48164314	22.125	22.194
28)	SA Decachlor...	8.205	8.979	204.7E6	49765642	19.861	22.279
Target Compounds							
2)	A alpha-BHC	3.897	0.000	8755623	0	0.504	N.D. #
4)	MA Heptachlor	0.000	5.141	0	275380	N.D.	0.082 #
8)	B Heptachlo...	0.000	5.802	0	3490451	N.D.	1.293 #
14)	MA Endrin	6.009	0.000	994349	0	0.085	N.D. #
15)	B Endosulfa...	6.287	6.869f	-614748	1042555	N.D.	0.402
16)	A 4,4'-DDD	6.124	0.000	680430	0	0.068	N.D. #
22)	Mirex	7.339	0.000	142854	0	0.017	N.D. #
23)	Chlordane-1	4.355f	0.000	2290255	0	6.192	N.D. #
24)	Chlordane-2	4.832	0.000	1771953	0	4.389	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040320\
Data File : PL057792.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Apr 2020 21:17
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 04 07:04:47 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:41:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

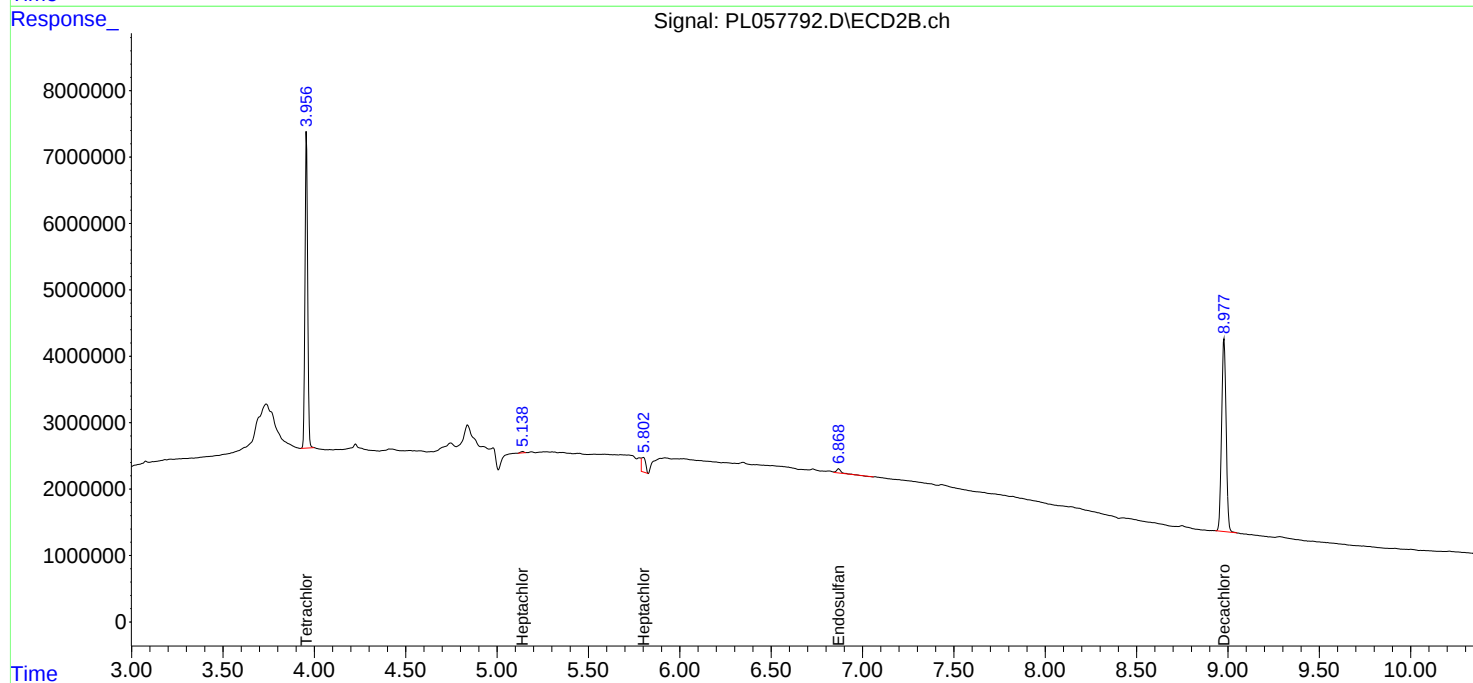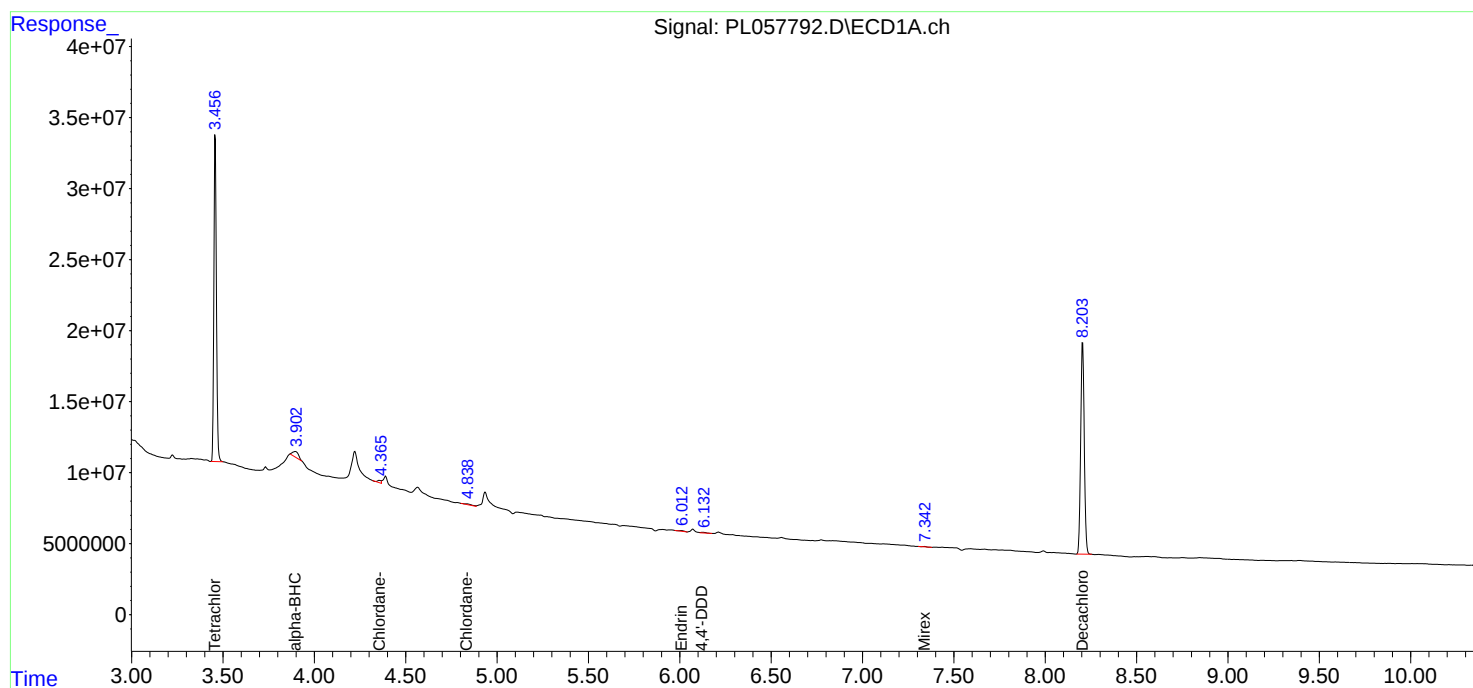


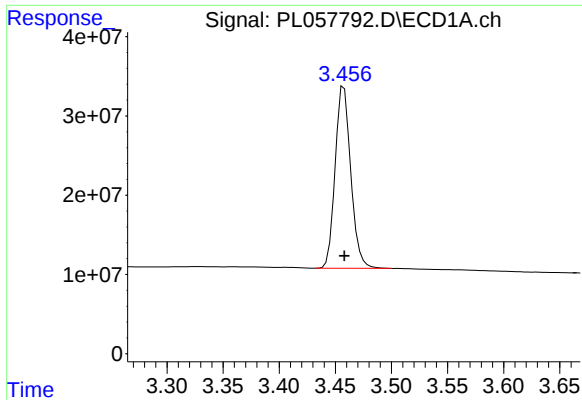

#1 Tetrachloro-m-xylene


R.T.: 3.458 min
Delta R.T.: 0.000 min
Response: 223037752
Conc: 22.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

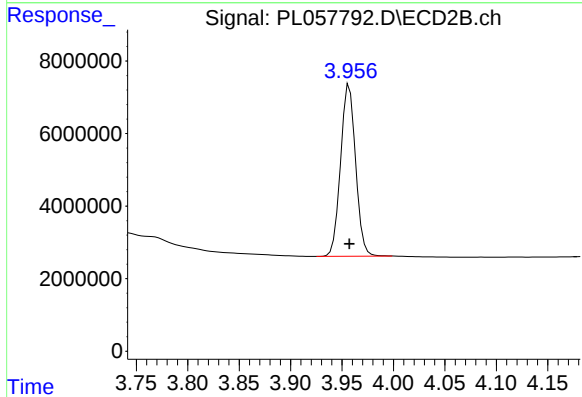


#1 Tetrachloro-m-xylene

R.T.: 3.957 min
Delta R.T.: 0.000 min
Response: 48164314
Conc: 22.19 ng/ml

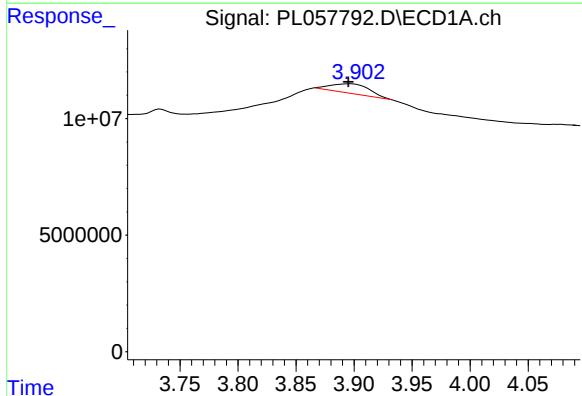


#2 alpha-BHC

R.T.: 3.897 min
Delta R.T.: 0.002 min
Response: 8755623
Conc: 0.50 ng/ml

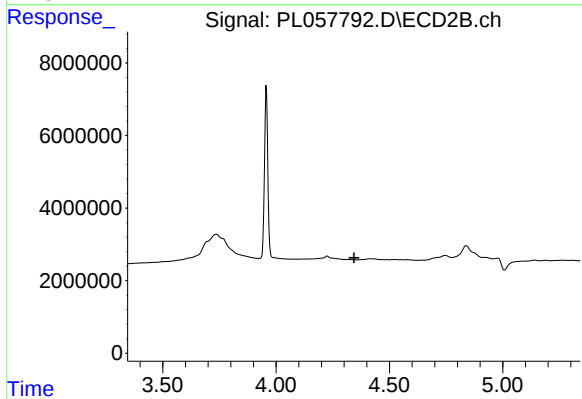

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.345 min
Response: 0
Conc: N.D.

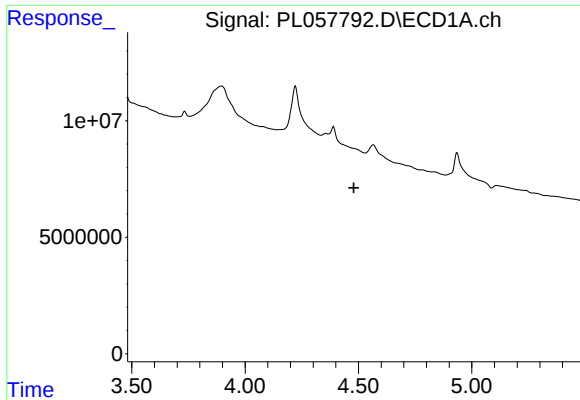

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 4.479 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

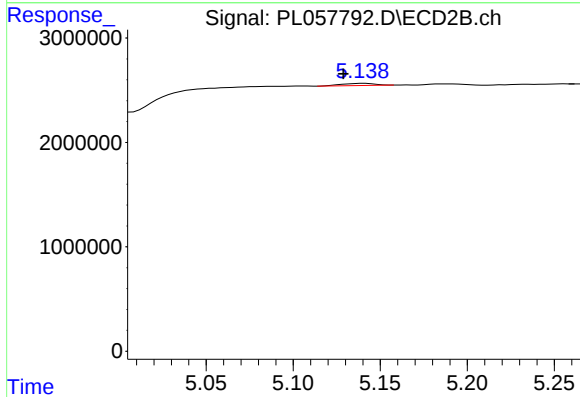


#4 Heptachlor

R.T.: 5.141 min
Delta R.T.: 0.012 min
Response: 275380
Conc: 0.08 ng/ml

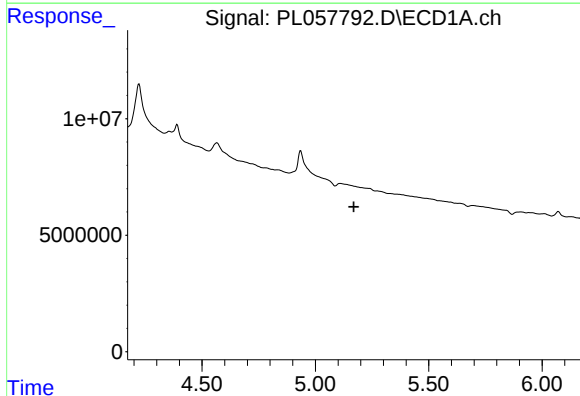


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.169 min
Response: 0
Conc: N.D.

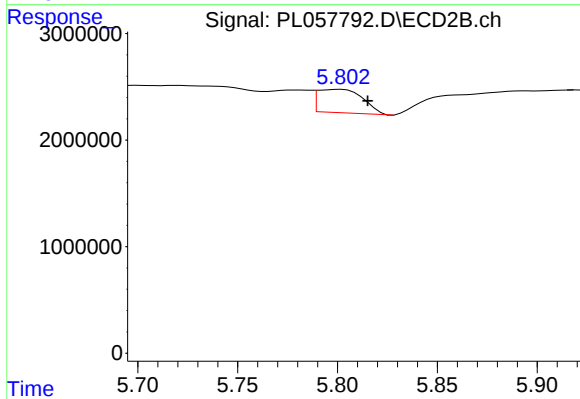

#8 Heptachlor epoxide


R.T.: 5.802 min
Delta R.T.: -0.013 min
Response: 3490451
Conc: 1.29 ng/ml

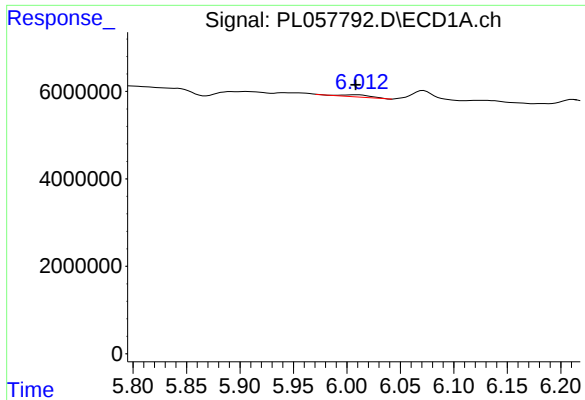

#14 Endrin


R.T.: 6.009 min
Delta R.T.: 0.001 min
Response: 994349
Conc: 0.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

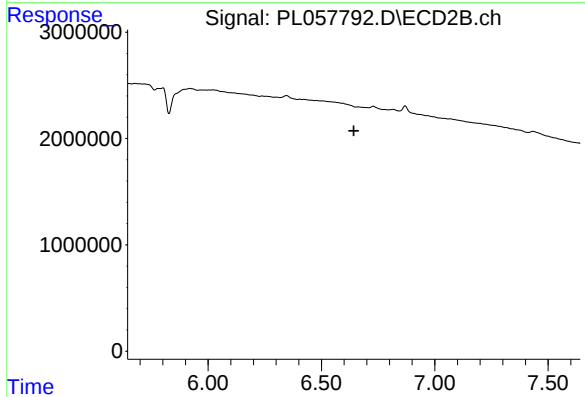


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.642 min
Response: 0
Conc: N.D.

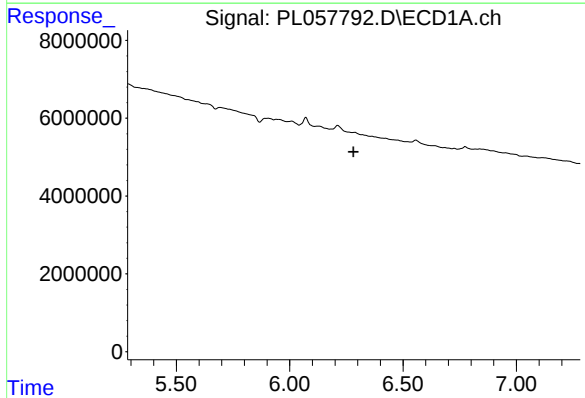


#15 Endosulfan II

R.T.: 6.287 min
Delta R.T.: 0.006 min
Response: -614748
Conc: N.D.

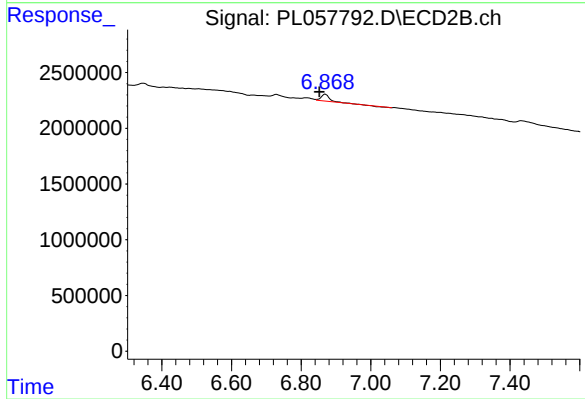

#15 Endosulfan II


R.T.: 6.869 min
Delta R.T.: 0.017 min
Response: 1042555
Conc: 0.40 ng/ml

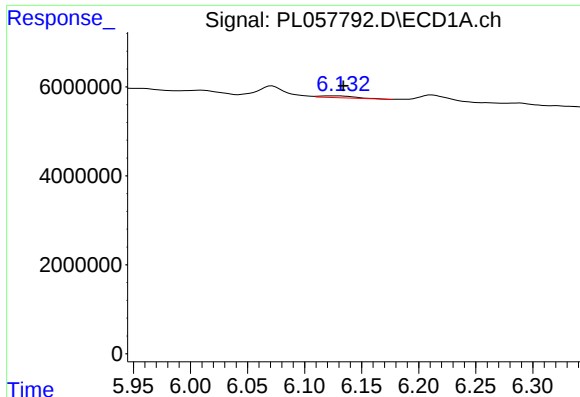

#16 4,4'-DDD


R.T.: 6.124 min
Delta R.T.: -0.010 min
Response: 680430
Conc: 0.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

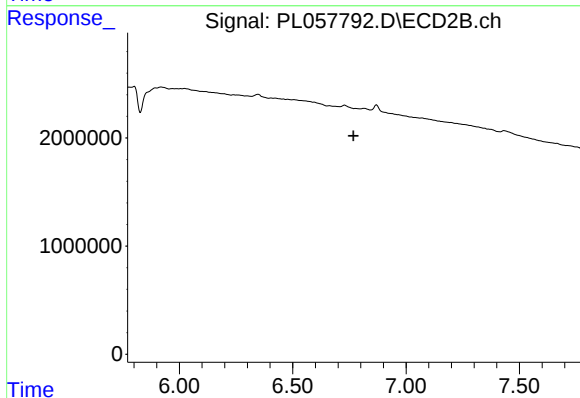


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.769 min
Response: 0
Conc: N.D.

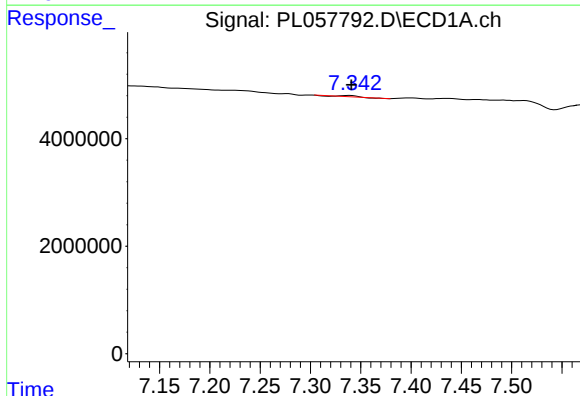


#22 Mirex

R.T.: 7.339 min
Delta R.T.: -0.002 min
Response: 142854
Conc: 0.02 ng/ml

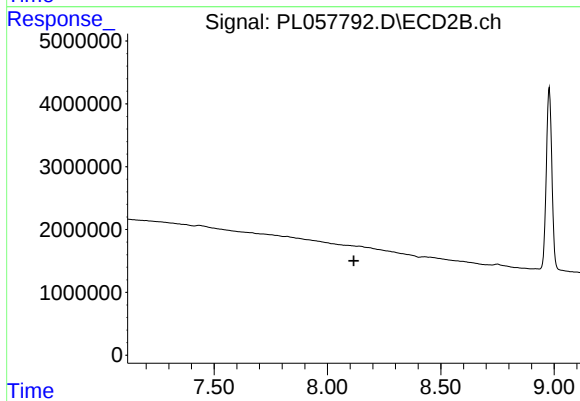

#22 Mirex


R.T.: 0.000 min
Exp R.T. : 8.117 min
Response: 0
Conc: N.D.

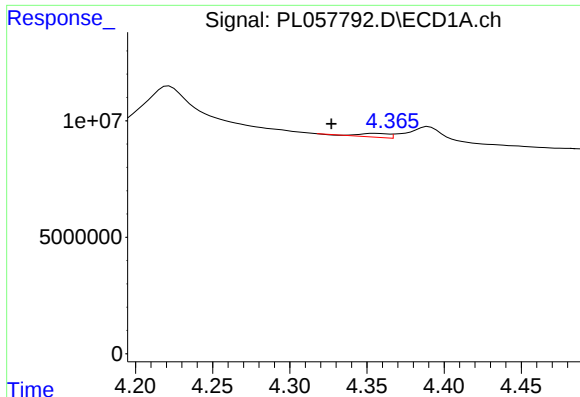

#23 Chlordane-1


R.T.: 4.355 min
Delta R.T.: 0.029 min
Response: 2290255
Conc: 6.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

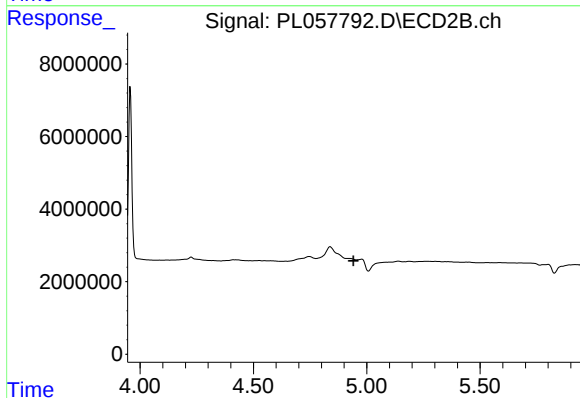


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.942 min
Response: 0
Conc: N.D.

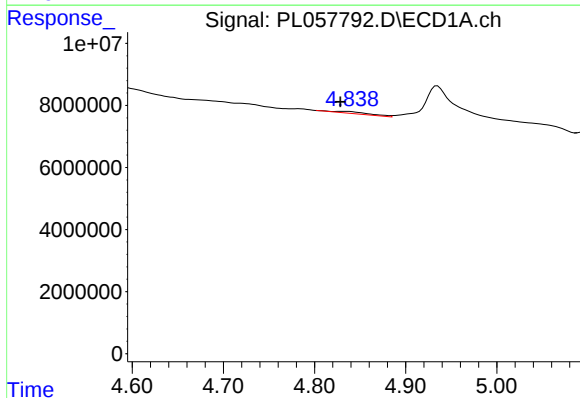


#24 Chlordane-2

R.T.: 4.832 min
Delta R.T.: 0.004 min
Response: 1771953
Conc: 4.39 ng/ml

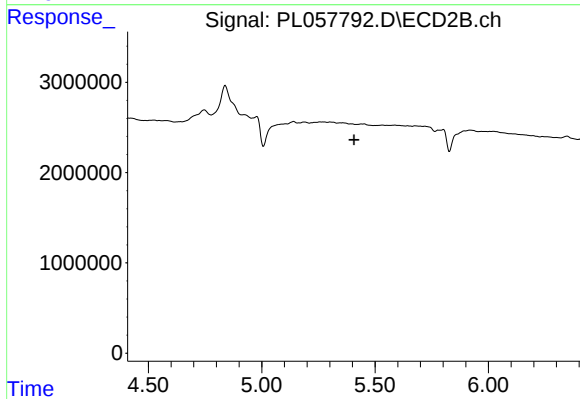

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.407 min
Response: 0
Conc: N.D.

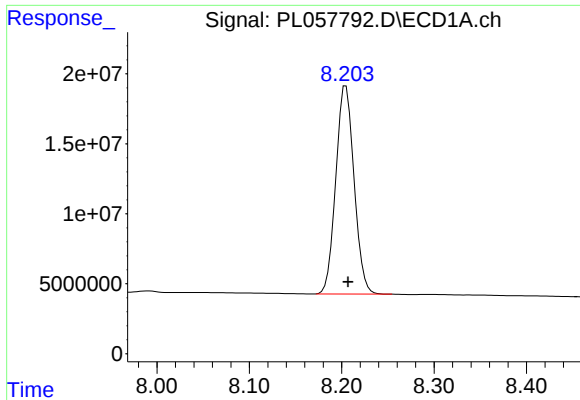

#28 Decachlorobiphenyl

R.T.: 8.205 min
Delta R.T.: -0.002 min
Response: 204740190
Conc: 19.86 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

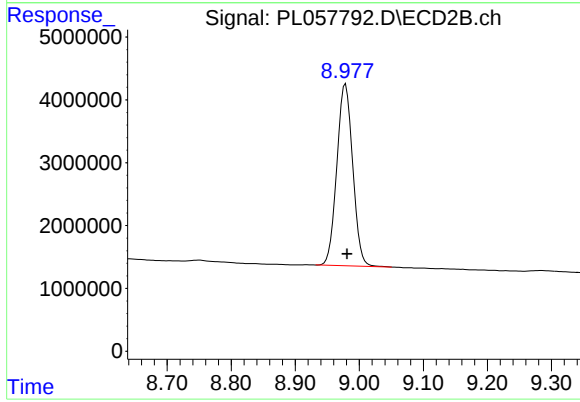

#28 Decachlorobiphenyl

R.T.: 8.979 min
Delta R.T.: -0.002 min
Response: 49765642
Conc: 22.28 ng/ml