

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040320\
 Data File : PL057756.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Apr 2020 10:32
 Operator : AJ\MA
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 04 07:27:07 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:41:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.458	3.957	218.5E6	47105086	21.671	21.706
28)	SA Decachlor...	8.207	8.981	219.3E6	49221711	21.279	22.035
Target Compounds							
9)	A Endosulfan I	5.509	6.170	118.2E6	29927595	9.643	10.037
10)	B gamma-Chl...	5.396	6.049	126.7E6	31804878	9.332	9.817
12)	B 4,4'-DDE	5.619	6.280	261.0E6	58416503	19.927	19.731
13)	MA Dieldrin	5.751	6.426	259.6E6	61460478	19.955	20.114
19)	B Endosulfa...	6.663	7.200	204.2E6	47472361	20.100	20.005
20)	A Methoxychlor	6.920	7.525	548.4E6	124.9E6	99.488	98.224
21)	B Endrin ke...	7.154	7.667	220.5E6	50192956	19.802	20.304



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040320\
Data File : PL057756.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Apr 2020 10:32
Operator : AJ\MA
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 04 07:27:07 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:41:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

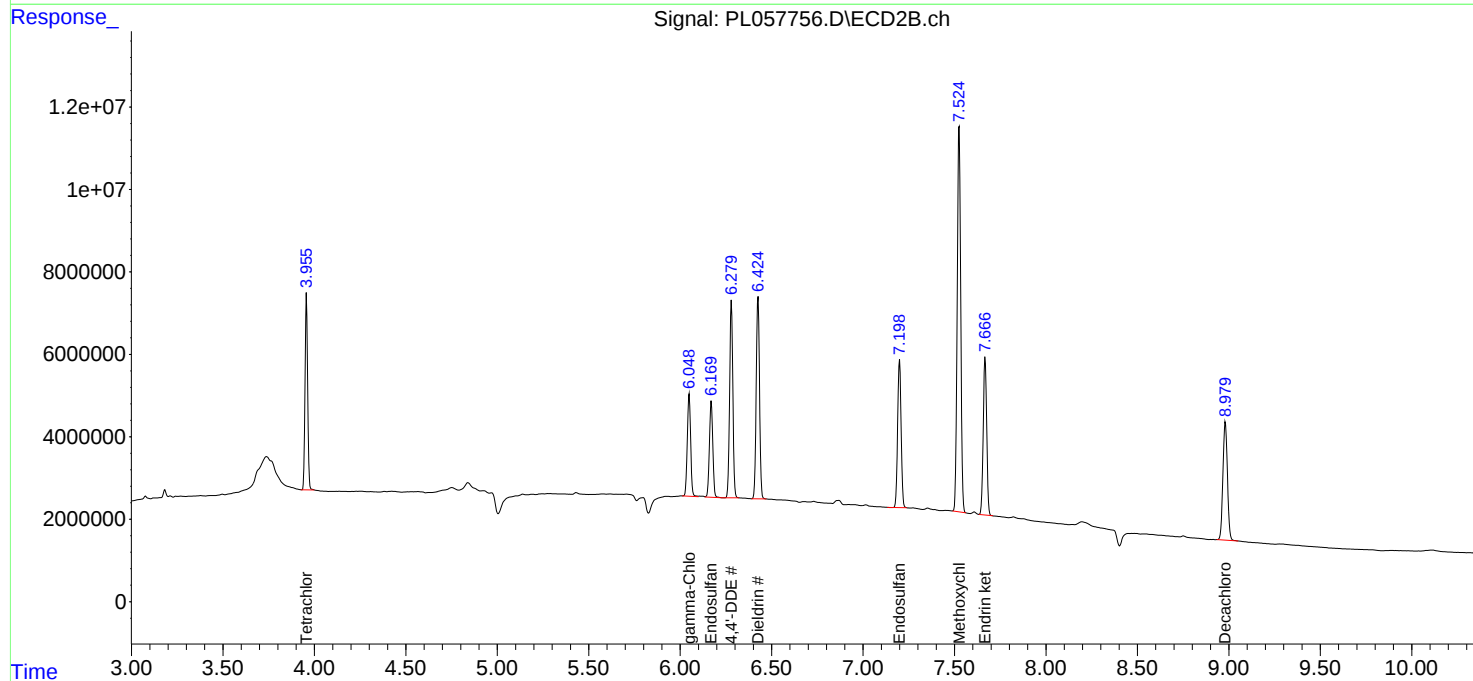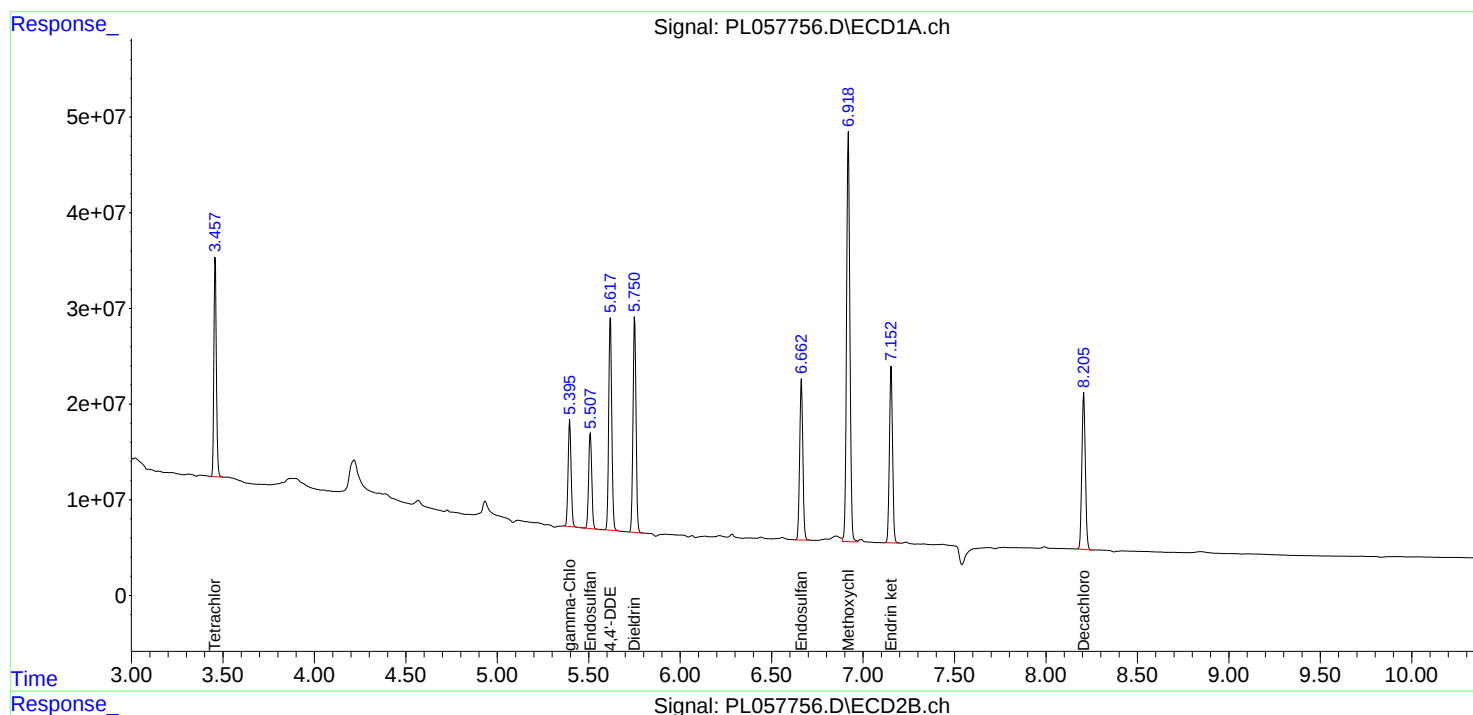


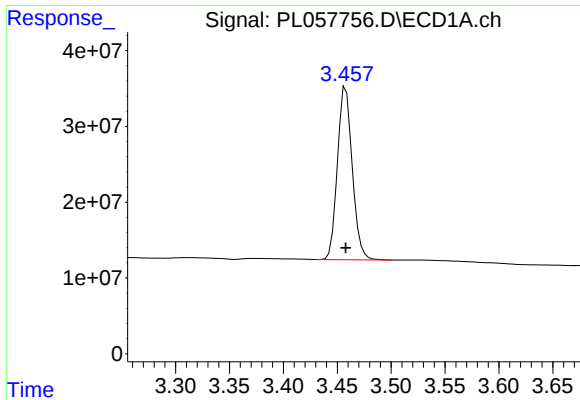

#1 Tetrachloro-m-xylene


R.T.: 3.458 min
Delta R.T.: 0.000 min
Response: 218465419
Conc: 21.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

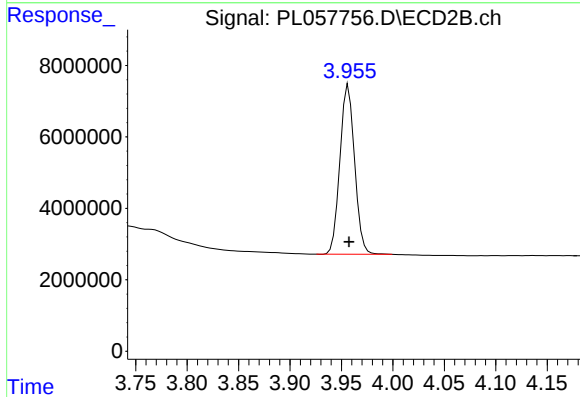


#1 Tetrachloro-m-xylene

R.T.: 3.957 min
Delta R.T.: 0.000 min
Response: 47105086
Conc: 21.71 ng/ml

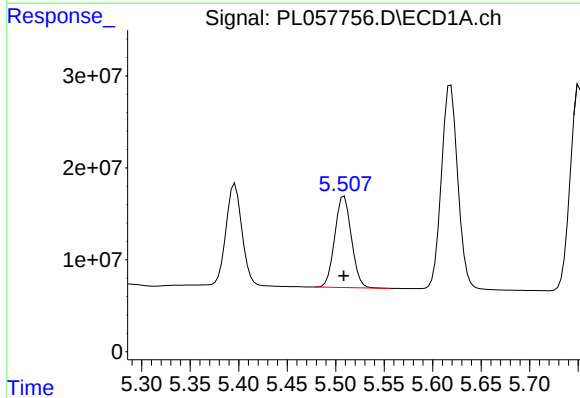


#9 Endosulfan I

R.T.: 5.509 min
Delta R.T.: 0.000 min
Response: 118191106
Conc: 9.64 ng/ml

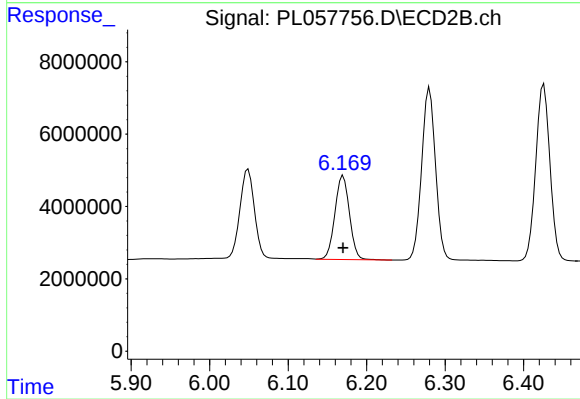

#9 Endosulfan I


R.T.: 6.170 min
Delta R.T.: 0.000 min
Response: 29927595
Conc: 10.04 ng/ml

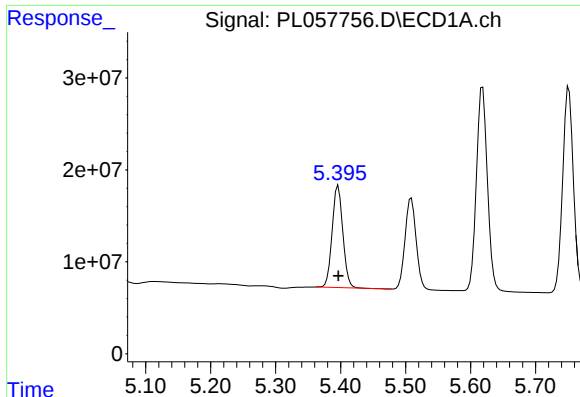

#10 gamma-Chlordane


R.T.: 5.396 min
Delta R.T.: 0.000 min
Response: 126736462
Conc: 9.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

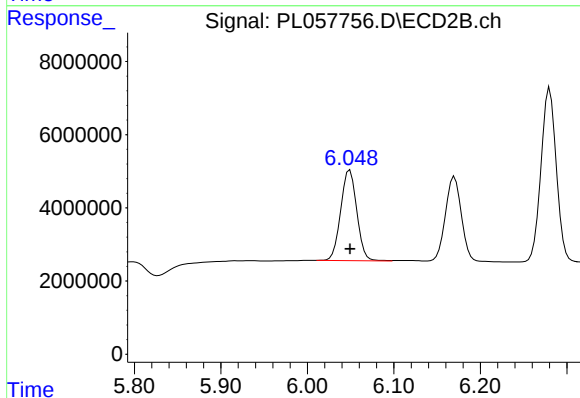


#10 gamma-Chlordane

R.T.: 6.049 min
Delta R.T.: 0.000 min
Response: 31804878
Conc: 9.82 ng/ml

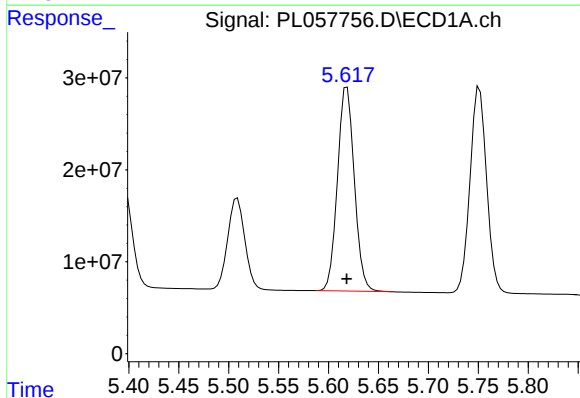


#12 4,4'-DDE

R.T.: 5.619 min
Delta R.T.: 0.000 min
Response: 261044293
Conc: 19.93 ng/ml

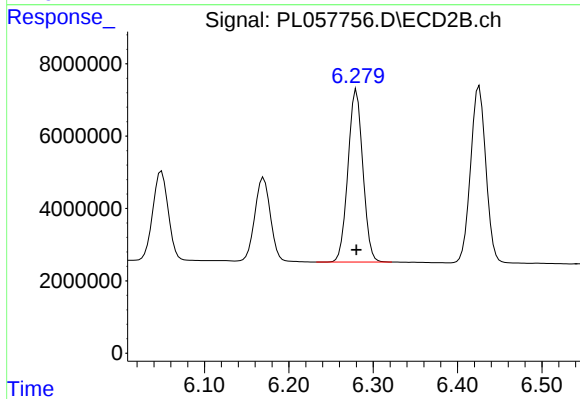

#12 4,4'-DDE


R.T.: 6.280 min
Delta R.T.: 0.000 min
Response: 58416503
Conc: 19.73 ng/ml

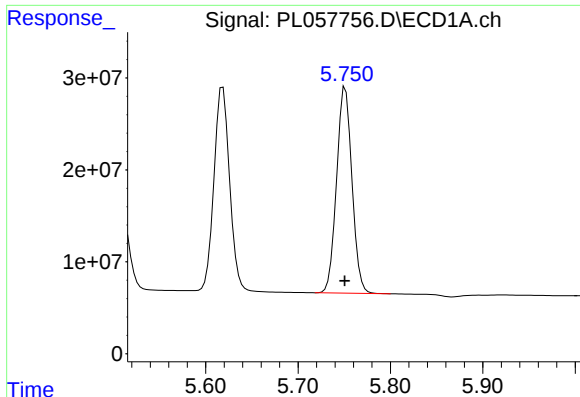

#13 Dieldrin


R.T.: 5.751 min
Delta R.T.: 0.000 min
Response: 259598932
Conc: 19.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

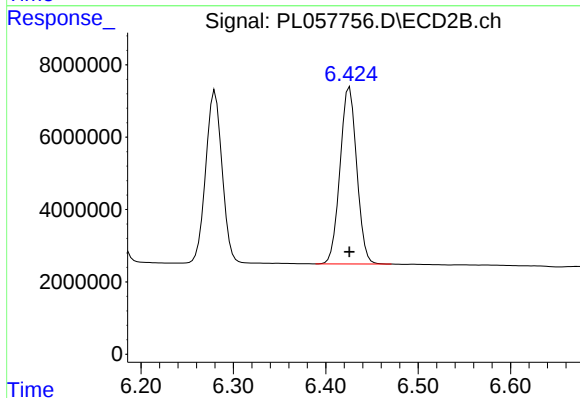


#13 Dieldrin

R.T.: 6.426 min
Delta R.T.: 0.000 min
Response: 61460478
Conc: 20.11 ng/ml

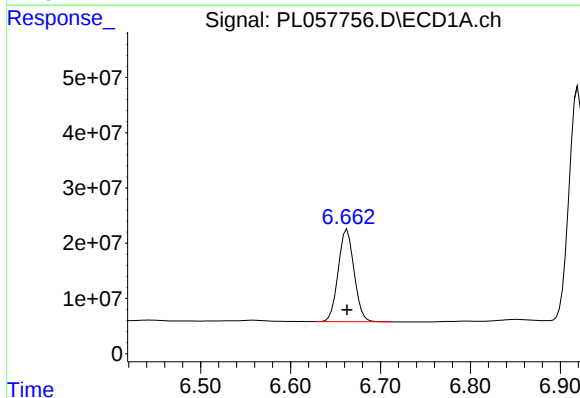


#19 Endosulfan Sulfate

R.T.: 6.663 min
Delta R.T.: 0.000 min
Response: 204214303
Conc: 20.10 ng/ml

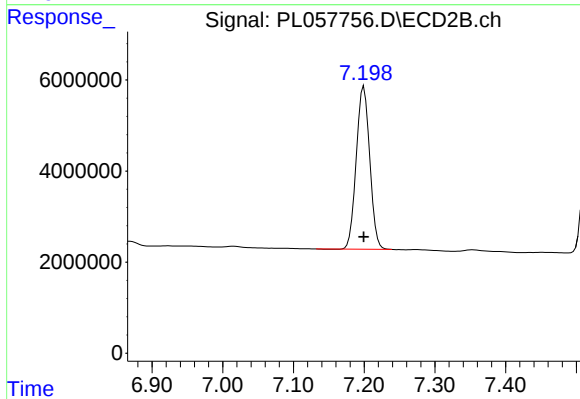

#19 Endosulfan Sulfate


R.T.: 7.200 min
Delta R.T.: 0.000 min
Response: 47472361
Conc: 20.00 ng/ml

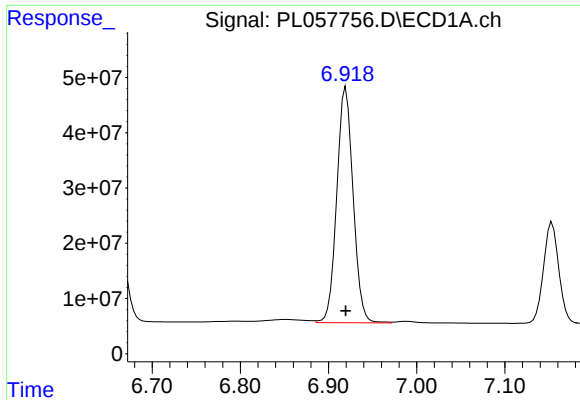

#20 Methoxychlor


R.T.: 6.920 min
Delta R.T.: 0.000 min
Response: 548436275
Conc: 99.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

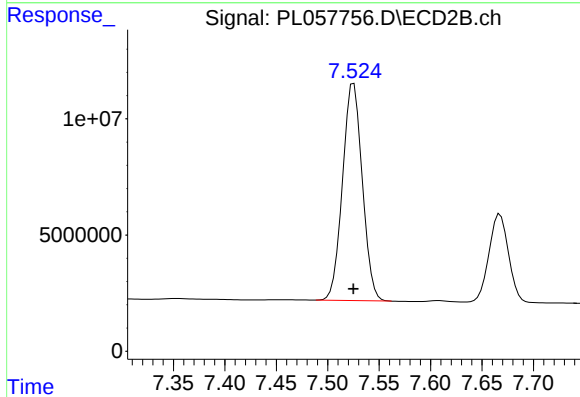


#20 Methoxychlor

R.T.: 7.525 min
Delta R.T.: 0.000 min
Response: 124943200
Conc: 98.22 ng/ml

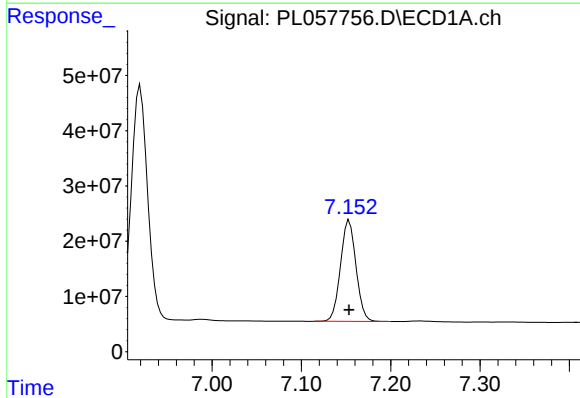


#21 Endrin ketone

R.T.: 7.154 min
Delta R.T.: 0.000 min
Response: 220455099
Conc: 19.80 ng/ml

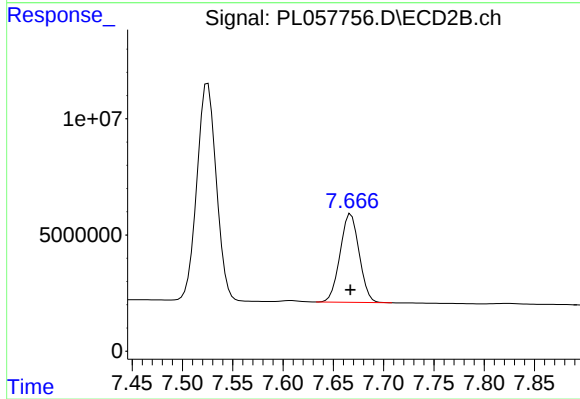

#21 Endrin ketone


R.T.: 7.667 min
Delta R.T.: 0.000 min
Response: 50192956
Conc: 20.30 ng/ml

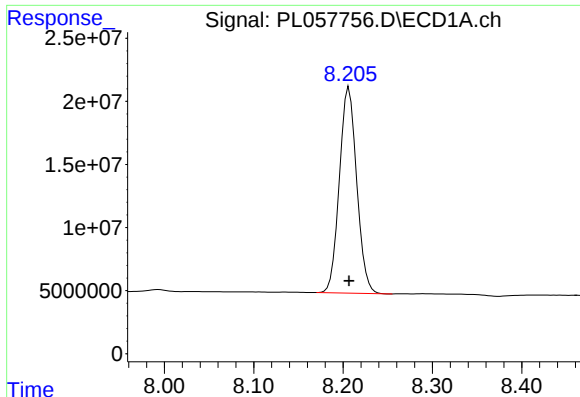

#28 Decachlorobiphenyl

R.T.: 8.207 min
Delta R.T.: 0.000 min
Response: 219349354
Conc: 21.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

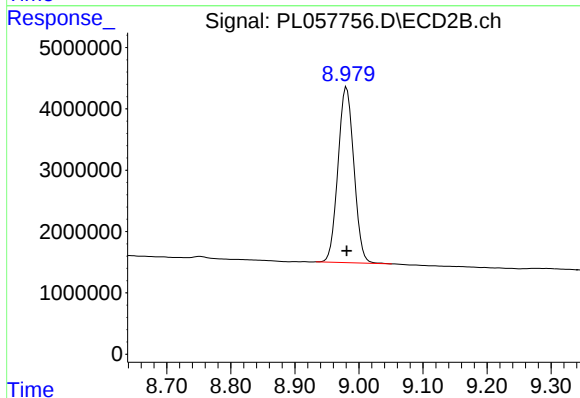

#28 Decachlorobiphenyl

R.T.: 8.981 min
Delta R.T.: 0.000 min
Response: 49221711
Conc: 22.04 ng/ml