

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040324\
 Data File : PL088901.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Apr 2024 13:40
 Operator : AR\AJ
 Sample : PB159873BS
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB159873BS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 04 01:15:16 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031324.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 13 15:45:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.640	2.851	49947677	32891354	18.848	24.679 #
28)	SA Decachlor...	9.310	8.081	42363329	28623215	17.138	21.110
Target Compounds							
23)	Chlordane-1	4.825	3.874	23966652	10790375	206.105	222.228
24)	Chlordane-2	5.361	4.461	29129292	14310275	221.569	235.694
25)	Chlordane-3	6.081	5.102	104.3E6	38640995	209.725	226.407
26)	Chlordane-4	6.165	5.167	128.0E6	36484300	213.414	228.685
27)	Chlordane-5	7.024	5.843	22588823	12242464	213.699	241.395



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040324\
Data File : PL088901.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Apr 2024 13:40
Operator : AR\AJ
Sample : PB159873BS
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB159873BS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 04 01:15:16 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031324.M
Quant Title : GC Extractables
QLast Update : Wed Mar 13 15:45:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

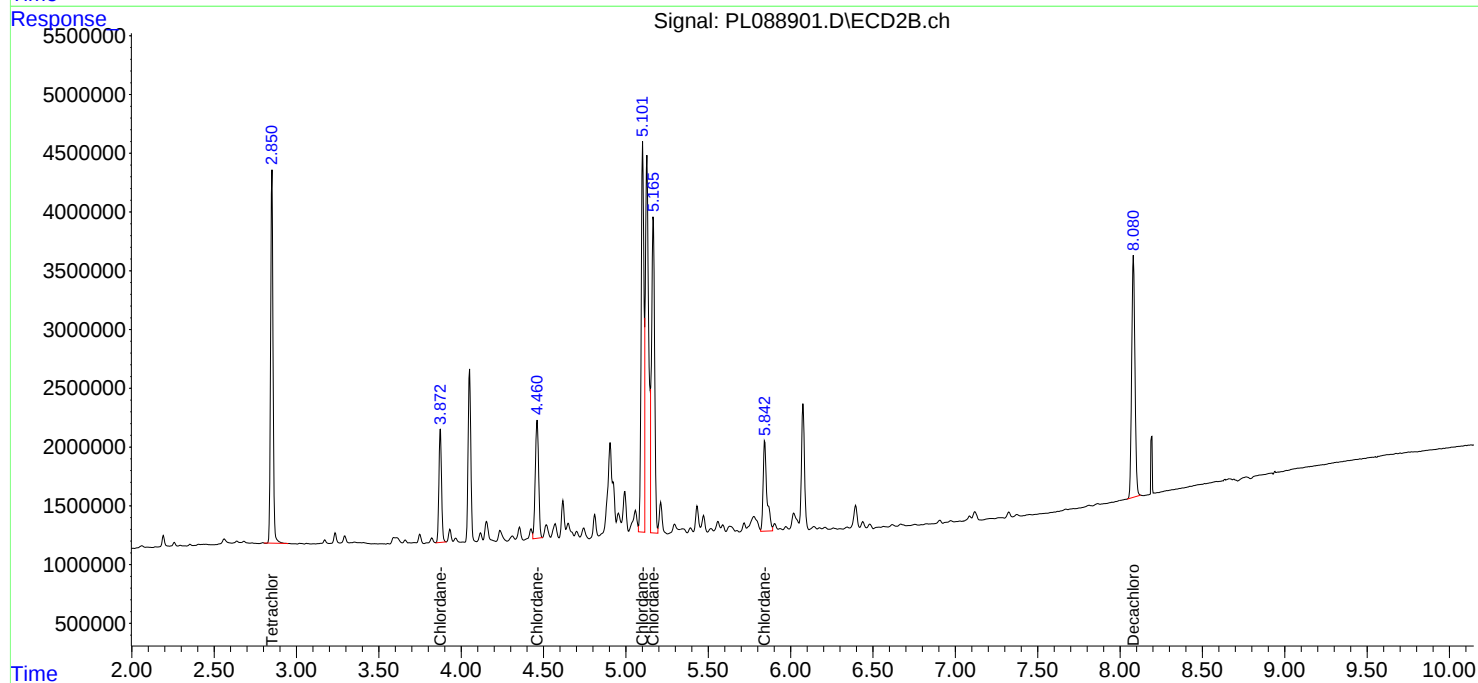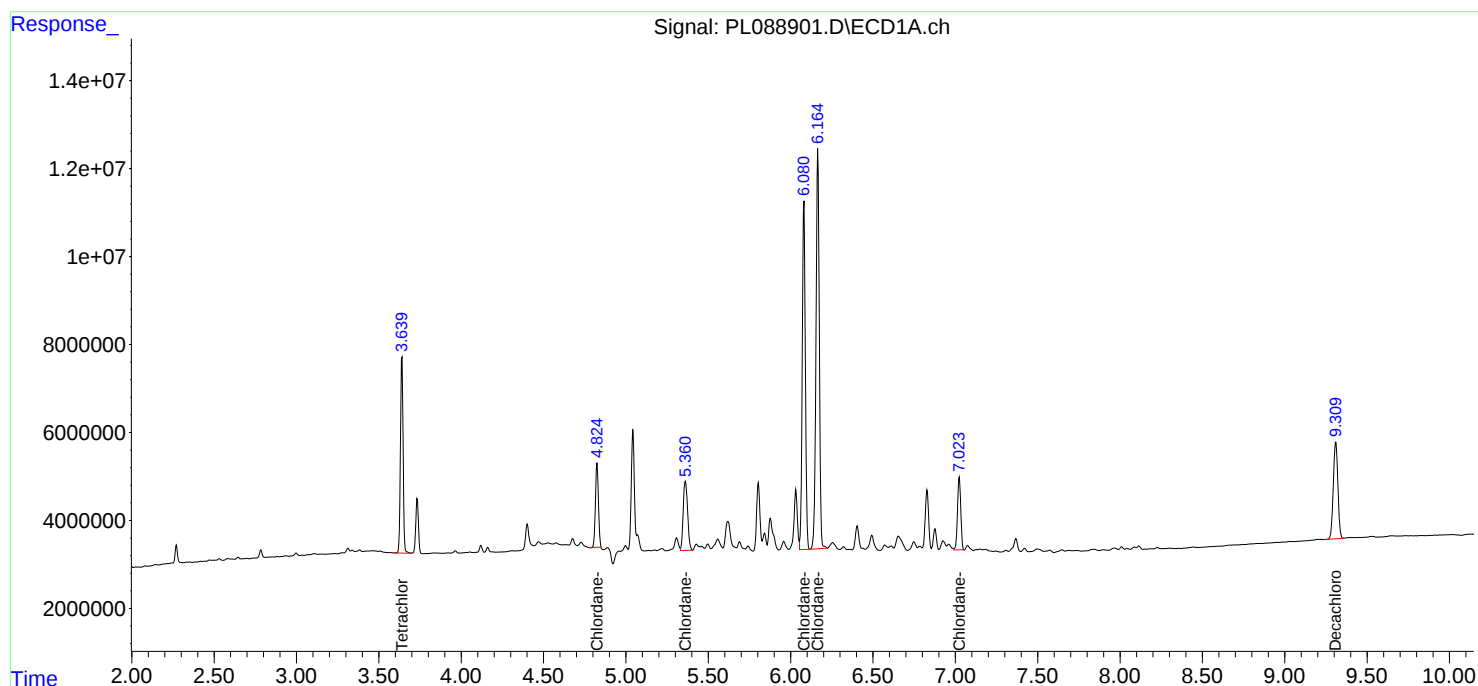


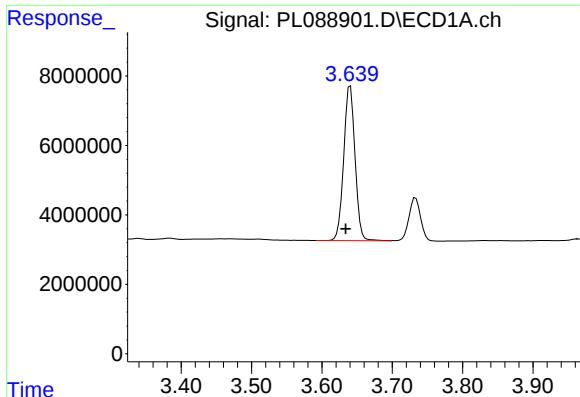

#1 Tetrachloro-m-xylene


R.T.: 3.640 min
Delta R.T.: 0.006 min
Response: 49947677
Conc: 18.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB159873BS

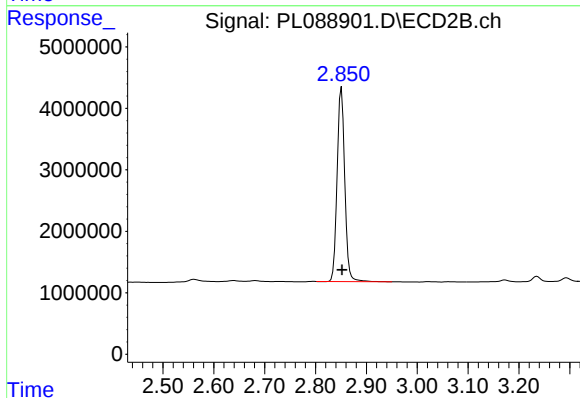


#1 Tetrachloro-m-xylene

R.T.: 2.851 min
Delta R.T.: -0.001 min
Response: 32891354
Conc: 24.68 ng/ml

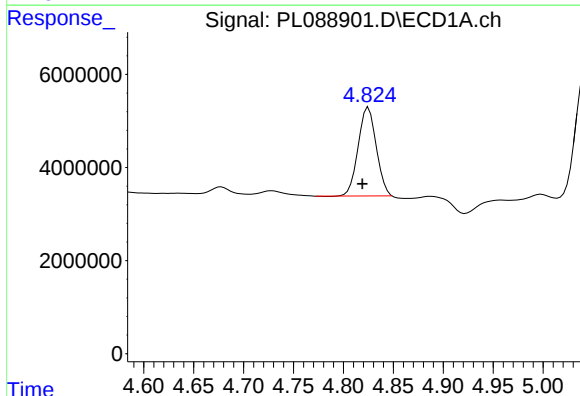


#23 Chlordane-1

R.T.: 4.825 min
Delta R.T.: 0.006 min
Response: 23966652
Conc: 206.11 ng/ml

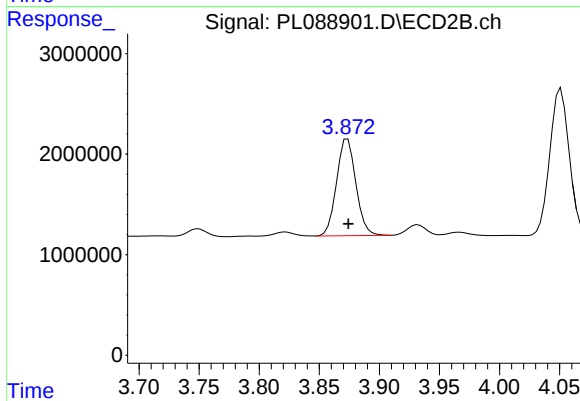

#23 Chlordane-1


R.T.: 3.874 min
Delta R.T.: 0.000 min
Response: 10790375
Conc: 222.23 ng/ml

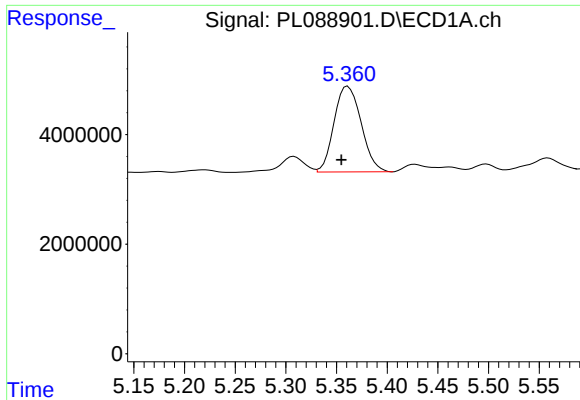

#24 Chlordane-2


R.T.: 5.361 min
Delta R.T.: 0.006 min
Response: 29129292
Conc: 221.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB159873BS

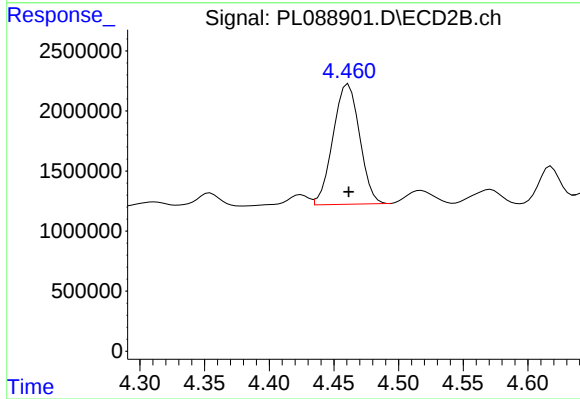


#24 Chlordane-2

R.T.: 4.461 min
Delta R.T.: 0.000 min
Response: 14310275
Conc: 235.69 ng/ml

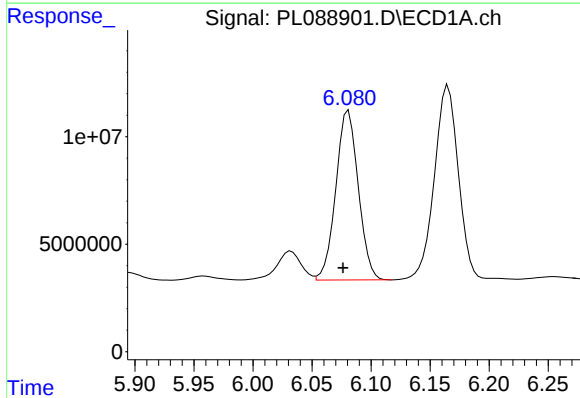


#25 Chlordane-3

R.T.: 6.081 min
Delta R.T.: 0.005 min
Response: 104282825
Conc: 209.73 ng/ml

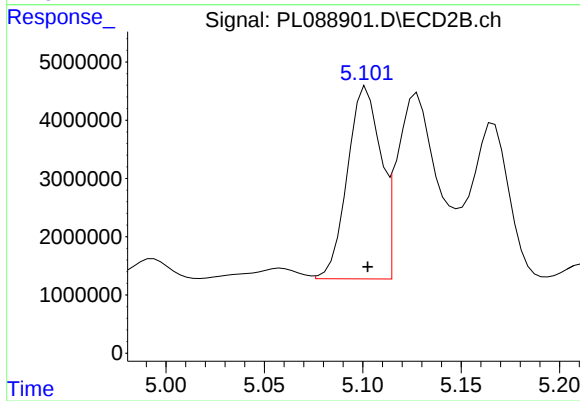

#25 Chlordane-3


R.T.: 5.102 min
Delta R.T.: 0.000 min
Response: 38640995
Conc: 226.41 ng/ml

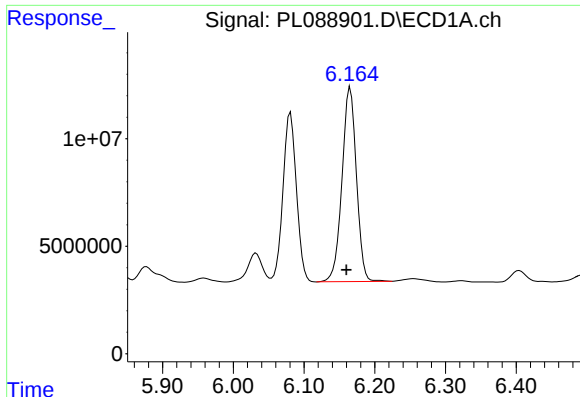

#26 Chlordane-4


R.T.: 6.165 min
Delta R.T.: 0.006 min
Response: 128019856
Conc: 213.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB159873BS

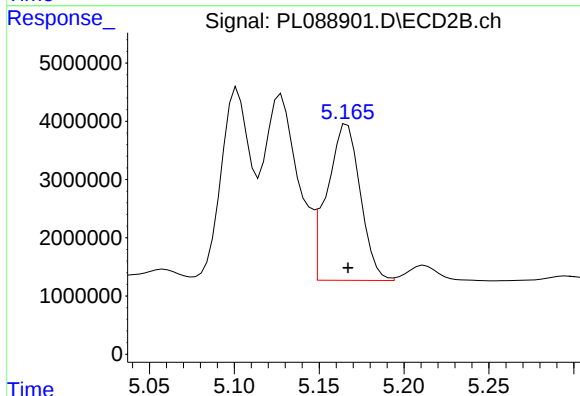


#26 Chlordane-4

R.T.: 5.167 min
Delta R.T.: 0.000 min
Response: 36484300
Conc: 228.68 ng/ml

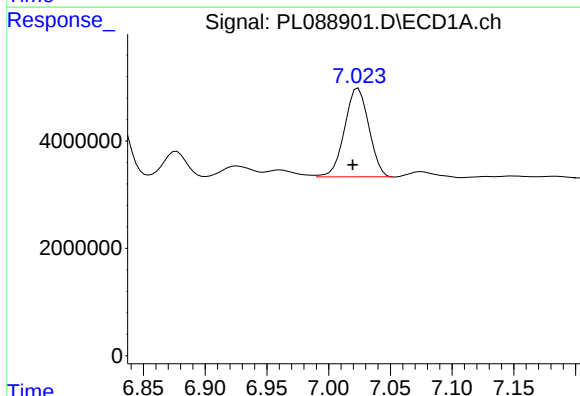


#27 Chlordane-5

R.T.: 7.024 min
Delta R.T.: 0.005 min
Response: 22588823
Conc: 213.70 ng/ml

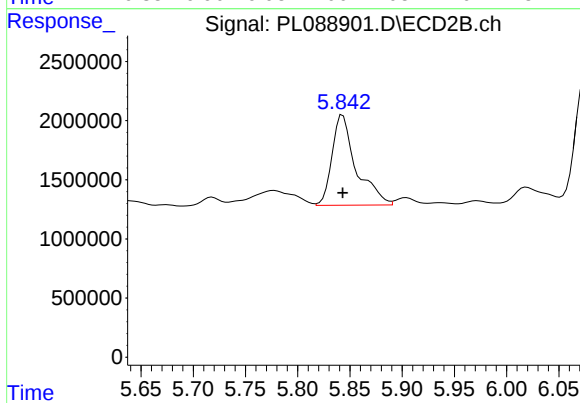

#27 Chlordane-5


R.T.: 5.843 min
Delta R.T.: 0.000 min
Response: 12242464
Conc: 241.40 ng/ml

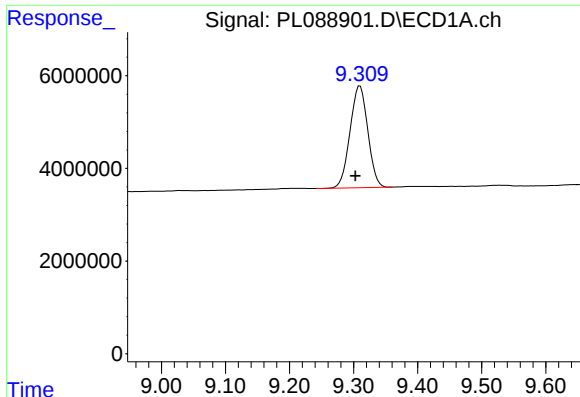

#28 Decachlorobiphenyl

R.T.: 9.310 min
Delta R.T.: 0.007 min
Response: 42363329
Conc: 17.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB159873BS

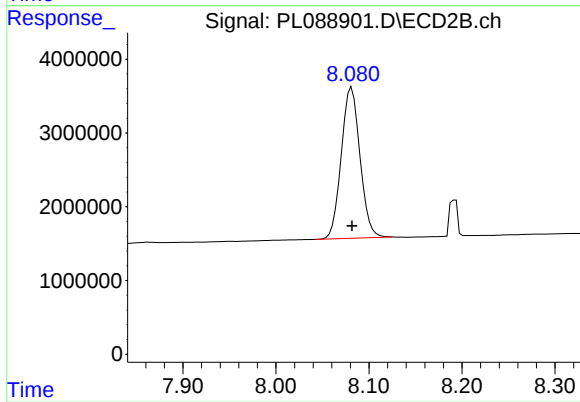

#28 Decachlorobiphenyl

R.T.: 8.081 min
Delta R.T.: 0.000 min
Response: 28623215
Conc: 21.11 ng/ml