

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040324\
 Data File : PL088904.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Apr 2024 15:11
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 04 01:16:12 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031324.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 13 15:45:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.633	2.850	110.8E6	74237078	41.821	55.703 #
28)	SA Decachlor...	9.304	8.079	108.1E6	73864298	43.749	54.475
Target Compounds							
23)	Chlordane-1	4.818	3.872	48974863	22725336	421.168	468.030
24)	Chlordane-2	5.355	4.459	54892645	28481732	417.535	469.103
25)	Chlordane-3	6.075	5.100	205.6E6	81644507	413.517	478.375
26)	Chlordane-4	6.158	5.164	247.7E6	75759183	412.965	474.861
27)	Chlordane-5	7.019	5.840	43978244	24565740	416.051	484.384

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040324\
Data File : PL088904.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Apr 2024 15:11
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e

Integration File signal 2: autoint2.e

Quant Time: Apr 04 01:16:12 2024

Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031324.M

Quant Title : GC Extractables

QLast Update : Wed Mar 13 15:45:55 2024

Response via : Initial Calibration



Integrator: ChemStation


Volume Inj. : 1 µl

Signal #1 Phase : ZB-MR2

Signal #2 Phase: ZB-MR1

Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

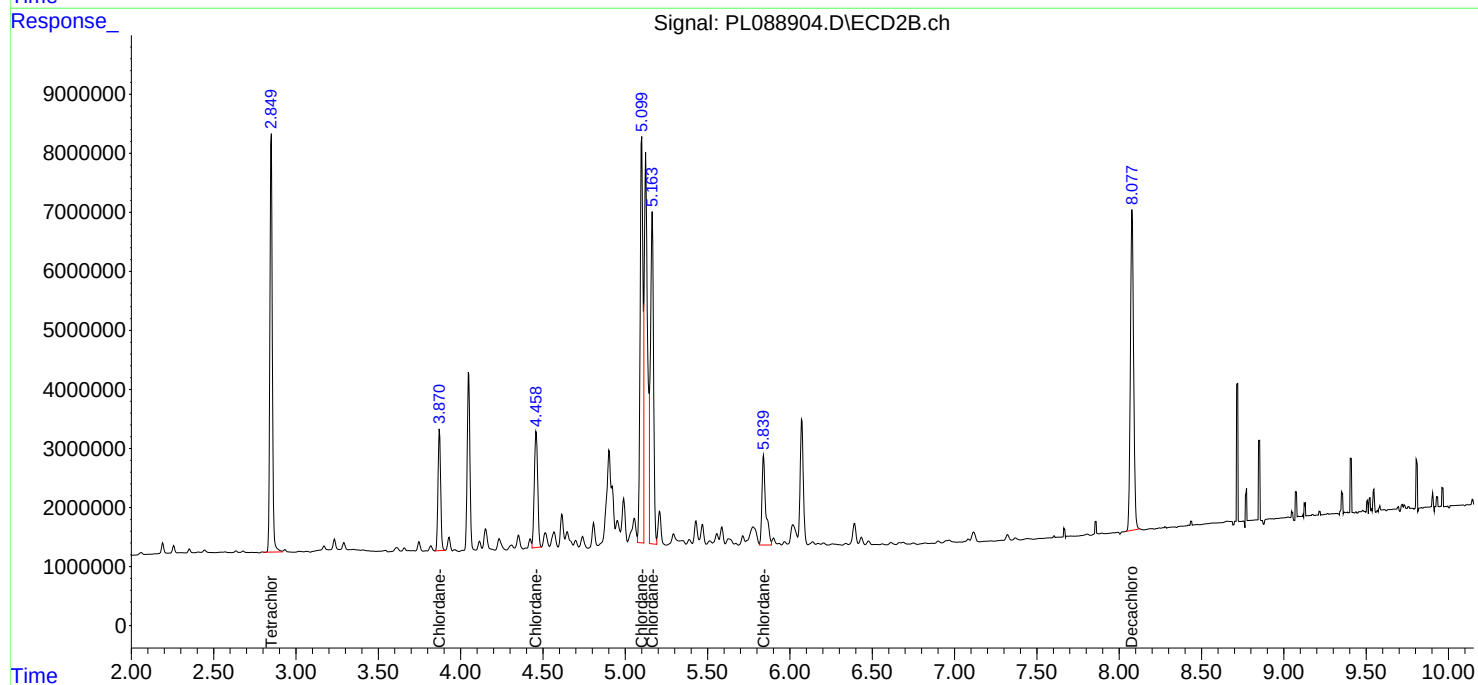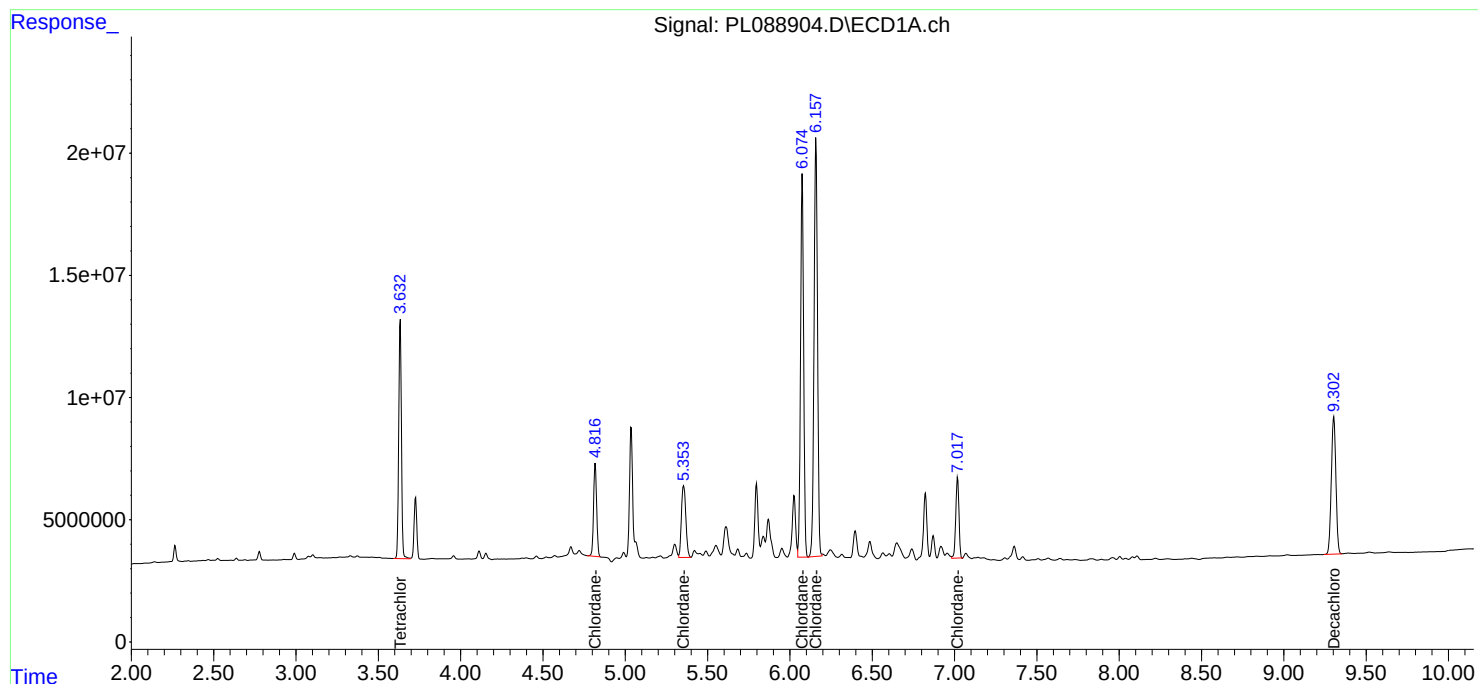


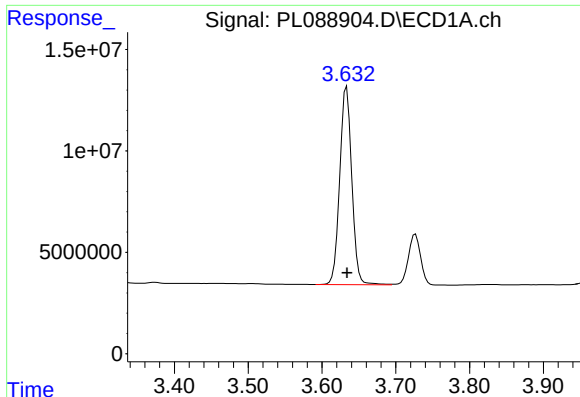

#1 Tetrachloro-m-xylene


R.T.: 3.633 min
Delta R.T.: 0.000 min
Response: 110825546
Conc: 41.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

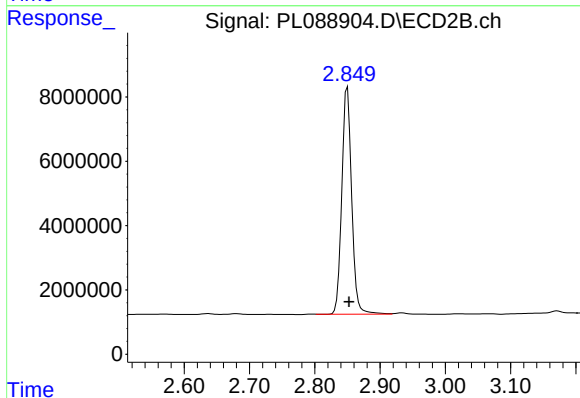


#1 Tetrachloro-m-xylene

R.T.: 2.850 min
Delta R.T.: -0.002 min
Response: 74237078
Conc: 55.70 ng/ml

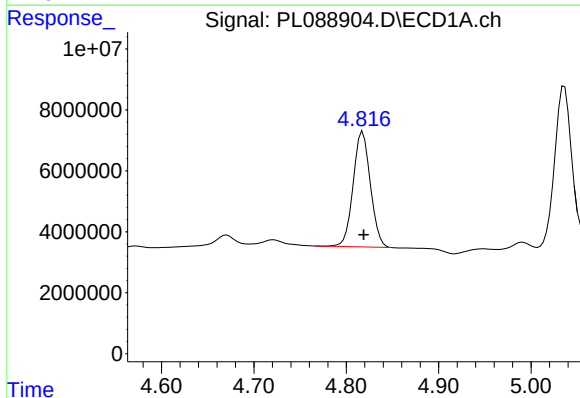


#23 Chlordane-1

R.T.: 4.818 min
Delta R.T.: -0.001 min
Response: 48974863
Conc: 421.17 ng/ml

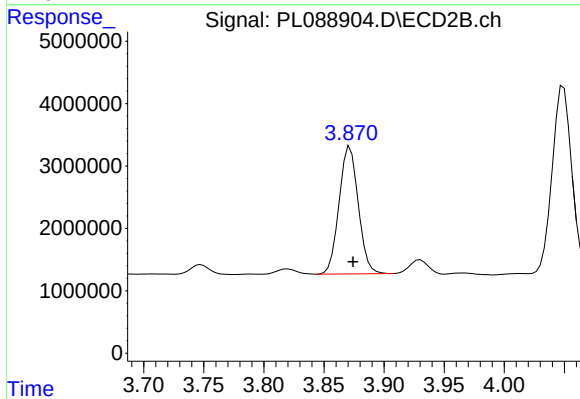

#23 Chlordane-1


R.T.: 3.872 min
Delta R.T.: -0.002 min
Response: 22725336
Conc: 468.03 ng/ml

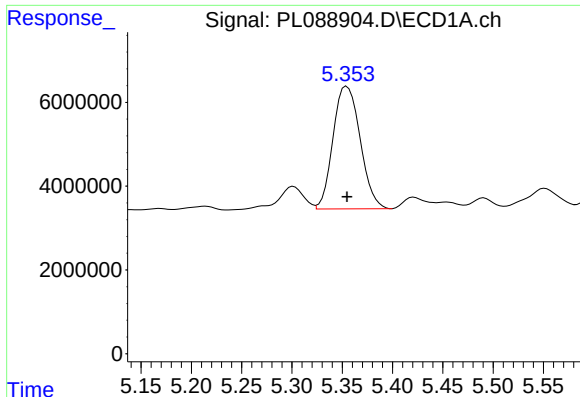

#24 Chlordane-2


R.T.: 5.355 min
Delta R.T.: 0.000 min
Response: 54892645
Conc: 417.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

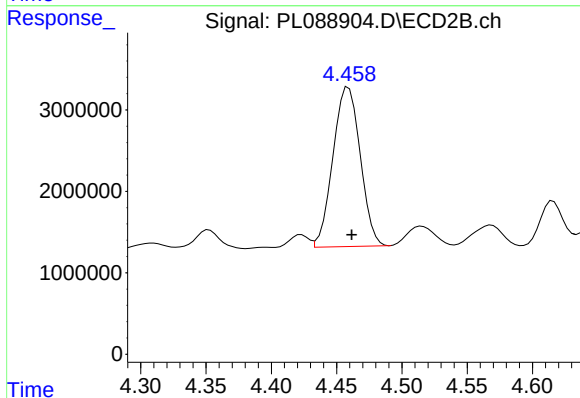


#24 Chlordane-2

R.T.: 4.459 min
Delta R.T.: -0.002 min
Response: 28481732
Conc: 469.10 ng/ml

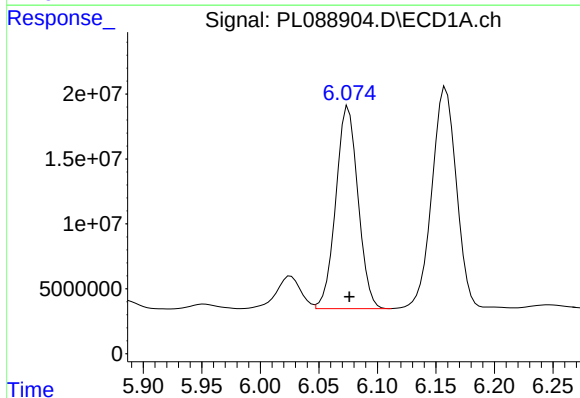


#25 Chlordane-3

R.T.: 6.075 min
Delta R.T.: -0.001 min
Response: 205615472
Conc: 413.52 ng/ml

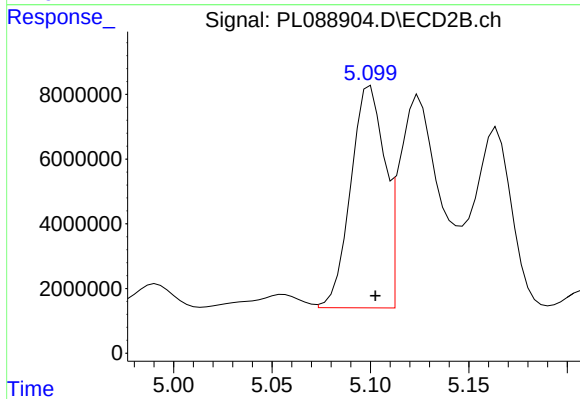

#25 Chlordane-3


R.T.: 5.100 min
Delta R.T.: -0.002 min
Response: 81644507
Conc: 478.37 ng/ml

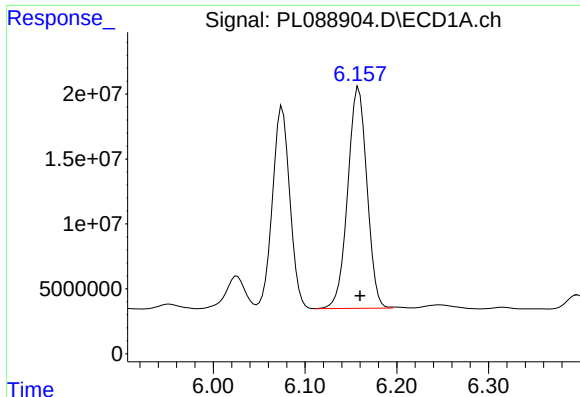

#26 Chlordane-4


R.T.: 6.158 min
Delta R.T.: -0.001 min
Response: 247724168
Conc: 412.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

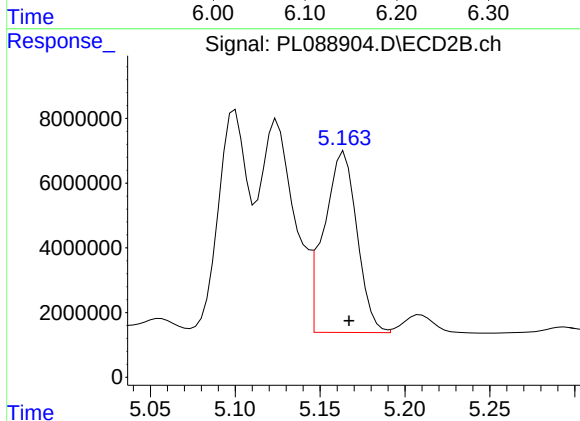


#26 Chlordane-4

R.T.: 5.164 min
Delta R.T.: -0.003 min
Response: 75759183
Conc: 474.86 ng/ml

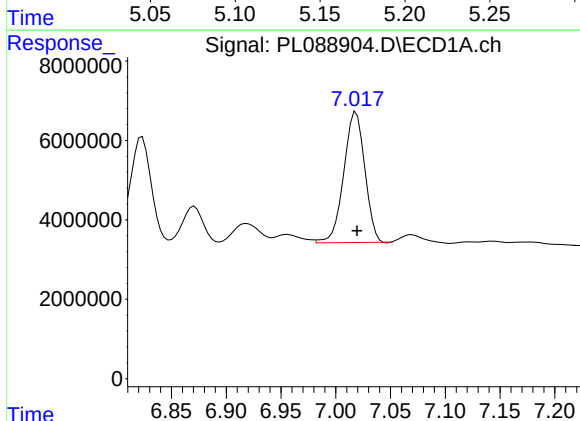


#27 Chlordane-5

R.T.: 7.019 min
Delta R.T.: 0.000 min
Response: 43978244
Conc: 416.05 ng/ml

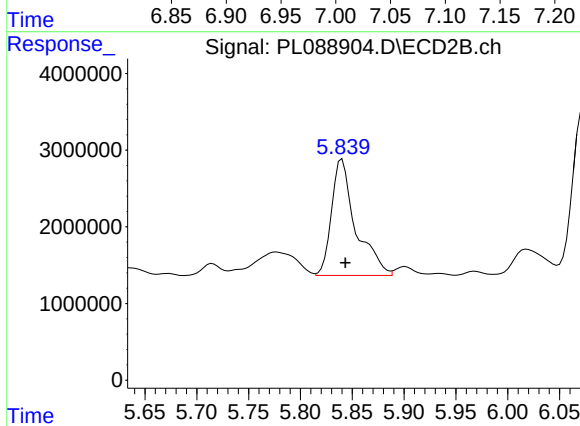

#27 Chlordane-5


R.T.: 5.840 min
Delta R.T.: -0.003 min
Response: 24565740
Conc: 484.38 ng/ml

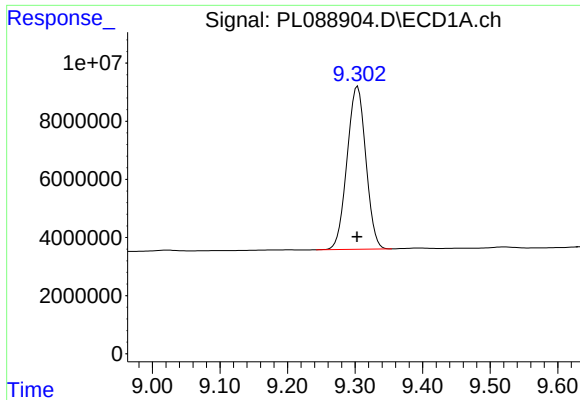

#28 Decachlorobiphenyl

R.T.: 9.304 min
Delta R.T.: 0.001 min
Response: 108143356
Conc: 43.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

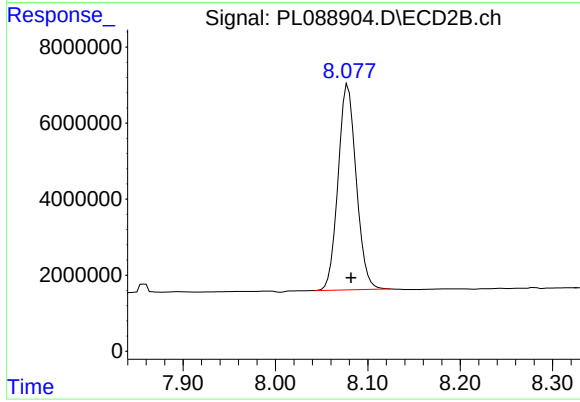

#28 Decachlorobiphenyl

R.T.: 8.079 min
Delta R.T.: -0.003 min
Response: 73864298
Conc: 54.48 ng/ml