

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040419\
 Data File : PL047027.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Apr 2019 15:21
 Operator : AJ\SJ
 Sample : K2240-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 00:55:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.358	3.976	121.1E6	38183946	16.647	16.677
28)	SA Decachlor...	8.034	9.027	120.8E6	35541628	14.359	15.330
Target Compounds							
11)	B alpha-Chl...	0.000	6.155	0	1470855	N.D.	0.519 #
26)	Chlordane-4	0.000	6.155	0	1470855	N.D.	3.188 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040419\
Data File : PL047027.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Apr 2019 15:21
Operator : AJ\SJ
Sample : K2240-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 00:55:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

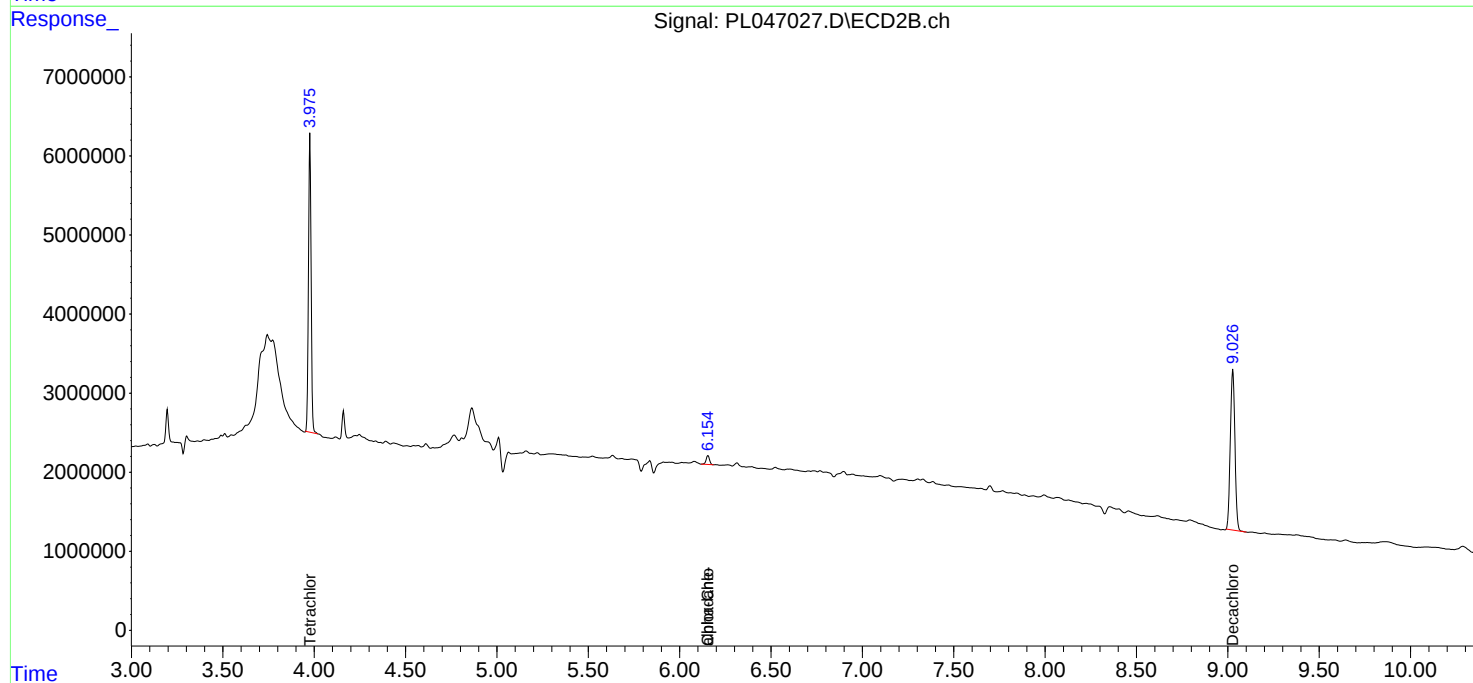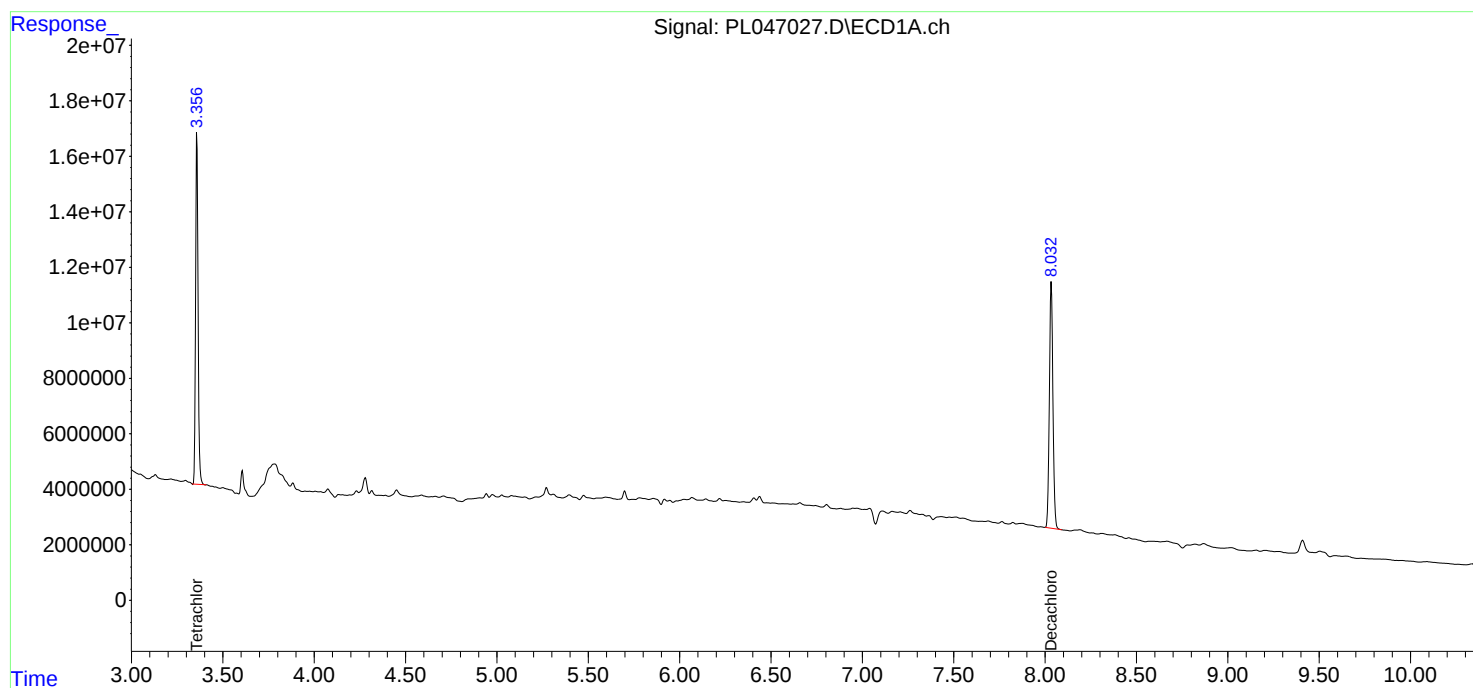


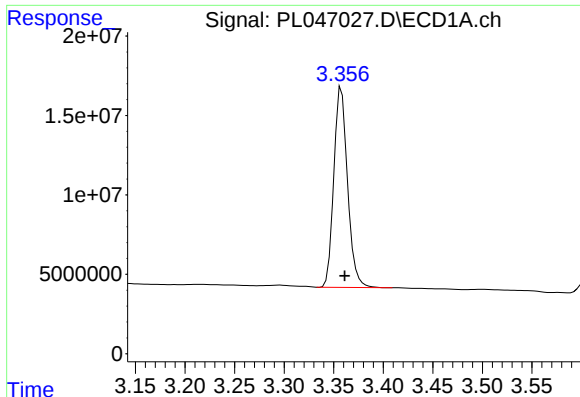

#1 Tetrachloro-m-xylene


R.T.: 3.358 min
Delta R.T.: -0.003 min
Response: 121097741
Conc: 16.65 ng/ml

Instrument :
ECD_L
ClientSampleId :

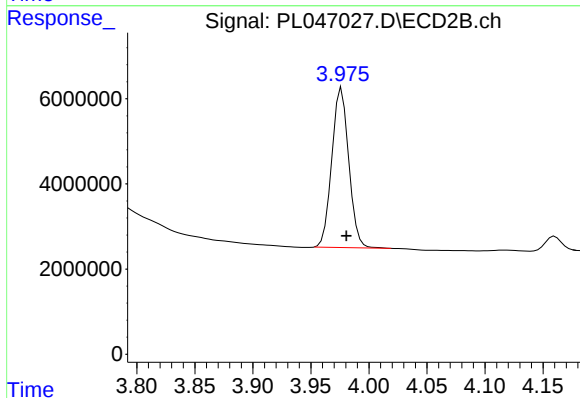


#1 Tetrachloro-m-xylene

R.T.: 3.976 min
Delta R.T.: -0.004 min
Response: 38183946
Conc: 16.68 ng/ml

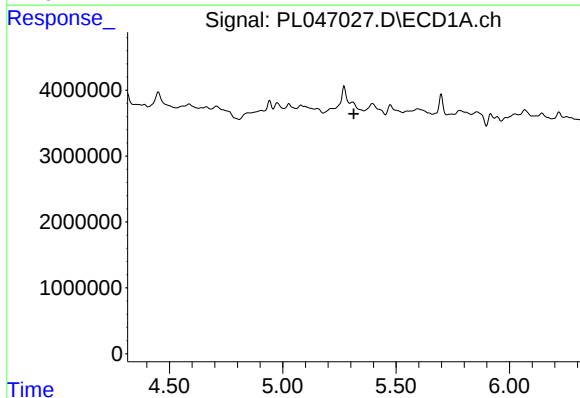


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.314 min
Response: 0
Conc: N.D.

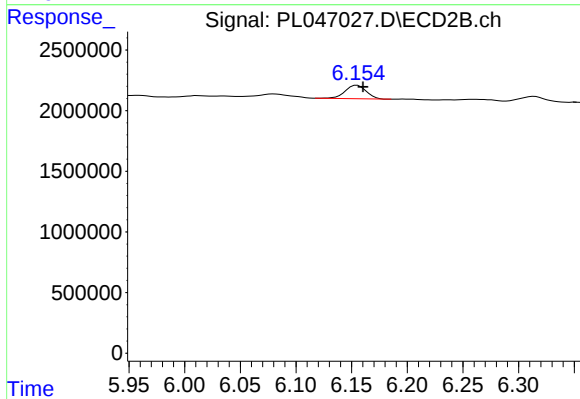

#11 alpha-Chlordane


R.T.: 6.155 min
Delta R.T.: -0.005 min
Response: 1470855
Conc: 0.52 ng/ml

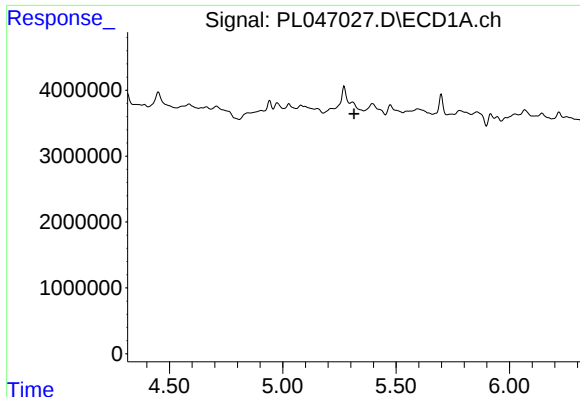

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.314 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

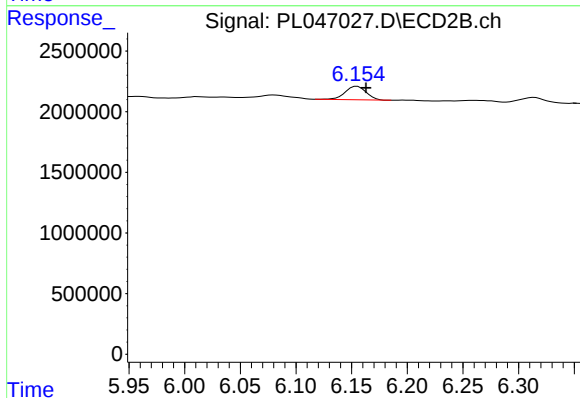


#26 Chlordane-4

R.T.: 6.155 min
Delta R.T.: -0.008 min
Response: 1470855
Conc: 3.19 ng/ml

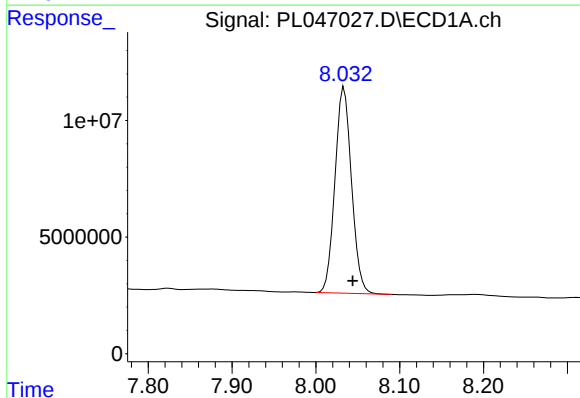

#28 Decachlorobiphenyl

R.T.: 8.034 min
Delta R.T.: -0.010 min
Response: 120771177
Conc: 14.36 ng/ml

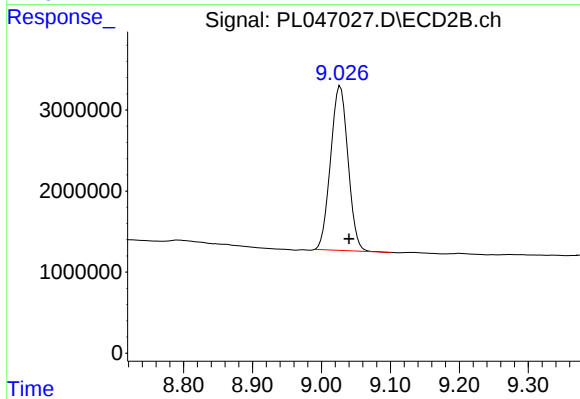

#28 Decachlorobiphenyl

R.T.: 9.027 min
Delta R.T.: -0.012 min
Response: 35541628
Conc: 15.33 ng/ml