

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040419\
 Data File : PL047059.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Apr 2019 23:29
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 01:21:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.357	3.976	157.2E6	50950393	21.609	22.253
28)	SA Decachlor...	8.033	9.027	187.9E6	56700459	22.342	24.456
Target Compounds							
8)	B Heptachlo...	0.000	5.841	0	9739033	N.D.	3.693 #
10)	B gamma-Chl...	0.000	6.088	0	9150520	N.D.	3.224 #
14)	MA Endrin	0.000	6.678	0	5959596	N.D.	2.494 #
24)	Chlordane-2	4.709	0.000	38390080	0	101.181	N.D. #
25)	Chlordane-3	0.000	6.088	0	9150520	N.D.	24.000 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040419\
Data File : PL047059.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Apr 2019 23:29
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 01:21:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

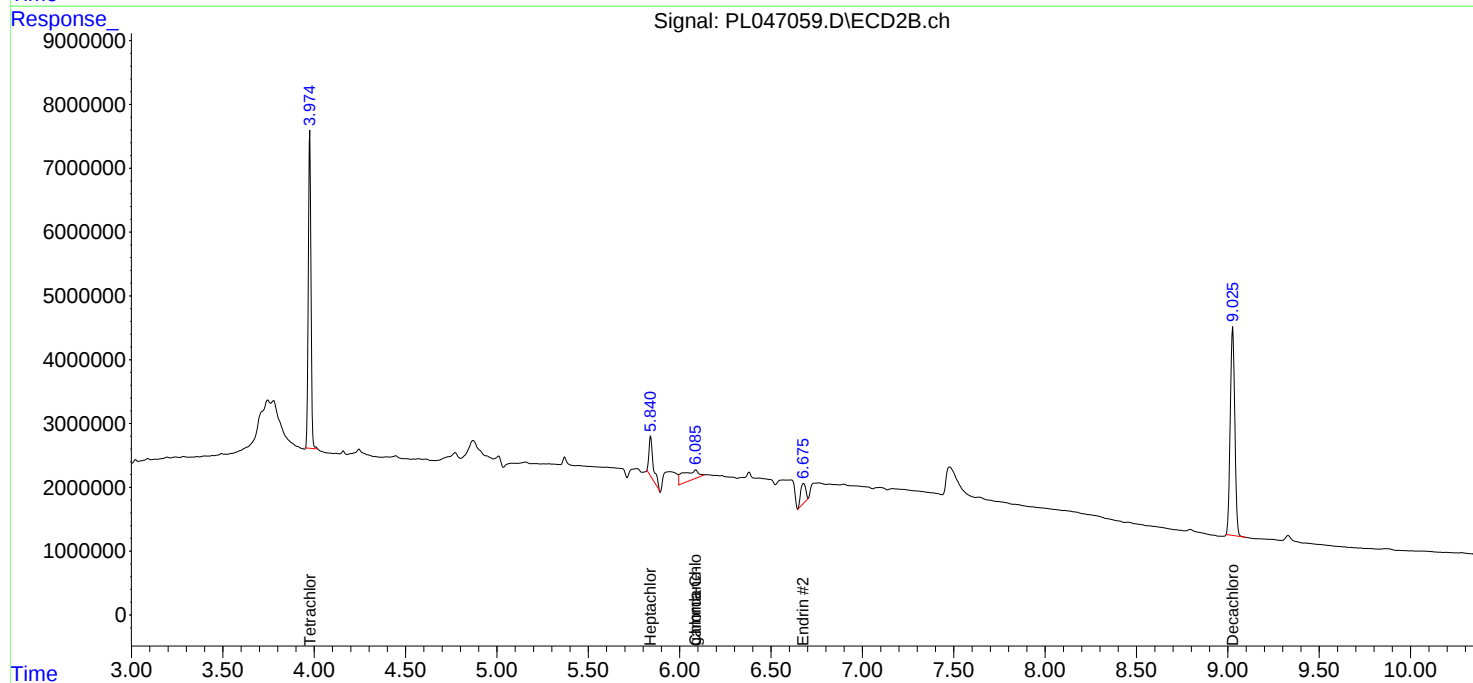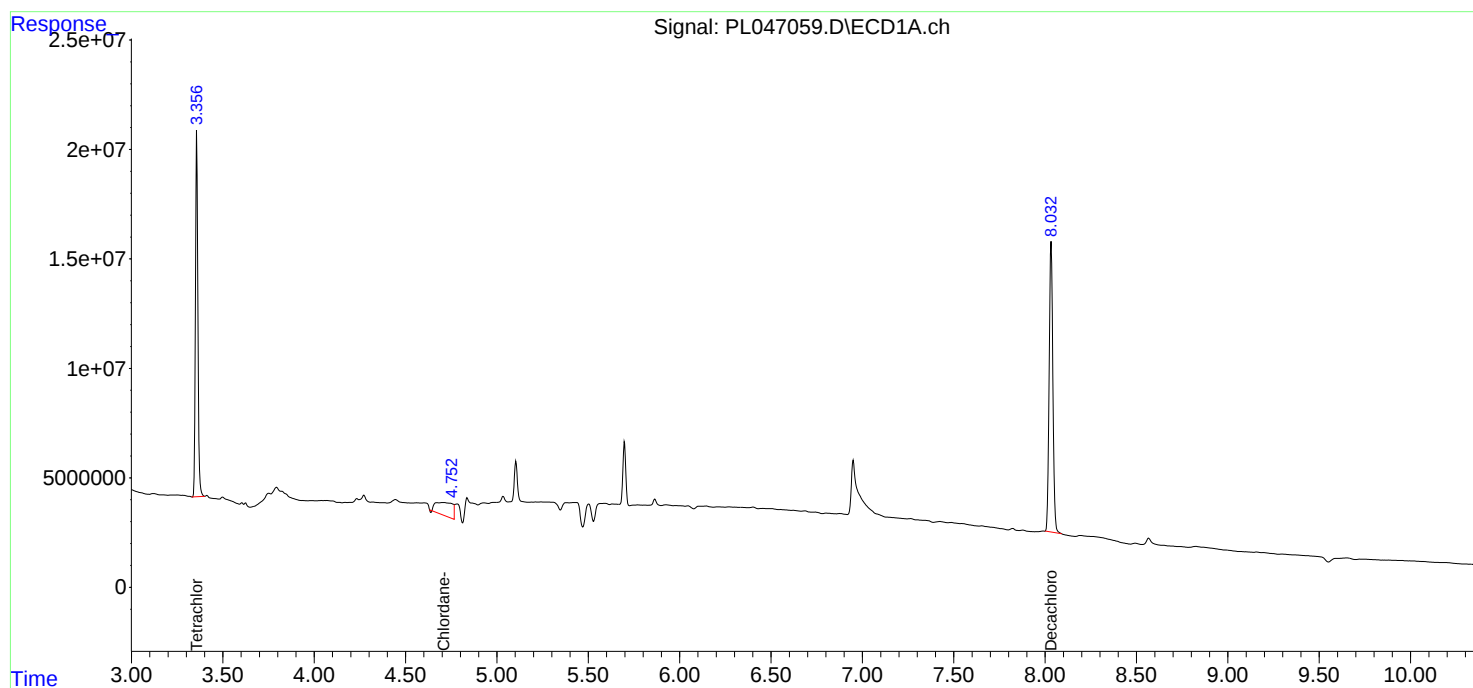


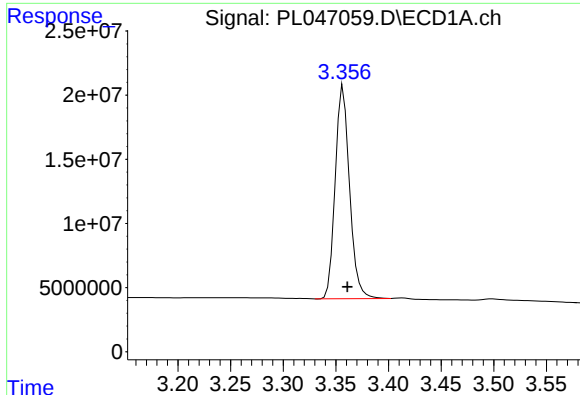

#1 Tetrachloro-m-xylene


R.T.: 3.357 min
Delta R.T.: -0.004 min
Response: 157198622
Conc: 21.61 ng/ml

Instrument :
ECD_L
ClientSampleId :

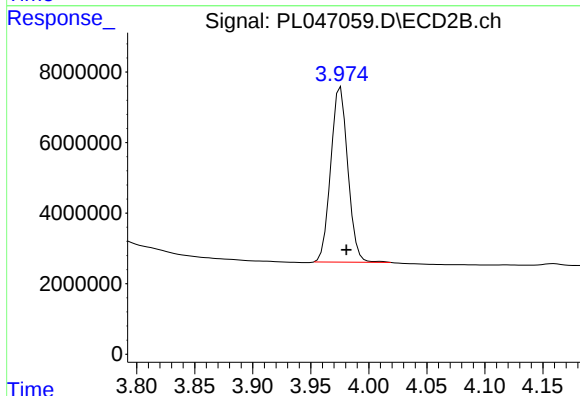


#1 Tetrachloro-m-xylene

R.T.: 3.976 min
Delta R.T.: -0.005 min
Response: 50950393
Conc: 22.25 ng/ml

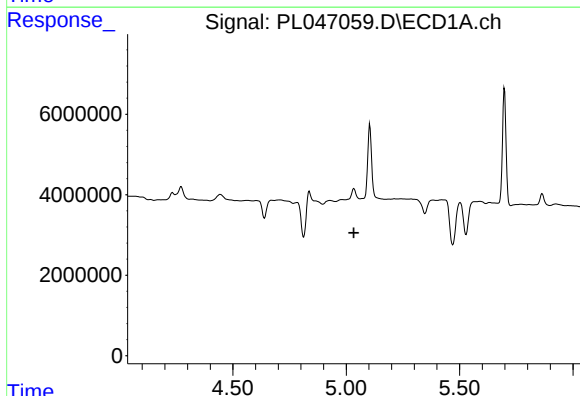


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.034 min
Response: 0
Conc: N.D.

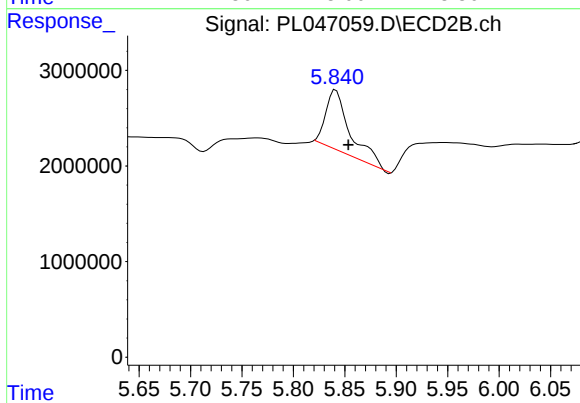

#8 Heptachlor epoxide


R.T.: 5.841 min
Delta R.T.: -0.012 min
Response: 9739033
Conc: 3.69 ng/ml

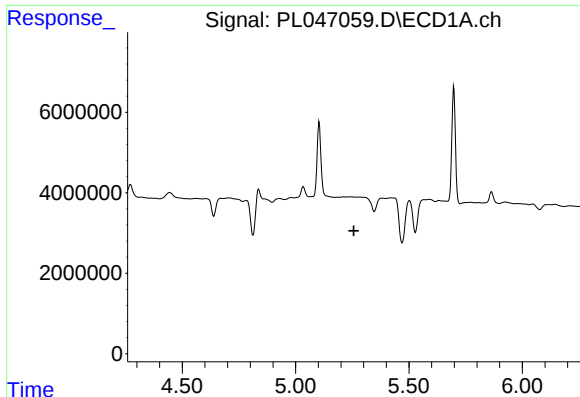

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.257 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

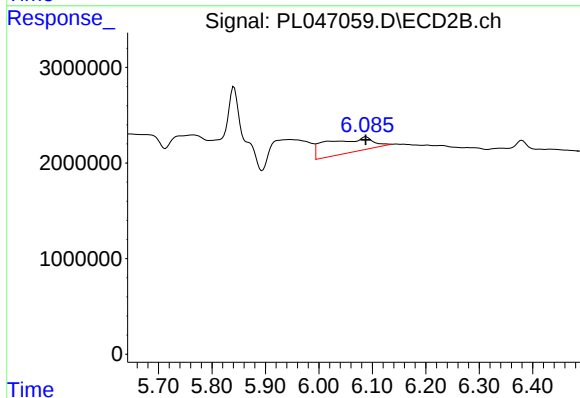


#10 gamma-Chlordane

R.T.: 6.088 min
Delta R.T.: 0.000 min
Response: 9150520
Conc: 3.22 ng/ml

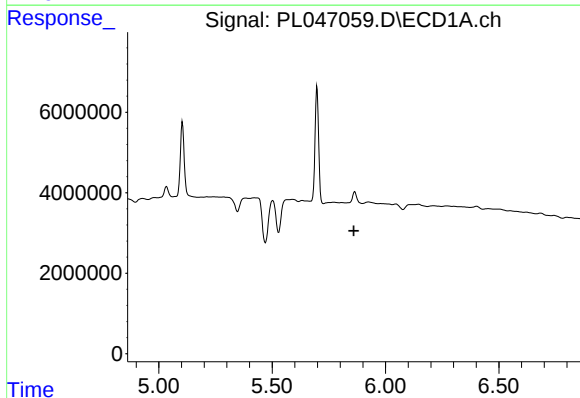


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 5.860 min
Response: 0
Conc: N.D.

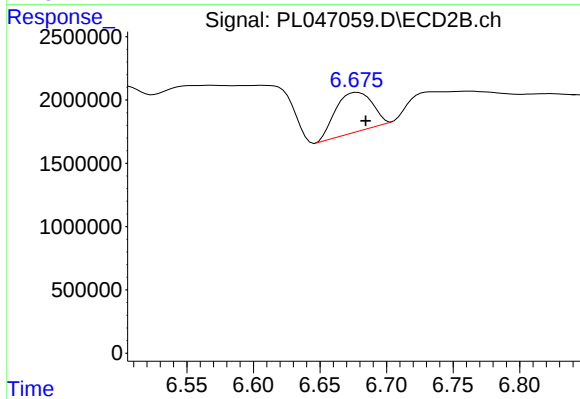

#14 Endrin


R.T.: 6.678 min
Delta R.T.: -0.006 min
Response: 5959596
Conc: 2.49 ng/ml

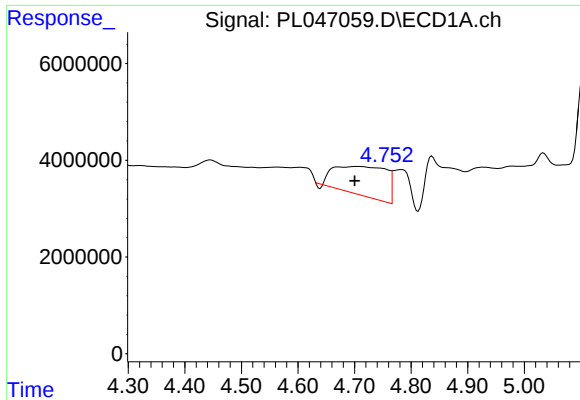

#24 Chlordane-2


R.T.: 4.709 min
Delta R.T.: 0.009 min
Response: 38390080
Conc: 101.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

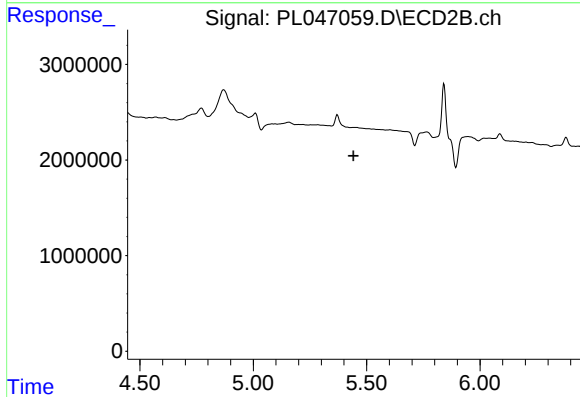


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.443 min
Response: 0
Conc: N.D.

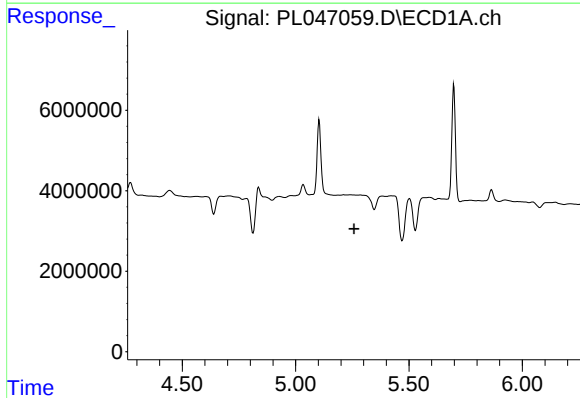


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.258 min
Response: 0
Conc: N.D.

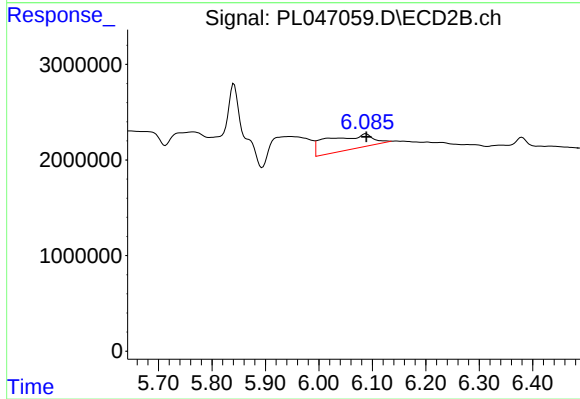

#25 Chlordane-3


R.T.: 6.088 min
Delta R.T.: 0.000 min
Response: 9150520
Conc: 24.00 ng/ml

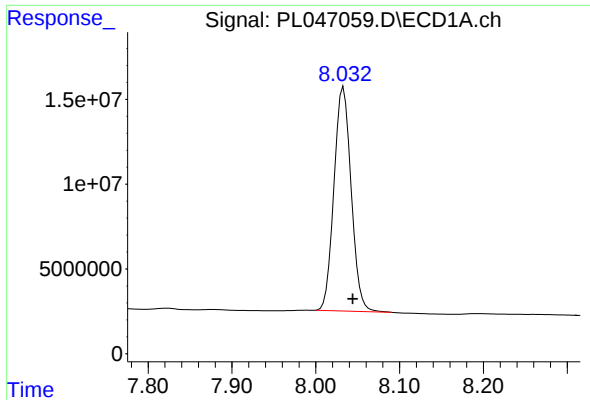

#28 Decachlorobiphenyl

R.T.: 8.033 min
Delta R.T.: -0.011 min
Response: 187920623
Conc: 22.34 ng/ml

Instrument :
ECD_L
ClientSampleId :

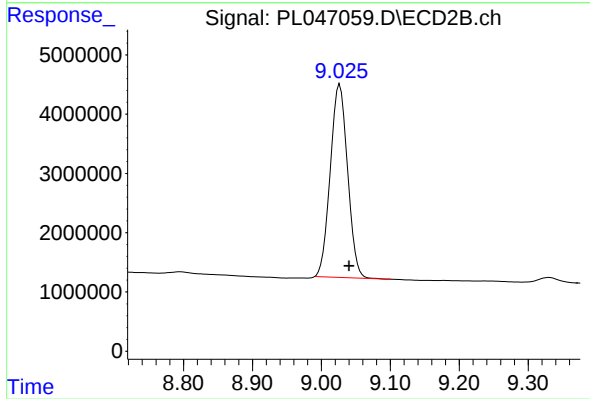

#28 Decachlorobiphenyl

R.T.: 9.027 min
Delta R.T.: -0.013 min
Response: 56700459
Conc: 24.46 ng/ml