

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040419\
 Data File : PL047044.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Apr 2019 19:39
 Operator : AJ\SJ
 Sample : K2244-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FK-EF-01-007-ABCD

Manual Integrations
 APPROVED

Sohil
 4/5/2019 11:32:33 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 01:18:33 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.357	3.976	60783709	19908583	8.356	8.695
28)	SA Decachlor...	8.033	9.026	76452547	24770160	9.090	10.684
Target Compounds							
12)	B 4,4'-DDE	5.471	6.310	85385038	32822355	9.274m	13.222 #
17)	MA 4,4'-DDT	6.218	7.096	82933001	14136094	10.949	6.741m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040419\
Data File : PL047044.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Apr 2019 19:39
Operator : AJ\SJ
Sample : K2244-01
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
FK-EF-01-007-ABCD


Manual Integrations
APPROVED

Sohil
4/5/2019 11:32:33 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 01:18:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

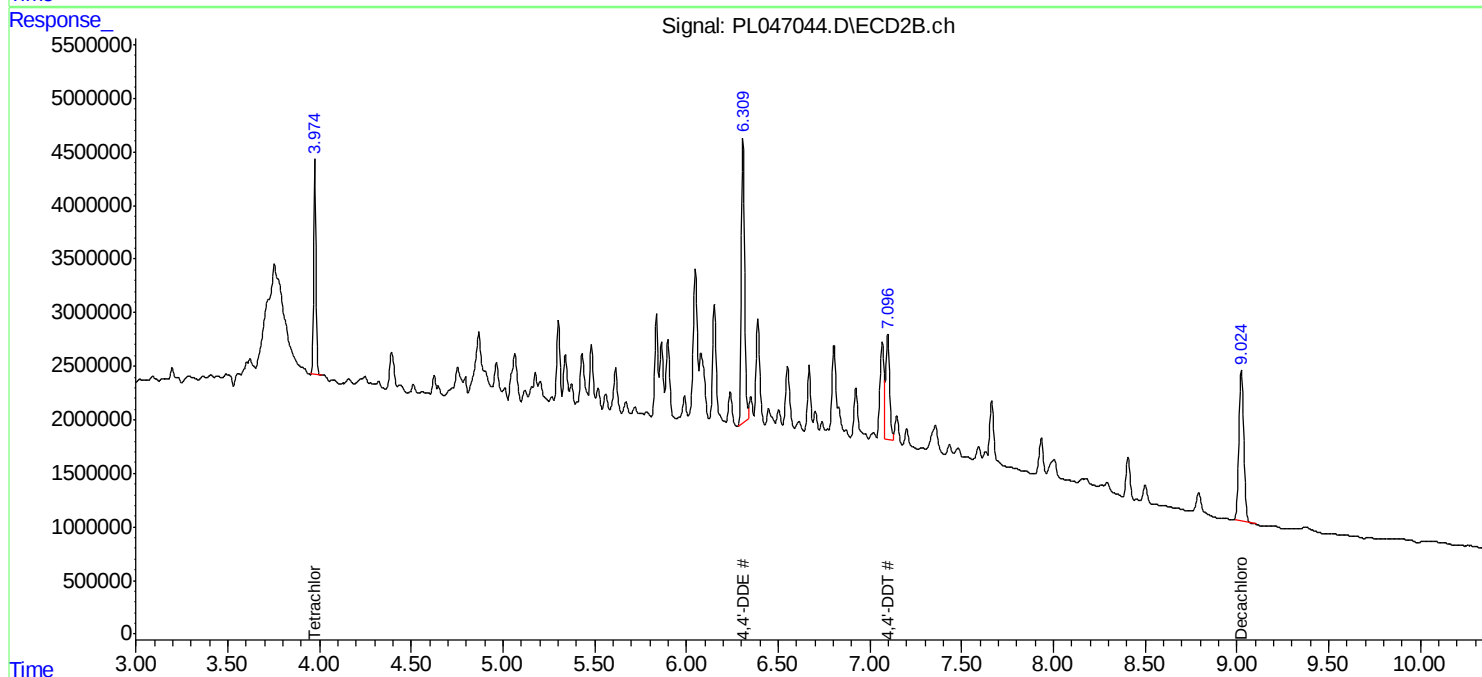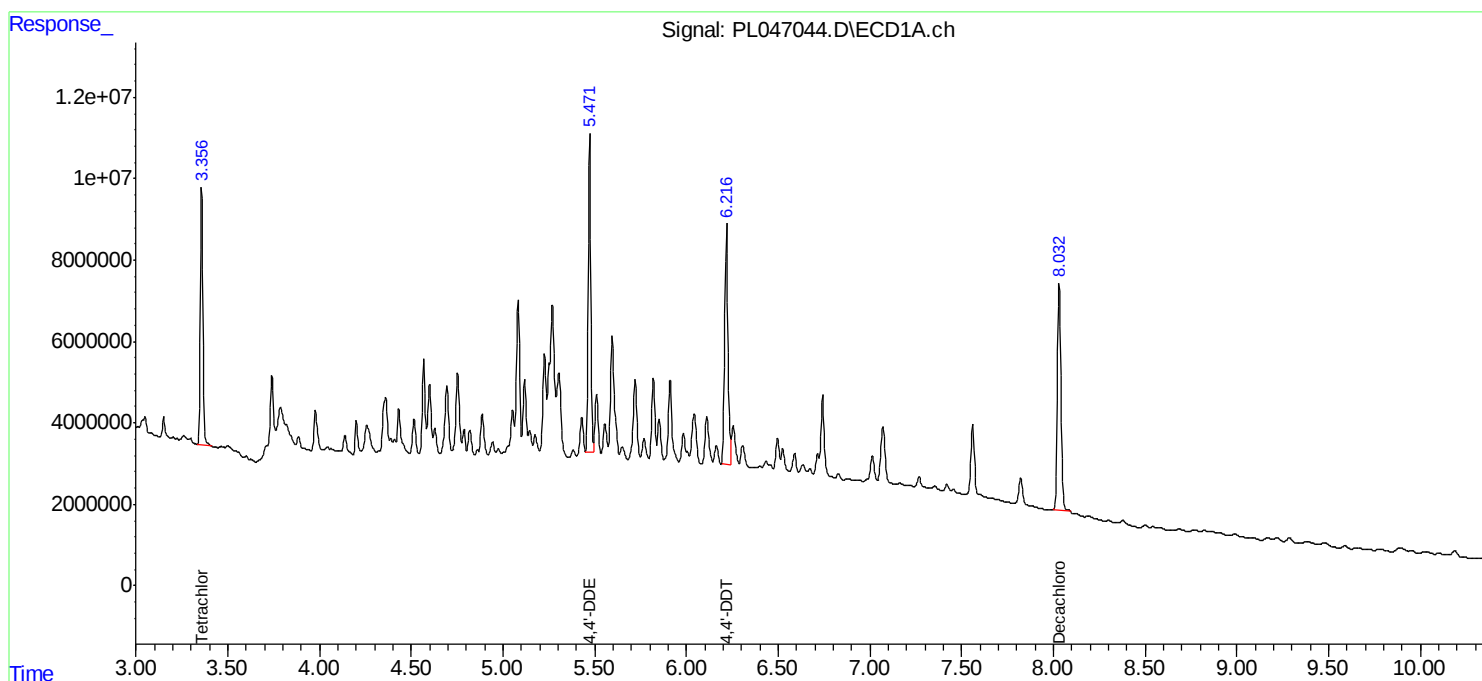

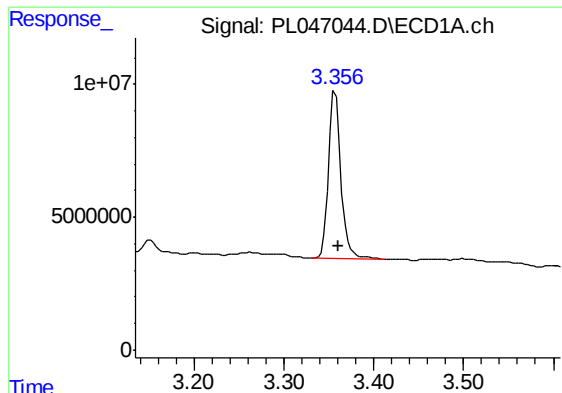


#1 Tetrachloro-m-xylene

R.T.: 3.357 min
Delta R.T.: -0.004 min
Response: 60783709
Conc: 8.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-EF-01-007-ABCD


Manual Integrations
APPROVED

Sohil
4/5/2019 11:32:33 AM

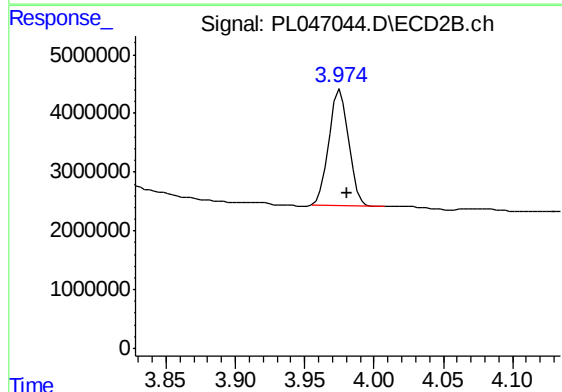


#1 Tetrachloro-m-xylene

R.T.: 3.976 min
Delta R.T.: -0.005 min
Response: 19908583
Conc: 8.70 ng/ml

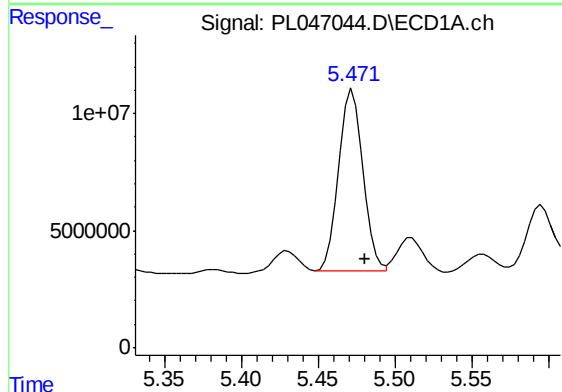


#12 4,4'-DDE

R.T.: 5.471 min
Delta R.T.: -0.010 min
Response: 85385038
Conc: 9.27 ng/ml m

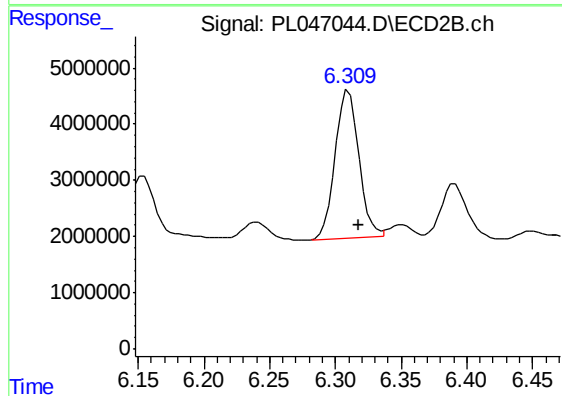

#12 4,4'-DDE

R.T.: 6.310 min
Delta R.T.: -0.008 min
Response: 32822355
Conc: 13.22 ng/ml

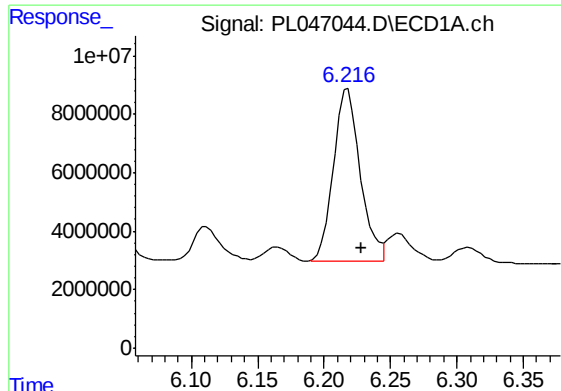


#17 4,4'-DDT

R.T.: 6.218 min
Delta R.T.: -0.010 min
Response: 82933001
Conc: 10.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-EF-01-007-ABCD


Manual Integrations
APPROVED

Sohil
4/5/2019 11:32:33 AM

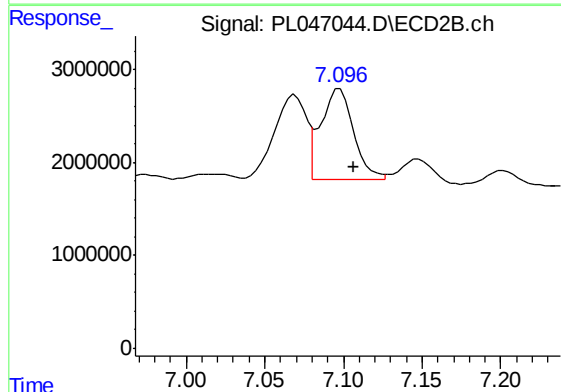


#17 4,4'-DDT

R.T.: 7.096 min
Delta R.T.: -0.010 min
Response: 14136094
Conc: 6.74 ng/ml m

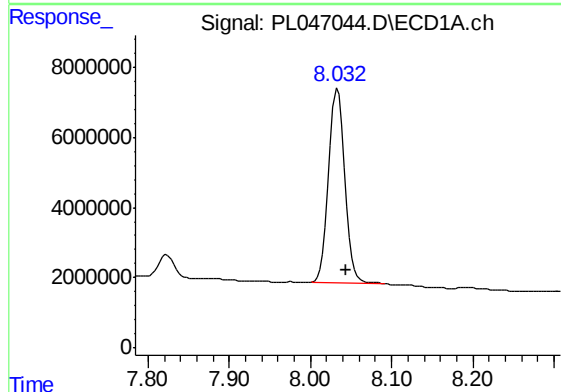

#28 Decachlorobiphenyl

R.T.: 8.033 min
Delta R.T.: -0.011 min
Response: 76452547
Conc: 9.09 ng/ml

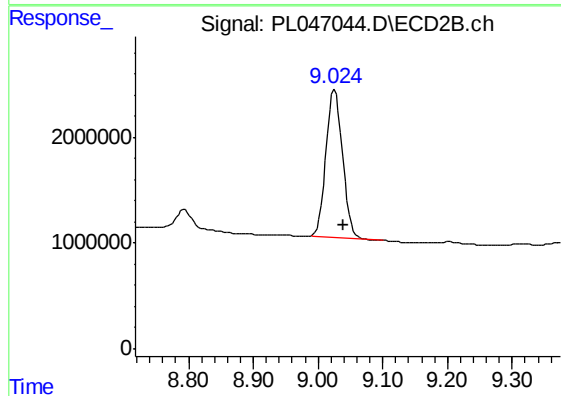

#28 Decachlorobiphenyl

R.T.: 9.026 min
Delta R.T.: -0.014 min
Response: 24770160
Conc: 10.68 ng/ml